

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022516\
 Data File : BM004404.D
 Acq On : 25 Feb 2016 17:55
 Operator : SJ/UM
 Sample : H1572-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-S56-0312

Quant Time: Feb 26 01:32:50 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 26 01:28:38 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	23738	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	115778	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.28	164	73607	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	162441	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	140339	20.00	ng/ul	0.00
86) Perylene-d12	23.47	264	123525	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.08	96	1080	2.40	ng/uL	0.00
5) Phenol-d5	6.81	99	25118	12.62	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	14142	13.97	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	23351	13.60	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	21389	12.03	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	11941	13.56	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	13386	13.33	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	23707	13.06	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	32209	14.24	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	91465	14.49	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	108155	14.63	ng/ul	0.00
52) 4-Nitrophenol-d4	14.54	143	8129	8.01	ng/ul	0.01
58) Fluorene-d10	15.28	176	78809	14.68	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	8204	8.22	ng/ul	0.00
71) Anthracene-d10	17.13	188	118488	14.89	ng/ul	0.00
79) Pyrene-d10	19.44	212	121667	17.92	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.33	264	96155	14.83	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.74	163	47530	7.22	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022516\
Data File : BM004404.D
Acq On : 25 Feb 2016 17:55
Operator : SJ/UM
Sample : H1572-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-S56-0312

Quant Time: Feb 26 01:32:50 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 26 01:28:38 2016
Response via : Initial Calibration

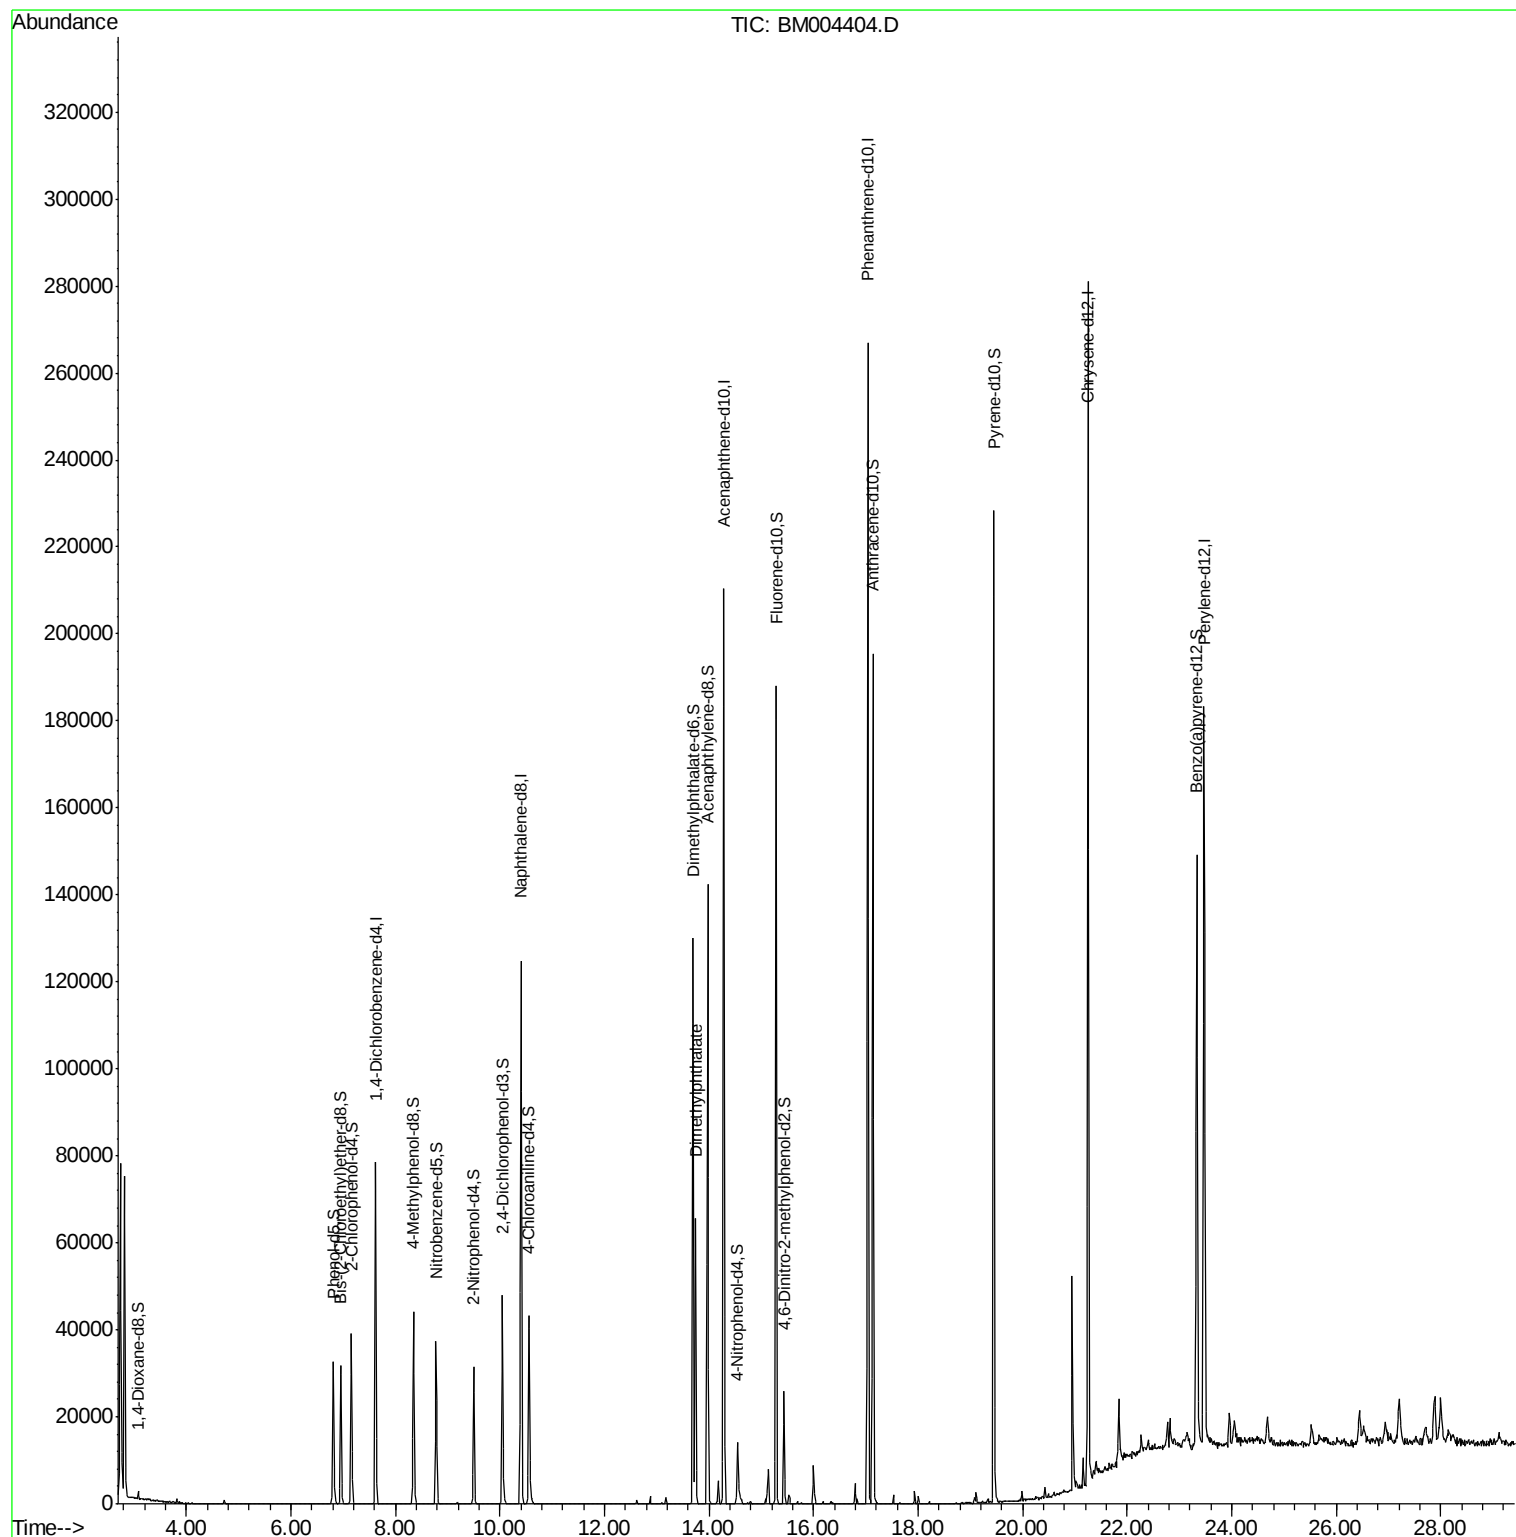

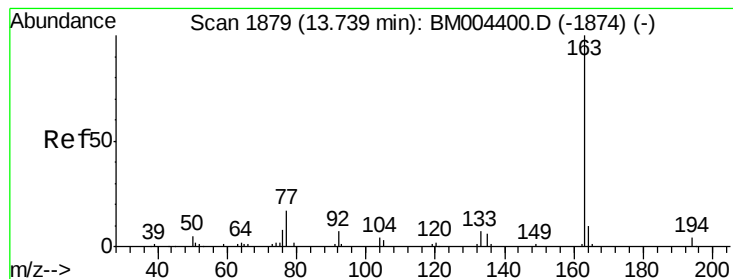

#45

Dimethylphthalate

Concen: 7.22 ng/ul

RT: 13.74 min Scan# 1879

Delta R.T. 0.00 min

Lab File: BM004404.D


Acq: 25 Feb 2016 17:55

Instrument :

BNA_M

ClientSampleId :

0311-S56-0312

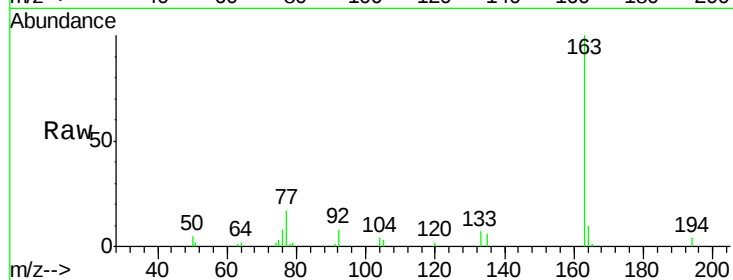

Tgt Ion:163 Resp: 47530

Ion Ratio Lower Upper

163 100

194 4.0 3.2 4.8

164 10.2 7.8 11.8

