

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022516\
 Data File : BM004407.D
 Acq On : 25 Feb 2016 19:44
 Operator : SJ/UM
 Sample : H1572-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-S44-0003

Quant Time: Feb 26 01:33:16 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 26 01:28:38 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	24713	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	117987	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.28	164	71555	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	148328	20.00	ng/ul	0.00
78) Chrysene-d12	21.25	240	133552	20.00	ng/ul	0.00
86) Perylene-d12	23.47	264	125384	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.08	96	2499	5.33	ng/uL	0.00
5) Phenol-d5	6.80	99	57735	27.86	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	30908	29.33	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	52837	29.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	50726	27.39	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	26581	29.61	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	31203	30.49	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	53298	28.82	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	67619	29.33	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	181281	29.54	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	222340	30.95	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	20160	20.44	ng/ul	0.00
58) Fluorene-d10	15.28	176	154742	29.65	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	20106	22.07	ng/ul	0.00
71) Anthracene-d10	17.13	188	226790	31.20	ng/ul	0.00
79) Pyrene-d10	19.44	212	231295	35.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.33	264	209234	31.80	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.74	163	89988	14.06	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022516\
Data File : BM004407.D
Acq On : 25 Feb 2016 19:44
Operator : SJ/UM
Sample : H1572-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-S44-0003

Quant Time: Feb 26 01:33:16 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 26 01:28:38 2016
Response via : Initial Calibration

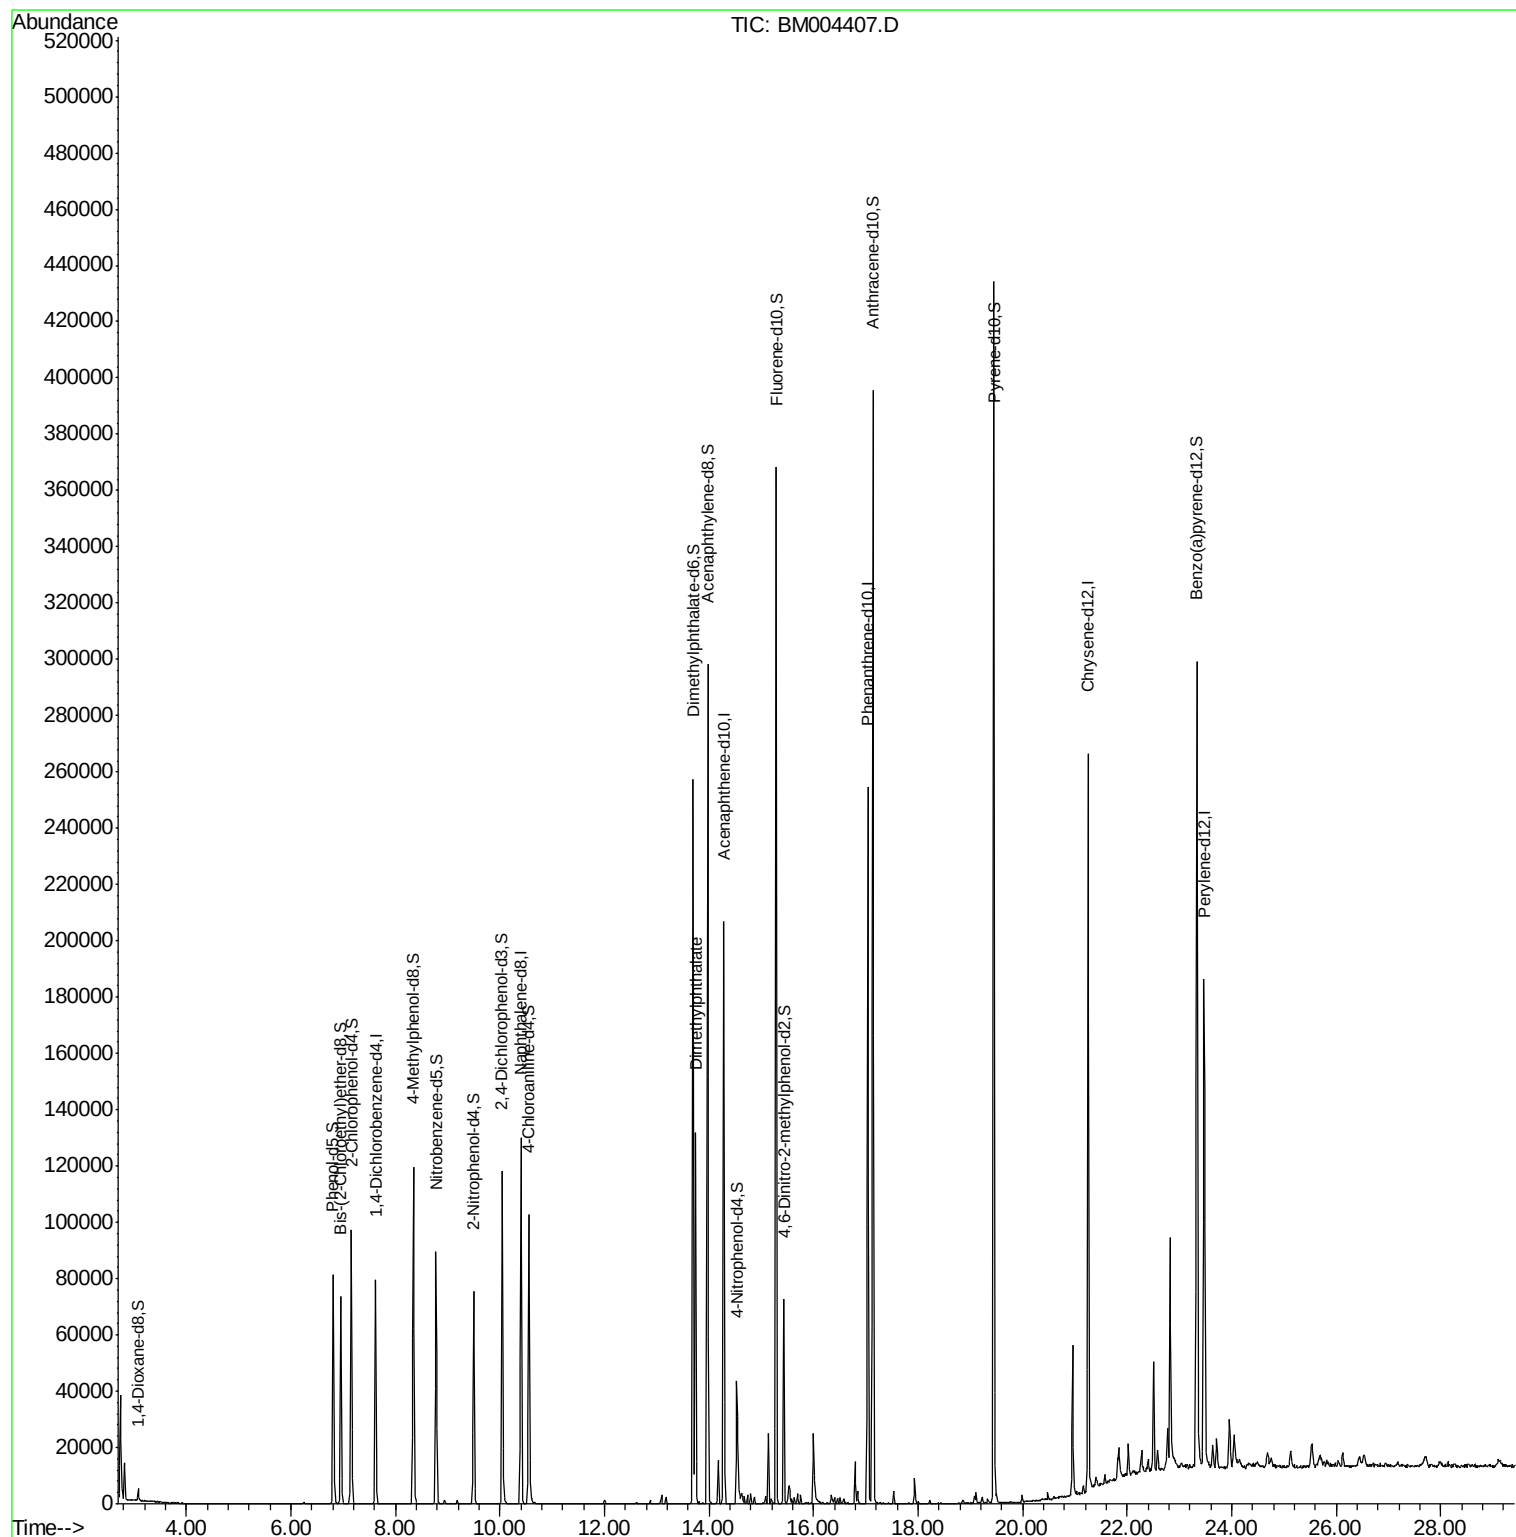

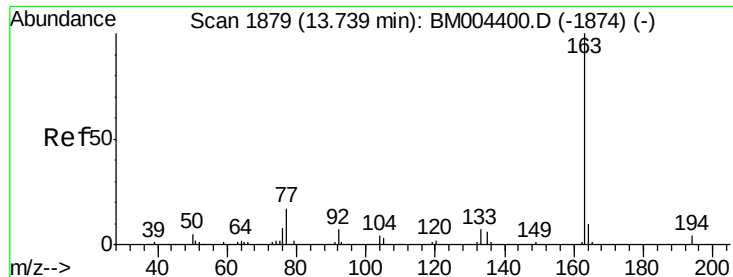

#45

Dimethylphthalate

Concen: 14.06 ng/ul

RT: 13.74 min Scan# 1879

Delta R.T. 0.00 min

Lab File: BM004407.D


Acq: 25 Feb 2016 19:44

Instrument :

BNA_M

ClientSampleId :

0311-S44-0003

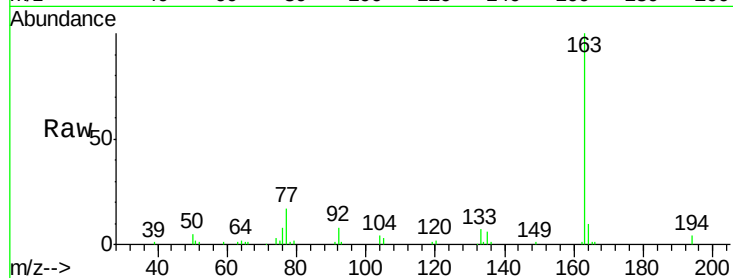

Tgt Ion:163 Resp: 89988

Ion Ratio Lower Upper

163 100

194 4.2 3.2 4.8

164 9.7 7.8 11.8

