

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022516\
 Data File : BM004412.D
 Acq On : 25 Feb 2016 23:21
 Operator : SJ/UM
 Sample : H1572-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-S54-0003

Quant Time: Feb 26 03:56:12 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 26 03:49:40 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	27679	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	131978	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	81558	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	175176	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	151517	20.00	ng/ul	0.00
86) Perylene-d12	23.47	264	139374	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.08	96	2233	4.25	ng/uL	0.00
5) Phenol-d5	6.80	99	52996	22.83	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	28975	24.55	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	49106	24.53	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	47545	22.92	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	24736	24.64	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	28696	25.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	49890	24.11	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	71253	27.63	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	179470	25.66	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	216366	26.42	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	19998	17.79	ng/ul	0.00
58) Fluorene-d10	15.27	176	154956	26.05	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.42	200	19791	18.39	ng/ul	0.00
71) Anthracene-d10	17.13	188	232499	27.09	ng/ul	0.00
79) Pyrene-d10	19.44	212	233061	31.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.33	264	204045	27.90	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.74	163	96698	13.26	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022516\
Data File : BM004412.D
Acq On : 25 Feb 2016 23:21
Operator : SJ/UM
Sample : H1572-12
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-S54-0003

Quant Time: Feb 26 03:56:12 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 26 03:49:40 2016
Response via : Initial Calibration

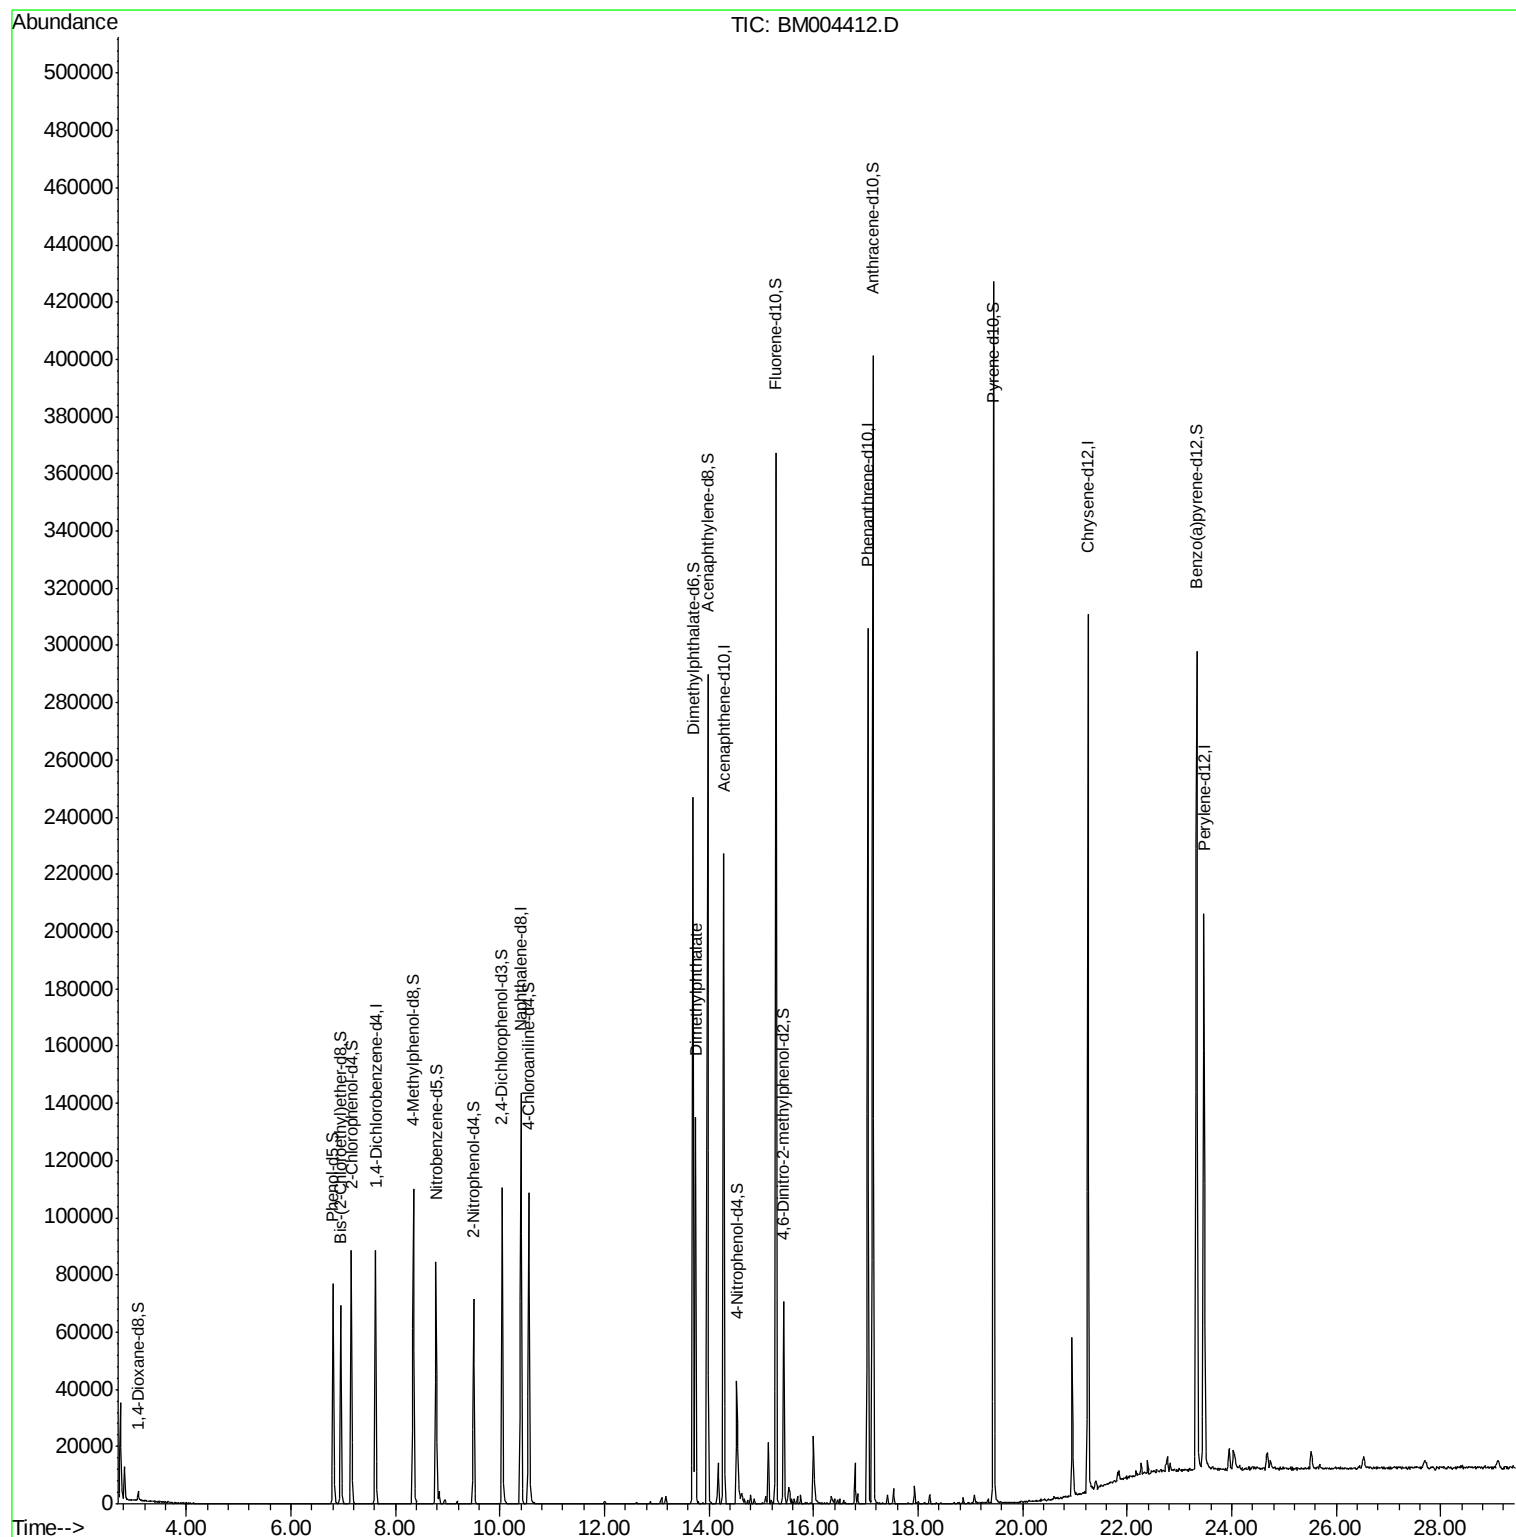

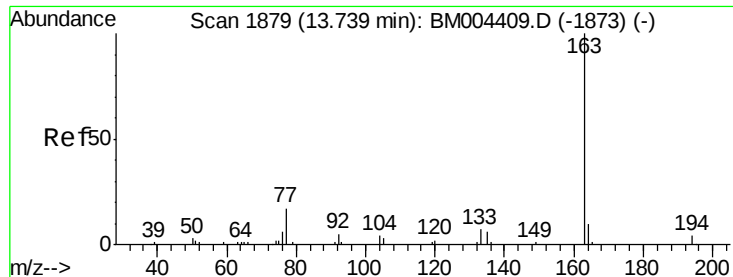

#45

Dimethylphthalate

Concen: 13.26 ng/ul

RT: 13.74 min Scan# 1879

Delta R.T. 0.00 min

Lab File: BM004412.D


Acq: 25 Feb 2016 23:21

Instrument :

BNA_M

ClientSampleId :

0311-S54-0003

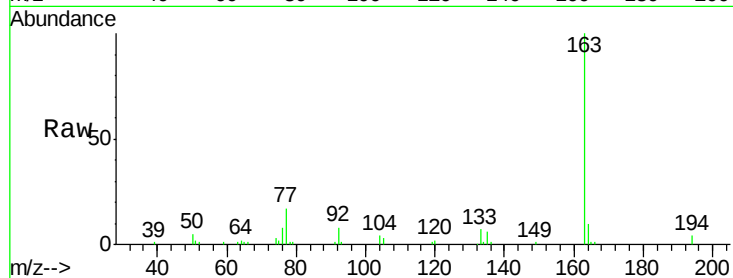


Tgt Ion:163 Resp: 96698

Ion Ratio Lower Upper

163 100

194 4.1 3.2 4.8

164 9.8 7.8 11.8

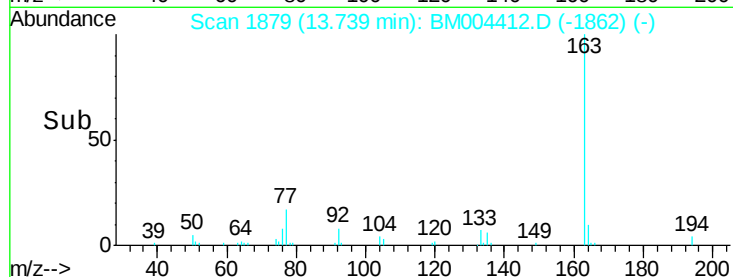

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

