

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022516\
 Data File : BM004414.D
 Acq On : 26 Feb 2016 00:34
 Operator : SJ/UM
 Sample : H1572-14
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 0311-S59-0003

Quant Time: Feb 26 03:56:27 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 26 03:49:40 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	24951	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	113169	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.28	164	62978	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	131757	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	134118	20.00	ng/ul	0.00
86) Perylene-d12	23.46	264	131502	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.08	96	2115	4.47	ng/uL	0.00
5) Phenol-d5	6.80	99	50400	24.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	27280	25.64	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	47092	26.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	44195	23.64	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	22849	26.54	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	26031	26.52	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	45314	25.54	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	62428	28.23	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	144743	26.80	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	180795	28.59	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	14734	16.97	ng/ul	0.00
58) Fluorene-d10	15.27	176	124884	27.19	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	14760	18.24	ng/ul	0.00
71) Anthracene-d10	17.13	188	183291	28.39	ng/ul	0.00
79) Pyrene-d10	19.44	212	195474	30.13	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.32	264	200012	28.98	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.74	163	77194	13.71	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022516\
Data File : BM004414.D
Acq On : 26 Feb 2016 00:34
Operator : SJ/UM
Sample : H1572-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
0311-S59-0003

Quant Time: Feb 26 03:56:27 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 26 03:49:40 2016
Response via : Initial Calibration

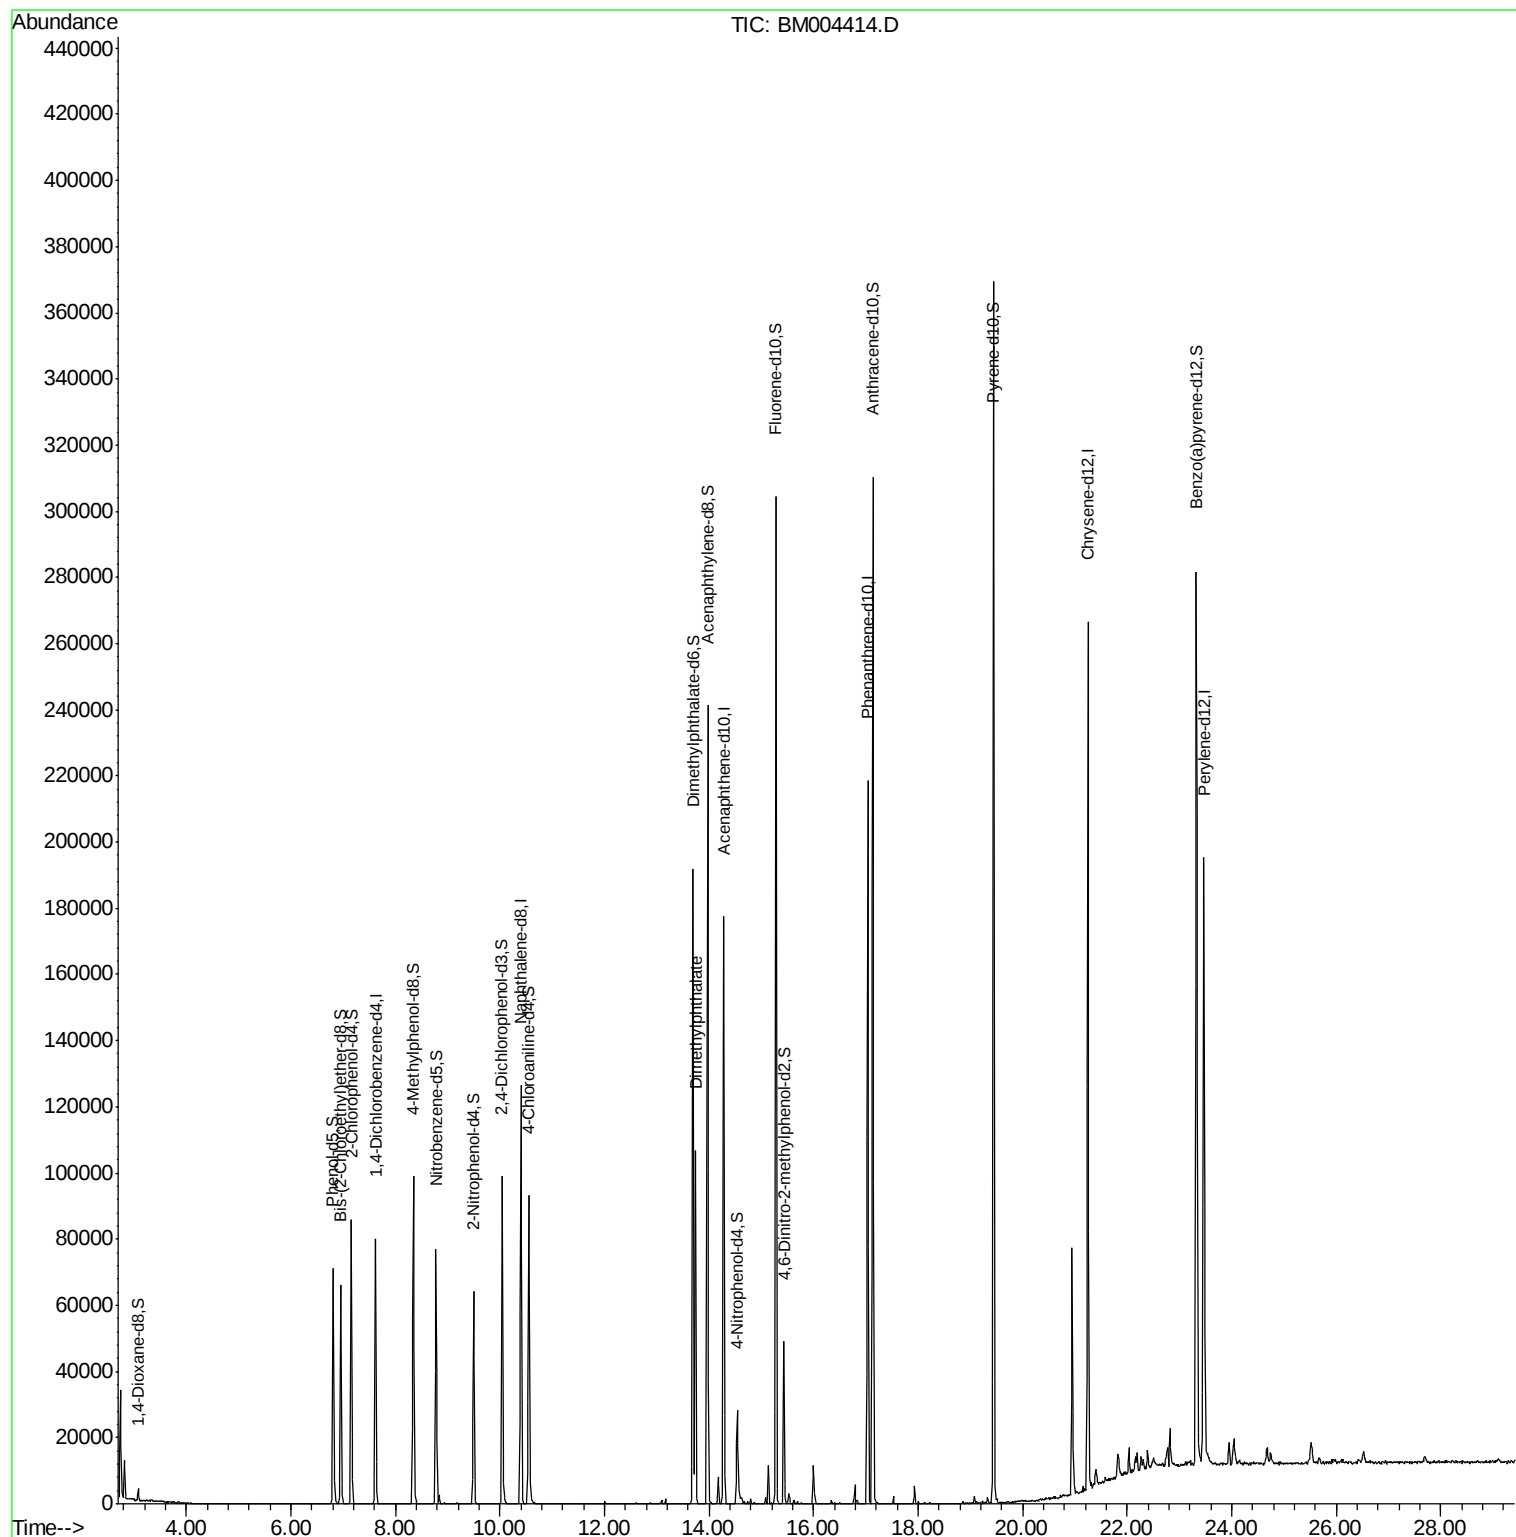

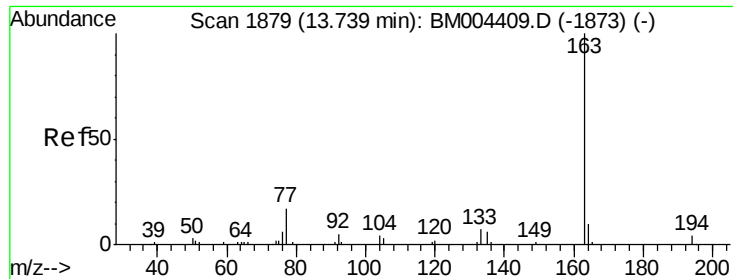

#45

Dimethylphthalate

Concen: 13.71 ng/ul

RT: 13.74 min Scan# 1879

Delta R.T. 0.00 min

Lab File: BM004414.D


Acq: 26 Feb 2016 00:34

Instrument :

BNA_M

ClientSampleId :

0311-S59-0003

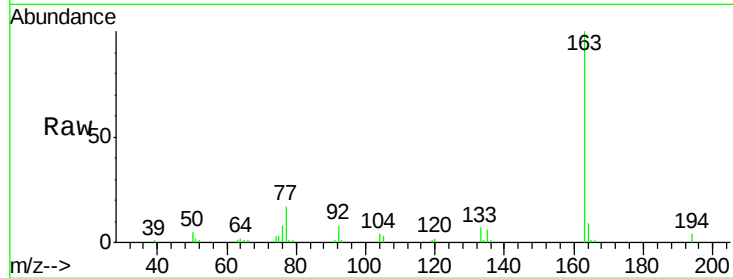

Tgt Ion:	163	Resp:	77194
Ion	Ratio	Lower	Upper
163	100		
194	3.9	3.2	4.8
164	9.4	7.8	11.8

