


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022516\
 Data File : BM004399.D
 Acq On : 25 Feb 2016 10:37
 Operator : SJ/UM
 Sample : DFTPP56
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP56

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Title : SVOA CALIBRATION
 Last Update : Fri Feb 26 03:49:40 2016

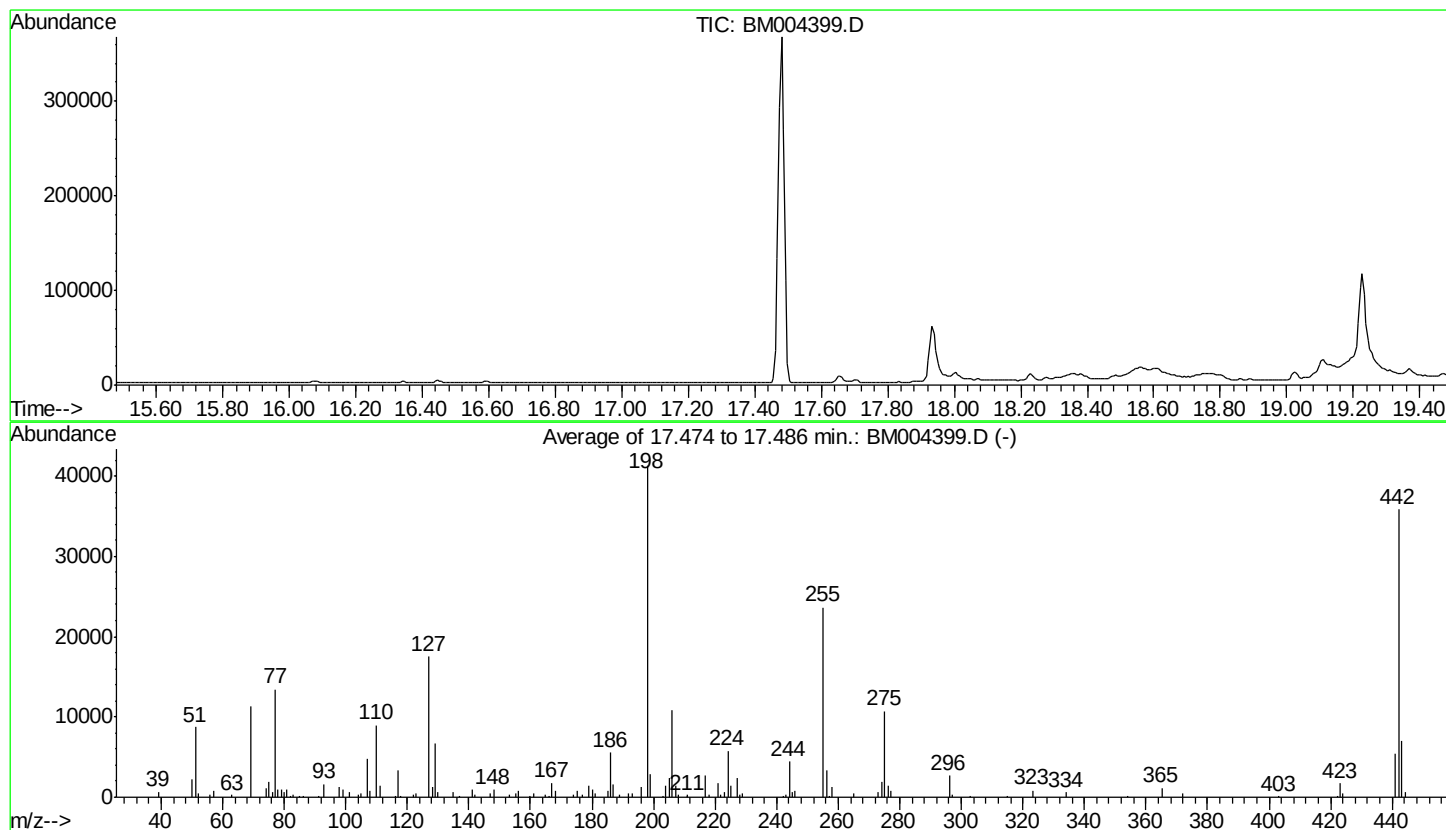

AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.1	8715	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	27.5	11371	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.3	17462	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	41290	PASS
199	198	5	9	6.9	2829	PASS
275	198	10	60	26.0	10743	PASS
365	198	1	100	2.8	1169	PASS
441	443	0.01	100	77.6	5487	PASS
442	198	50	100	86.7	35810	PASS
443	442	15	24	19.8	7074	PASS

Scan 2509 (17.445 min): BM004399.D
DFTPP56

m/z	Abundance
43.10	1204.0
45.00	925.0
60.00	729.0

Instrument :
BNA_M
ClientSampleId :
DFTPP56

m/z	Abundance
39.10	762.0
43.10	1072.0
45.00	728.0
50.10	2445.0
51.10	9550.0
52.00	550.0
56.00	378.0
57.00	910.0
60.00	662.0
63.00	440.0
69.00	12409.0
74.00	1236.0
75.00	1949.0
76.10	727.0
77.10	14497.0
78.00	995.0
79.00	1033.0
80.00	676.0
81.00	1068.0
83.00	395.0
85.10	306.0
86.00	331.0
91.00	319.0
93.00	1733.0
98.00	1370.0
99.00	1024.0
101.00	612.0
104.00	456.0
105.00	470.0
107.00	5070.0
108.00	837.0
110.00	9264.0
111.00	1457.0
117.00	3440.0
118.00	304.0
122.00	351.0
123.00	578.0
127.10	18128.0
128.10	1408.0
129.00	7008.0
130.00	633.0
135.00	628.0
137.10	329.0
141.00	952.0
142.00	300.0
147.00	483.0
148.00	986.0
153.00	306.0
155.00	544.0
156.10	778.0
161.00	470.0
165.00	381.0
167.00	1762.0
168.00	770.0
174.00	388.0
175.00	706.0
176.90	372.0
179.00	1381.0
180.00	1015.0
181.00	493.0
185.00	766.0
186.10	5408.0
187.10	1671.0
189.00	374.0
192.00	361.0
193.00	507.0
196.00	1227.0
198.00	39752.0
199.00	2764.0
204.00	1303.0
205.10	2291.0
206.10	10043.0
207.10	1402.0
208.00	329.0
210.90	409.0
217.00	2546.0
218.00	350.0
221.10	1668.0
221.80	468.0
223.00	539.0
224.10	5453.0
225.00	1420.0
227.00	2332.0
228.00	308.0
229.00	498.0
243.10	346.0
244.10	4003.0
245.10	569.0
246.00	762.0
255.10	21264.0
256.10	3150.0

Instrument :
BNA_M
ClientSampleId :
DFTPP56

258.00	1116.0
265.00	438.0
273.00	596.0
274.00	1682.0
275.10	9403.0
276.10	1204.0
277.10	691.0
296.10	2279.0
297.00	326.0
323.10	737.0
334.10	517.0
365.10	951.0
372.10	375.0
423.10	1252.0
424.10	339.0
441.10	4078.0
442.10	26232.0
443.10	5412.0
444.10	558.0

Instrument :
BNA_M
ClientSampleId :
DFTPP56

m/z	Abundance
39.00	737.0
43.00	1075.0
45.00	753.0
50.10	2635.0
51.10	10059.0
52.10	522.0
56.00	404.0
57.00	982.0
60.00	637.0
63.00	505.0
69.00	13116.0
74.00	1371.0
75.00	2302.0
76.10	704.0
77.10	15570.0
78.10	1049.0
79.00	1082.0
80.00	866.0
81.00	1240.0
82.00	369.0
83.00	314.0
86.00	346.0
91.00	364.0
93.00	1844.0
98.00	1520.0
99.00	1150.0
101.00	674.0
104.00	491.0
105.00	503.0
107.00	5398.0
108.00	846.0
110.00	10372.0
111.00	1793.0
116.00	356.0
117.00	3927.0
122.10	403.0
123.00	577.0
127.00	20520.0
128.10	1531.0
129.00	7803.0
130.00	731.0
135.00	746.0
141.00	1191.0
142.00	350.0
147.00	563.0
148.00	1055.0
153.00	373.0
155.00	570.0
156.00	956.0
160.00	321.0
161.00	586.0
164.90	366.0
166.00	326.0
167.00	2213.0
168.00	879.0
174.00	469.0
175.00	861.0
177.00	434.0
179.00	1612.0
180.00	1046.0
181.00	546.0
185.00	915.0
186.10	6592.0
187.10	1928.0
189.00	435.0
192.00	546.0
193.00	592.0
196.00	1533.0
198.00	48512.0
199.00	3295.0
203.00	321.0
204.00	1752.0
205.10	2932.0
206.10	13159.0
207.10	1539.0
208.10	425.0
211.10	395.0
217.00	3156.0
218.00	429.0
221.10	2183.0
221.80	534.0
223.00	697.0
224.10	6965.0
225.00	1765.0
227.00	2903.0
228.00	373.0
229.00	544.0
242.00	333.0
243.10	351.0
244.10	5265.0
245.10	720.0

Instrument :
BNA_M
ClientSampleId :
DFTPP56

246.00	951.0
255.10	27960.0
256.10	3855.0
257.10	329.0
258.00	1519.0
265.10	611.0
273.00	752.0
274.10	2273.0
275.10	12962.0
276.10	1743.0
277.00	1153.0
296.10	3228.0
297.00	465.0
303.10	360.0
315.00	395.0
323.10	1009.0
334.10	726.0
354.10	344.0
365.10	1391.0
372.10	543.0
403.20	321.0
422.10	304.0
423.20	2045.0
424.10	467.0
441.10	6353.0
442.20	42456.0
443.20	8581.0
444.10	754.0

Instrument :
BNA_M
ClientSampleId :
DFTPP56

m/z	Abundance
39.00	572.0
43.00	1100.0
45.00	813.0
50.00	1650.0
51.10	6537.0
52.00	335.0
57.00	574.0
60.00	714.0
69.00	8590.0
74.00	785.0
75.00	1401.0
76.10	555.0
77.10	10117.0
78.10	675.0
79.00	697.0
80.00	541.0
81.00	799.0
83.00	305.0
93.00	1272.0
98.00	960.0
99.00	772.0
101.00	477.0
105.00	339.0
107.00	3810.0
108.00	595.0
110.00	7167.0
111.00	1098.0
117.00	2662.0
123.00	478.0
127.10	13739.0
128.00	1085.0
129.00	5325.0
130.00	479.0
135.00	534.0
141.00	701.0
142.00	308.0
147.00	434.0
148.00	832.0
153.00	304.0
155.10	450.0
156.00	691.0
161.00	375.0
167.10	1453.0
168.00	643.0
174.00	314.0
175.00	608.0
179.00	1136.0
180.00	848.0
181.00	417.0
185.00	575.0
186.10	4604.0
187.00	1301.0
192.00	383.0
193.00	417.0
196.00	972.0
198.00	35608.0
199.00	2430.0
204.10	1216.0
205.10	2096.0
206.10	9420.0
207.10	1314.0
208.00	317.0
211.00	370.0
217.00	2400.0
218.00	355.0
221.10	1547.0
223.10	598.0
224.10	5014.0
225.10	1367.0
227.00	2187.0
228.00	334.0
229.00	477.0
243.10	308.0
244.10	3973.0
245.10	595.0
246.00	741.0
255.10	21760.0
256.10	3199.0
258.00	1203.0
265.00	421.0
273.10	600.0
274.10	1627.0
275.10	9864.0
276.10	1305.0
277.00	774.0
296.10	2508.0
297.00	313.0
303.00	354.0
315.00	301.0
323.10	862.0
334.10	598.0

Instrument :
BNA_M
ClientSampleId :
DFTPP56

365.10	1165.0
372.10	428.0
423.10	1852.0
424.10	408.0
441.20	6031.0
442.20	38744.0
443.10	7229.0
444.10	558.0

Instrument :
BNA_M
ClientSampleId :
DFTPP56