
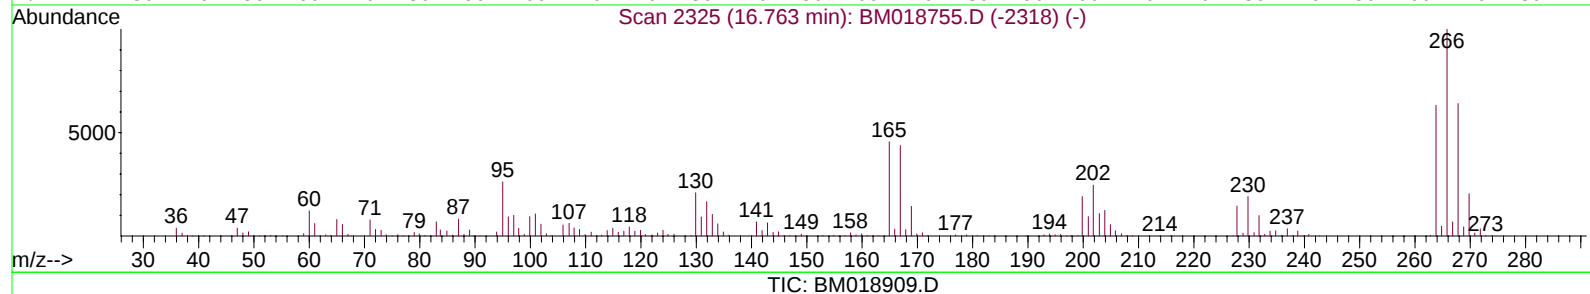
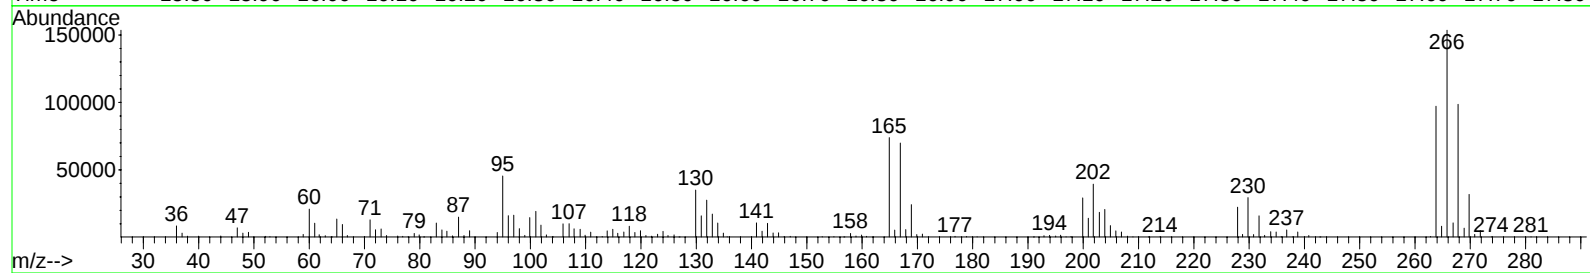


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022519\
Data File : BM018909.D
Acq On : 25 Feb 2019 10:59
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 25 18:09:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

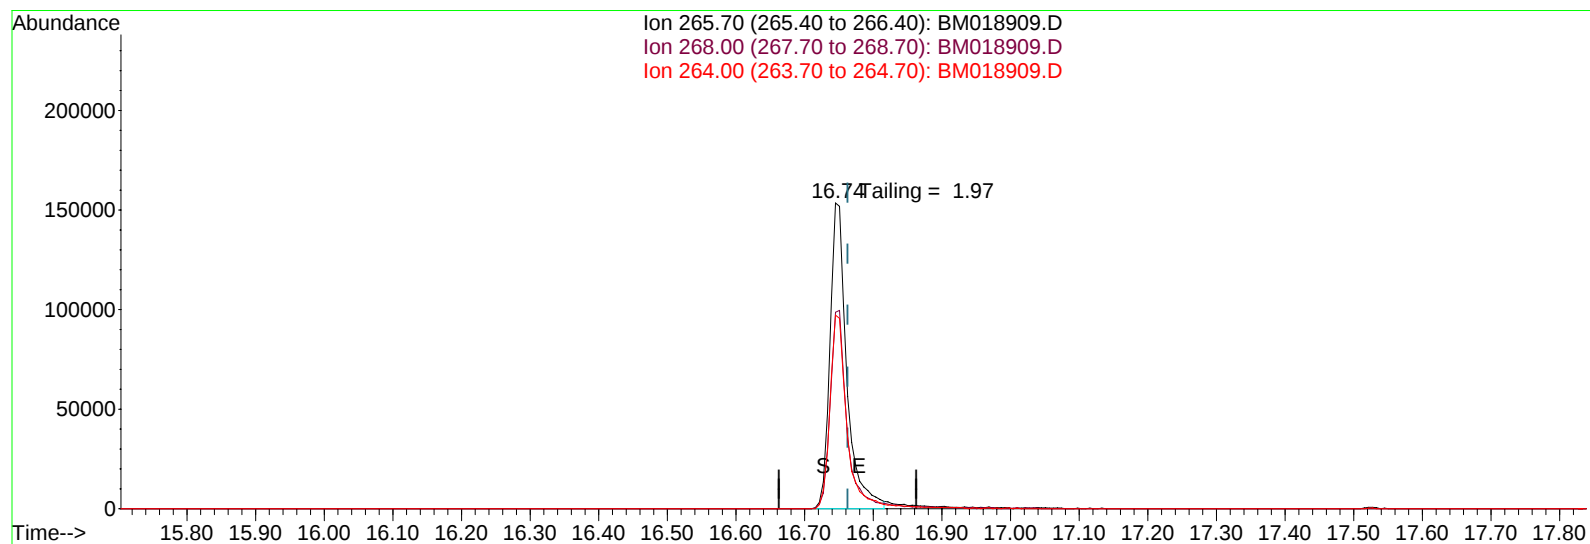

TIC: BM018909.D

(70) Pentachlorophenol (C)




16.745min (-0.018) 254502.83ng

response 266502

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	64.26
264.00	63.20	63.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022519\
Data File : BM018909.D
Acq On : 25 Feb 2019 10:59
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 25 18:09:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

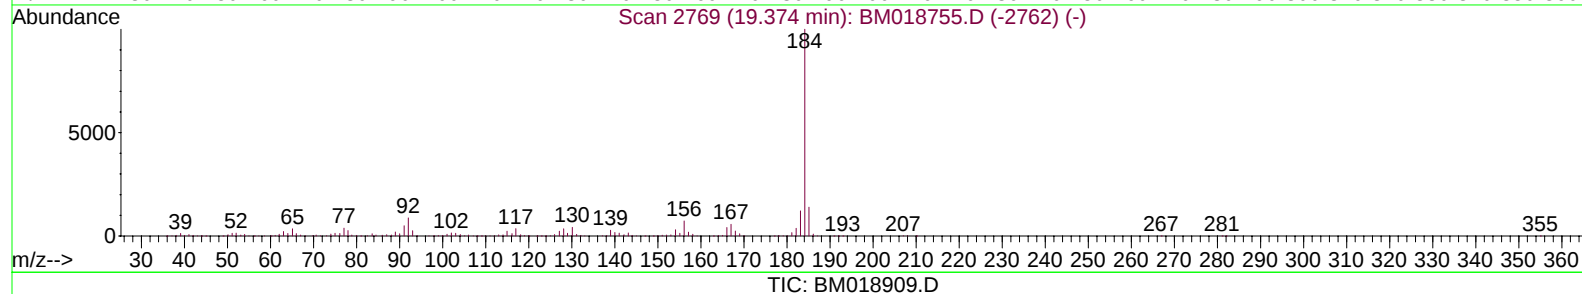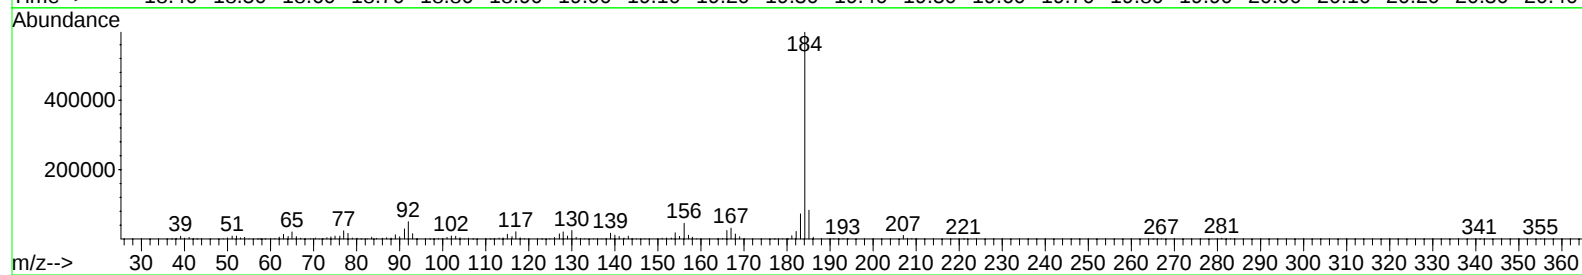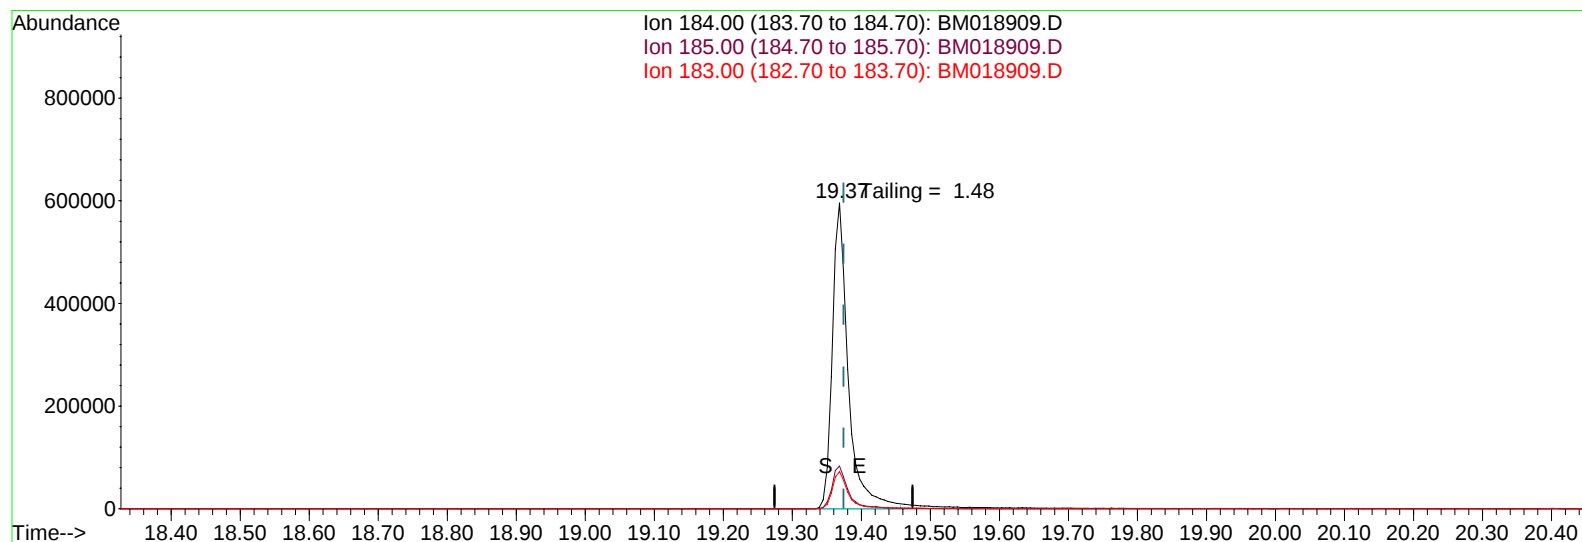

(77) Benzidine

19.368min (-0.006) 30023.82ng

response 948003

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	13.97
183.00	12.10	12.18
0.00	0.00	0.00