

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022522\
 Data File : BM034077.D
 Acq On : 25 Feb 2022 14:44
 Operator : CG/JU
 Sample : PB142933BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB142933BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034077.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.554	387	394	404	rBV	3317039	4636375	44.97%	10.239%
2	7.160	658	667	674	rBV	2962707	4695692	45.54%	10.370%
3	8.007	803	811	819	rVB	602108	966212	9.37%	2.134%
4	9.166	1000	1008	1016	rBV	1867897	2981417	28.92%	6.584%
5	10.819	1281	1289	1297	rBV	734947	1226877	11.90%	2.709%
6	13.271	1696	1706	1715	rBV	5406397	7655399	74.25%	16.906%
7	14.636	1932	1938	1945	rBV	1105986	1659711	16.10%	3.665%
8	16.118	2183	2190	2208	rVB	4010191	5491529	53.26%	12.127%
9	17.377	2398	2404	2413	rBV	1364846	1901958	18.45%	4.200%
10	19.995	2843	2849	2854	rBV	8530425	10310149	100.00%	22.769%
11	21.547	3108	3113	3122	rBV	1513577	1892681	18.36%	4.180%
12	24.000	3523	3530	3540	rVB	926223	1863879	18.08%	4.116%




Sum of corrected areas: 45281879

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022522\
Data File : BM034077.D
Acq On : 25 Feb 2022 14:44
Operator : CG/JU
Sample : PB142933BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB142933BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

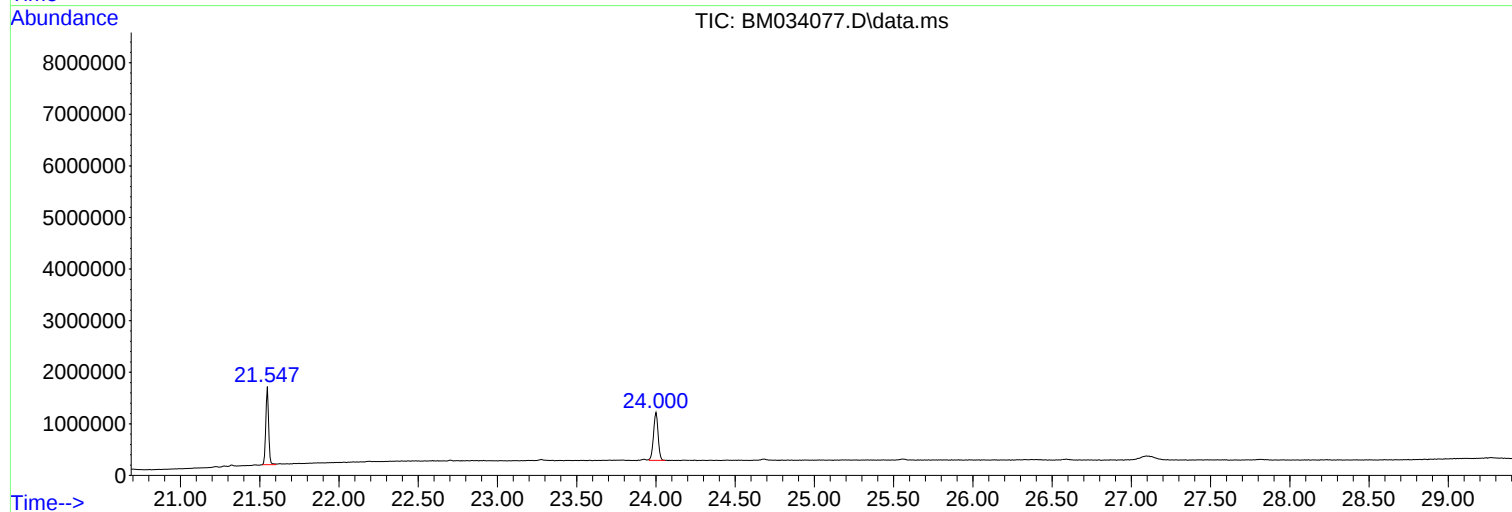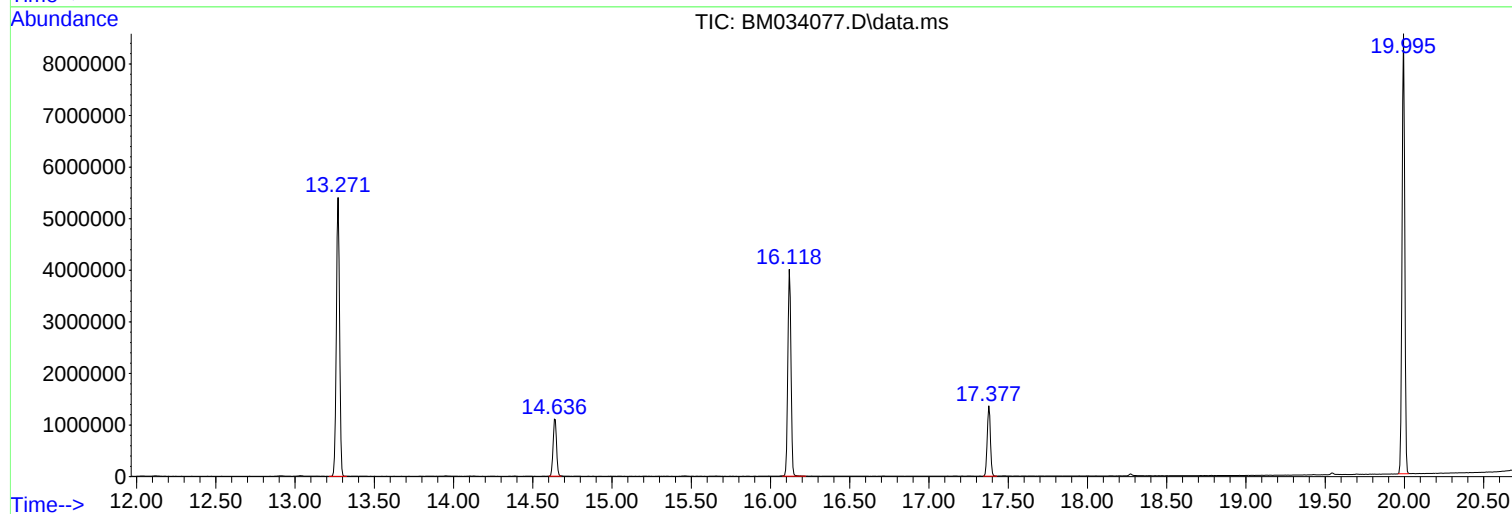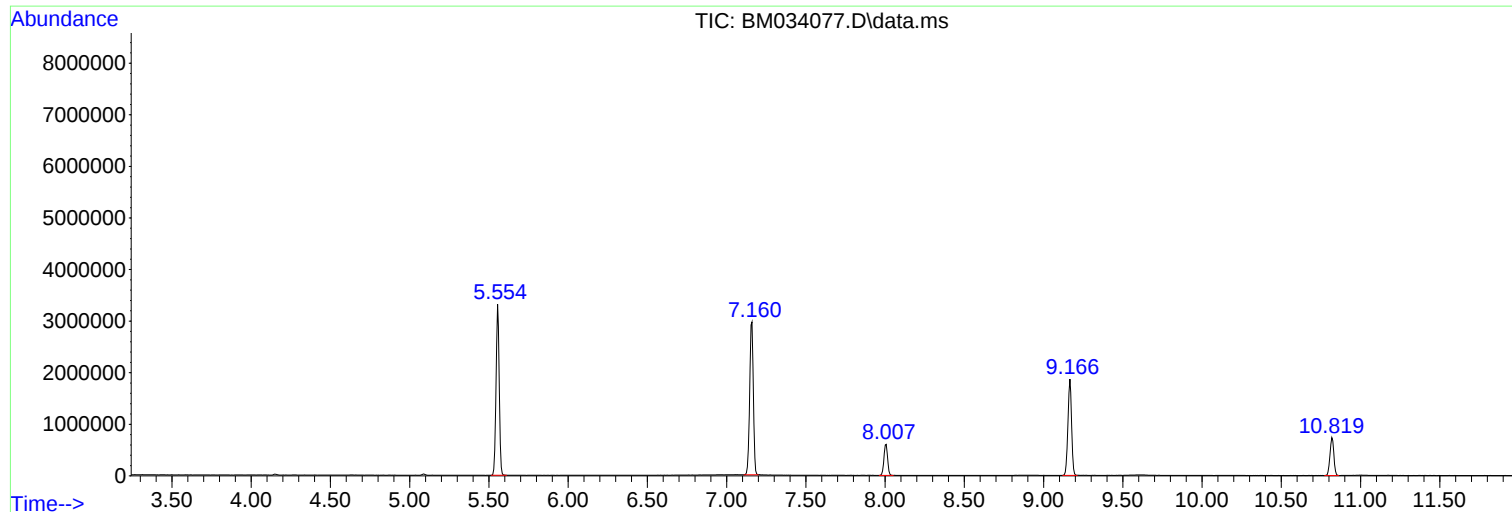

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022522\
Data File : BM034077.D
Acq On : 25 Feb 2022 14:44
Operator : CG/JU
Sample : PB142933BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB142933BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022522\
Data File : BM034077.D
Acq On : 25 Feb 2022 14:44
Operator : CG/JU
Sample : PB142933BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB142933BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------