

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022522\
 Data File : BM034081.D
 Acq On : 25 Feb 2022 17:14
 Operator : CG/JU
 Sample : N1653-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SP-DUP01-20210223E

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034081.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.554	387	394	403	rVB	1198153	1723998	18.12%	4.864%
2	7.148	659	665	678	rVB	652314	1052595	11.07%	2.970%
3	8.001	803	810	817	rBV	482520	759305	7.98%	2.142%
4	9.166	1000	1008	1018	rBV	1581139	2534887	26.65%	7.152%
5	10.819	1281	1289	1297	rBV	568986	944334	9.93%	2.664%
6	13.271	1699	1706	1715	rBV	4523414	6464466	67.96%	18.238%
7	14.636	1932	1938	1945	rBV	867503	1265657	13.30%	3.571%
8	16.118	2183	2190	2205	rBV	3766251	5185773	54.51%	14.631%
9	17.377	2397	2404	2410	rBV	1099497	1551257	16.31%	4.377%
10	18.271	2552	2556	2564	rBV2	109920	152273	1.60%	0.430%
11	19.542	2768	2772	2780	rBV3	89029	132781	1.40%	0.375%
12	19.994	2843	2849	2854	rBV	8068582	9512767	100.00%	26.839%
13	21.259	3061	3064	3070	rBV6	68734	95166	1.00%	0.268%
14	21.547	3108	3113	3118	rBV	1518663	1939639	20.39%	5.472%
15	24.000	3523	3530	3540	rVB2	1030933	2129442	22.39%	6.008%




Sum of corrected areas: 35444340

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022522\
Data File : BM034081.D
Acq On : 25 Feb 2022 17:14
Operator : CG/JU
Sample : N1653-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP-DUP01-20210223E

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

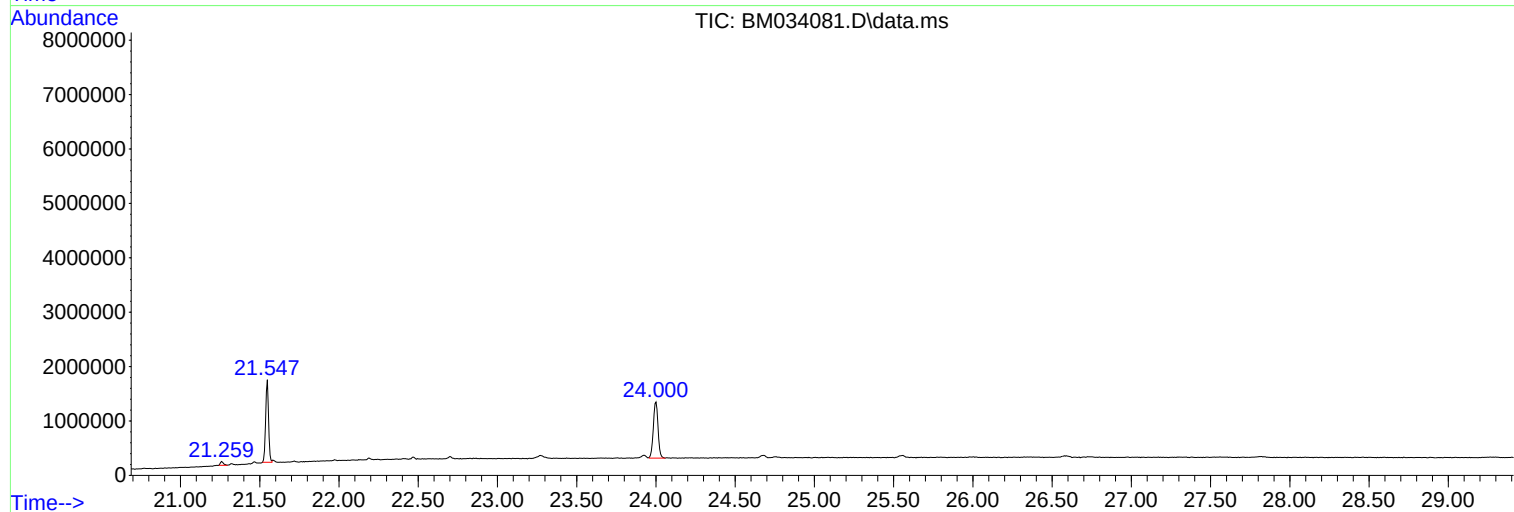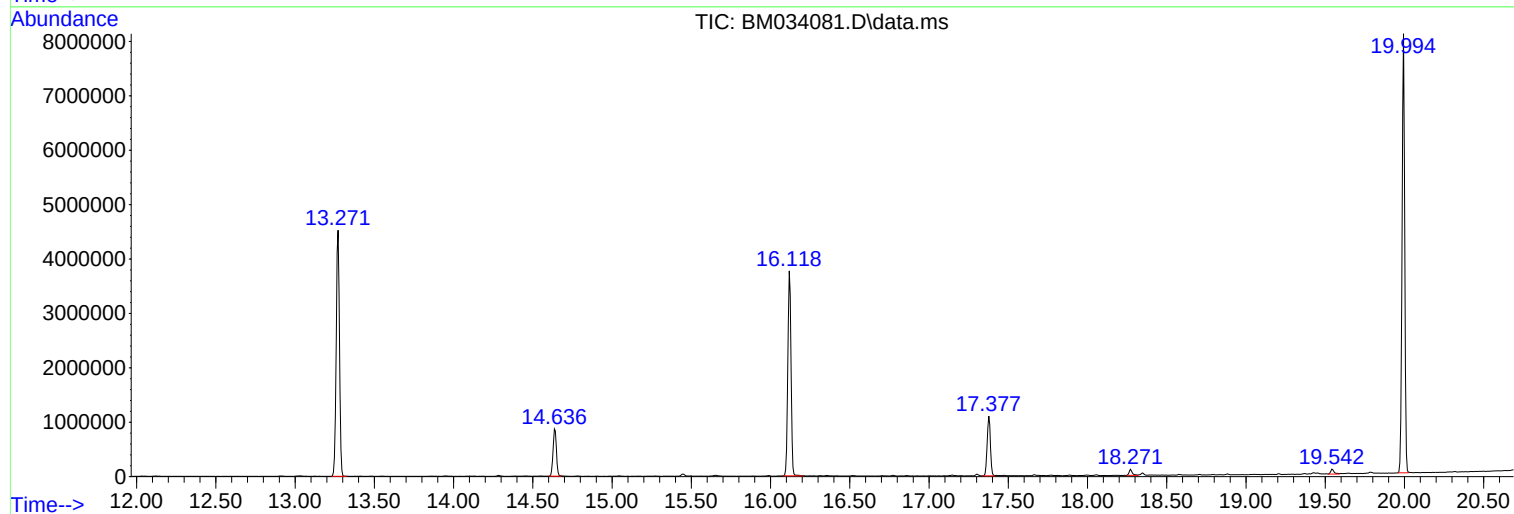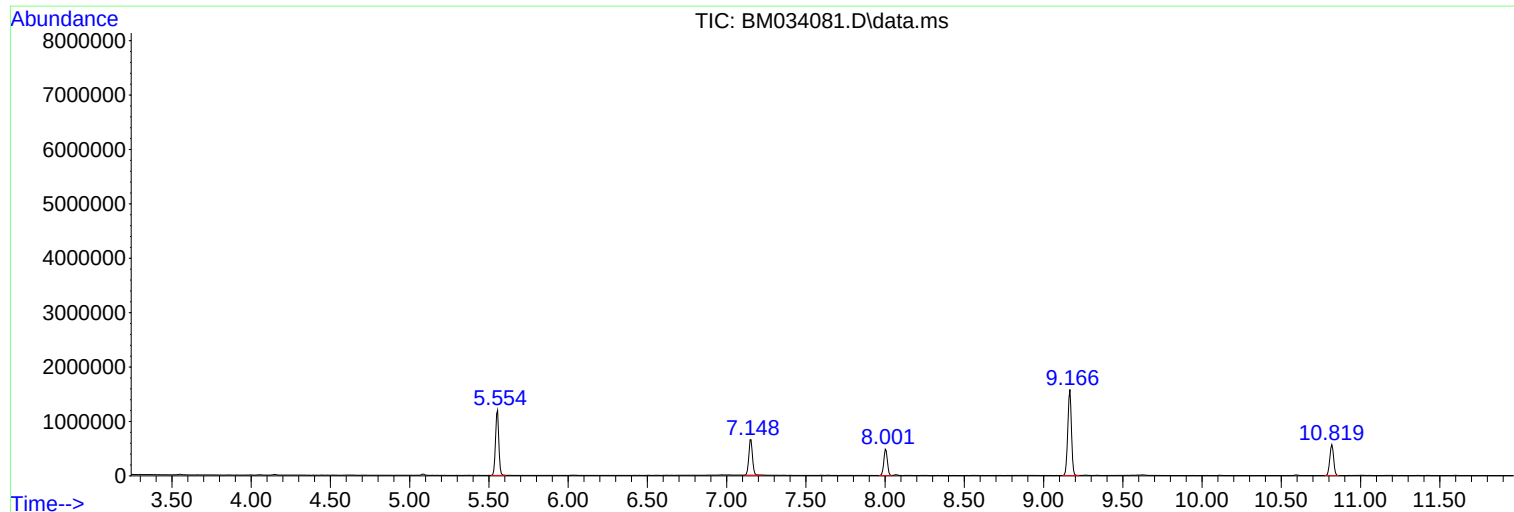

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022522\
Data File : BM034081.D
Acq On : 25 Feb 2022 17:14
Operator : CG/JU
Sample : N1653-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP-DUP01-20210223E

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022522\
Data File : BM034081.D
Acq On : 25 Feb 2022 17:14
Operator : CG/JU
Sample : N1653-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP-DUP01-20210223E

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------