

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022522\
 Data File : BM034082.D
 Acq On : 25 Feb 2022 17:50
 Operator : CG/JU
 Sample : N1653-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SP-303-20220223F

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034082.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.548	386	393	405	rBV	1086580	1586832	18.69%	5.108%
2	7.148	658	665	675	rVB	602569	953987	11.24%	3.071%
3	8.001	803	810	817	rBV	445891	696842	8.21%	2.243%
4	9.166	999	1008	1021	rBV	1478146	2388860	28.14%	7.689%
5	10.819	1281	1289	1297	rBV	511903	852134	10.04%	2.743%
6	13.271	1698	1706	1716	rBV	4094847	5906232	69.56%	19.011%
7	14.636	1931	1938	1945	rBV	757846	1107423	13.04%	3.565%
8	16.118	2183	2190	2203	rBV	3236776	4463134	52.57%	14.366%
9	17.377	2398	2404	2410	rBV	949949	1320951	15.56%	4.252%
10	19.995	2843	2849	2854	rBV	7077843	8490531	100.00%	27.329%
11	21.547	3108	3113	3118	rBV	1273535	1609089	18.95%	5.179%
12	24.000	3523	3530	3541	rVB2	835438	1692068	19.93%	5.446%




Sum of corrected areas: 31068083

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022522\
Data File : BM034082.D
Acq On : 25 Feb 2022 17:50
Operator : CG/JU
Sample : N1653-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP-303-20220223F

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

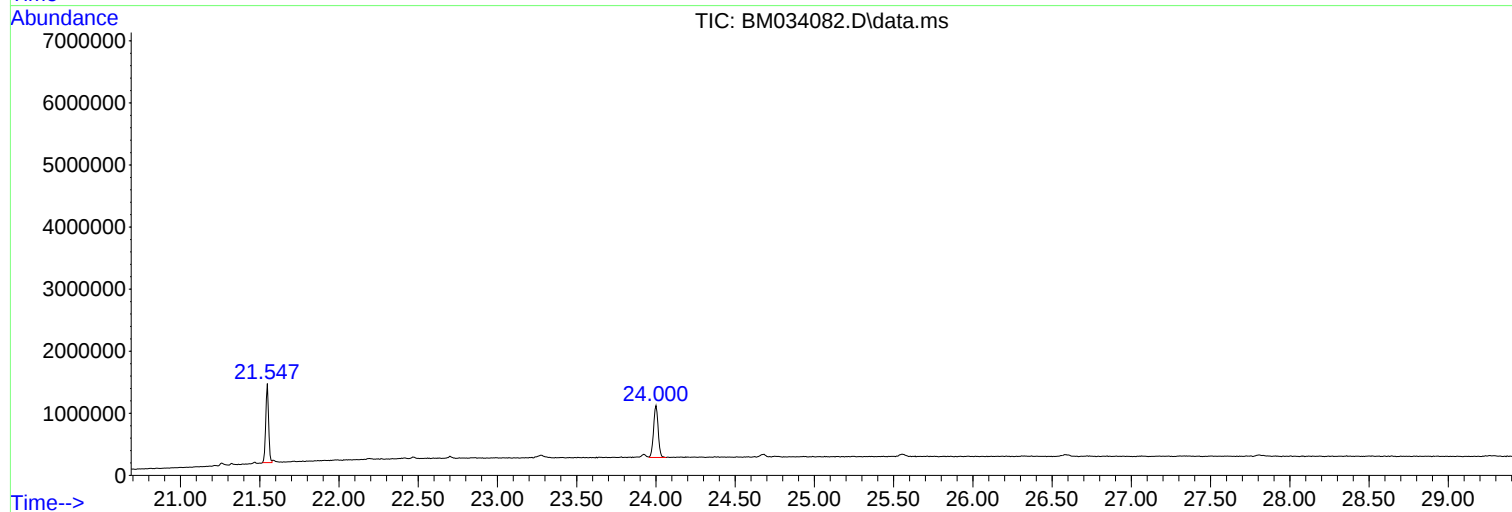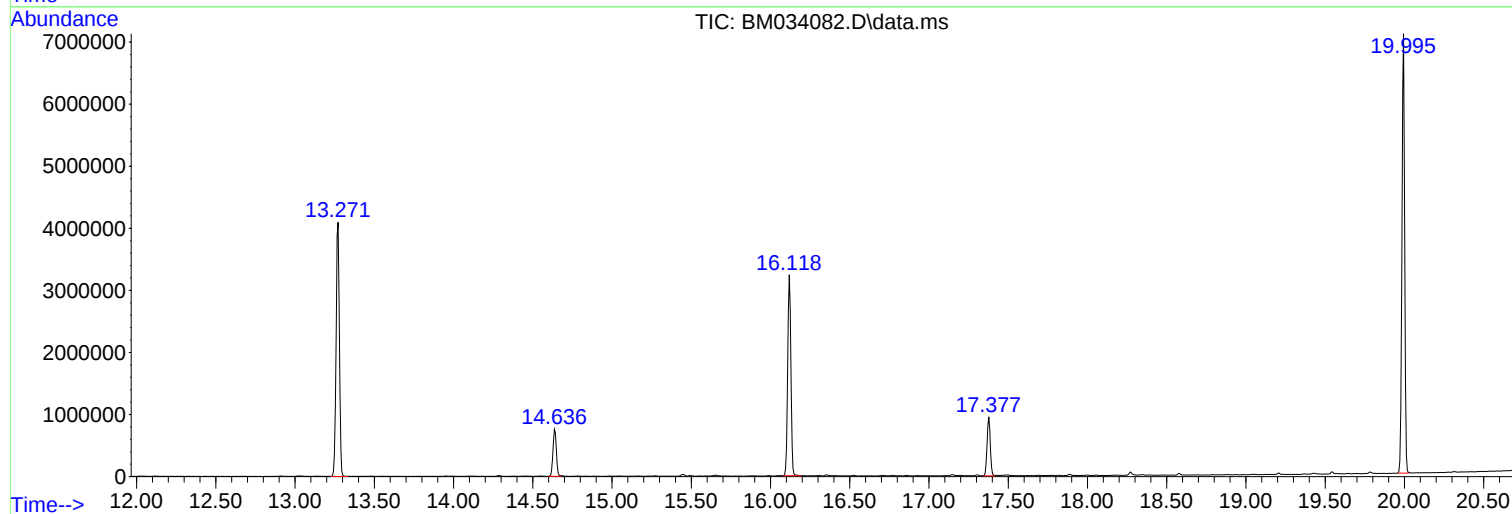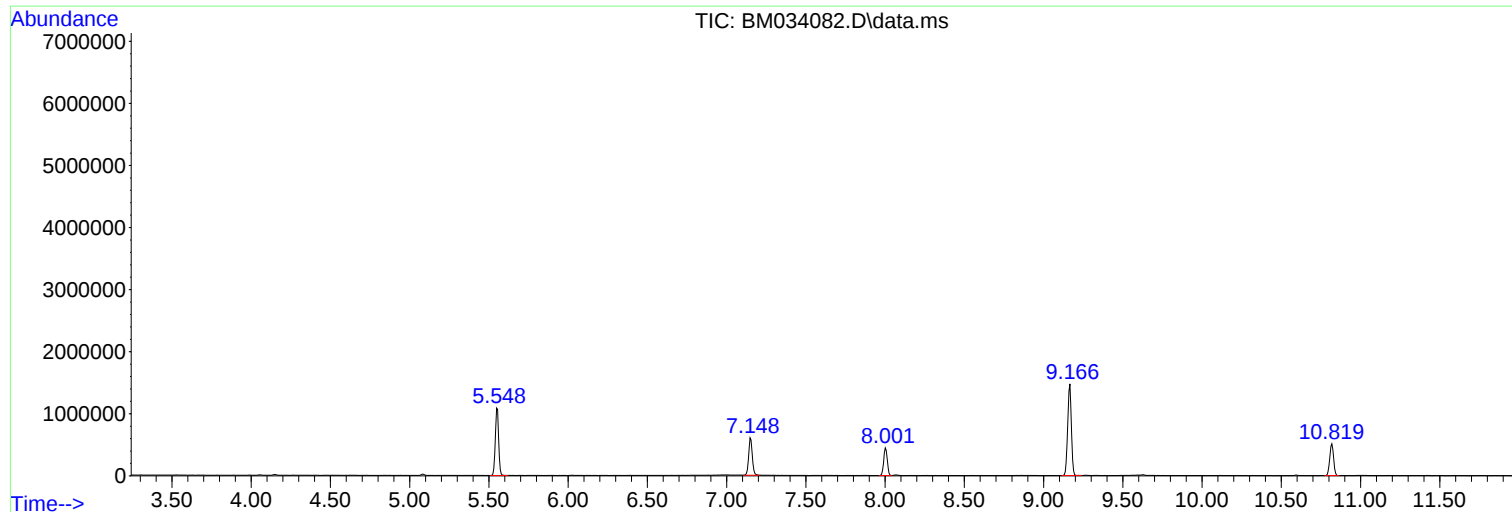

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022522\
Data File : BM034082.D
Acq On : 25 Feb 2022 17:50
Operator : CG/JU
Sample : N1653-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP-303-20220223F

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022522\
Data File : BM034082.D
Acq On : 25 Feb 2022 17:50
Operator : CG/JU
Sample : N1653-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP-303-20220223F

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------