


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022522\
 Data File : BM034075.D
 Acq On : 25 Feb 2022 11:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Feb 26 03:45:21 2022

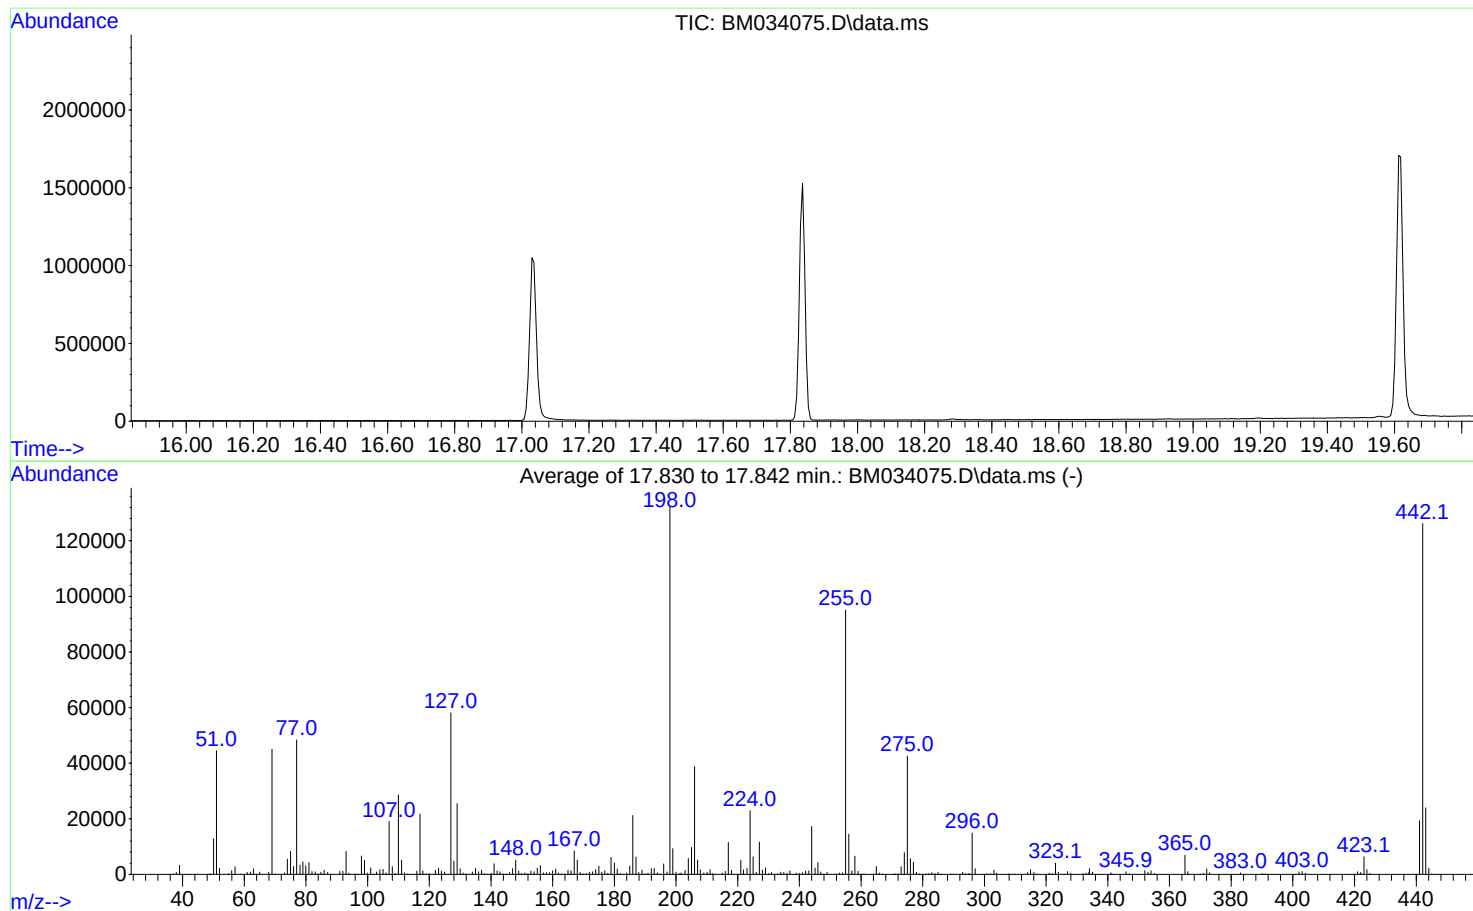




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	44501	PASS
68	69	0.00	2	1.7	777	PASS
69	198	0.00	100	34.0	45032	PASS
70	69	0.00	2	0.5	231	PASS
127	198	10	80	43.9	58059	PASS
197	198	0.00	2	0.6	846	PASS
198	198	100	100	100.0	132323	PASS
199	198	5	9	7.0	9278	PASS
275	198	10	60	32.1	42525	PASS
365	198	1	100	5.2	6881	PASS
441	198	0.01	100	14.6	19300	PASS
442	442	50	100	100.0	126227	PASS
443	442	15	24	19.0	23941	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022522\
Data File : BM034075.D
Acq On : 25 Feb 2022 11:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 26 05:10:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 26 03:45:21 2022
Response via : Initial Calibration

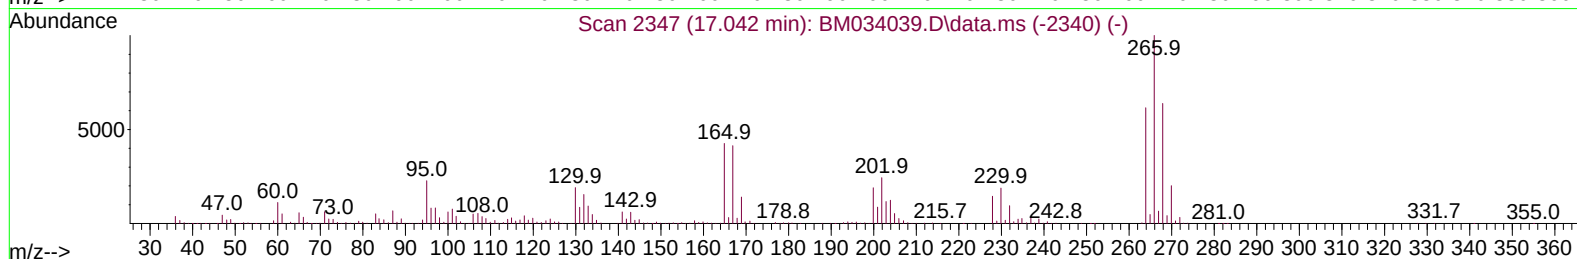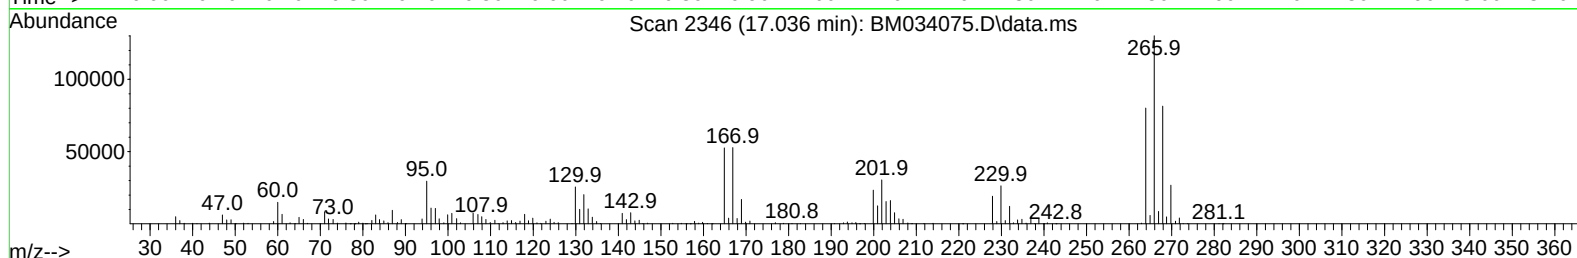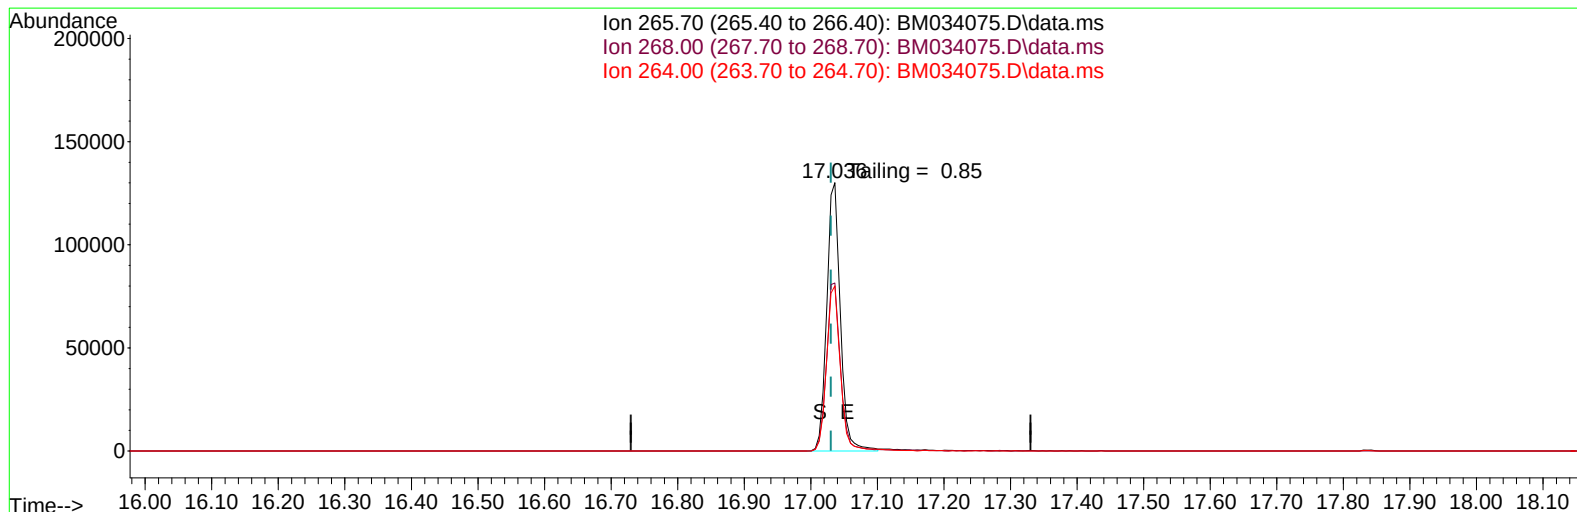

TIC: BM034075.D\data.ms

(70) Pentachlorophenol (C)

17.036min (+ 0.006) 0.00 ng




response 187300

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	62.59
264.00	61.40	61.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022522\
 Data File : BM034075.D
 Acq On : 25 Feb 2022 11:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Feb 26 05:10:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 26 03:45:21 2022
 Response via : Initial Calibration

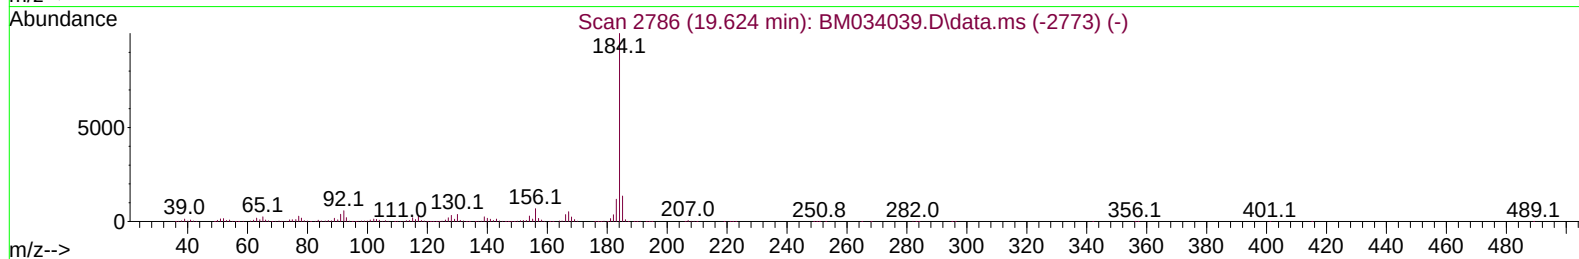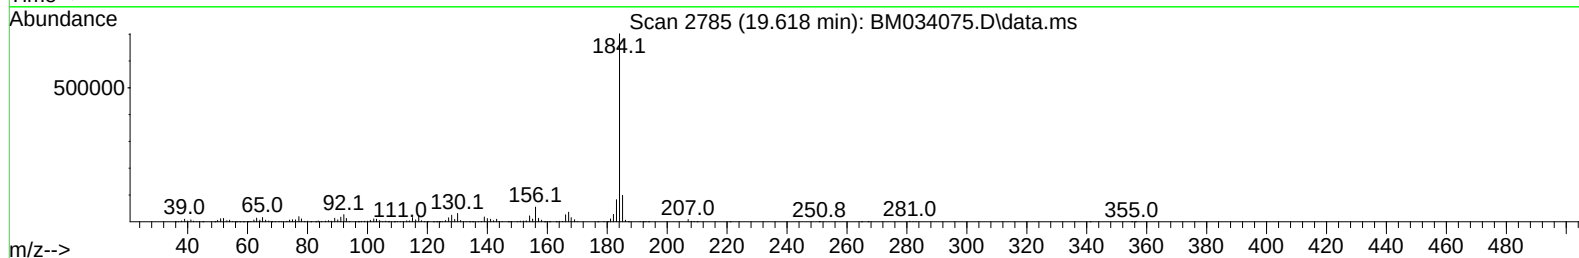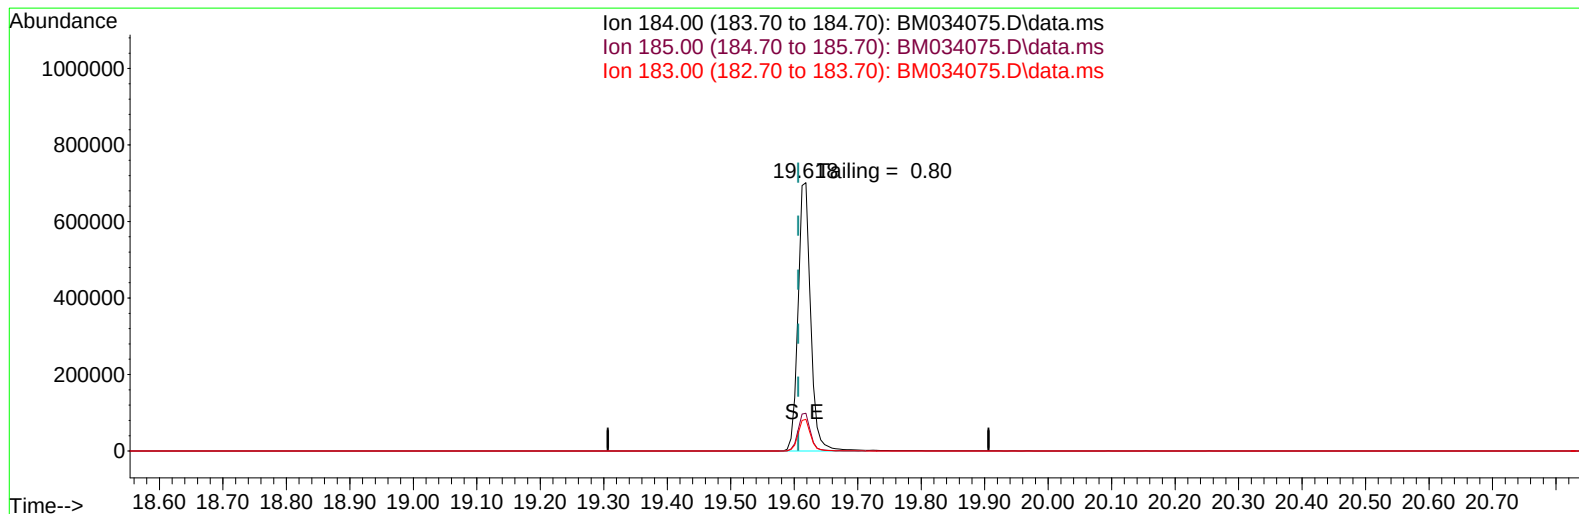

TIC: BM034075.D\data.ms

(77) Benzidine

19.618min (+ 0.012) 0.00 ng

response 972590

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.08
183.00	12.10	11.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/25/2022	BNA_M	<u>BM034075.D</u>
Compound Name	Response	Retention Time
DDT	525618	20.854
DDD	6428	20.418
DDE	693	19.912
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7121	532739	1.34

Instrument :
BNA_M
ClientSampleId :
DFTPP