
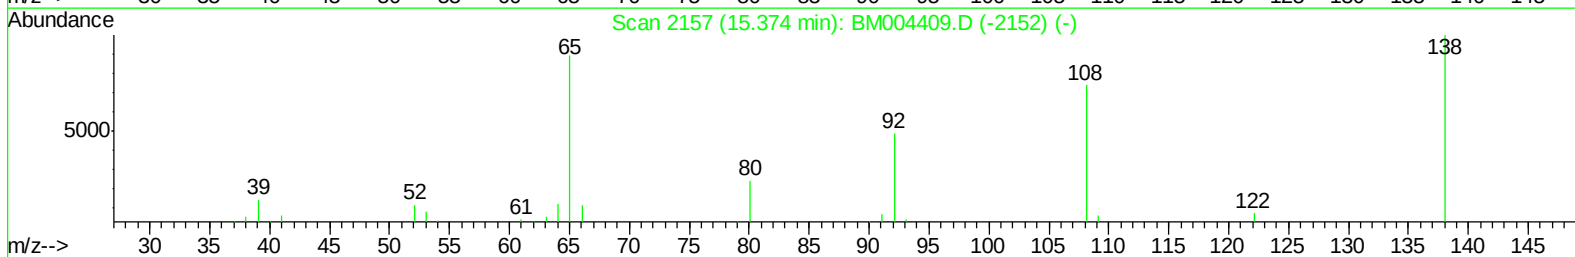
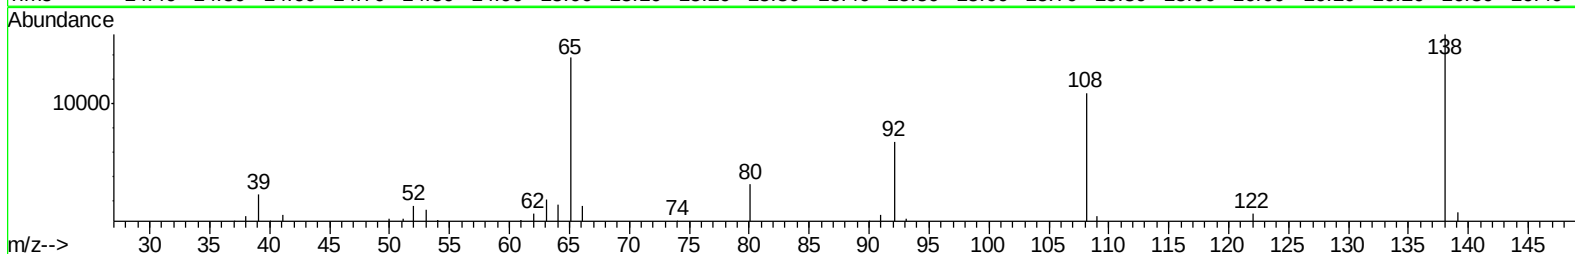


Data Path : Z:\HPCHEM1\BNA_M\Data\BM022616\
Data File : BM004422.D
Acq On : 26 Feb 2016 09:39
Operator : SJ/UM
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Feb 26 23:19:08 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 26 03:49:40 2016
Response via : Initial Calibration

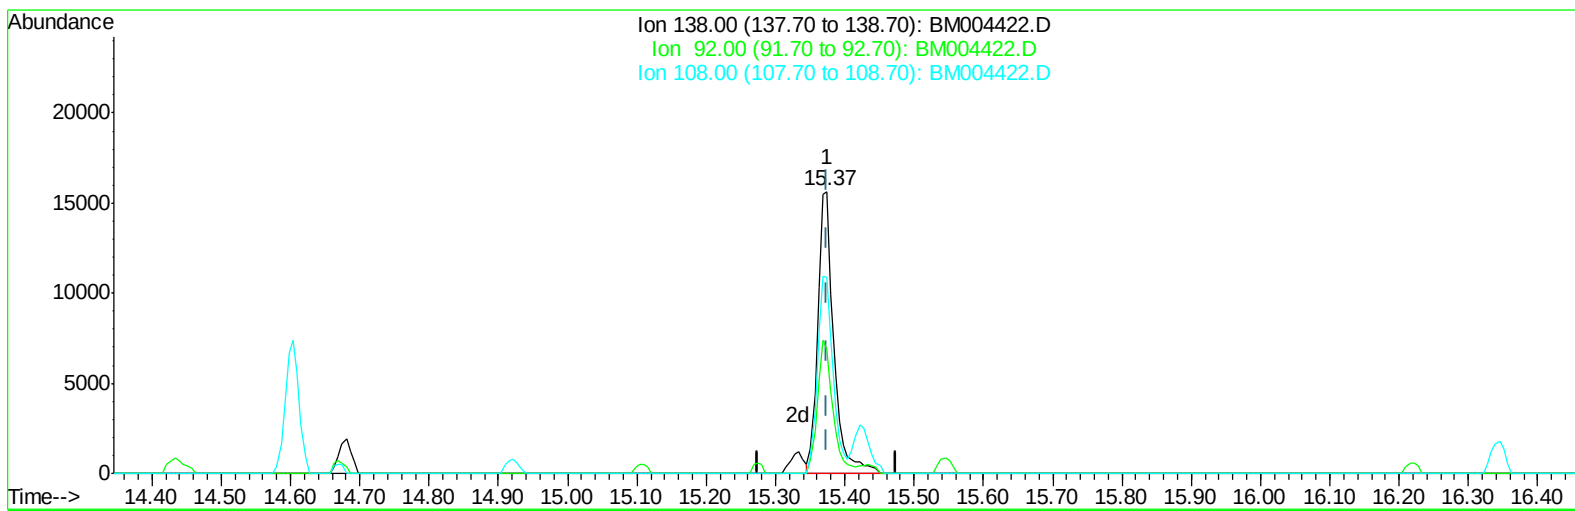

TIC: BM004422.D

(61) 4-Nitroaniline

15.374min (-0.000) 17.17ng/ul m

response 25212

Ion	Exp%	Act%
138.00	100	100
92.00	50.70	43.91
108.00	83.80	69.46
0.00	0.00	0.00