
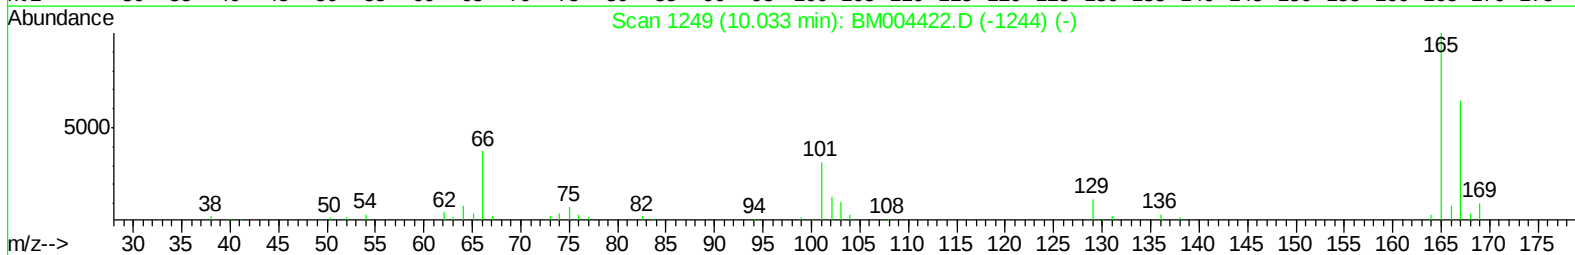
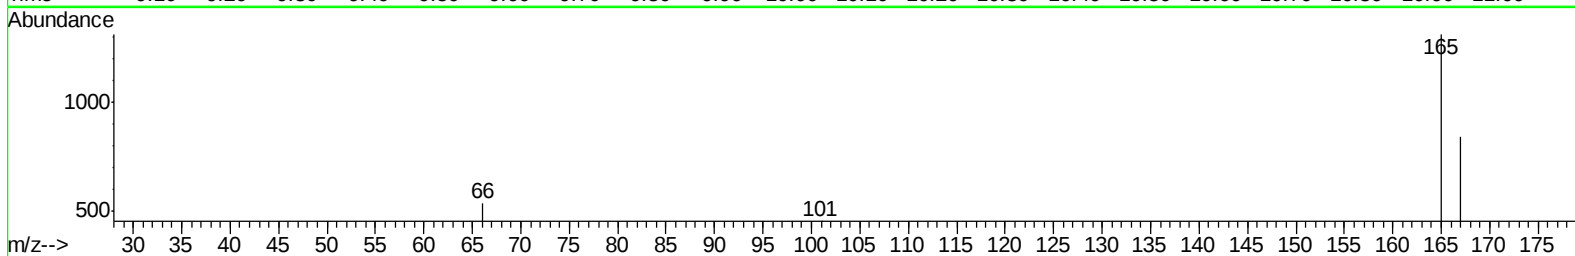


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022616\
Data File : BM004433.D
Acq On : 26 Feb 2016 18:52
Operator : SJ/UM
Sample : H1564-13MS
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Feb 26 23:26:25 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 26 23:20:20 2016
Response via : Initial Calibration

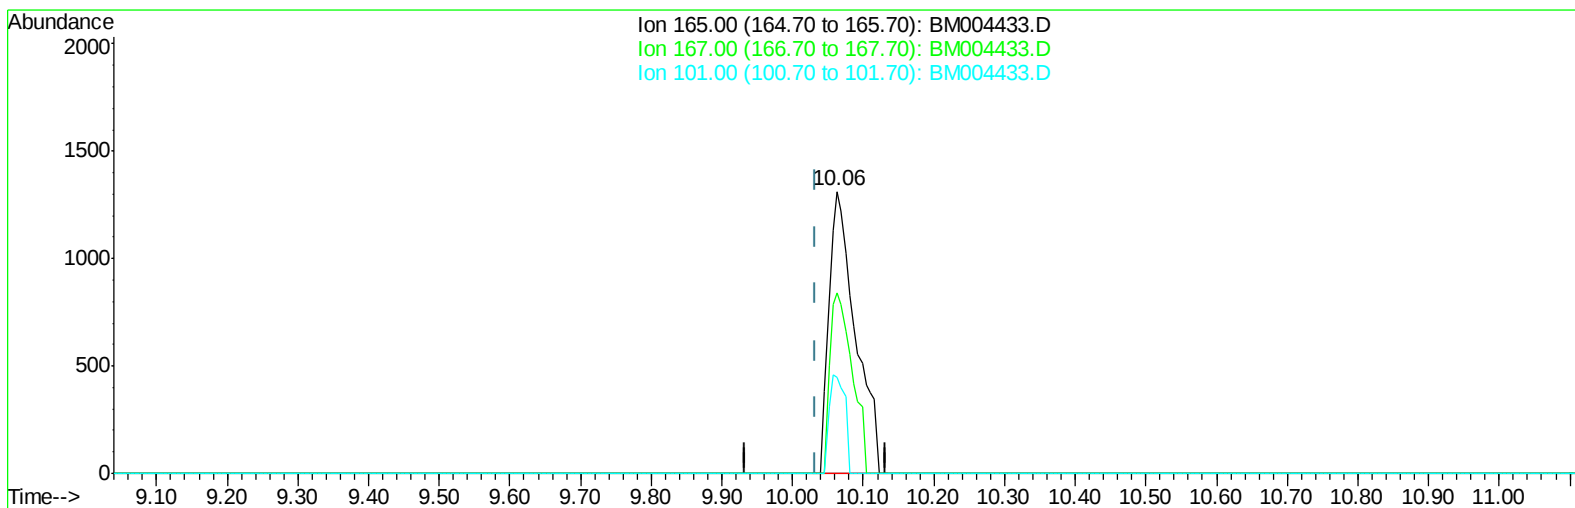

TIC: BM004433.D

(26) 2,4-Dichlorophenol-d3 (S)

10.063min (+0.030) 2.19ng/ul m

response 3387

Ion	Exp%	Act%
165.00	100	100
167.00	65.30	63.92
101.00	34.20	34.32
0.00	0.00	0.00