
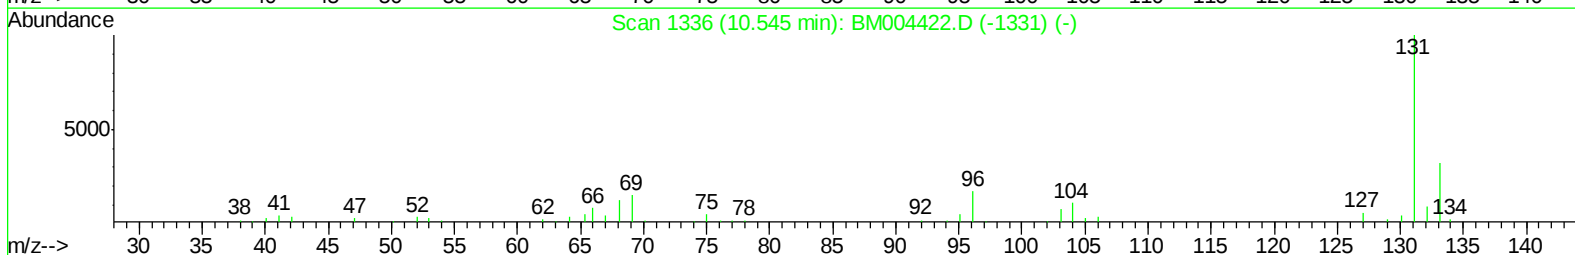
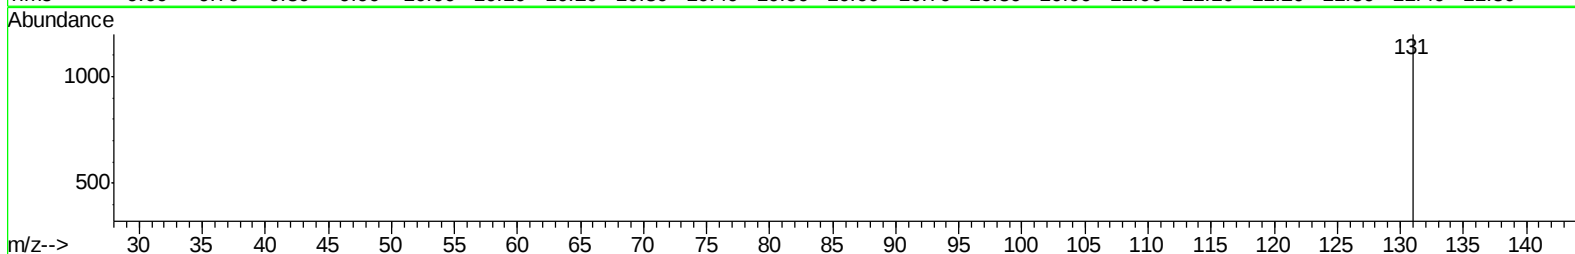


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022616\
Data File : BM004433.D
Acq On : 26 Feb 2016 18:52
Operator : SJ/UM
Sample : H1564-13MS
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Feb 26 23:26:25 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 26 23:20:20 2016
Response via : Initial Calibration

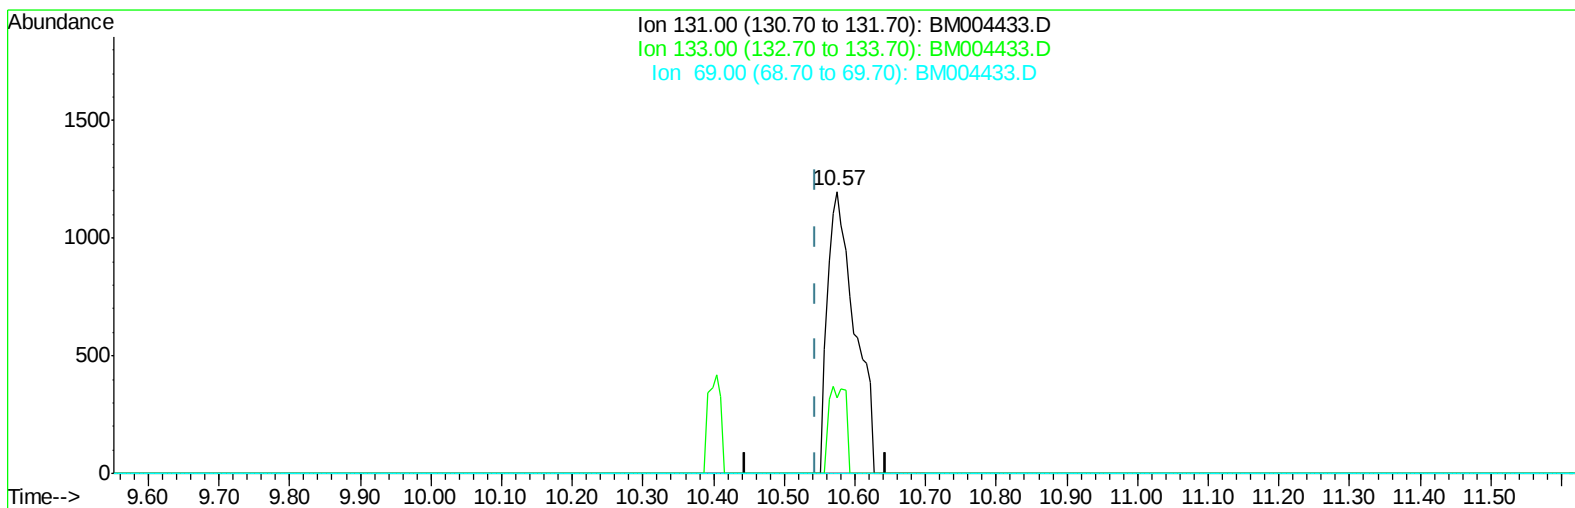

TIC: BM004433.D

(29) 4-Chloroaniline-d4 (S)

10.575min (+0.030) 1.65ng/ul m

response 3176

Ion	Exp%	Act%
131.00	100	100
133.00	32.10	26.98
69.00	16.20	0.00#
0.00	0.00	0.00