
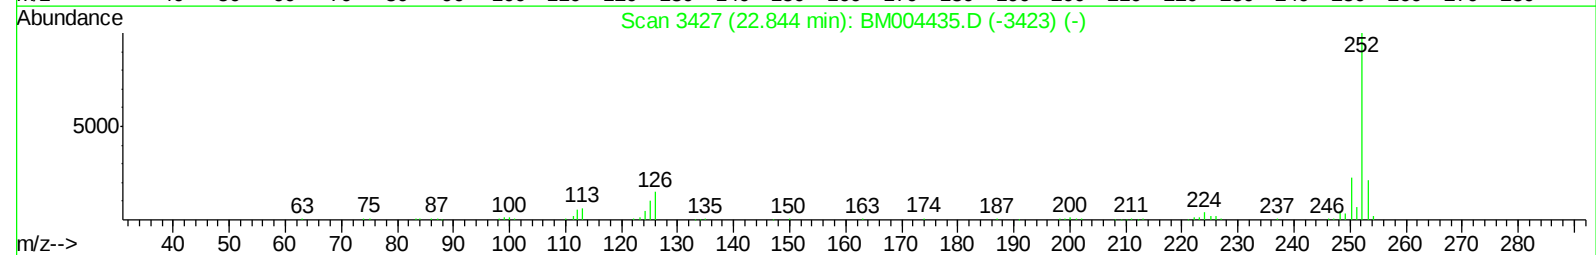
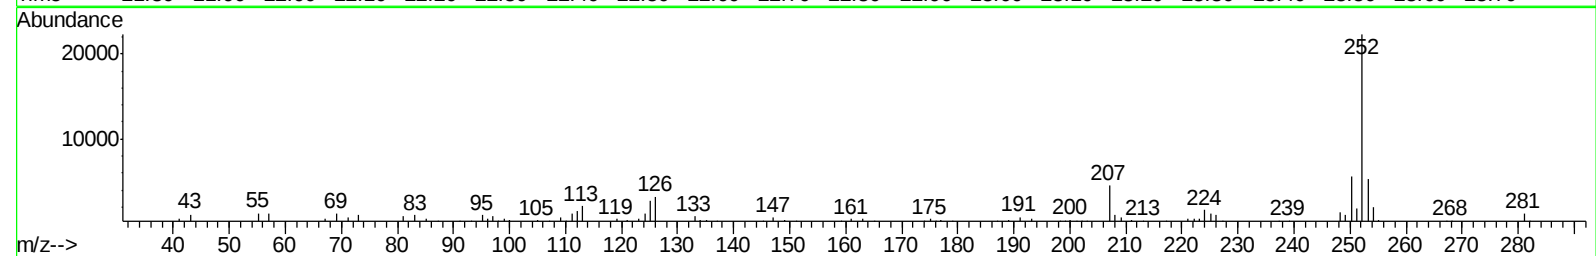


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022616\
Data File : BM004441.D
Acq On : 27 Feb 2016 00:16
Operator : SJ/UM
Sample : H1564-07
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Feb 27 01:08:26 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 27 00:43:30 2016
Response via : Initial Calibration

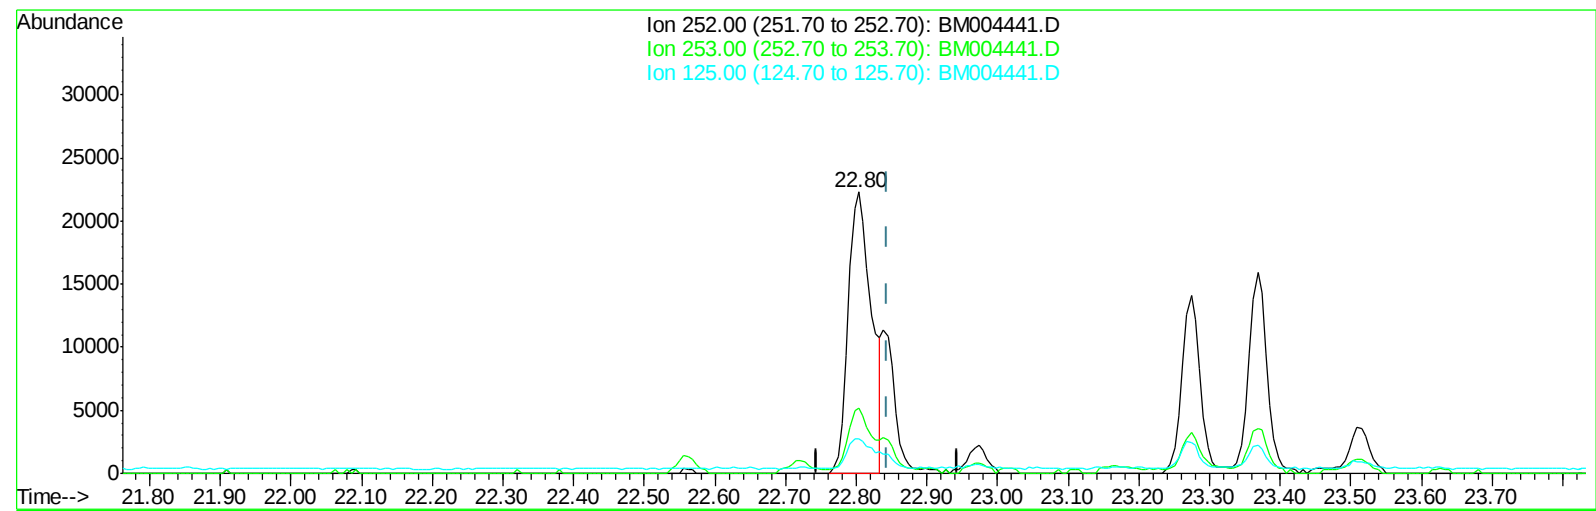

TIC: BM004441.D

(89) Benzo(k)fluoranthene
22.803min (-0.041) 5.78ng/ul
response 51249

Ion	Exp%	Act%
252.00	100	100
253.00	21.60	23.37
125.00	10.20	12.14
0.00	0.00	0.00