

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022616\
Data File : BM004438.D
Acq On : 26 Feb 2016 22:28
Operator : SJ/UM
Sample : H1564-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9R28

Quant Time: Feb 27 00:48:48 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 27 00:43:30 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

UMANGI
2/29/2016 2:53:17 PM

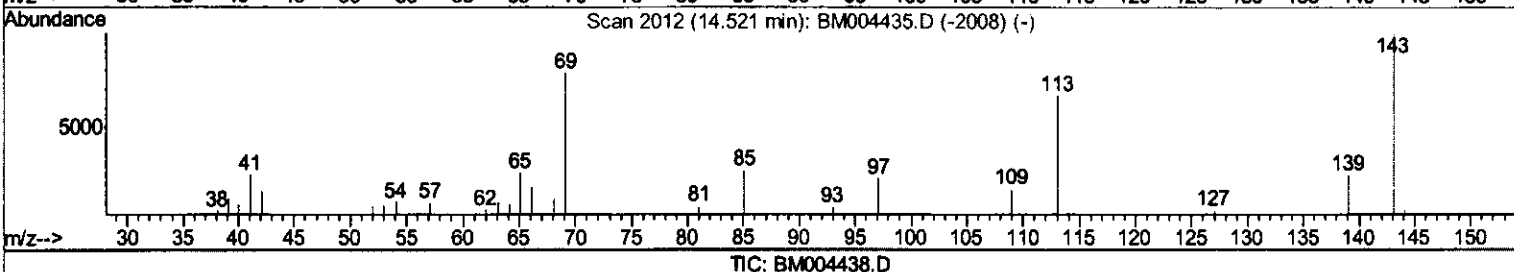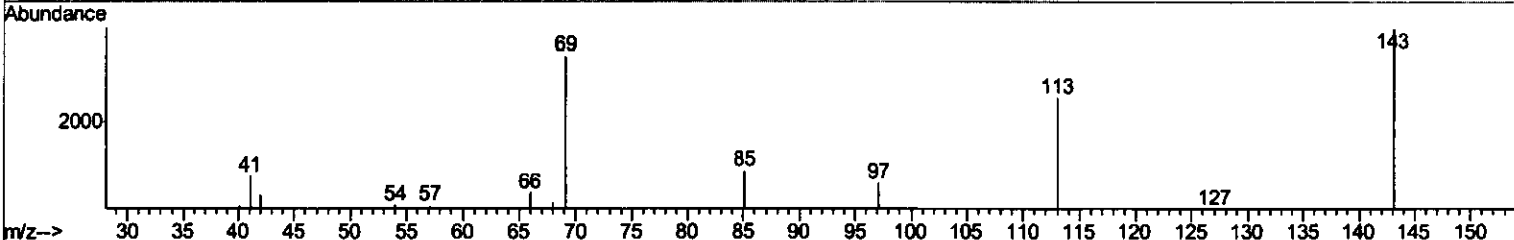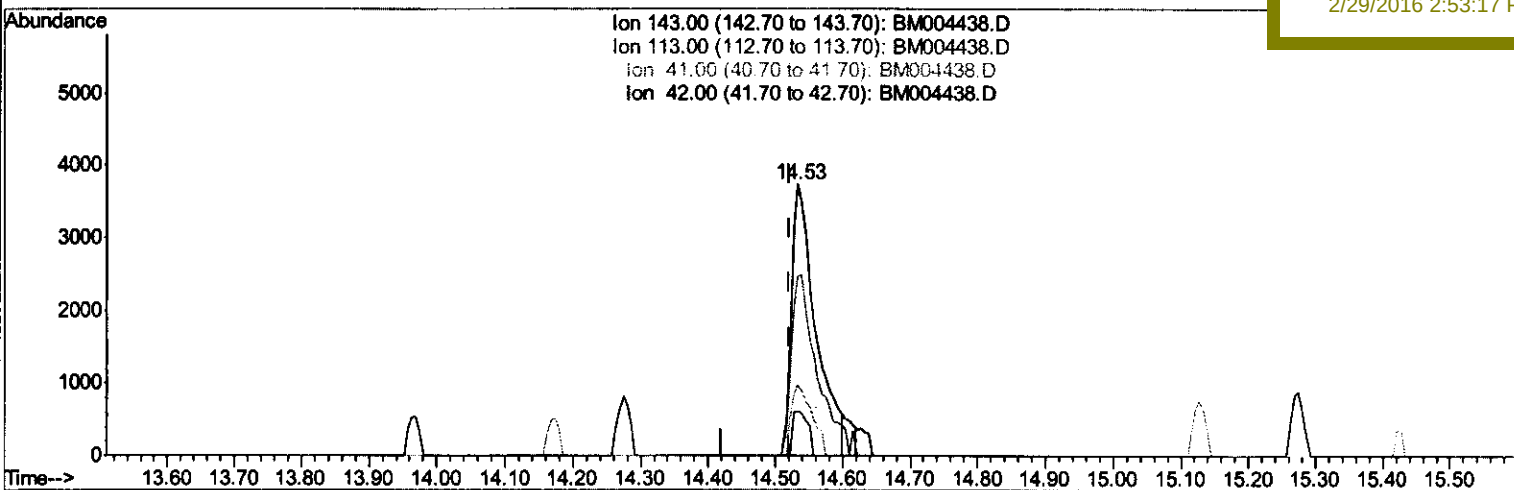

(52) 4-Nitrophenol-d4 (S)

14.533min (+0.012) 10.43ng/ul

response 9304

Ion	Exp%	Act%
143.00	100	100
113.00	75.10	65.49
41.00	28.80	25.87
42.00	19.10	16.59




```
Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022616\  
Data File : BM004438.D  
Acq On    : 26 Feb 2016   22:28  
Operator  : SJ/UM  
Sample    : H1564-03  
Misc      :  
ALS Vial  : 17      Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
D9R28

Manual Integrations

UMANGI
2/29/2016 2:53:17 PM

Quant Time: Feb 27 00:48:48 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 27 00:43:30 2016
Response via : Initial Calibration

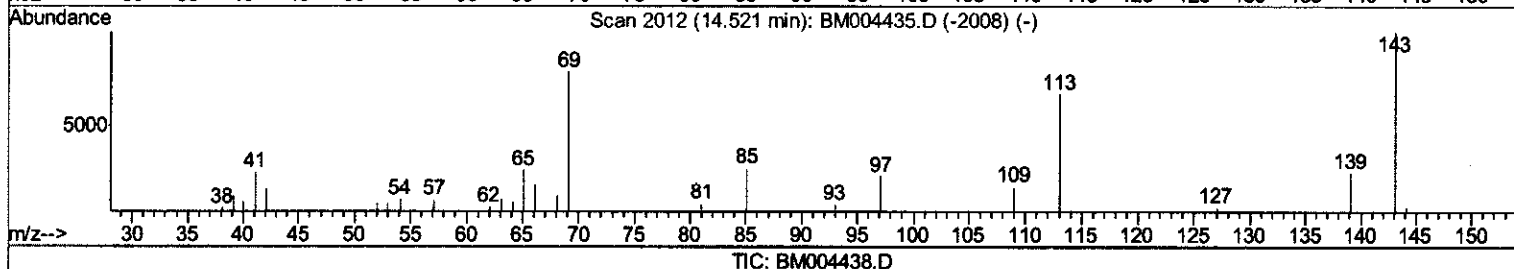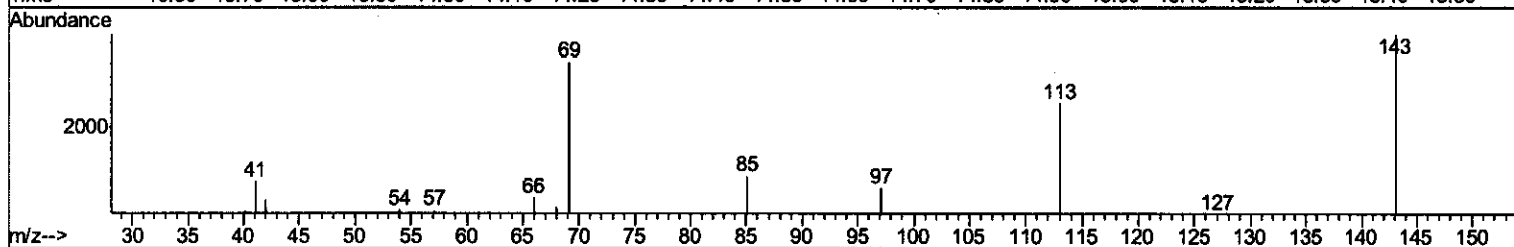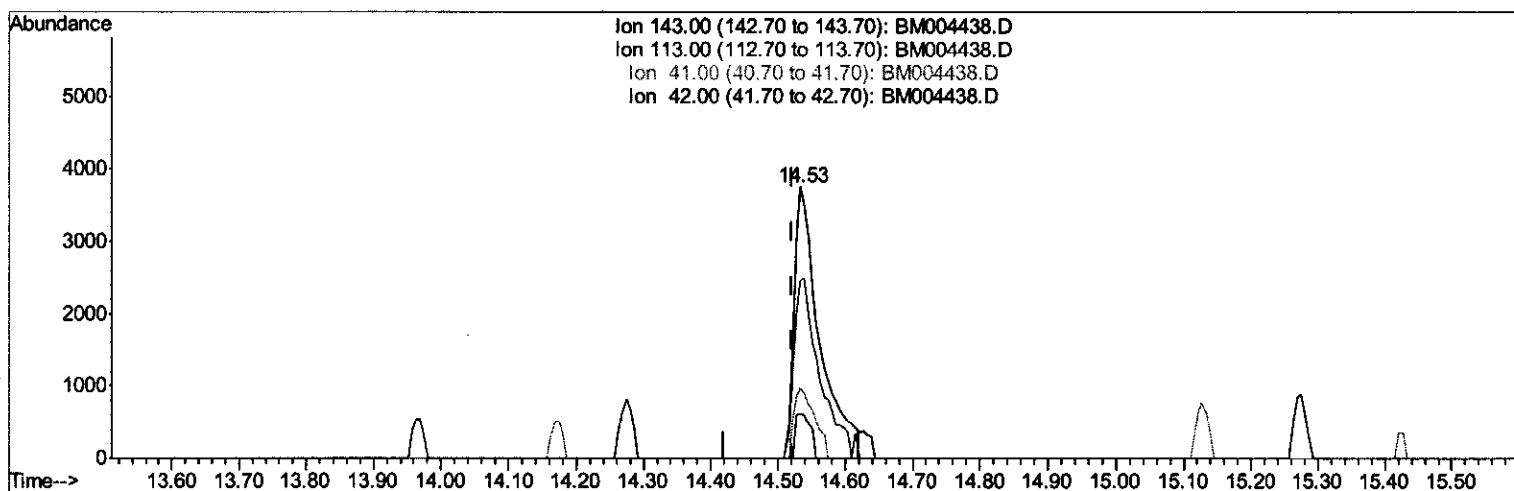

TIC: BM004438.D

(52) 4-Nitrophenol-d4 (S)

14.533min (+0.012) 11.54ng/ul m

response 10289

Ion	Exp%	Act%
143.00	100	100
113.00	75.10	65.49
41.00	28.80	25.87
42.00	19.10	16.59

> S.T
03/08/16




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022616\
Data File : BM004438.D
Acq On : 26 Feb 2016 22:28
Operator : SJ/UM
Sample : H1564-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9R28

Quant Time: Feb 27 00:48:48 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 27 00:43:30 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

UMANGI
2/29/2016 2:53:17 PM

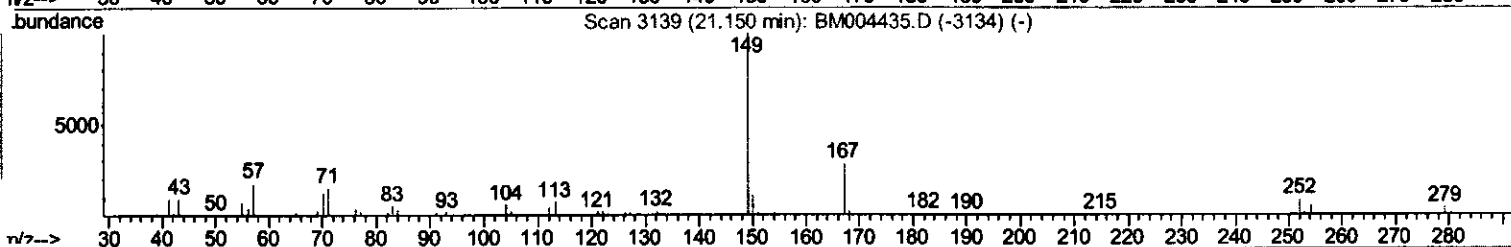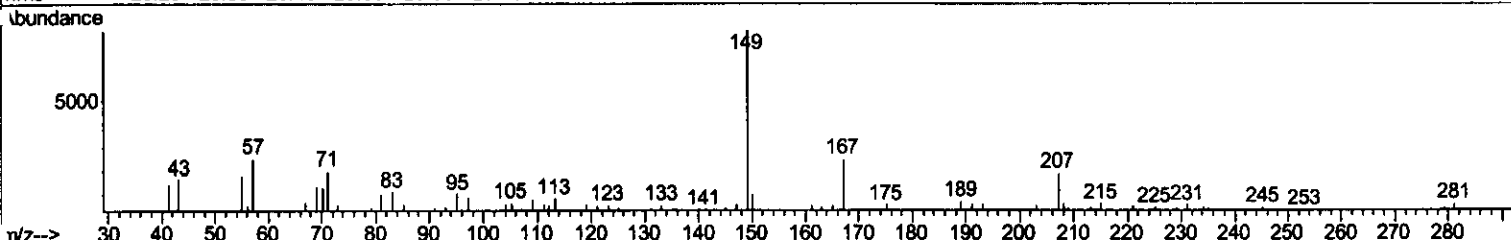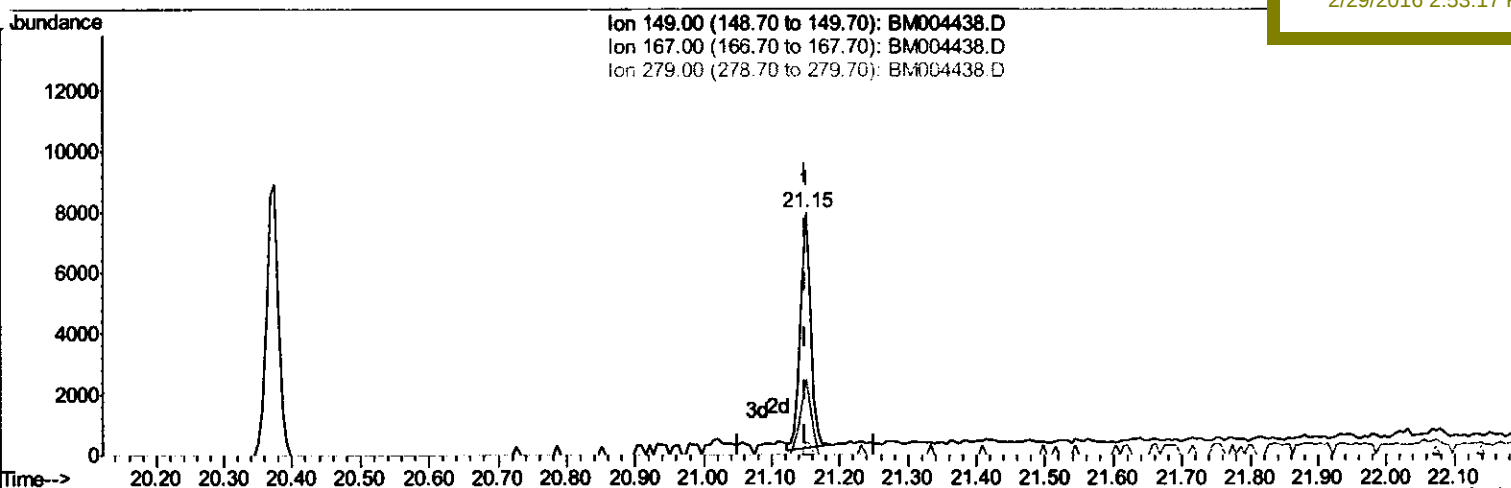

TIC: BM004438.D

(84) Bis(2-ethylhexyl)phthalate

21.150min (+0.000) 1.32ng/ul

response 8378

Ion	Exp%	Act%
149.00	100	100
167.00	27.00	31.04
279.00	3.70	5.18#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022616\
 Data File : BM004438.D
 Acq On : 26 Feb 2016 22:28
 Operator : SJ/UM
 Sample : H1564-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9R28

Manual Integrations
 APPROVED

UMANGI
 2/29/2016 2:53:17 PM

Quant Time: Feb 27 00:48:48 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Feb 27 00:43:30 2016
 Response via : Initial Calibration

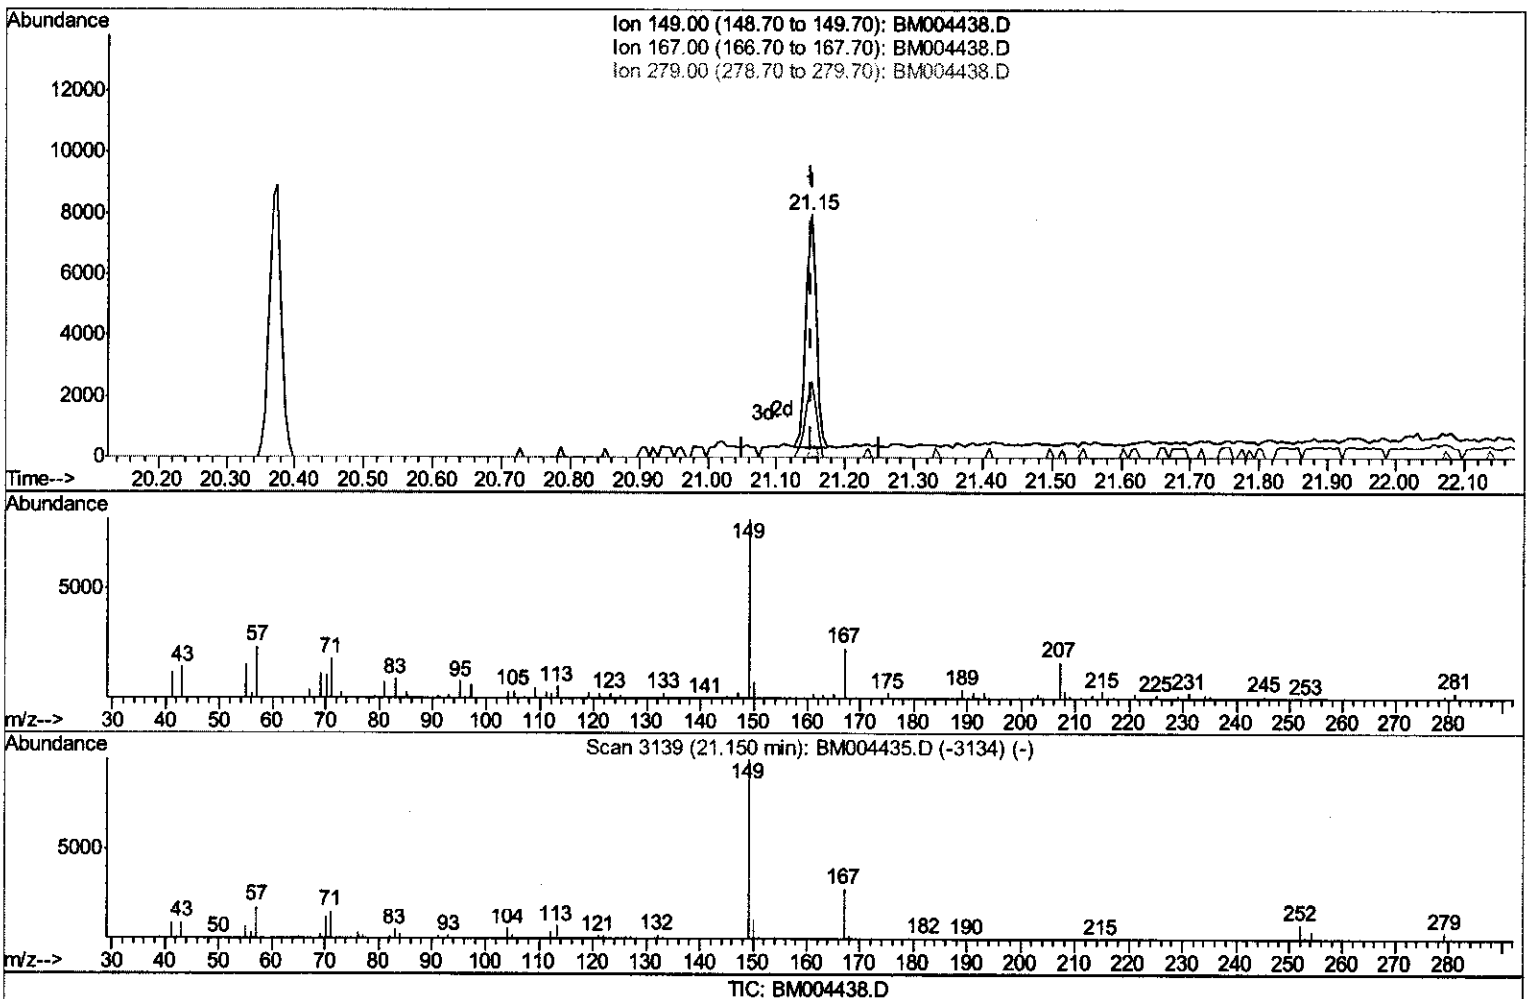

(84) Bis(2-ethylhexyl)phthalate

21.150min (+0.000) 1.25ng/ul m

response 7922

Ion	Exp%	Act%
149.00	100	100
167.00	27.00	31.04
279.00	3.70	5.18#
0.00	0.00	0.00

> 9.7
 03/08/16




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022616\
Data File : BM004438.D
Acq On : 26 Feb 2016 22:28
Operator : SJ/UM
Sample : H1564-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9R28

Quant Time: Feb 27 00:48:48 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 27 00:43:30 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

UMANGI
2/29/2016 2:53:17 PM

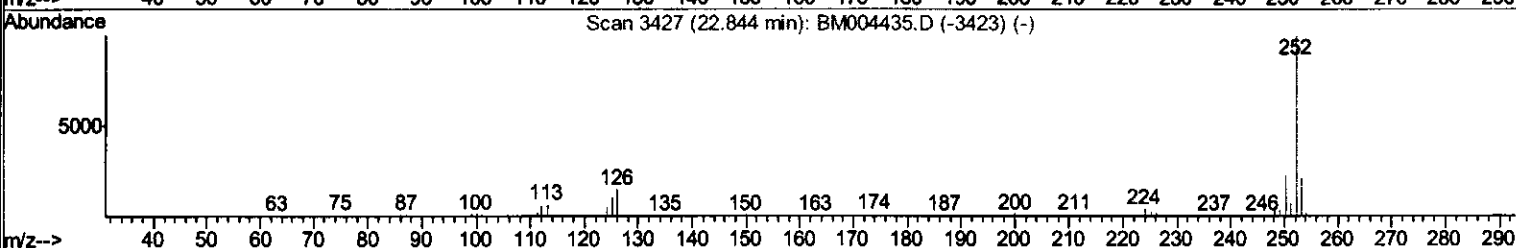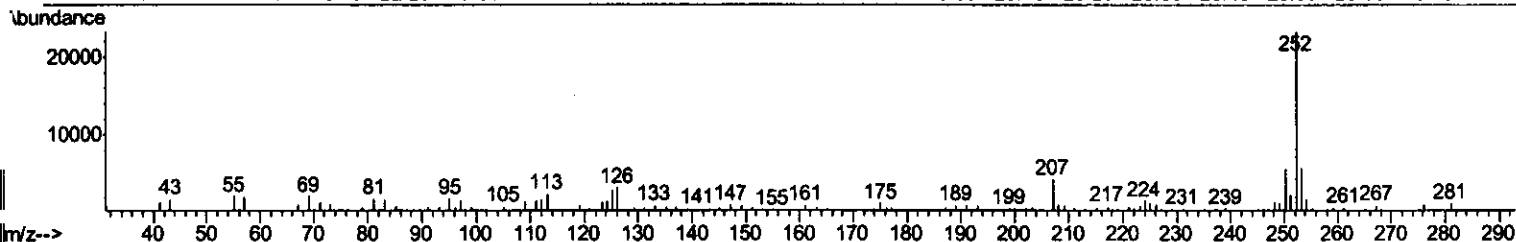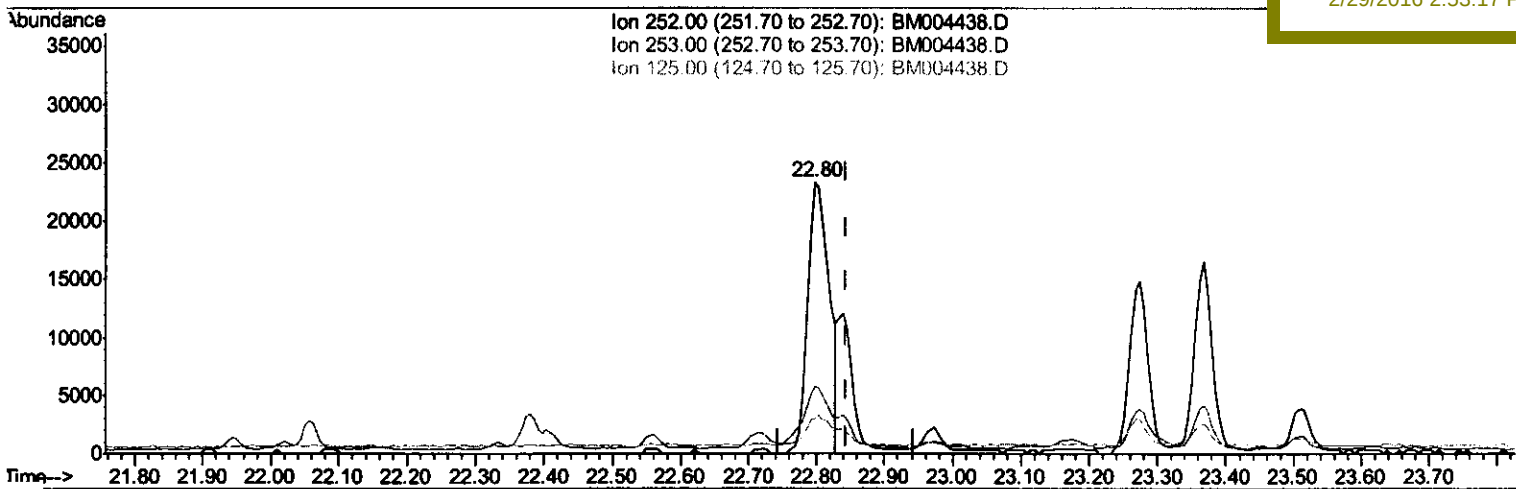

TIC: BM004438.D

(89) Benzo(k)fluoranthene

22.797min (-0.047) 5.39ng/ul

response 50821

Ion	Exp%	Act%
252.00	100	100
253.00	21.60	24.70
125.00	10.20	12.93#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022616\
 Data File : BM004438.D
 Acq On : 26 Feb 2016 22:28
 Operator : SJ/UM
 Sample : H1564-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9R28

Manual Integrations
 APPROVED

UMANGI
 2/29/2016 2:53:17 PM

Quant Time: Feb 27 00:48:48 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Feb 27 00:43:30 2016
 Response via : Initial Calibration

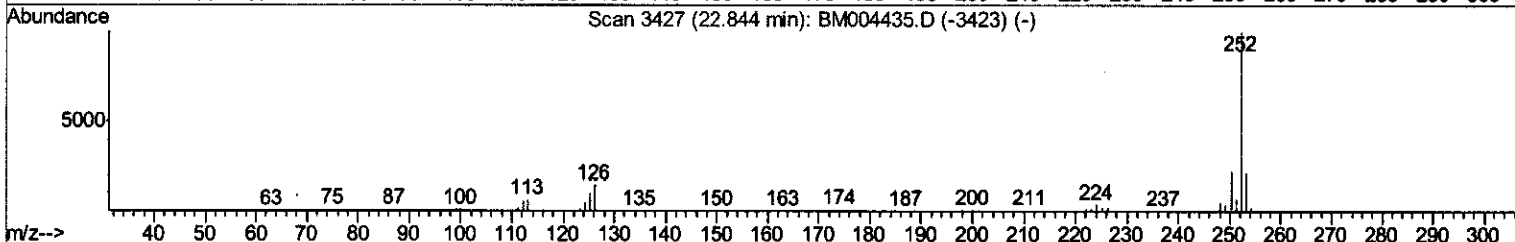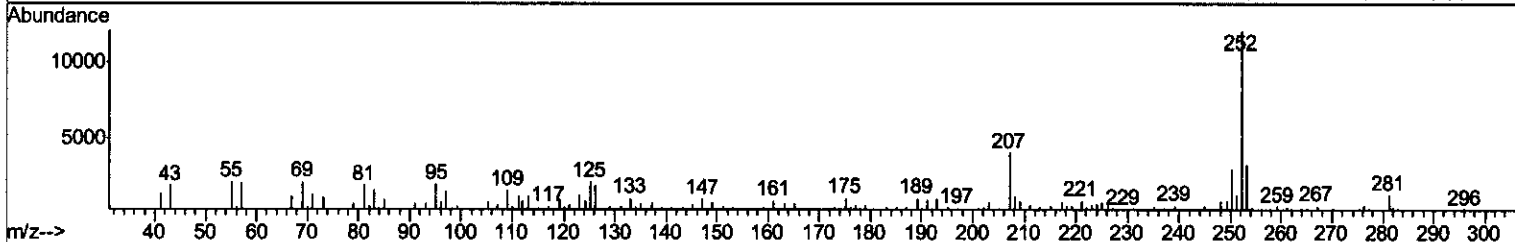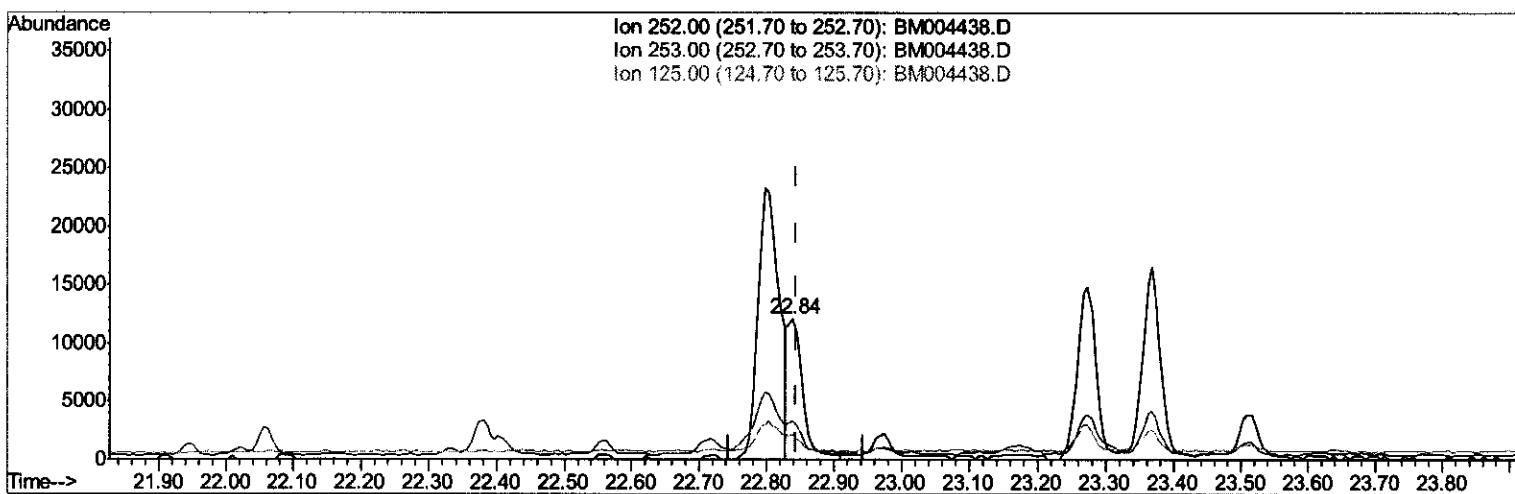

TIC: BM004438.D

(89) Benzo(k)fluoranthene

22.839min (-0.006) 1.99ng/ul m

response 18746

Ion	Exp%	Act%
252.00	100	100
253.00	21.60	27.18#
125.00	10.20	17.55#
0.00	0.00	0.00

9.3
 03/08/16

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022616\
 Data File : BM004438.D
 Acq On : 26 Feb 2016 22:28
 Operator : SJ/UM
 Sample : H1564-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9R28

Manual Integrations
 APPROVED

UMANGI
 2/29/2016 2:53:17 PM

Quant Time: Feb 27 01:01:58 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Feb 27 00:43:30 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	29148	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	121435	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	64701	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	137613	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	149560	20.00	ng/ul	0.00
86) Perylene-d12	23.46	264	148061	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.08	96	1901	3.44	ng/uL	0.00
5) Phenol-d5	6.80	99	40363	16.51	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	20991	16.89	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	37937	18.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	30733	14.07	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	16996	18.40	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	18620	17.68	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	32747	17.20	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	34386	14.49	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	101231	18.24	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	127511	19.63	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	10289m	11.54	ng/ul	0.01
58) Fluorene-d10	15.27	176	91155	19.32	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	8643	10.22	ng/ul	0.00
71) Anthracene-d10	17.13	188	138118	20.48	ng/ul	0.00
79) Pyrene-d10	19.44	212	152758	21.12	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.32	264	164804	21.21	ng/ul	0.00

> S.I
 03/08/16

Target Compounds

						Qvalue
45) Dimethylphthalate	13.73	163	33467	5.78	ng/ul	98
70) Phenanthrene	17.07	178	10183	1.23	ng/ul	97
77) Fluoranthene	19.10	202	49671	5.30	ng/ul	98
80) Pyrene	19.47	202	45771	4.68	ng/ul	99
81) Butylbenzylphthalate	20.37	149	10892	2.53	ng/ul	94
83) Benzo(a)anthracene	21.23	228	17333	1.80	ng/ul	96
84) Bis(2-ethylhexyl)phthalate	21.15	149	7922m	1.25	ng/ul	
85) Chrysene	21.28	228	31904	3.45	ng/ul	97
88) Benzo(b)fluoranthene	22.80	252	50821	5.08	ng/ul#	94
89) Benzo(k)fluoranthene	22.84	252	18746m	1.99	ng/ul	
91) Benzo(a)pyrene	23.37	252	29303	3.15	ng/ul#	91
92) Indeno(1,2,3-cd)pyrene	25.70	276	30640	3.52	ng/ul#	94
94) Benzo(g,h,i)perylene	26.39	276	21749	3.04	ng/ul	97

2 S.I
 03/08/16

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022616\
 Data File : BM004438.D
 Acq On : 26 Feb 2016 22:28
 Operator : SJ/UM
 Sample : H1564-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9R28

Manual Integrations
 APPROVED

UMANGI
 2/29/2016 2:53:17 PM

Quant Time: Feb 27 01:01:58 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Feb 27 00:43:30 2016
 Response via : Initial Calibration

