


Data Path : Z:\HPCHEM1\BNA M\Data\BM022616\
 Data File : BM004421.D
 Acq On : 26 Feb 2016 09:03
 Operator : SJ/UM
 Sample : DFTPP57
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP57

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Title : SVOA CALIBRATION
 Last Update : Sat Feb 27 00:43:30 2016

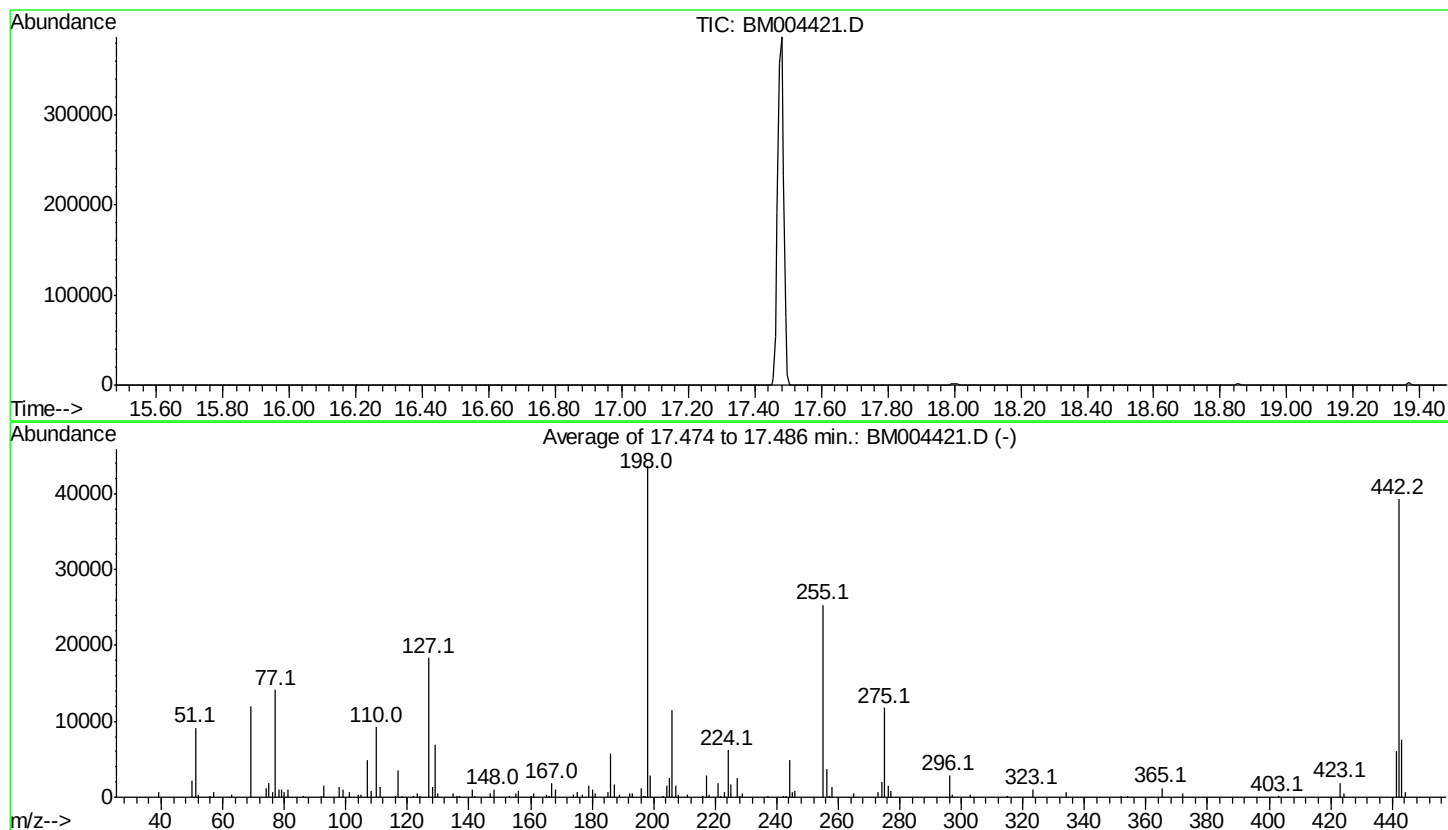

AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	21.0	9178	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	27.5	12021	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.0	18332	PASS
197	198	0.00	2	0.3	111	PASS
198	198	100	100	100.0	43672	PASS
199	198	5	9	6.7	2932	PASS
275	198	10	60	26.9	11730	PASS
365	198	1	100	2.8	1202	PASS
441	443	0.01	100	79.5	6098	PASS
442	198	50	100	89.9	39256	PASS
443	442	15	24	19.5	7671	PASS

m/z

Abundance

Instrument :

BNA_M

ClientSampleId :

DFTPP57

m/z	Abundance
39.00	768.0
50.10	2787.0
51.10	11413.0
52.00	590.0
56.00	340.0
57.00	854.0
63.00	497.0
69.00	14800.0
74.00	1371.0
75.00	2403.0
76.10	793.0
77.10	17104.0
78.10	1252.0
79.00	1179.0
80.00	888.0
81.00	1273.0
86.00	374.0
92.00	319.0
93.00	1847.0
98.00	1592.0
99.00	1235.0
101.00	698.0
104.00	435.0
105.00	478.0
107.00	5861.0
108.00	1015.0
110.00	10923.0
111.00	1700.0
116.10	355.0
117.00	4323.0
118.00	356.0
122.00	387.0
123.00	598.0
124.00	300.0
127.10	21760.0
128.00	1651.0
129.00	8111.0
130.00	718.0
135.00	652.0
137.10	403.0
141.00	1085.0
142.10	379.0
147.00	564.0
148.00	1179.0
153.00	327.0
155.00	658.0
156.10	965.0
160.00	386.0
161.10	508.0
165.00	432.0
166.00	324.0
167.00	2184.0
168.00	1196.0
174.00	453.0
175.10	870.0
177.00	444.0
179.00	1597.0
180.00	1210.0
181.00	560.0
185.10	733.0
186.10	6370.0
187.00	1870.0
189.00	373.0
192.10	513.0
193.00	581.0
196.00	1381.0
198.00	48360.0
199.00	3125.0
202.90	316.0
204.10	1628.0
205.10	2963.0
206.10	12619.0
207.10	1727.0
208.00	401.0
211.10	482.0
217.00	3077.0
218.00	382.0
221.10	2264.0
223.00	677.0
224.10	6812.0
225.10	1844.0
227.00	2631.0
228.00	387.0
229.00	550.0
242.10	312.0
243.10	361.0
244.10	5475.0
245.10	683.0
246.00	933.0
255.10	26648.0
256.10	4091.0
257.10	313.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57

258.00	1457.0
265.10	587.0
273.00	778.0
274.10	2121.0
275.10	12183.0
276.10	1703.0
277.10	893.0
296.10	2959.0
297.00	401.0
303.00	333.0
315.00	319.0
323.10	910.0
334.10	662.0
354.10	322.0
365.10	1168.0
372.10	446.0
423.10	1730.0
424.10	481.0
441.20	5294.0
442.20	34400.0
443.20	6974.0
444.10	665.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57

m/z	Abundance
39.00	744.0
50.10	2692.0
51.10	10693.0
52.00	527.0
56.00	314.0
57.00	802.0
63.00	519.0
69.00	13742.0
74.10	1451.0
75.10	2210.0
76.10	736.0
77.10	16313.0
78.10	1120.0
79.00	1054.0
80.00	831.0
81.00	1187.0
86.00	400.0
93.00	1913.0
98.00	1414.0
99.00	1127.0
101.00	733.0
104.00	498.0
105.10	416.0
107.00	5570.0
108.00	856.0
110.00	10683.0
111.00	1589.0
115.90	330.0
117.00	3960.0
118.00	315.0
122.00	374.0
123.10	623.0
124.00	308.0
127.10	21256.0
128.00	1565.0
129.00	7995.0
130.00	667.0
135.00	648.0
136.00	318.0
137.10	323.0
141.00	1175.0
142.00	388.0
147.00	620.0
148.00	1152.0
153.00	352.0
155.00	625.0
156.10	948.0
160.00	357.0
161.00	555.0
165.00	466.0
166.00	313.0
167.00	2015.0
168.00	1021.0
174.00	405.0
175.00	879.0
177.00	444.0
179.00	1779.0
180.00	1191.0
181.10	566.0
185.00	797.0
186.10	6957.0
187.10	2040.0
189.00	439.0
192.00	498.0
193.10	670.0
196.00	1506.0
196.80	333.0
197.10	319.0
198.00	51448.0
199.00	3601.0
203.00	323.0
204.10	1761.0
205.10	2974.0
206.10	13552.0
207.10	1954.0
208.00	527.0
211.10	541.0
216.00	320.0
217.00	3319.0
218.00	440.0
221.10	2177.0
223.00	741.0
224.10	7374.0
225.10	2043.0
227.10	2956.0
228.00	363.0
229.00	616.0
237.10	315.0
242.10	392.0
243.10	365.0
244.10	5658.0
245.10	712.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57

246.00	1098.0
255.10	30160.0
256.10	4214.0
257.10	302.0
258.00	1684.0
265.00	668.0
273.00	879.0
274.10	2381.0
275.10	13905.0
276.10	1725.0
277.10	1121.0
296.10	3426.0
297.00	410.0
303.00	447.0
315.10	379.0
323.10	1162.0
334.10	668.0
352.10	364.0
354.10	408.0
365.10	1416.0
372.10	582.0
403.10	395.0
423.10	2181.0
424.10	579.0
441.20	7369.0
442.20	46528.0
443.20	9141.0
444.10	893.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57

m/z	Abundance
39.00	400.0
50.00	1343.0
51.10	5428.0
57.00	440.0
69.00	7521.0
74.00	702.0
75.00	1141.0
76.10	354.0
77.10	8901.0
78.00	569.0
79.00	615.0
80.00	495.0
81.00	625.0
93.00	1007.0
98.00	806.0
99.00	671.0
101.00	363.0
107.10	3060.0
108.00	503.0
110.00	6125.0
111.00	928.0
117.00	2373.0
123.00	377.0
127.10	11981.0
128.00	881.0
129.10	4637.0
130.00	367.0
135.00	363.0
141.00	577.0
147.00	345.0
148.00	674.0
155.00	360.0
156.00	532.0
161.00	327.0
167.00	1321.0
168.00	613.0
175.00	495.0
179.00	951.0
180.10	773.0
181.00	320.0
185.00	486.0
186.10	4129.0
187.10	1146.0
192.10	382.0
193.10	347.0
196.00	880.0
198.00	31208.0
199.00	2072.0
204.00	1056.0
205.10	1862.0
206.10	8069.0
207.10	1126.0
217.00	2174.0
221.10	1252.0
221.80	316.0
223.00	469.0
224.10	4334.0
225.10	1206.0
227.00	1807.0
229.00	419.0
244.10	3453.0
245.10	439.0
246.00	673.0
255.10	19240.0
256.10	2744.0
258.10	939.0
265.00	440.0
273.10	495.0
274.10	1601.0
275.10	9104.0
276.10	1099.0
277.00	692.0
296.00	2165.0
323.10	777.0
334.10	493.0
365.10	1024.0
372.10	397.0
423.10	1788.0
424.20	438.0
441.20	5633.0
442.20	36840.0
443.20	6899.0
444.10	592.0

Instrument :
BNA_M
ClientSampleId :
DFTPP57