




Data Path : Z:\HPCHEM1\BNA M\DATA\BM022618\
Data File : BM014374.D
Acq On : 27 Feb 2018 01:47
Operator : SJ/JU
Sample : J1646-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE5X7

Manual Integrations
APPROVED

Sohil
2/27/2018 4:58:50 PM

Quant Time: Feb 27 03:27:33 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 03:22:24 2018
Response via : Initial Calibration

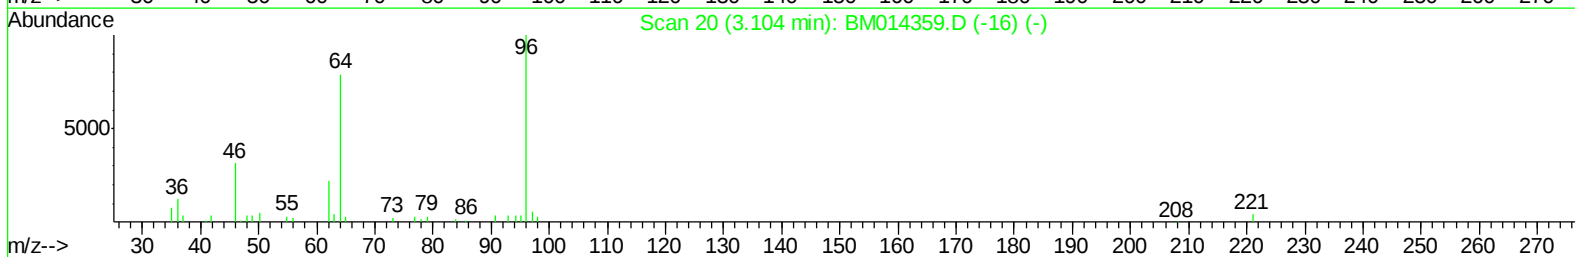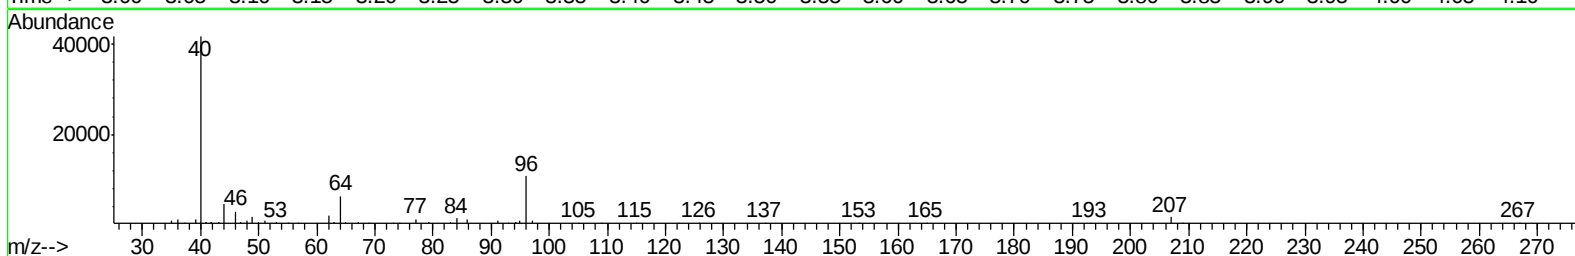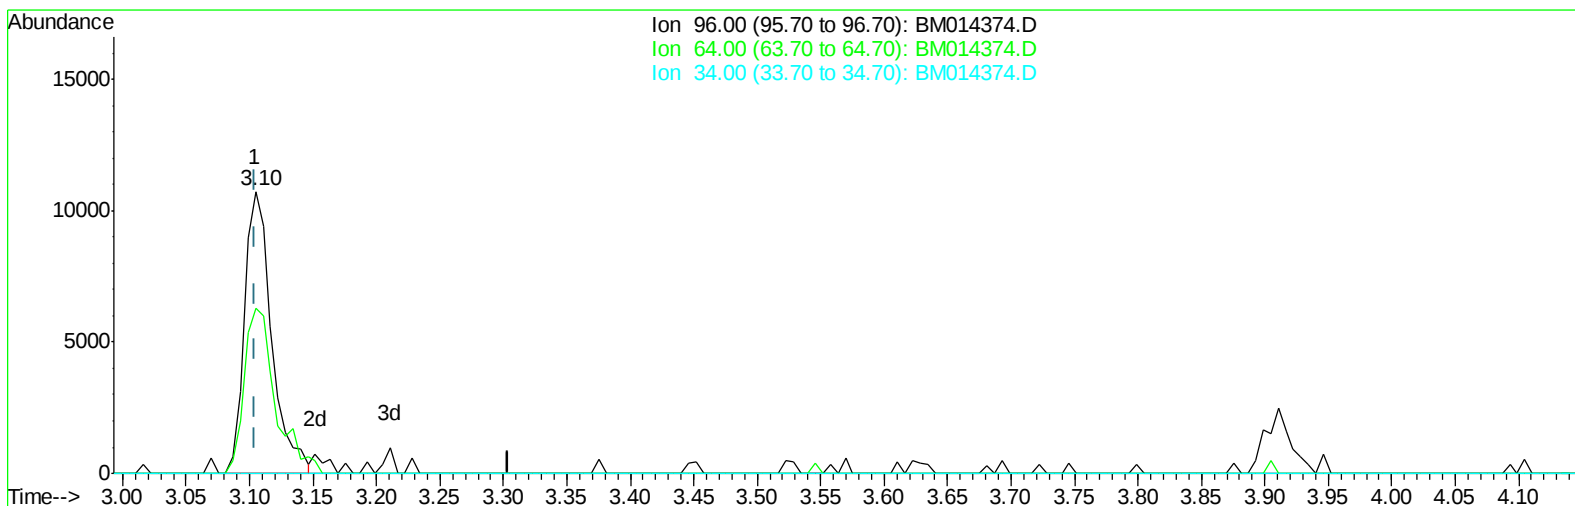

TIC: BM014374.D

(3) 1,4-Dioxane-d8 (S)

3.105min (+0.000) 4.33ng/uL

response 15919

Ion	Exp%	Act%
96.00	100	100
64.00	74.90	60.35
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\DATA\BM022618\
Data File : BM014374.D
Acq On : 27 Feb 2018 01:47
Operator : SJ/JU
Sample : J1646-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE5X7

Manual Integrations
APPROVED

Sohil
2/27/2018 4:58:50 PM

Quant Time: Feb 27 03:27:33 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 03:22:24 2018
Response via : Initial Calibration

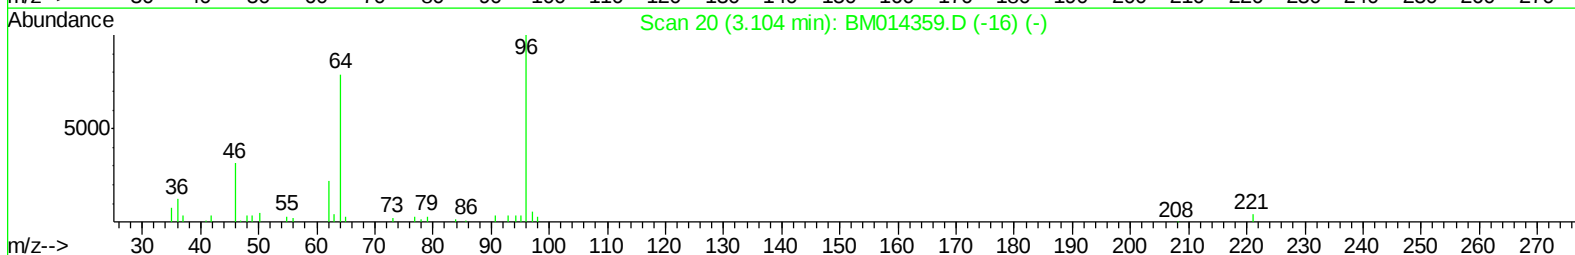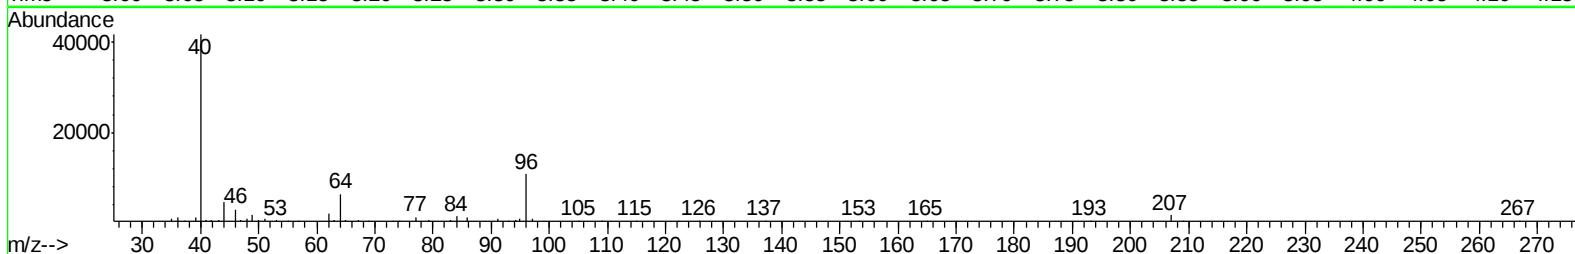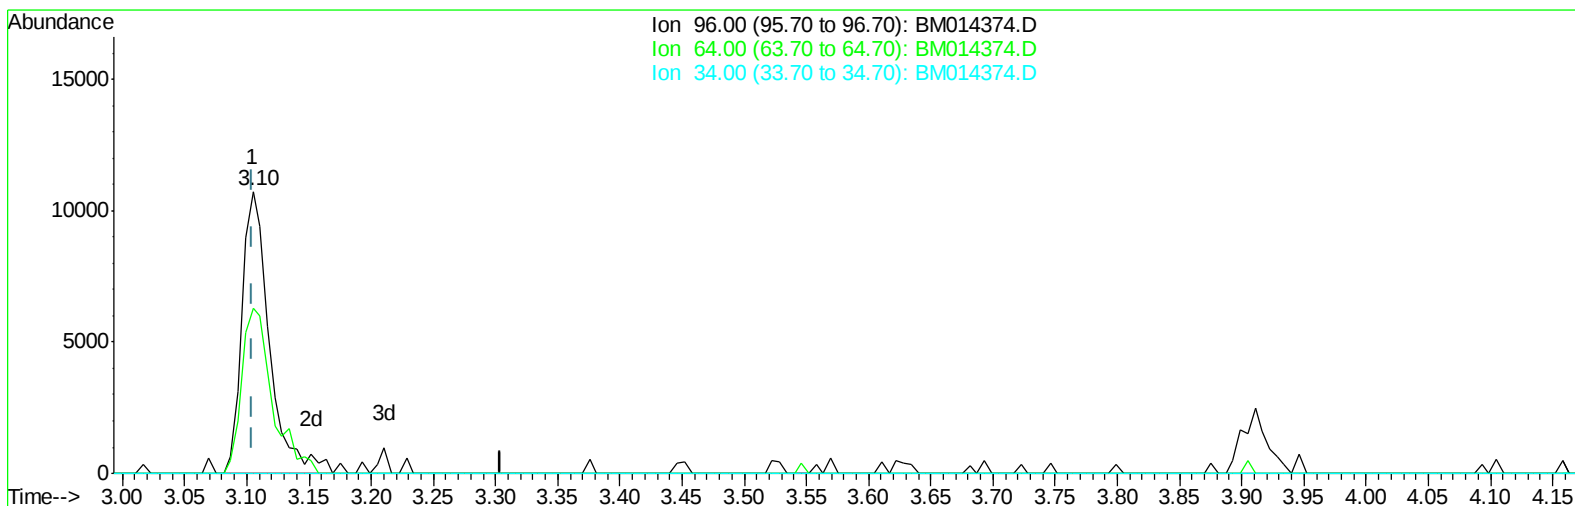

TIC: BM014374.D

(3) 1,4-Dioxane-d8 (S)

3.105min (+0.000) 4.49ng/uL m

response 16502

Ion	Exp%	Act%
96.00	100	100
64.00	74.90	58.22#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\DATA\BM022618\
Data File : BM014374.D
Acq On : 27 Feb 2018 01:47
Operator : SJ/JU
Sample : J1646-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE5X7

Manual Integrations
APPROVED

Sohil
2/27/2018 4:58:50 PM

Quant Time: Feb 27 06:52:27 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 03:22:24 2018
Response via : Initial Calibration

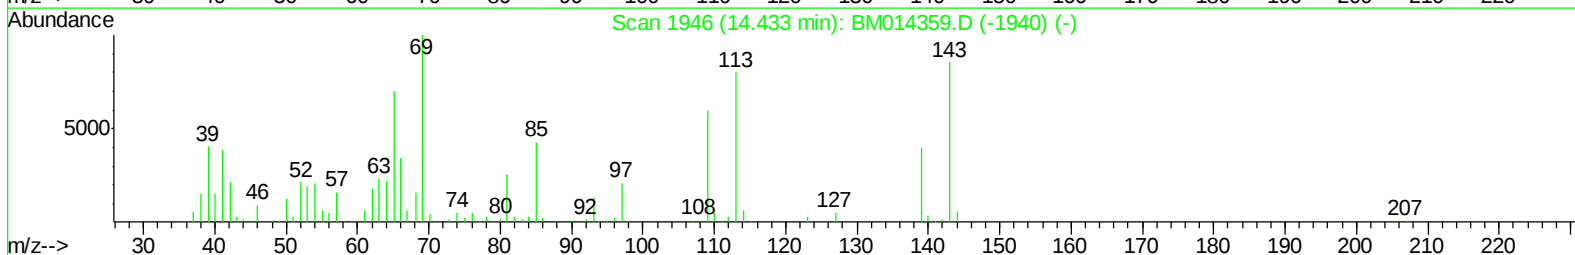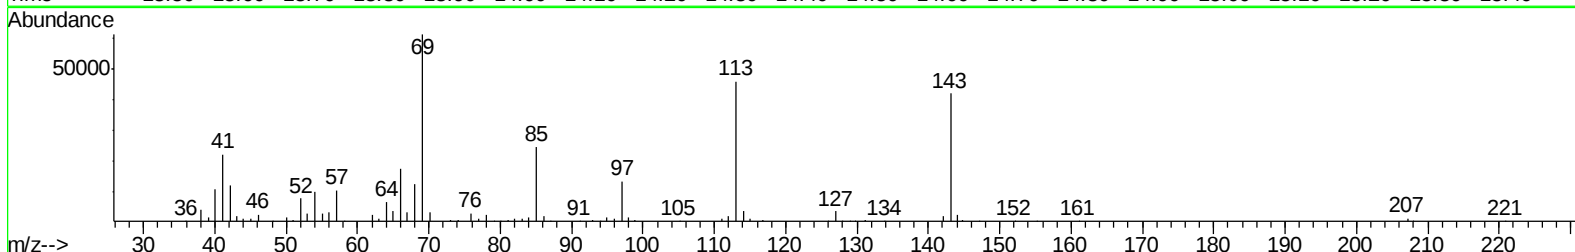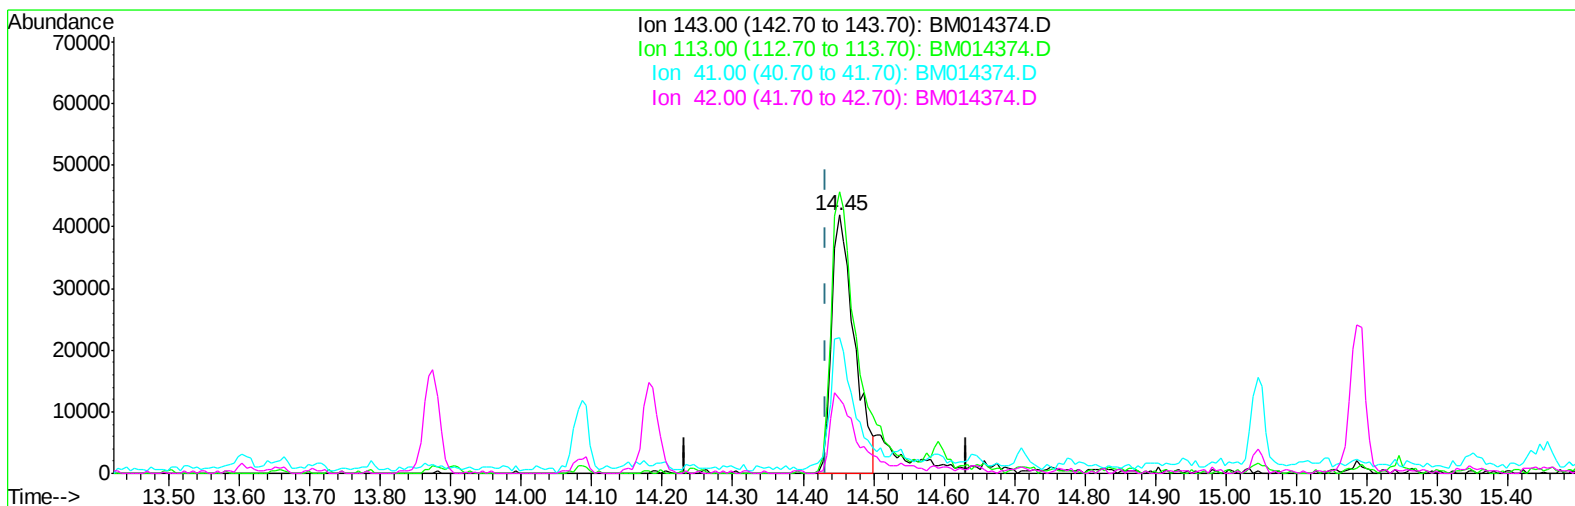

TIC: BM014374.D

(51) 4-Nitrophenol-d4 (S)

14.451min (+0.018) 20.36ng/ul

response 92908

Ion	Exp%	Act%
143.00	100	100
113.00	114.60	108.97
41.00	34.80	52.43#
42.00	20.50	28.77#




Data Path : Z:\HPCHEM1\BNA M\DATA\BM022618\
Data File : BM014374.D
Acq On : 27 Feb 2018 01:47
Operator : SJ/JU
Sample : J1646-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE5X7

Manual Integrations
APPROVED

Sohil
2/27/2018 4:58:50 PM

Quant Time: Feb 27 06:52:27 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 03:22:24 2018
Response via : Initial Calibration

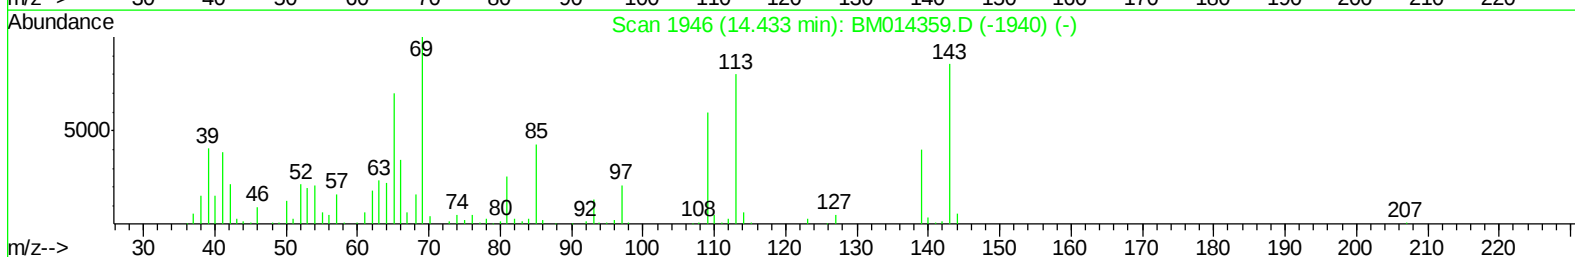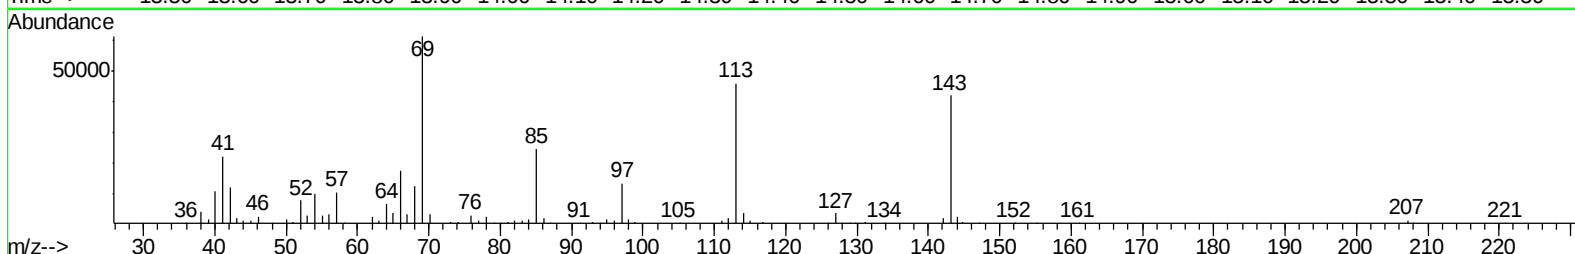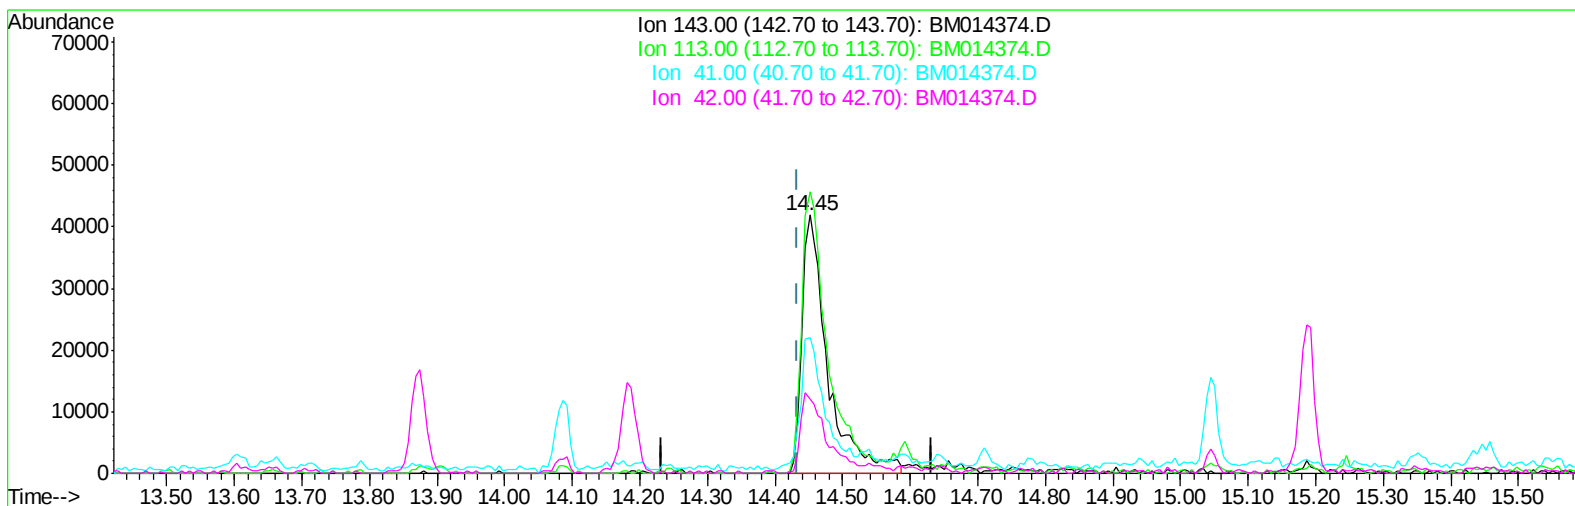

TIC: BM014374.D

(51) 4-Nitrophenol-d4 (S)

14.451min (+0.018) 23.97ng/ul m

response 109356

Ion	Exp%	Act%
143.00	100	100
113.00	114.60	108.97
41.00	34.80	52.43#
42.00	20.50	28.77#




Data Path : Z:\HPCHEM1\BNA M\DATA\BM022618\
Data File : BM014374.D
Acq On : 27 Feb 2018 01:47
Operator : SJ/JU
Sample : J1646-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE5X7

Manual Integrations
APPROVED

Sohil
2/27/2018 4:58:50 PM

Quant Time: Feb 27 06:53:45 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 03:22:24 2018
Response via : Initial Calibration

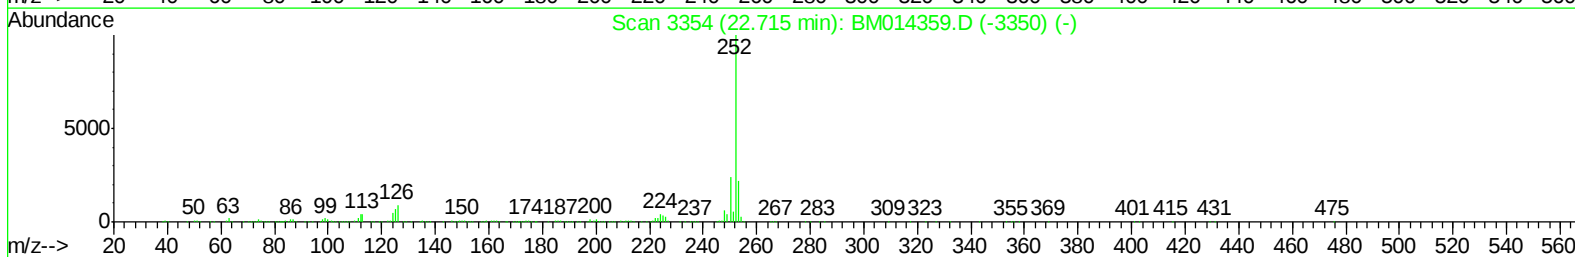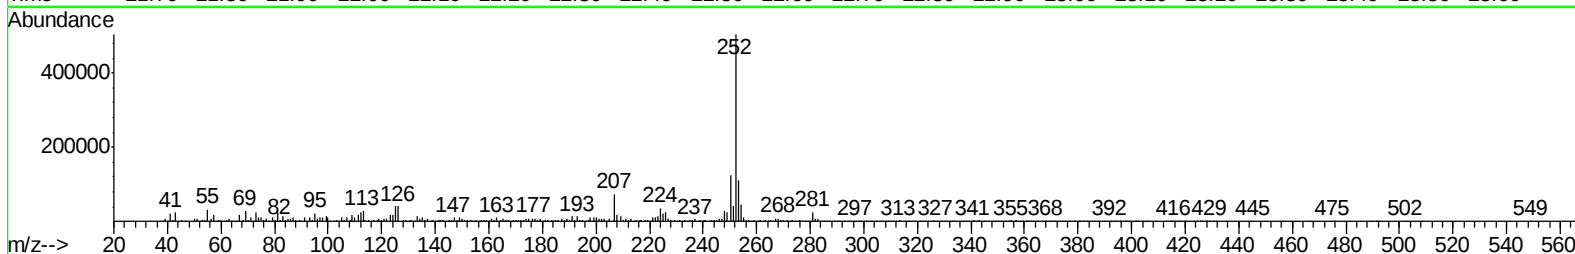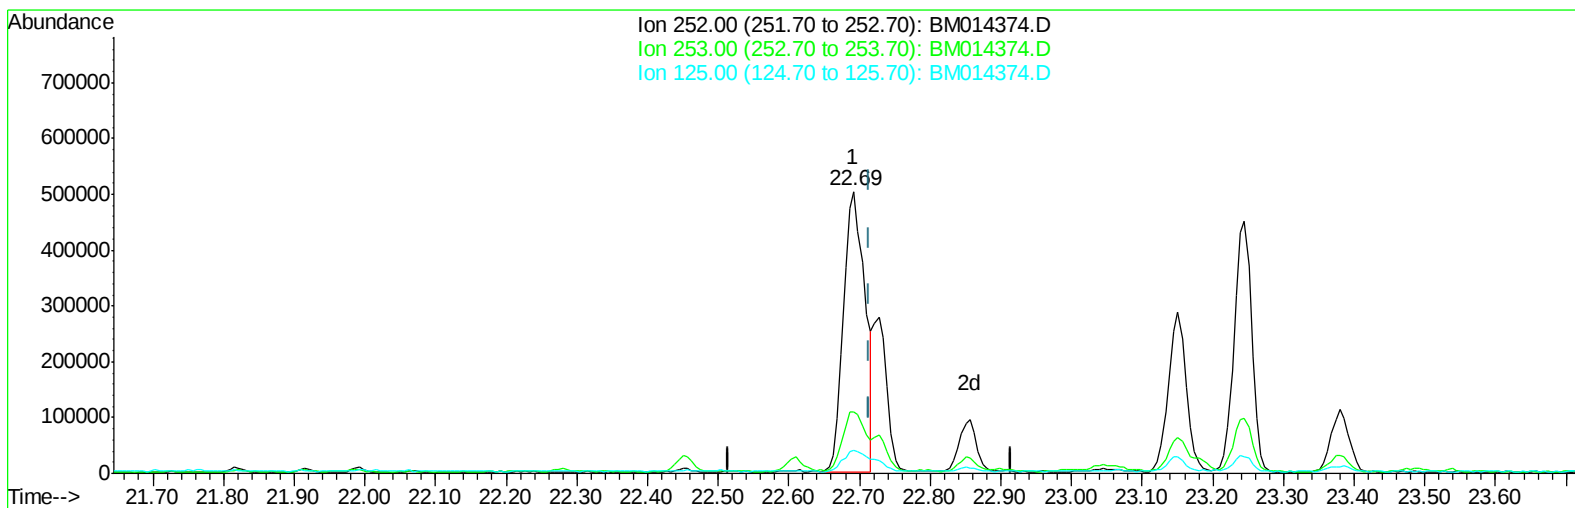

TIC: BM014374.D

(86) Benzo(k)fluoranthene

22.692min (-0.023) 34.65ng/ul

response 1067148

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	21.77
125.00	4.30	7.98#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA M\DATA\BM022618\
Data File : BM014374.D
Acq On : 27 Feb 2018 01:47
Operator : SJ/JU
Sample : J1646-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE5X7

Manual Integrations
APPROVED

Sohil
2/27/2018 4:58:50 PM

Quant Time: Feb 27 06:53:45 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 03:22:24 2018
Response via : Initial Calibration

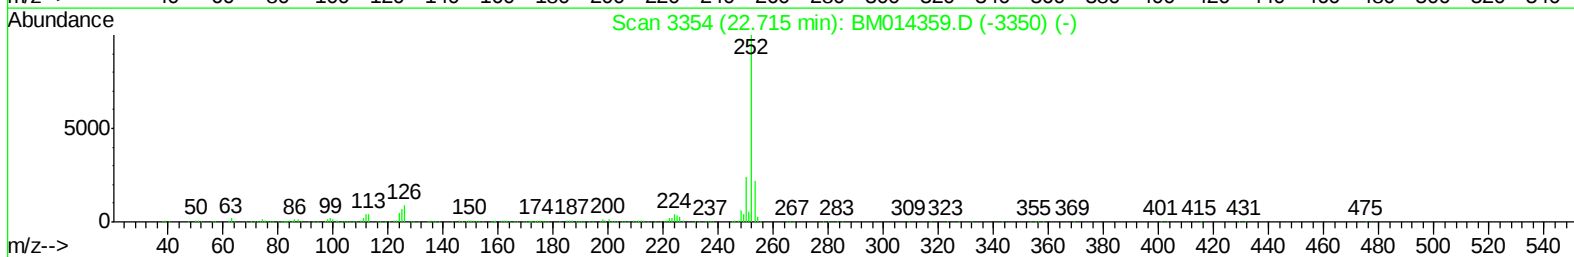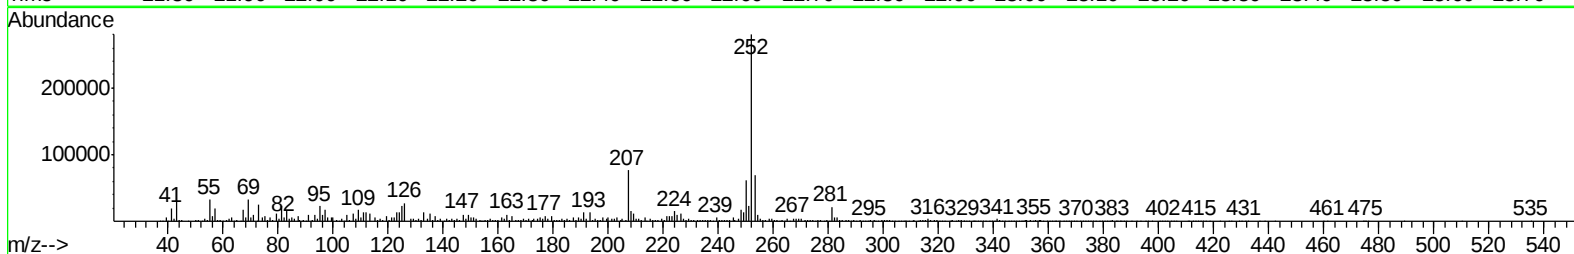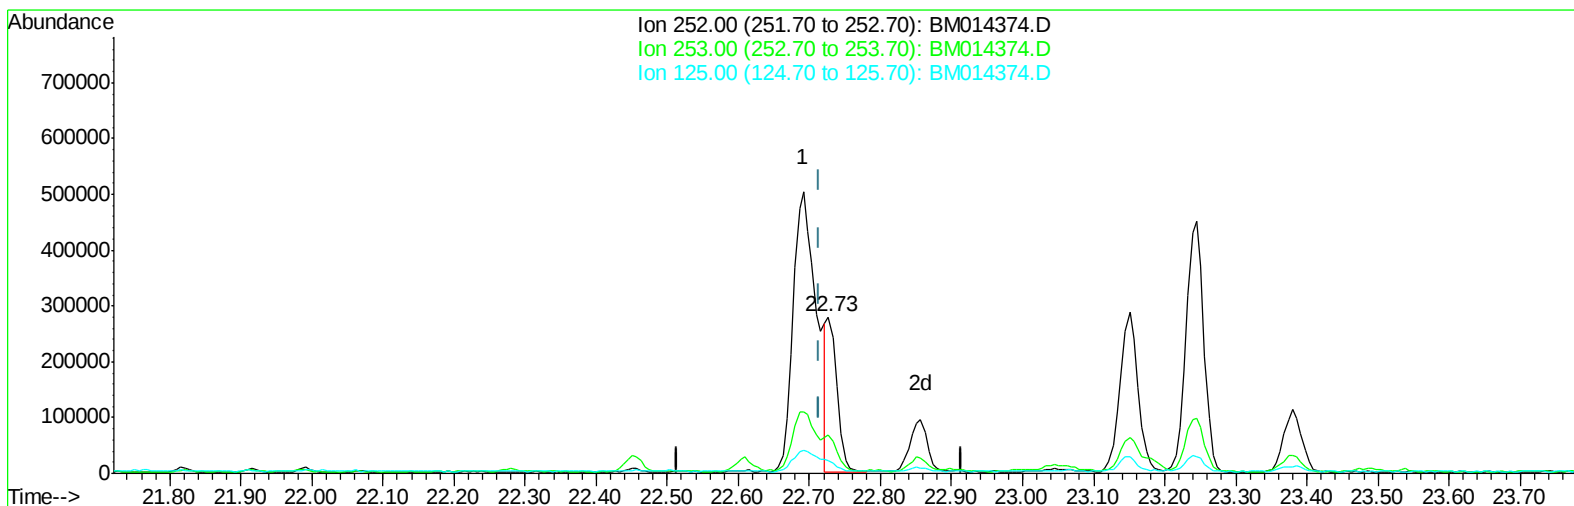

TIC: BM014374.D

(86) Benzo(k)fluoranthene

22.727min (+0.012) 9.00ng/ul m

response 277245

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	24.61
125.00	4.30	8.02#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022618\
 Data File : BM014374.D
 Acq On : 27 Feb 2018 01:47
 Operator : SJ/JU
 Sample : J1646-13
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BE5X7

Manual Integrations
 APPROVED

Sohil
 2/27/2018 4:58:50 PM

Quant Time: Feb 27 06:58:02 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 27 03:22:24 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	157419	20.00	ng/ul	0.00
18) Naphthalene-d8	10.30	136	712778	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.18	164	400166	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.95	188	789350	20.00	ng/ul	0.00
75) Chrysene-d12	21.16	240	542968	20.00	ng/ul	0.00
83) Perylene-d12	23.33	264	483820	20.00	ng/ul	0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.10	96	16502m	4.49	ng/uL	0.00
5) Phenol-d5	6.73	99	377439	28.37	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	6.88	67	227707	28.27	ng/ul	0.00
9) 2-Chlorophenol-d4	7.06	132	314704	30.85	ng/ul	0.00
13) 4-Methylphenol-d8	8.25	113	303355	26.06	ng/ul	0.00
19) Nitrobenzene-d5	8.69	128	162535	30.86	ng/ul	0.00
22) 2-Nitrophenol-d4	9.40	143	180179	33.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.94	165	332431	29.44	ng/ul	0.01
29) 4-Chloroaniline-d4	10.46	131	283000	25.44	ng/ul	0.00
43) Dimethylphthalate-d6	13.61	166	1070659	32.40	ng/ul	0.00
46) Acenaphthylene-d8	13.87	160	1350313	33.14	ng/ul	0.00
51) 4-Nitrophenol-d4	14.45	143	109356m	23.97	ng/ul	0.02
57) Fluorene-d10	15.19	176	862652	29.14	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	32515	6.87	ng/ul	0.02
70) Anthracene-d10	17.05	188	1238340	32.52	ng/ul	0.00
76) Pyrene-d10	19.36	212	1071846	38.27	ng/ul	0.01
87) Benzo(a)pyrene-d12	23.20	264	737912	31.34	ng/ul	0.02

Target Compounds

					Ovalue	
6) Phenol	6.75	94	44497	3.187	ng/ul	97
28) Naphthalene	10.35	128	128233	3.503	ng/ul	97
44) Dimethylphthalate	13.65	163	268824	8.250	ng/ul	100
47) Acenaphthylene	13.90	152	120587	3.131	ng/ul	96
49) Acenaphthene	14.25	153	77577	2.860	ng/ul	98
53) Dibenzofuran	14.59	168	61368	1.509	ng/ul	88
58) Fluorene	15.25	166	83871	2.389	ng/ul	95
69) Phenanthrene	16.99	178	1823700	40.100	ng/ul	99
71) Anthracene	17.08	178	405226	8.860	ng/ul	98
72) Carbazole	17.36	167	150981	3.926	ng/ul#	96
74) Fluoranthene	19.02	202	2847485	52.406	ng/ul#	93
77) Pyrene	19.39	202	2390307	66.243	ng/ul#	93
80) Benzo(a)anthracene	21.14	228	1086905	32.075	ng/ul	97
82) Chrysene	21.19	228	923557	29.215	ng/ul	97
85) Benzo(b)fluoranthene	22.69	252	1067148	32.941	ng/ul#	97
86) Benzo(k)fluoranthene	22.73	252	277245m	9.001	ng/ul	
88) Benzo(a)pyrene	23.24	252	781701	27.003	ng/ul#	98
89) Indeno(1,2,3-cd)pyrene	25.50	276	485542	17.284	ng/ul	98
90) Dibenzo(a,h)anthracene	25.50	278	138263	5.923	ng/ul#	87
91) Benzo(g,h,i)perylene	26.16	276	361327	15.878	ng/ul#	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022618\
Data File : BM014374.D
Acq On : 27 Feb 2018 01:47
Operator : SJ/JU
Sample : J1646-13
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE5X7

Quant Time: Feb 27 06:58:02 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 03:22:24 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
2/27/2018 4:58:50 PM

