

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044360.D
 Acq On : 27 Feb 2024 11:00
 Operator : MA/JU
 Sample : P1469-19
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Feb 27 22:27:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 27 00:07:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	246757	20.000	ng/ul	0.00
20) Naphthalene-d8	10.739	136	1048942	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.574	164	590174	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.327	188	1250076	20.000	ng/ul	0.00
79) Chrysene-d12	21.527	240	1124930	20.000	ng/ul	0.00
88) Perylene-d12	23.938	264	1246110	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	46820	5.987	ng/uL	0.00
4) Pyridine-d5	3.775	84	690697	32.338	ng/ul	0.00
7) Phenol-d5	7.098	99	878395	37.160	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	556236	36.337	ng/ul	0.00
11) 2-Chlorophenol-d4	7.463	132	704582	39.576	ng/ul	0.00
15) 4-Methylphenol-d8	8.645	113	701078	39.197	ng/ul	0.00
21) Nitrobenzene-d5	9.104	128	359282	42.126	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143	396208	45.534	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.357	165	627949	40.911	ng/ul	0.00
31) 4-Chloroaniline-d4	10.886	131	1007323	39.075	ng/ul	0.00
46) Dimethylphthalate-d6	13.998	166	1971150	43.306	ng/ul	0.00
49) Acenaphthylene-d8	14.268	160	2418966	46.191	ng/ul	0.00
54) 4-Nitrophenol-d4	14.780	143	390074	43.067	ng/ul	0.00
60) Fluorene-d10	15.568	176	1758687	45.650	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	286400	36.924	ng/ul	0.00
73) Anthracene-d10	17.427	188	2723356	45.690	ng/ul	0.00
81) Pyrene-d10	19.727	212	3130535	46.257	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.785	264	3038420	47.585	ng/ul	0.01
Target Compounds						
48) 2,6-Dinitrotoluene	14.004	165	10974	1.261	ng/ul#	30


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044360.D
Acq On : 27 Feb 2024 11:00
Operator : MA/JU
Sample : P1469-19
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Feb 27 22:27:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 00:07:53 2024
Response via : Initial Calibration

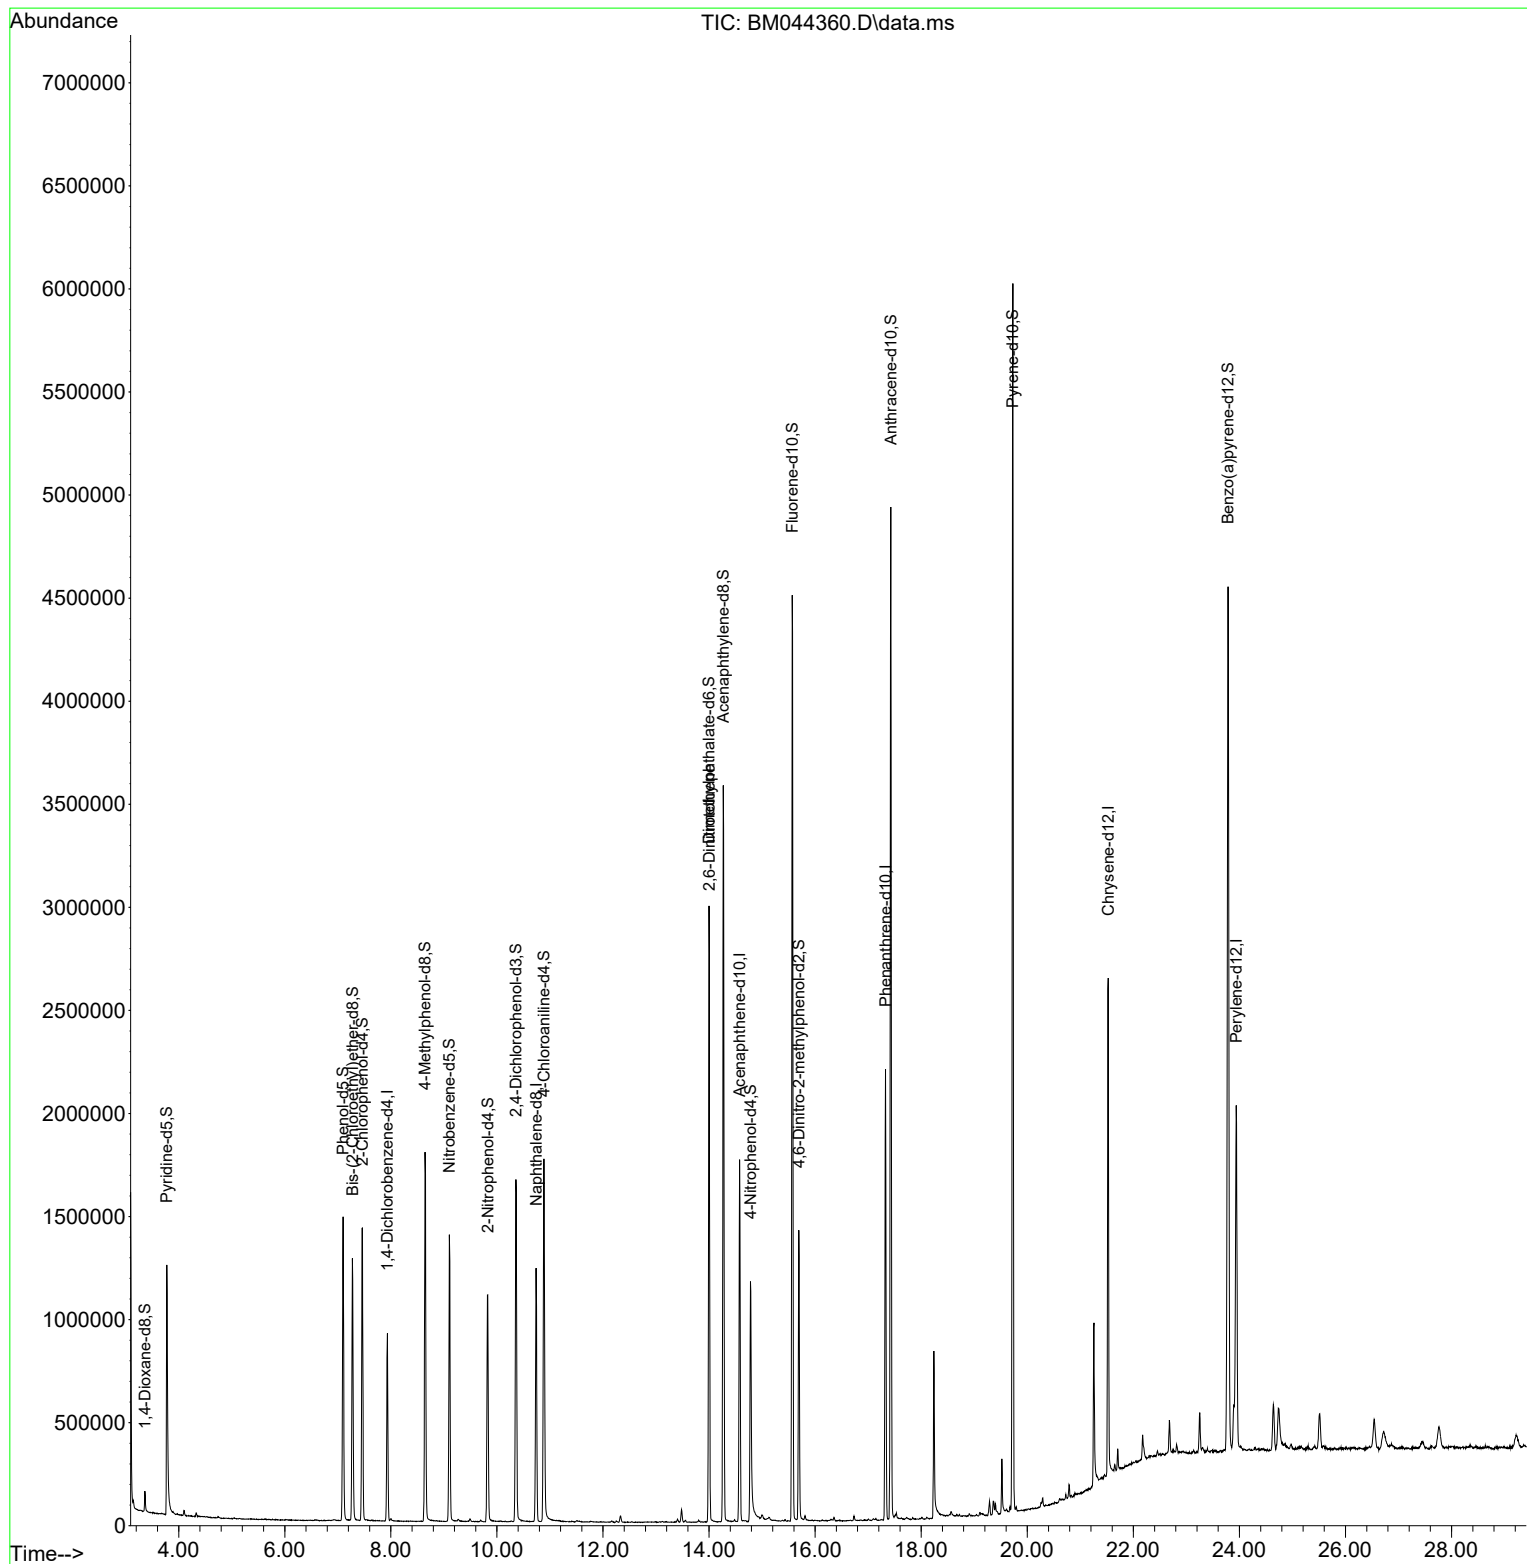

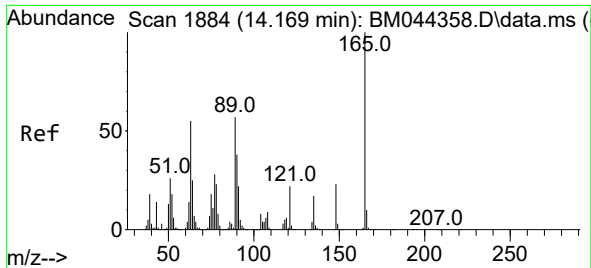

#48
2,6-Dinitrotoluene
Concen: 1.261 ng/ul
RT: 14.004 min Scan# 11
Delta R.T. -0.165 min
Lab File: BM044360.D
Acq: 27 Feb 2024 11:00

Instrument :
BNA_M
ClientSampleId :

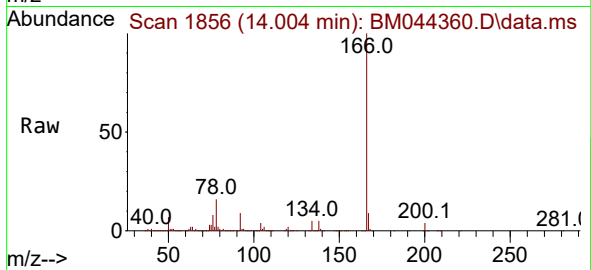

Tgt Ion	Ratio	Lower	Upper
165	100		
89	0.0	48.2	72.2#
121	45.3	18.7	28.1#

