

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030099.D
 Acq On : 27 Feb 2024 19:31
 Operator : MA/JU
 Sample : PB159254BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK254

Quant Time: Feb 27 23:51:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	3495	0.400	ng/ul	0.00
4) Naphthalene-d8	10.645	136	10187	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.493	164	5027	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.247	188	9739	0.400	ng/ul	-0.02
17) Chrysene-d12	21.460	240	6078	0.400	ng/ul	0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.83
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.311	96	30990	7.111	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.245	152	5058	0.390	ng/ul	0.00
18) Fluoranthene-d10	19.281	212	8831	0.442	ng/ul	-0.01
Target Compounds						
					Qvalue	
20) Pyrene	19.648	202	1492	0.052	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030099.D
Acq On : 27 Feb 2024 19:31
Operator : MA/JU
Sample : PB159254BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK254

Quant Time: Feb 27 23:51:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration

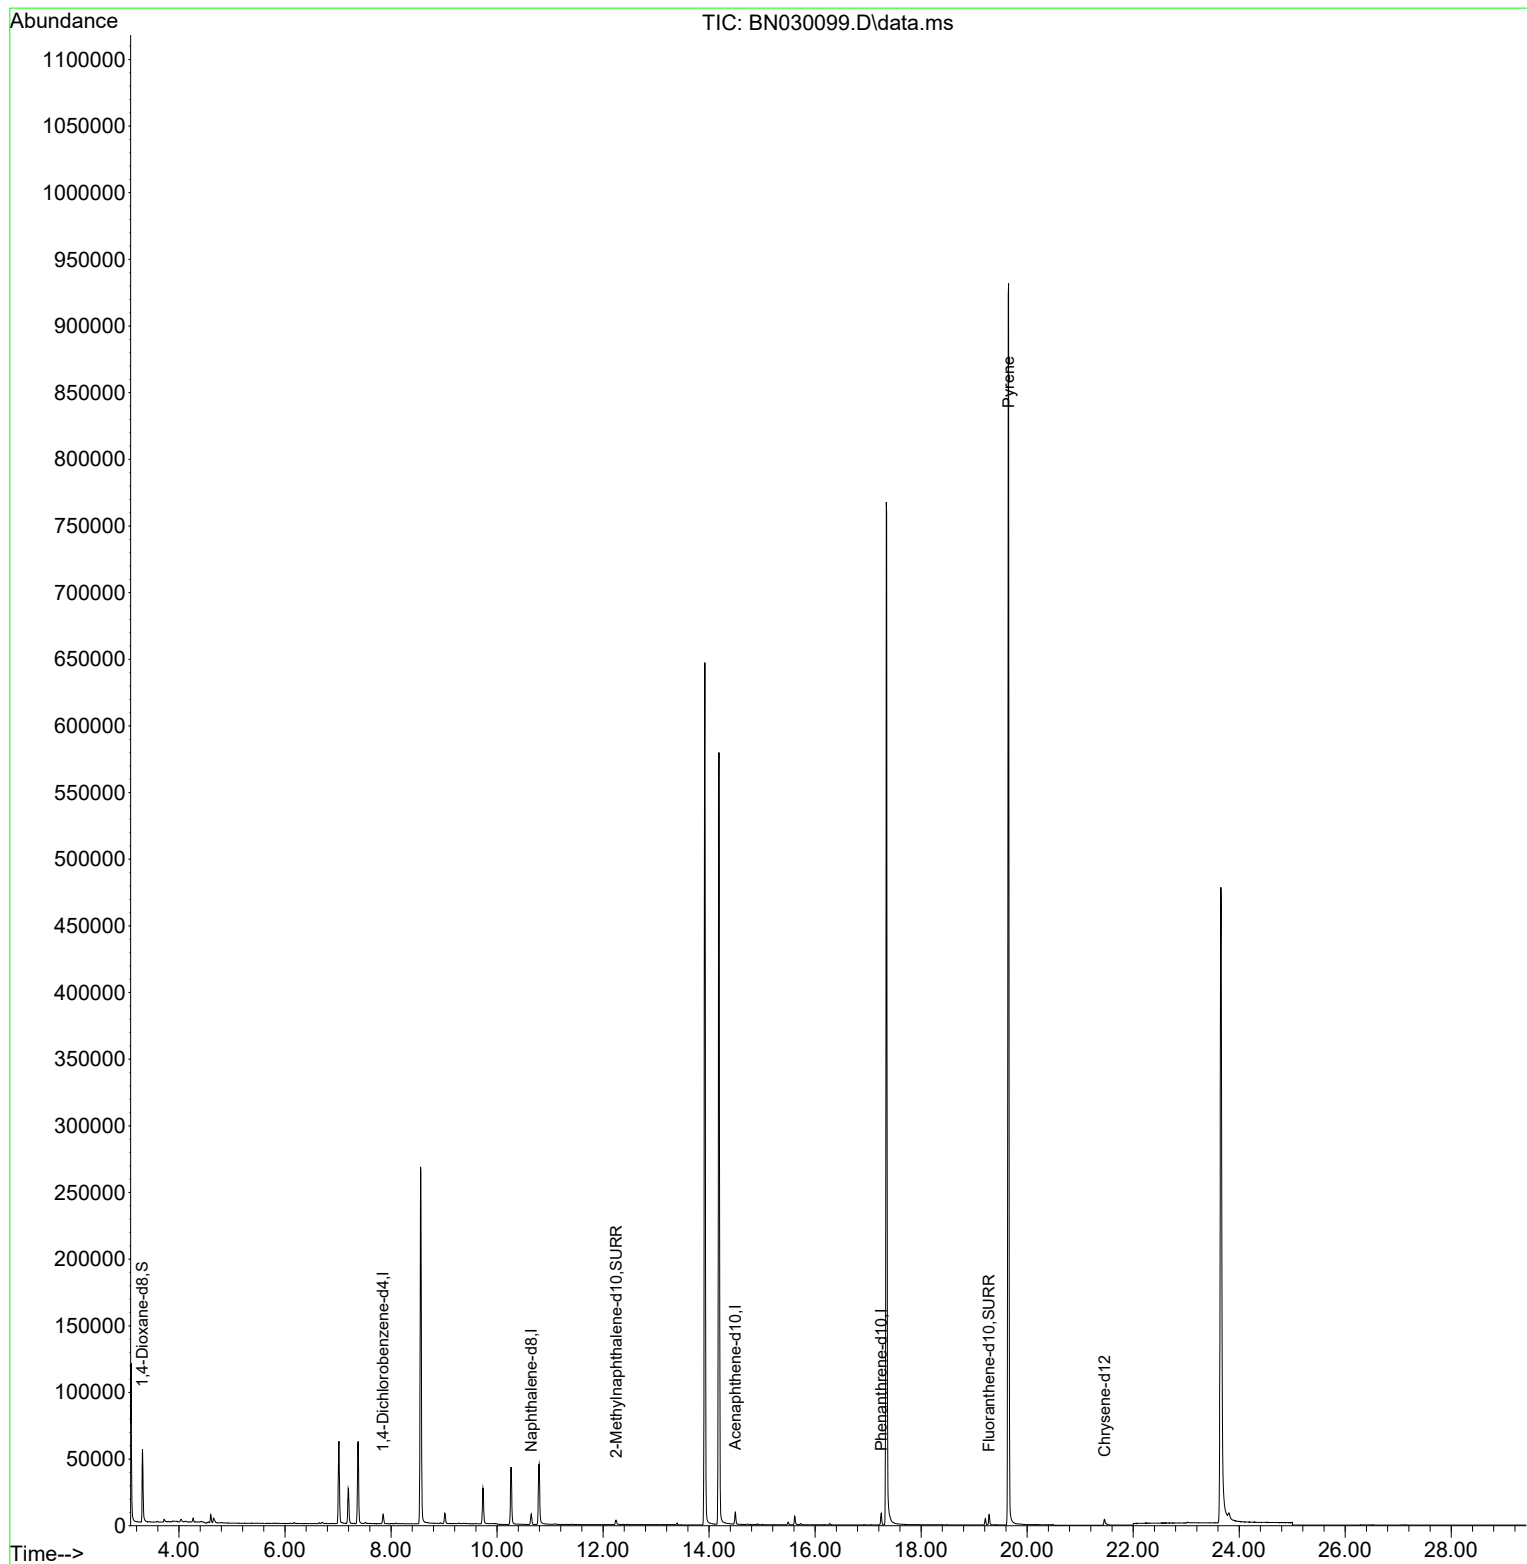

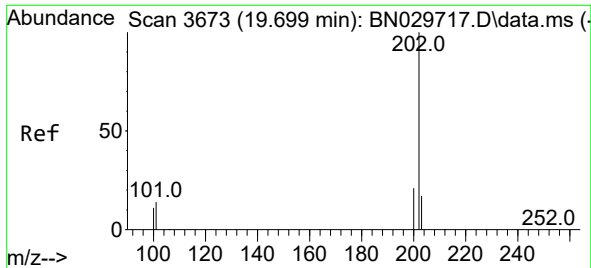

#20
 Pyrene
 Concen: 0.052 ng/ul
 RT: 19.648 min Scan# 30
 Delta R.T. -0.037 min
 Lab File: BN030099.D
 Acq: 27 Feb 2024 19:31

Instrument :
 BNA_M
 ClientSampleId :
 SBLK254

Tgt Ion:202 Resp: 1492
 Ion Ratio Lower Upper
 202 100
 101 203.7 12.5 18.7#
 100 1463.4 10.0 15.0#

