

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
 Data File : BN030102.D
 Acq On : 27 Feb 2024 21:20
 Operator : MA/JU
 Sample : P1508-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Feb 27 23:51:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 27 23:49:29 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.851	152	4008	0.400	ng/ul	0.00
4) Naphthalene-d8	10.645	136	11766	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.493	164	5891	0.400	ng/ul #	0.00
13) Phenanthrene-d10	17.247	188	11138	0.400	ng/ul	-0.02
17) Chrysene-d12	21.453	240	6827	0.400	ng/ul	-0.01
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.83
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.315	96	21993	4.401	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.245	152	5985	0.400	ng/ul	0.00
18) Fluoranthene-d10	19.282	212	12391	0.552	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.349	88	146	0.027	ng/ul#	60
20) Pyrene	19.644	202	2305	0.072	ng/ul#	1
22) Chrysene	21.491	228	539	0.020	ng/ul#	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022824\
Data File : BN030102.D
Acq On : 27 Feb 2024 21:20
Operator : MA/JU
Sample : P1508-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Feb 27 23:51:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 27 23:49:29 2024
Response via : Initial Calibration




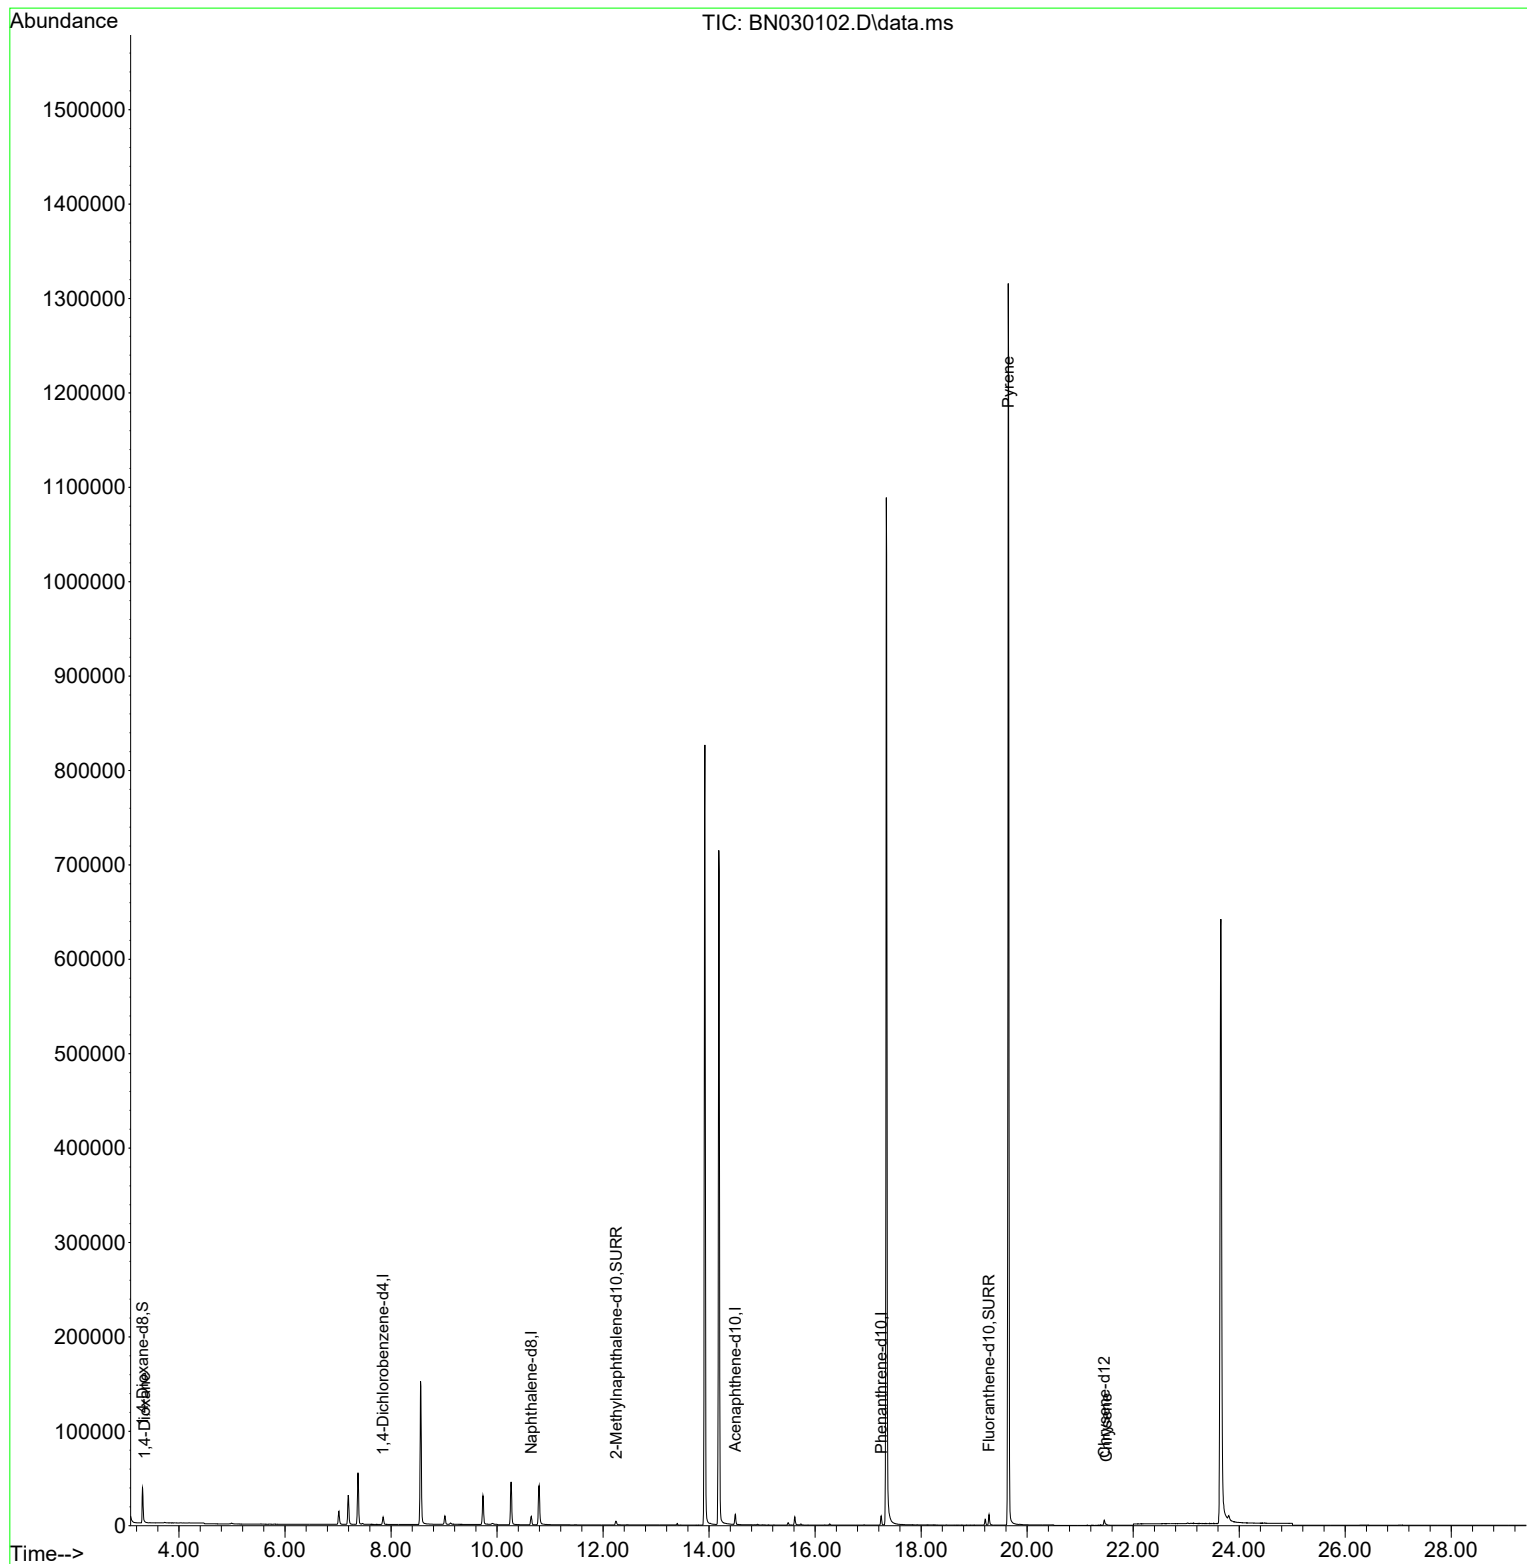


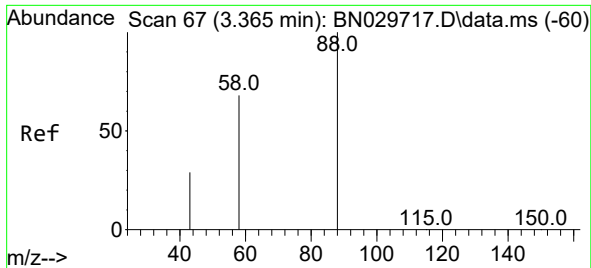

#2
 1,4-Dioxane
 Concen: 0.027 ng/ul
 RT: 3.349 min Scan# 61
 Delta R.T. -0.004 min
 Lab File: BN030102.D
 Acq: 27 Feb 2024 21:20




Instrument :
 BNA_M
 ClientSampleId :


Tgt Ion: 88 Resp: 146
 Ion Ratio Lower Upper
 88 100
 43 36.3 21.8 32.6#
 58 13.5 39.3 58.9#

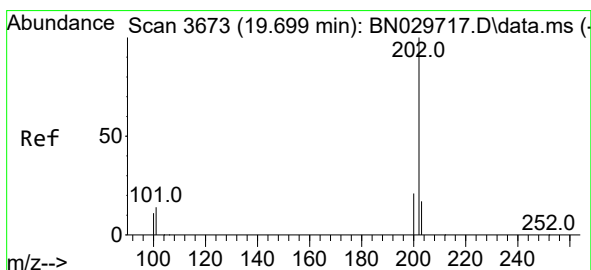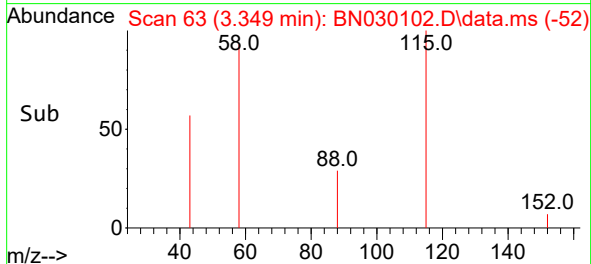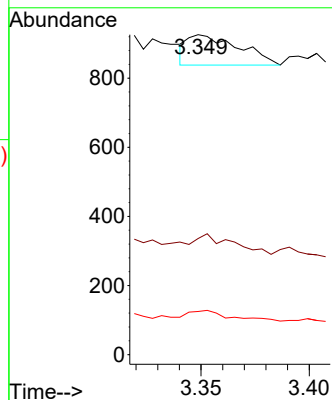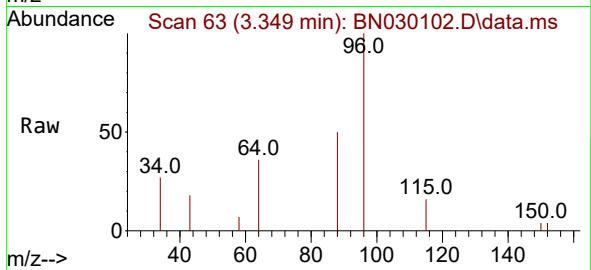

#20
 Pyrene
 Concen: 0.072 ng/ul
 RT: 19.644 min Scan# 3661
 Delta R.T. -0.041 min
 Lab File: BN030102.D
 Acq: 27 Feb 2024 21:20


Tgt Ion: 202 Resp: 2305
 Ion Ratio Lower Upper
 202 100
 101 213.7 12.5 18.7#
 100 1659.3 10.0 15.0#

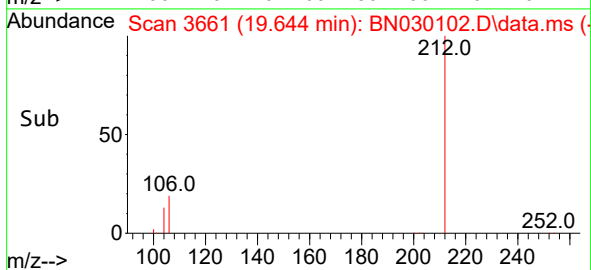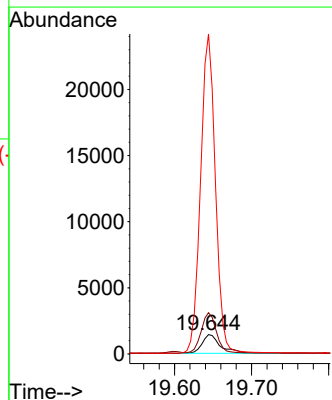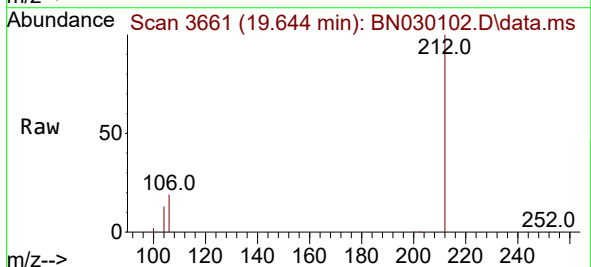

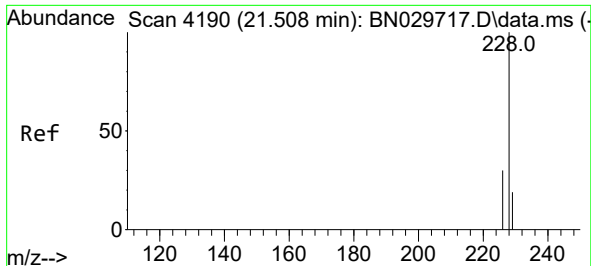

#22
Chrysene
Concen: 0.020 ng/ul
RT: 21.491 min Scan# 41
Delta R.T. -0.009 min
Lab File: BN030102.D
Acq: 27 Feb 2024 21:20

Instrument :
BNA_M
ClientSampleId :

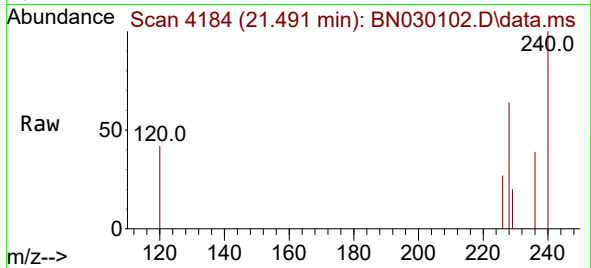

Tgt Ion:228 Resp: 539
Ion Ratio Lower Upper
228 100
226 42.1 24.2 36.2#
229 31.2 15.7 23.5#

