




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044383.D
Acq On : 28 Feb 2024 01:38
Operator : MA/JU
Sample : P1508-07
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH406

Manual IntegrationsAPPROVED

Quant Time: Feb 28 02:07:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 23:05:48 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/28/2024
Supervised By :mohammad ahmed 02/29/2024

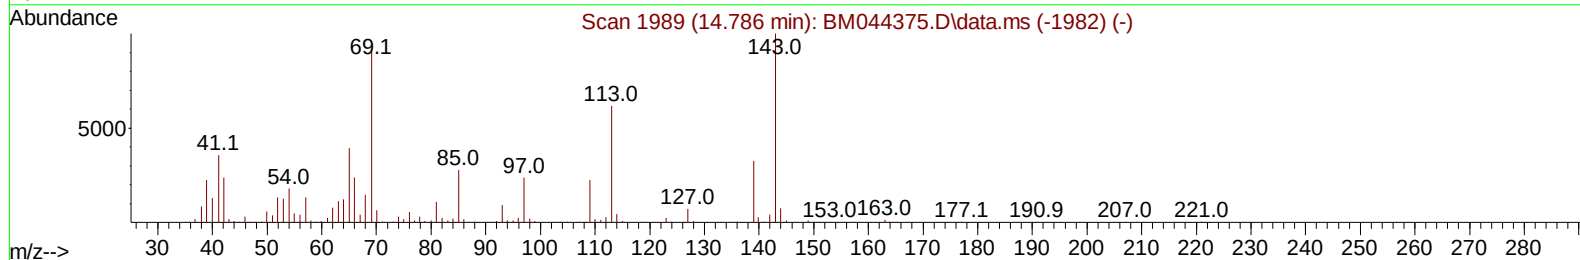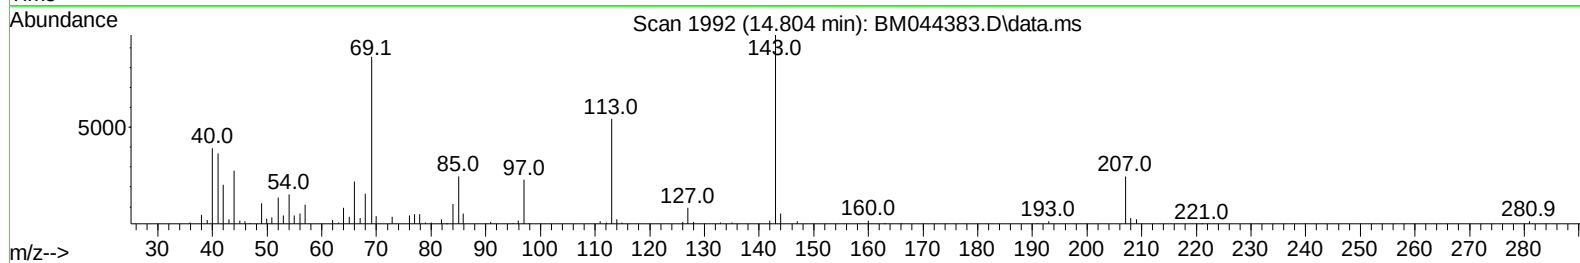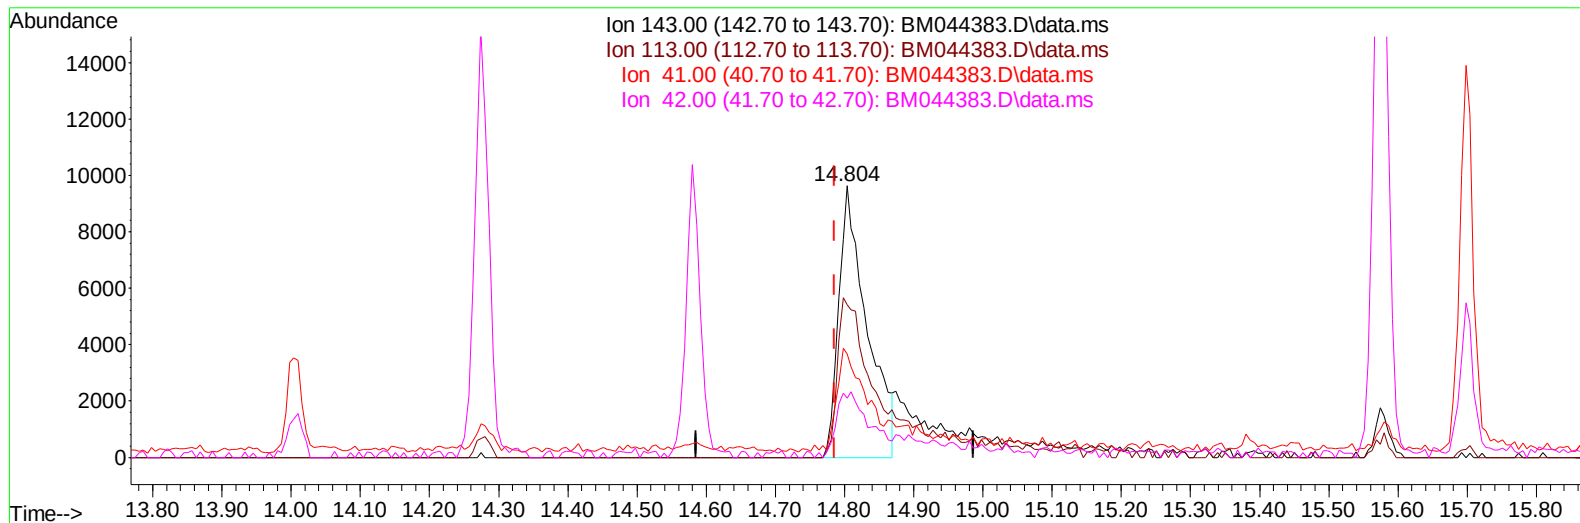

TIC: BM044383.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.804min (+ 0.018) 3.63 ng/ul

response 27251

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.00	56.28
41.00	38.20	38.15
42.00	25.30	21.81




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044383.D
Acq On : 28 Feb 2024 01:38
Operator : MA/JU
Sample : P1508-07
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH406

Manual IntegrationsAPPROVED

Quant Time: Feb 28 02:07:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 23:05:48 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/28/2024
Supervised By :mohammad ahmed 02/29/2024

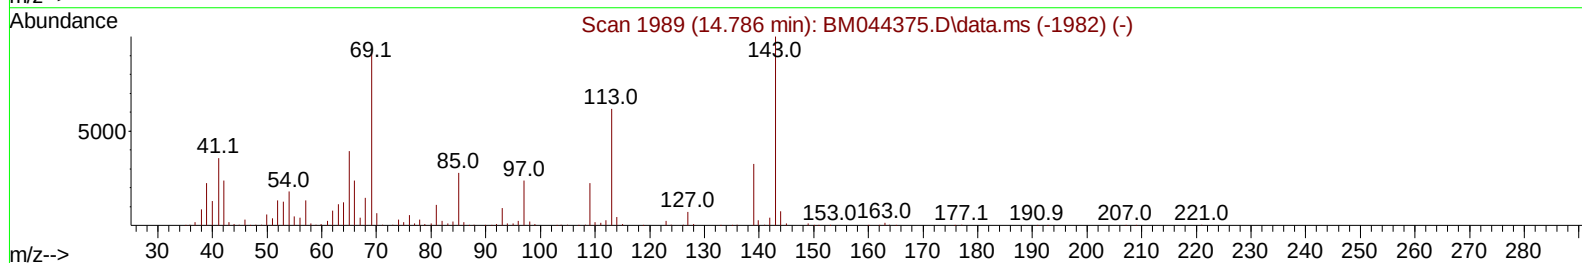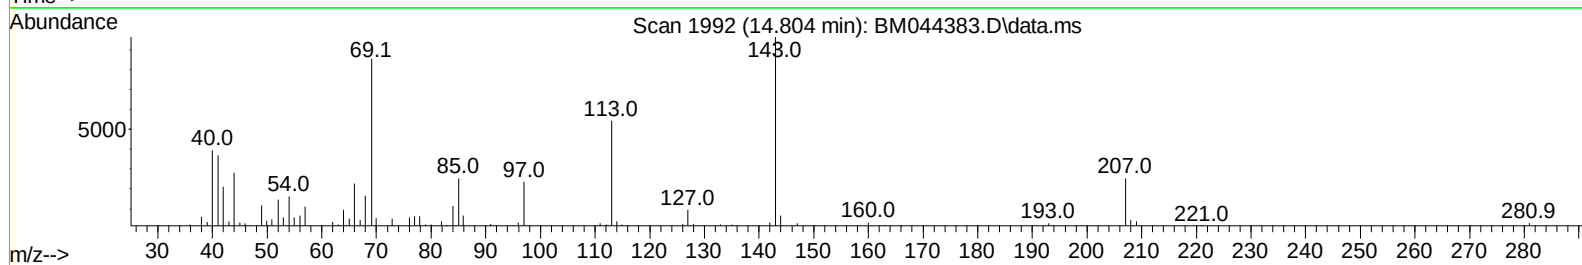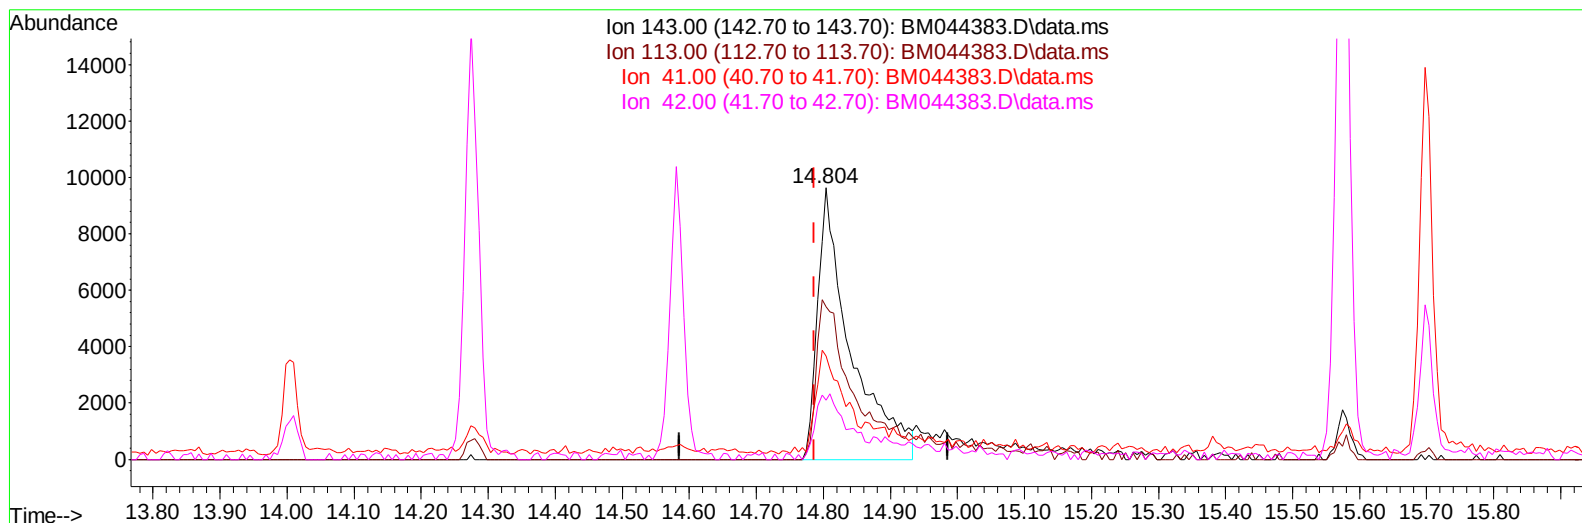

TIC: BM044383.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.804min (+ 0.018) 4.39 ng/ul m

response 33003

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.00	56.28
41.00	38.20	38.15
42.00	25.30	21.81

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044383.D
 Acq On : 28 Feb 2024 01:38
 Operator : MA/JU
 Sample : P1508-07
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH406

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/28/2024
 Supervised By :mohammad ahmed 02/29/2024

Quant Time: Feb 28 02:08:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 27 23:05:48 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.940	152		188840	20.000	ng/ul	0.00
20) Naphthalene-d8	10.745	136		834399	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.580	164		489408	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.333	188		994992	20.000	ng/ul	0.00
79) Chrysene-d12	21.527	240		786782	20.000	ng/ul	0.00
88) Perylene-d12	23.944	264		885923	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.363	96		27586	4.609	ng/uL	0.00
4) Pyridine-d5	3.787	84		200131	12.244	ng/ul	0.00
7) Phenol-d5	7.104	99		140520	7.768	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.281	67		460687	39.326	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132		436946	32.070	ng/ul	0.00
15) 4-Methylphenol-d8	8.651	113		255371	18.657	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128		282867	41.694	ng/ul	0.00
24) 2-Nitrophenol-d4	9.834	143		291751	42.150	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165		446891	36.601	ng/ul	0.00
31) 4-Chloroaniline-d4	10.898	131		643112	31.362	ng/ul	0.00
46) Dimethylphthalate-d6	14.010	166		1531364	40.571	ng/ul	0.00
49) Acenaphthylene-d8	14.274	160		1837805	42.319	ng/ul	0.00
54) 4-Nitrophenol-d4	14.804	143		33003m	4.394	ng/ul	0.02
60) Fluorene-d10	15.574	176		1391427	43.554	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.698	200		202222	32.755	ng/ul	0.00
73) Anthracene-d10	17.433	188		2248415	47.392	ng/ul	0.00
81) Pyrene-d10	19.727	212		2431661	51.372	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.791	264		2177458	47.966	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044383.D
Acq On : 28 Feb 2024 01:38
Operator : MA/JU
Sample : P1508-07
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH406

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/28/2024
Supervised By :mohammad ahmed 02/29/2024

Quant Time: Feb 28 02:08:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 23:05:48 2024
Response via : Initial Calibration

