




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044385.D
Acq On : 28 Feb 2024 02:51
Operator : MA/JU
Sample : P1526-02
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A5

Manual IntegrationsAPPROVED

Quant Time: Feb 28 03:25:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 23:05:48 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/28/2024
Supervised By :mohammad ahmed 02/29/2024

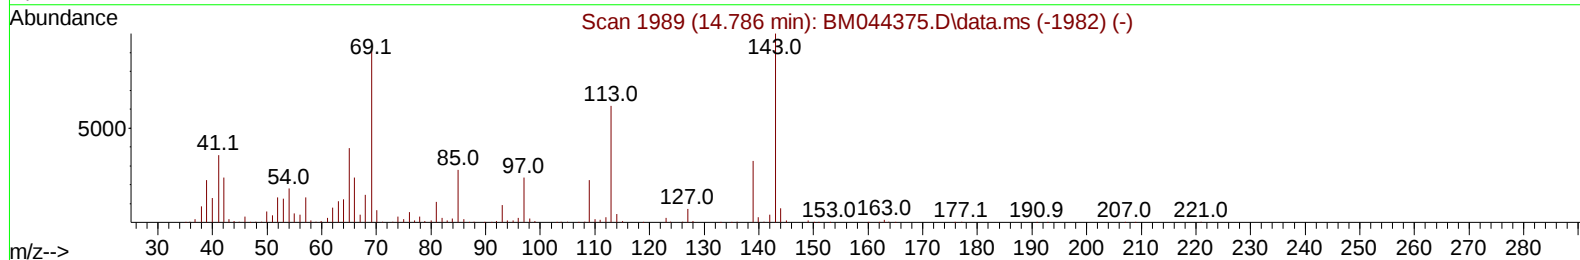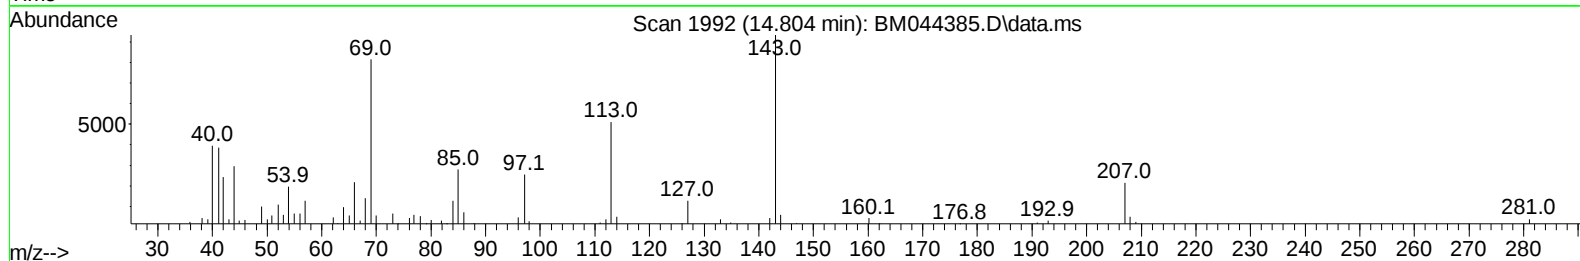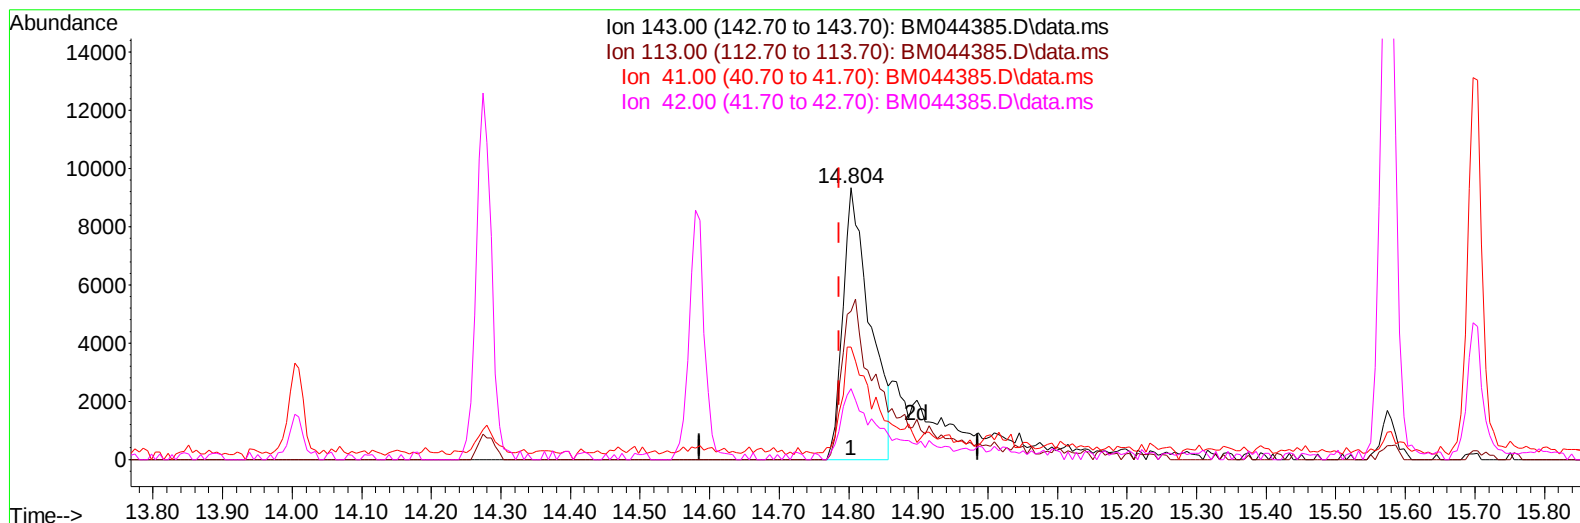

TIC: BM044385.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.804min (+ 0.018) 3.78 ng/u1

response 25166

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.00	54.66
41.00	38.20	41.39
42.00	25.30	26.10




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044385.D
Acq On : 28 Feb 2024 02:51
Operator : MA/JU
Sample : P1526-02
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A5

Manual IntegrationsAPPROVED

Quant Time: Feb 28 03:25:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 23:05:48 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/28/2024
Supervised By :mohammad ahmed 02/29/2024

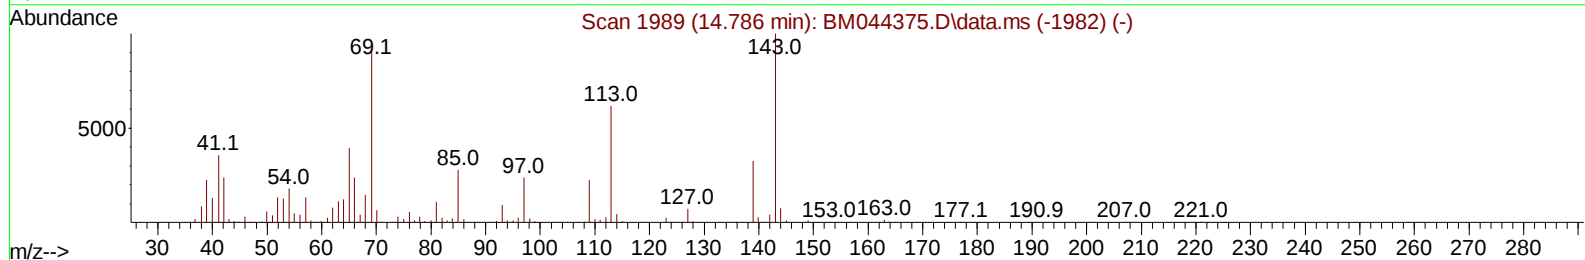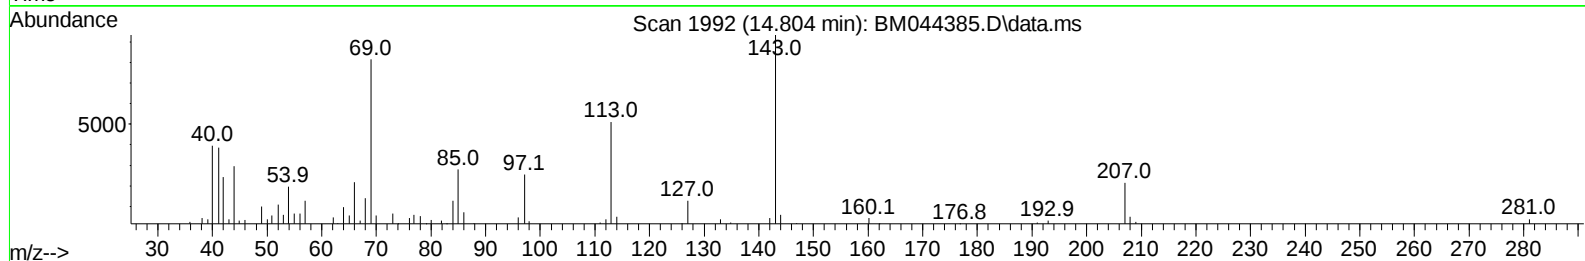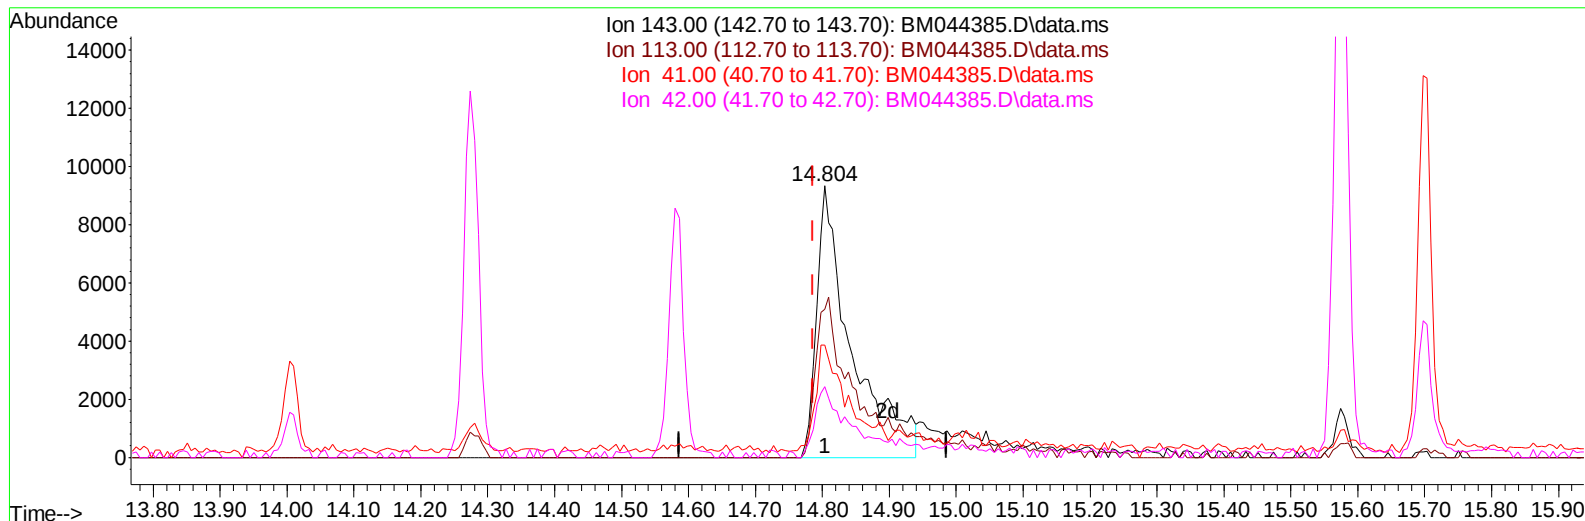

TIC: BM044385.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.804min (+ 0.018) 5.07 ng/ul m

response 33726

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.00	54.66
41.00	38.20	41.39
42.00	25.30	26.10

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044385.D
 Acq On : 28 Feb 2024 02:51
 Operator : MA/JU
 Sample : P1526-02
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E10A5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/28/2024
 Supervised By :mohammad ahmed 02/29/2024

Quant Time: Feb 28 03:26:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 27 23:05:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.939	152	167615	20.000	ng/ul	0.00
20) Naphthalene-d8	10.745	136	737937	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.580	164	433546	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.333	188	881167	20.000	ng/ul	0.00
79) Chrysene-d12	21.527	240	701692	20.000	ng/ul	0.00
88) Perylene-d12	23.944	264	790015	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	22269	4.192	ng/uL	0.00
4) Pyridine-d5	3.798	84	74306	5.122	ng/ul	0.02
7) Phenol-d5	7.104	99	127930	7.967	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.286	67	406274	39.073	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132	387387	32.033	ng/ul	0.00
15) 4-Methylphenol-d8	8.657	113	234002	19.260	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128	246990	41.165	ng/ul	0.00
24) 2-Nitrophenol-d4	9.833	143	254017	41.496	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	396611	36.729	ng/ul	0.00
31) 4-Chloroaniline-d4	10.898	131	391176	21.569	ng/ul	0.00
46) Dimethylphthalate-d6	14.010	166	1429629	42.756	ng/ul	0.00
49) Acenaphthylene-d8	14.274	160	1673868	43.510	ng/ul	0.00
54) 4-Nitrophenol-d4	14.804	143	33726m	5.069	ng/ul	0.02
60) Fluorene-d10	15.574	176	1283065	45.336	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	203464	37.213	ng/ul	0.00
73) Anthracene-d10	17.433	188	2282387	54.323	ng/ul	0.00
81) Pyrene-d10	19.727	212	2456391	58.188	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.791	264	2221076	54.867	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044385.D
Acq On : 28 Feb 2024 02:51
Operator : MA/JU
Sample : P1526-02
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/28/2024
Supervised By :mohammad ahmed 02/29/2024

Quant Time: Feb 28 03:26:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 23:05:48 2024
Response via : Initial Calibration

