




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044394.D
Acq On : 28 Feb 2024 08:55
Operator : MA/JU
Sample : P1508-04
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH402

Manual IntegrationsAPPROVED

Quant Time: Feb 28 09:40:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 23:05:48 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/28/2024
Supervised By :mohammad ahmed 02/29/2024

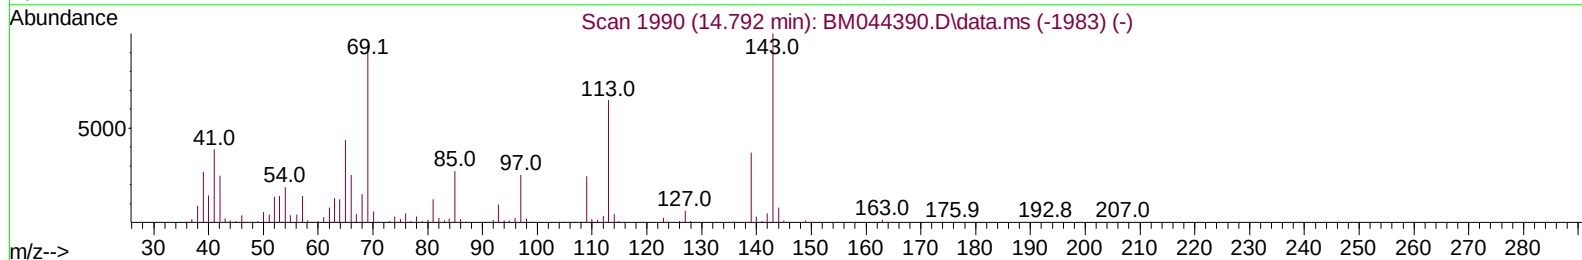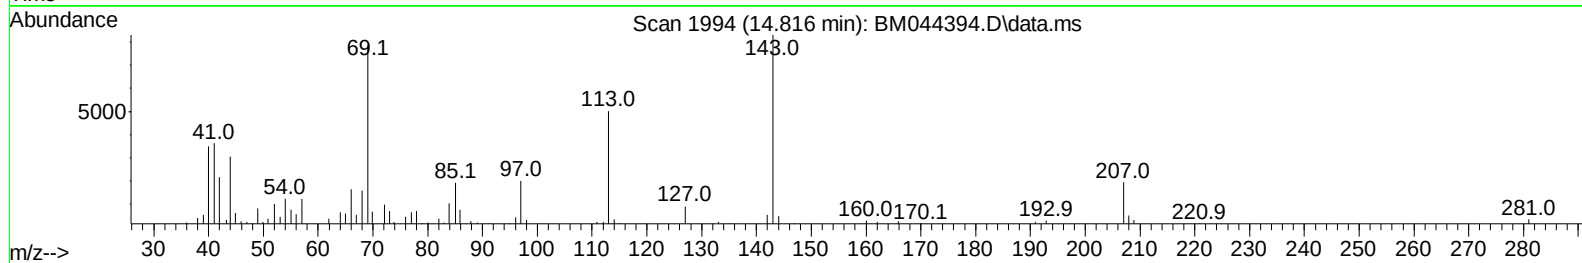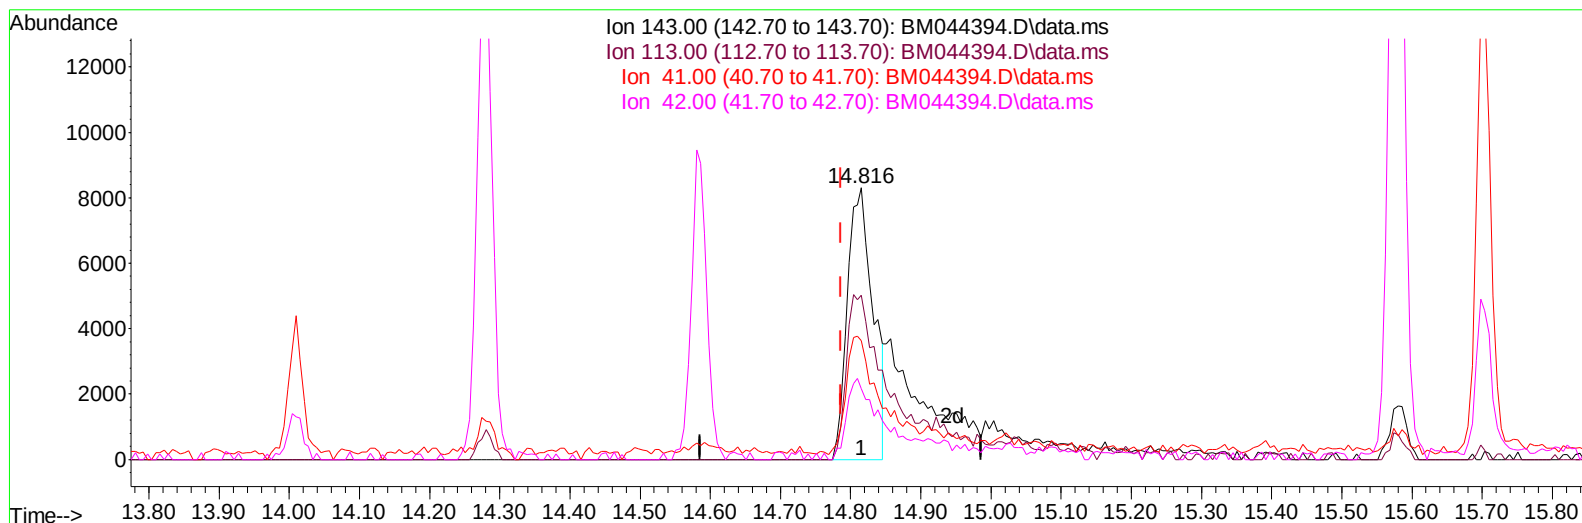

TIC: BM044394.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.816min (+ 0.030) 2.81 ng/ul

response 21082

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.00	60.51
41.00	38.20	43.69
42.00	25.30	26.01




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044394.D
Acq On : 28 Feb 2024 08:55
Operator : MA/JU
Sample : P1508-04
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH402

Manual IntegrationsAPPROVED

Quant Time: Feb 28 09:40:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 23:05:48 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/28/2024
Supervised By :mohammad ahmed 02/29/2024

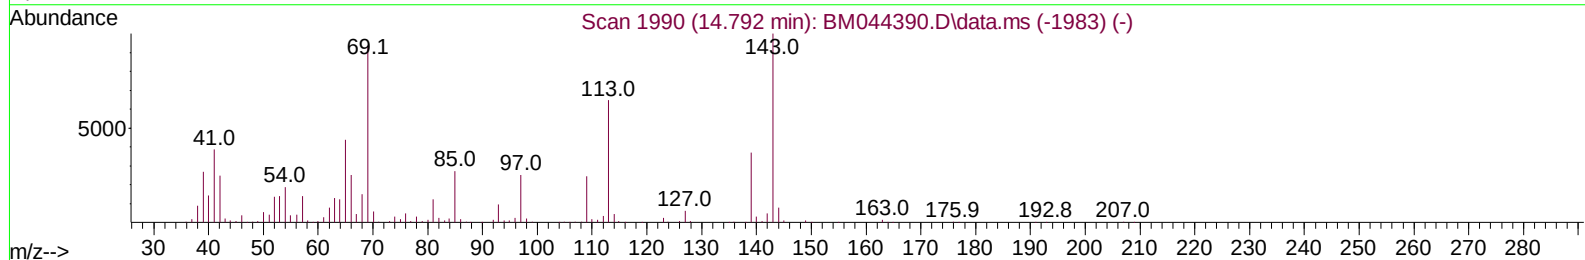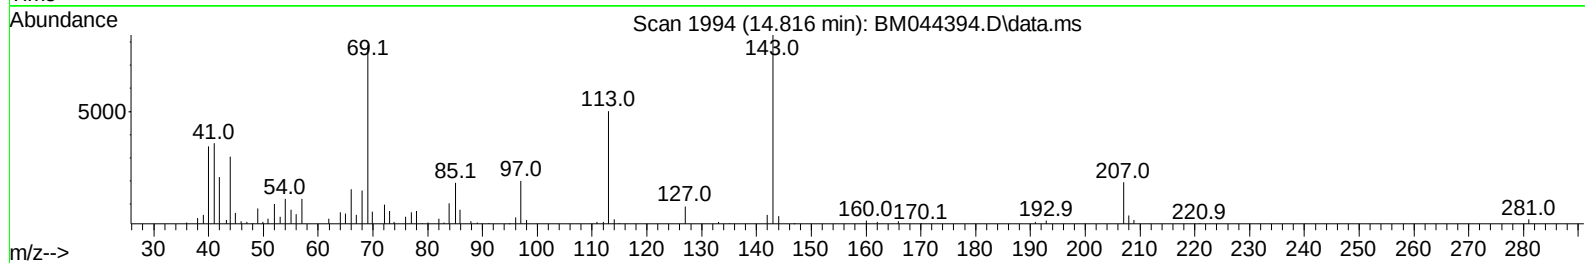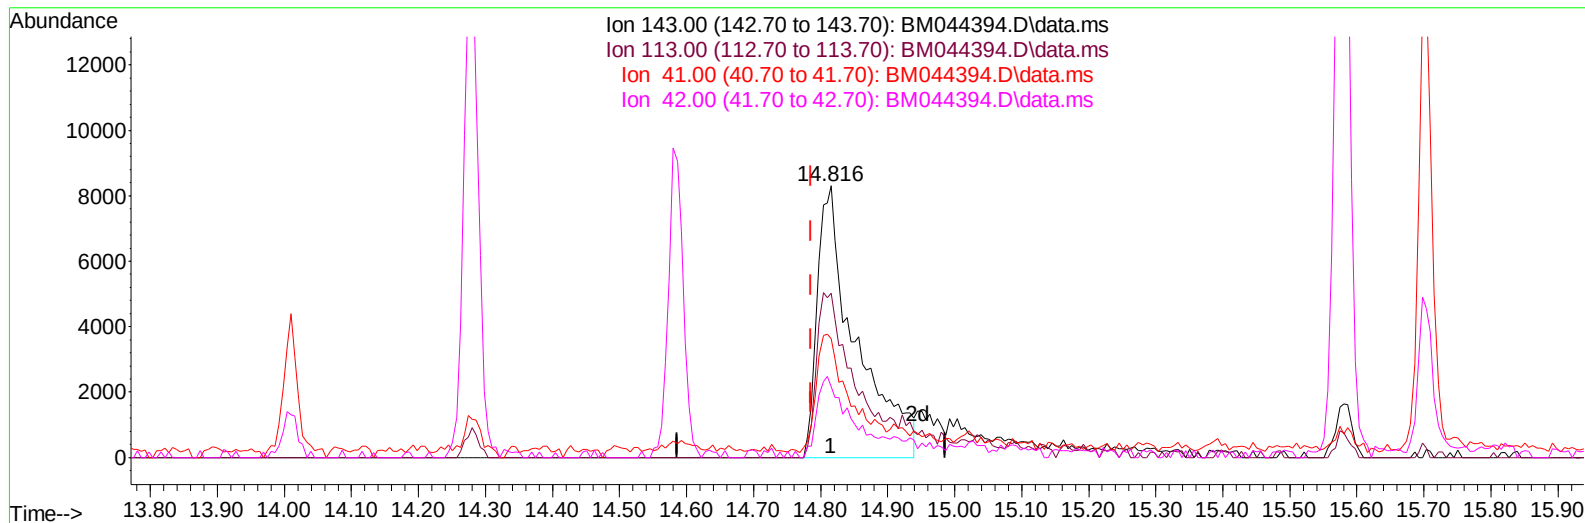

TIC: BM044394.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.816min (+ 0.030) 4.38 ng/ul m

response 32890

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.00	60.51
41.00	38.20	43.69
42.00	25.30	26.01

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044394.D
 Acq On : 28 Feb 2024 08:55
 Operator : MA/JU
 Sample : P1508-04
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH402

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/28/2024
 Supervised By :mohammad ahmed 02/29/2024

Quant Time: Feb 28 09:42:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 27 23:05:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.945	152	188399	20.000	ng/ul	0.00
20) Naphthalene-d8	10.751	136	831374	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.586	164	488824	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.333	188	988690	20.000	ng/ul	0.00
79) Chrysene-d12	21.533	240	780793	20.000	ng/ul	0.00
88) Perylene-d12	23.950	264	870354	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	29820	4.994	ng/uL	0.00
4) Pyridine-d5	3.799	84	70105	4.299	ng/ul	0.02
7) Phenol-d5	7.110	99	155678	8.626	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	525778	44.987	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132	490390	36.077	ng/ul	0.00
15) 4-Methylphenol-d8	8.657	113	289031	21.165	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128	321630	47.580	ng/ul	0.00
24) 2-Nitrophenol-d4	9.839	143	334759	48.540	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	503361	41.376	ng/ul	0.00
31) 4-Chloroaniline-d4	10.898	131	508931	24.909	ng/ul	0.00
46) Dimethylphthalate-d6	14.010	166	1716072	45.519	ng/ul	0.00
49) Acenaphthylene-d8	14.280	160	2015177	46.459	ng/ul	0.00
54) 4-Nitrophenol-d4	14.816	143	32890m	4.384	ng/ul	0.03
60) Fluorene-d10	15.580	176	1519539	47.620	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	224621	36.615	ng/ul	0.00
73) Anthracene-d10	17.433	188	2375870	50.398	ng/ul	0.00
81) Pyrene-d10	19.733	212	2614319	55.655	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.797	264	2329027	52.223	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044394.D
Acq On : 28 Feb 2024 08:55
Operator : MA/JU
Sample : P1508-04
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH402

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/28/2024
Supervised By :mohammad ahmed 02/29/2024

Quant Time: Feb 28 09:42:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 23:05:48 2024
Response via : Initial Calibration

