




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044395.D
Acq On : 28 Feb 2024 09:32
Operator : MA/JU
Sample : P1508-05
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH403

Manual IntegrationsAPPROVED

Quant Time: Feb 28 10:22:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 23:05:48 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/28/2024
Supervised By :mohammad ahmed 02/29/2024

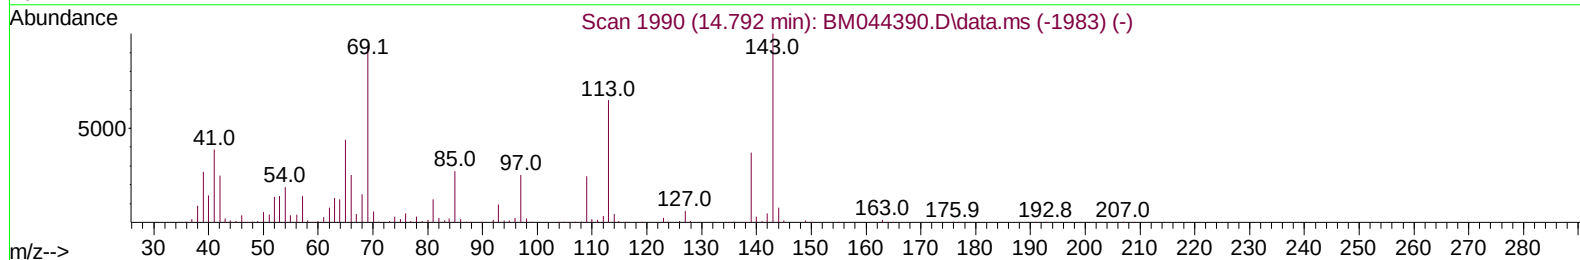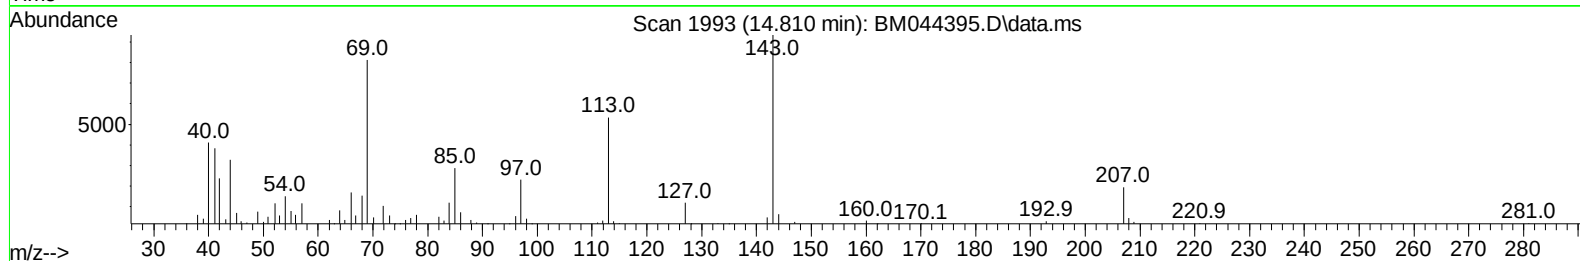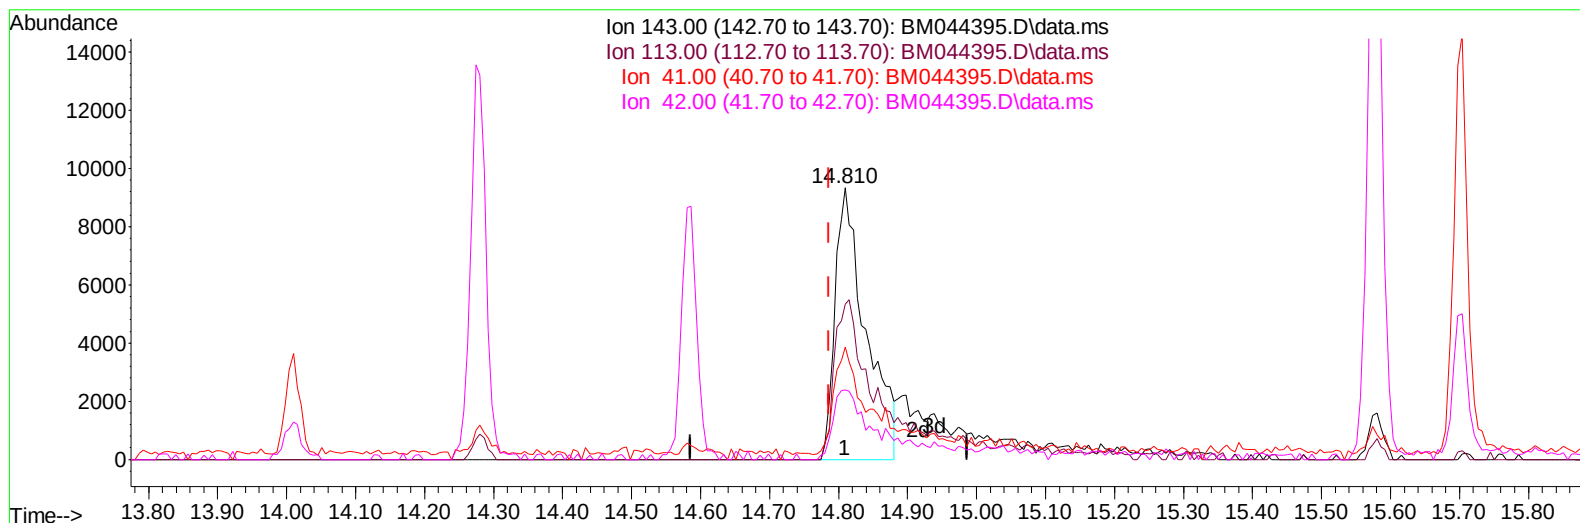

TIC: BM044395.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.810min (+ 0.024) 4.16 ng/ul

response 28851

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.00	57.18
41.00	38.20	41.28
42.00	25.30	25.59




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044395.D
Acq On : 28 Feb 2024 09:32
Operator : MA/JU
Sample : P1508-05
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH403

Manual IntegrationsAPPROVED

Quant Time: Feb 28 10:22:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 23:05:48 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/28/2024
Supervised By :mohammad ahmed 02/29/2024

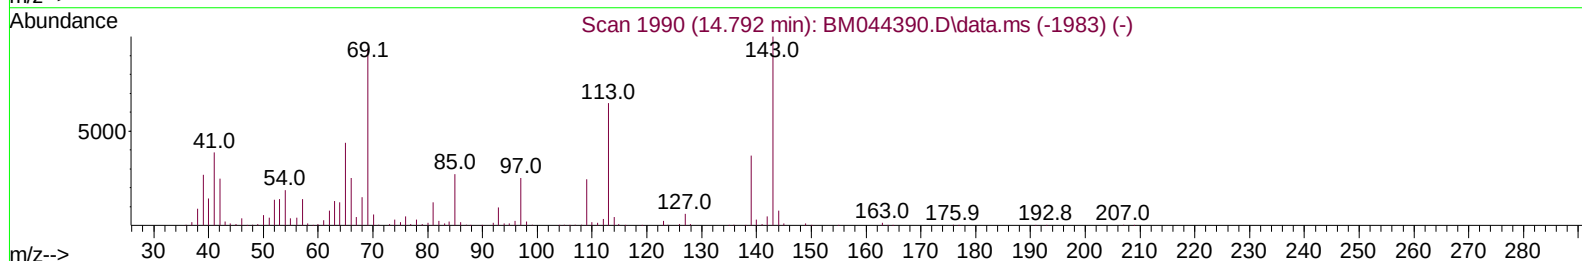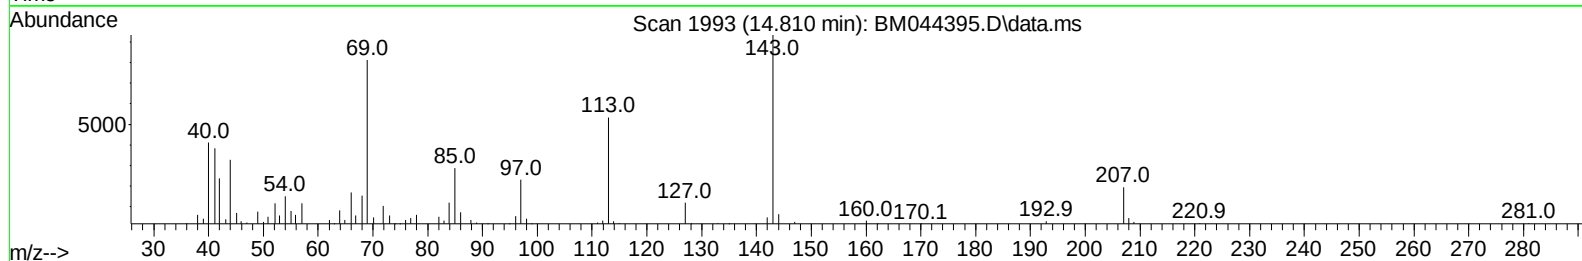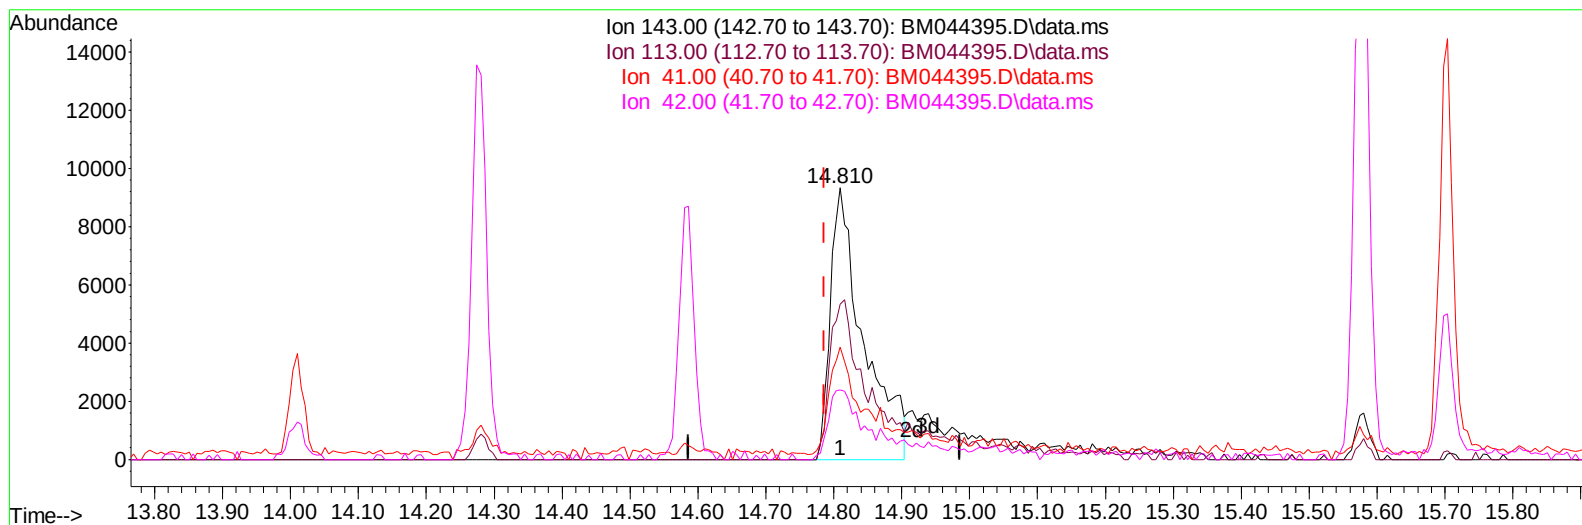

TIC: BM044395.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.810min (+ 0.024) 4.56 ng/ul m

response 31662

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	59.00	57.18
41.00	38.20	41.28
42.00	25.30	25.59

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044395.D
 Acq On : 28 Feb 2024 09:32
 Operator : MA/JU
 Sample : P1508-05
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH403

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/28/2024
 Supervised By :mohammad ahmed 02/29/2024

Quant Time: Feb 28 10:22:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 27 23:05:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.945	152	175434	20.000	ng/ul	0.00
20) Naphthalene-d8	10.751	136	781652	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.586	164	452243	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.333	188	914267	20.000	ng/ul	0.00
79) Chrysene-d12	21.533	240	742021	20.000	ng/ul	0.00
88) Perylene-d12	23.950	264	803491	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	24445	4.396	ng/uL	0.00
4) Pyridine-d5	3.787	84	204334	13.456	ng/ul	0.00
7) Phenol-d5	7.110	99	136196	8.104	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.287	67	446450	41.023	ng/ul	0.00
11) 2-Chlorophenol-d4	7.469	132	420448	33.217	ng/ul	0.00
15) 4-Methylphenol-d8	8.657	113	252458	19.853	ng/ul	0.00
21) Nitrobenzene-d5	9.116	128	273161	42.981	ng/ul	0.00
24) 2-Nitrophenol-d4	9.839	143	279953	43.175	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.369	165	428173	37.435	ng/ul	0.00
31) 4-Chloroaniline-d4	10.898	131	591764	30.805	ng/ul	0.00
46) Dimethylphthalate-d6	14.010	166	1552416	44.509	ng/ul	0.00
49) Acenaphthylene-d8	14.280	160	1795791	44.750	ng/ul	0.00
54) 4-Nitrophenol-d4	14.810	143	31662m	4.562	ng/ul	0.02
60) Fluorene-d10	15.580	176	1382507	46.831	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.704	200	214594	37.828	ng/ul	0.00
73) Anthracene-d10	17.433	188	2307018	52.921	ng/ul	0.00
81) Pyrene-d10	19.733	212	2534647	56.778	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.797	264	2299015	55.840	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044395.D
Acq On : 28 Feb 2024 09:32
Operator : MA/JU
Sample : P1508-05
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH403

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/28/2024
Supervised By :mohammad ahmed 02/29/2024

Quant Time: Feb 28 10:22:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 23:05:48 2024
Response via : Initial Calibration

