

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044353.D
 Acq On : 27 Feb 2024 04:28
 Operator : MA/JU
 Sample : P1469-15
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH9Q5

Quant Time: Feb 27 04:58:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 27 00:07:53 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	271754	20.000	ng/u1	0.00
20) Naphthalene-d8	10.740	136	1162473	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.575	164	651708	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.327	188	1316556	20.000	ng/u1	0.00
79) Chrysene-d12	21.521	240	1087836	20.000	ng/u1	0.00
88) Perylene-d12	23.939	264	1201459	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	19816	2.301	ng/uL	0.00
4) Pyridine-d5	3.781	84	201630	8.572	ng/u1	0.00
7) Phenol-d5	7.099	99	371463	14.269	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	247542	14.684	ng/u1	0.00
11) 2-Chlorophenol-d4	7.463	132	301306	15.367	ng/u1	0.00
15) 4-Methylphenol-d8	8.646	113	195724	9.936	ng/u1	0.00
21) Nitrobenzene-d5	9.104	128	141268	14.946	ng/u1	0.00
24) 2-Nitrophenol-d4	9.828	143	147639	15.310	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.357	165	250985	14.755	ng/u1	0.00
31) 4-Chloroaniline-d4	10.892	131	162797	5.698	ng/u1	0.01
46) Dimethylphthalate-d6	13.998	166	793182	15.781	ng/u1	0.00
49) Acenaphthylene-d8	14.269	160	927622	16.041	ng/u1	0.00
54) 4-Nitrophenol-d4	14.786	143	93101	9.309	ng/u1	0.01
60) Fluorene-d10	15.569	176	728208	17.117	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	85011	10.407	ng/u1	0.00
73) Anthracene-d10	17.427	188	1022471	16.288	ng/u1	0.00
81) Pyrene-d10	19.721	212	1253262	19.150	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.780	264	1102734	17.912	ng/u1	0.00
Target Compounds						
16) Acetophenone	8.769	105	62501	1.986	ng/u1	96
86) Bis(2-ethylhexyl)phtha...	21.456	149	61186	1.081	ng/u1	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044353.D
Acq On : 27 Feb 2024 04:28
Operator : MA/JU
Sample : P1469-15
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH9Q5

Quant Time: Feb 27 04:58:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 00:07:53 2024
Response via : Initial Calibration




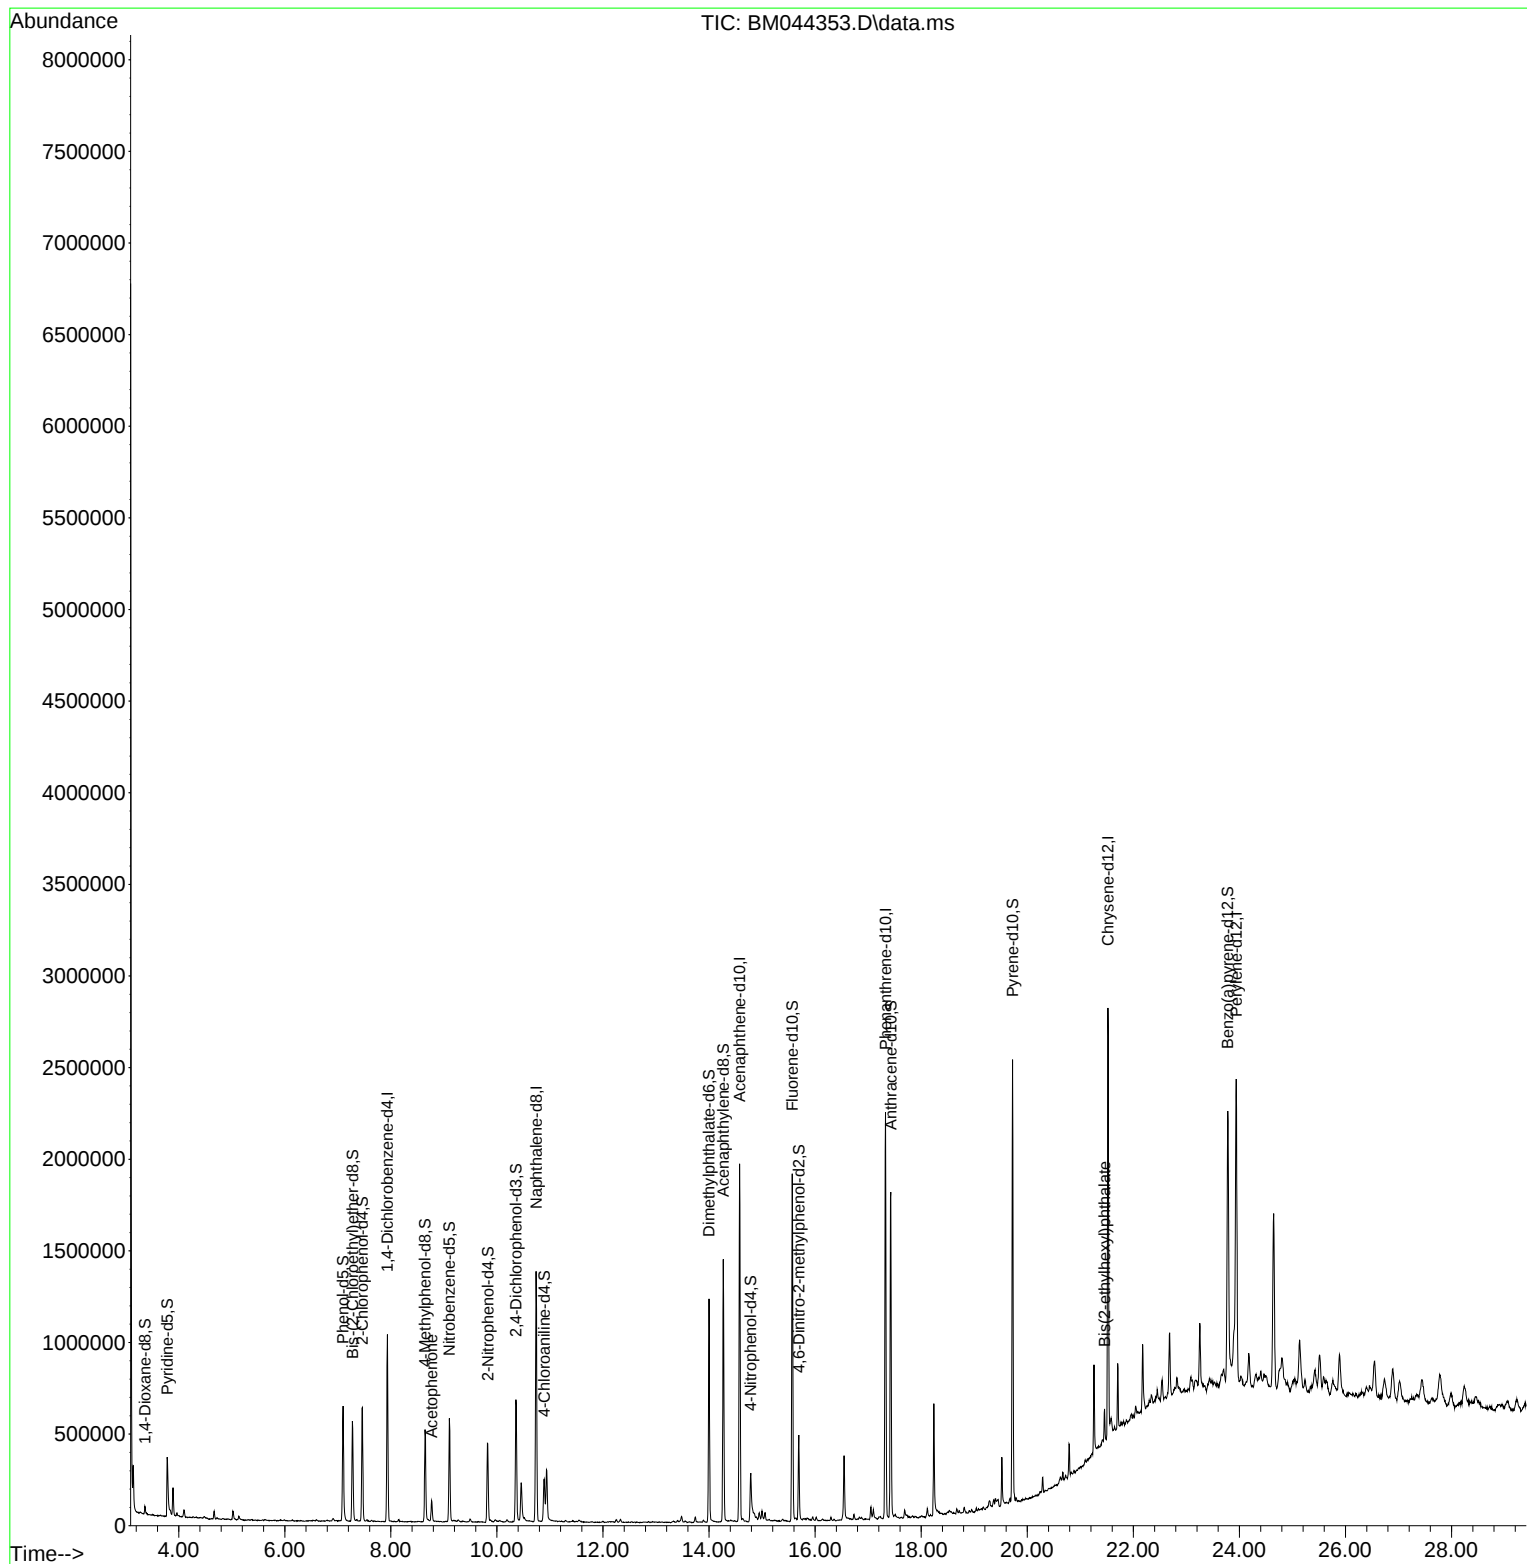


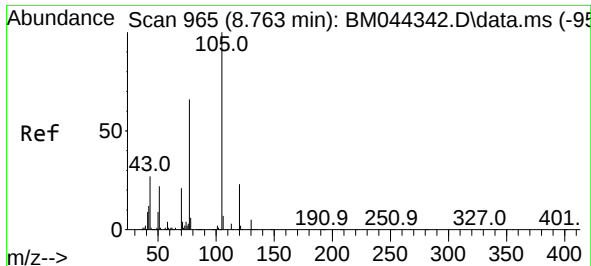

#16
 Acetophenone
 Concen: 1.986 ng/ul
 RT: 8.769 min Scan# 965
 Delta R.T. 0.006 min
 Lab File: BM044353.D
 Acq: 27 Feb 2024 04:28

Instrument :
 BNA_M
 ClientSampleId :
 BH9Q5

Tgt Ion:	105	Resp:	62501
Ion Ratio	Lower	Upper	
105	100		
77	79.8	61.2	91.8
51	28.2	21.1	31.7

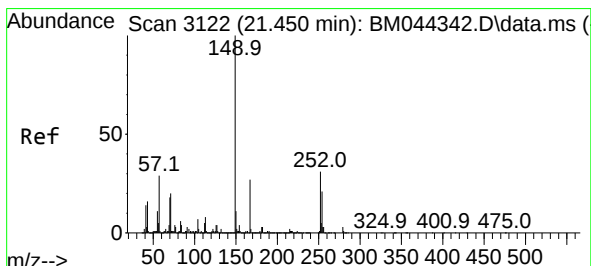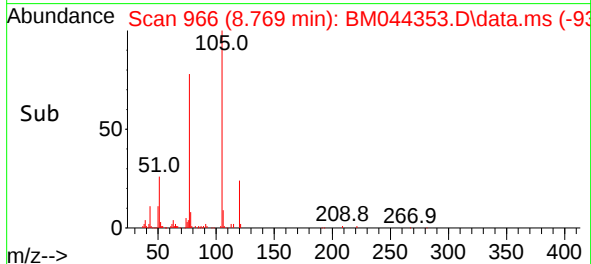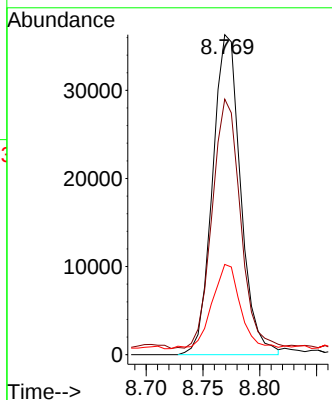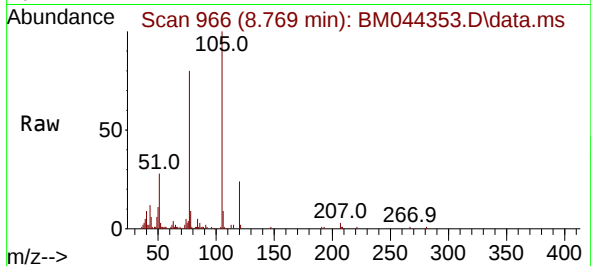

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.081 ng/ul
 RT: 21.456 min Scan# 3123
 Delta R.T. 0.006 min
 Lab File: BM044353.D
 Acq: 27 Feb 2024 04:28

Tgt Ion:	149	Resp:	61186
Ion Ratio	Lower	Upper	
149	100		
167	27.6	22.1	33.1
279	3.2	2.4	3.6

