

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044355.D
 Acq On : 27 Feb 2024 05:41
 Operator : MA/JU
 Sample : P1469-18
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH9S1

Quant Time: Feb 27 06:11:44 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 27 00:07:53 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	229393	20.000	ng/ul	0.00
20) Naphthalene-d8	10.740	136	995071	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.575	164	569154	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.328	188	1170399	20.000	ng/ul	0.00
79) Chrysene-d12	21.527	240	979912	20.000	ng/ul	0.00
88) Perylene-d12	23.945	264	1031708	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	19237	2.646	ng/uL	0.00
4) Pyridine-d5	3.770	84	293338	14.773	ng/ul	0.00
7) Phenol-d5	7.105	99	271742	12.366	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.275	67	219871	15.451	ng/ul	0.00
11) 2-Chlorophenol-d4	7.463	132	239699	14.483	ng/ul	0.00
15) 4-Methylphenol-d8	8.652	113	53342	3.208	ng/ul	0.00
21) Nitrobenzene-d5	9.105	128	127951	15.815	ng/ul	0.00
24) 2-Nitrophenol-d4	9.828	143	133194	16.136	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	164949	11.328	ng/ul	0.00
31) 4-Chloroaniline-d4	10.899	131	45488	1.860	ng/ul	0.02
46) Dimethylphthalate-d6	13.998	166	682944	15.558	ng/ul	0.00
49) Acenaphthylene-d8	14.269	160	759444	15.037	ng/ul	0.00
54) 4-Nitrophenol-d4	14.792	143	85356	9.772	ng/ul	0.02
60) Fluorene-d10	15.569	176	627128	16.880	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.692	200	52955	7.292	ng/ul	0.00
73) Anthracene-d10	17.428	188	810481	14.523	ng/ul	0.00
81) Pyrene-d10	19.721	212	1132646	19.213	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.786	264	821763	15.544	ng/ul	0.01
Target Compounds						
16) Acetophenone	8.769	105	38522	1.450	ng/ul	98
83) Butylbenzylphthalate	20.674	149	45510	1.366	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.457	149	108466	2.127	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044355.D
Acq On : 27 Feb 2024 05:41
Operator : MA/JU
Sample : P1469-18
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH9S1

Quant Time: Feb 27 06:11:44 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 00:07:53 2024
Response via : Initial Calibration




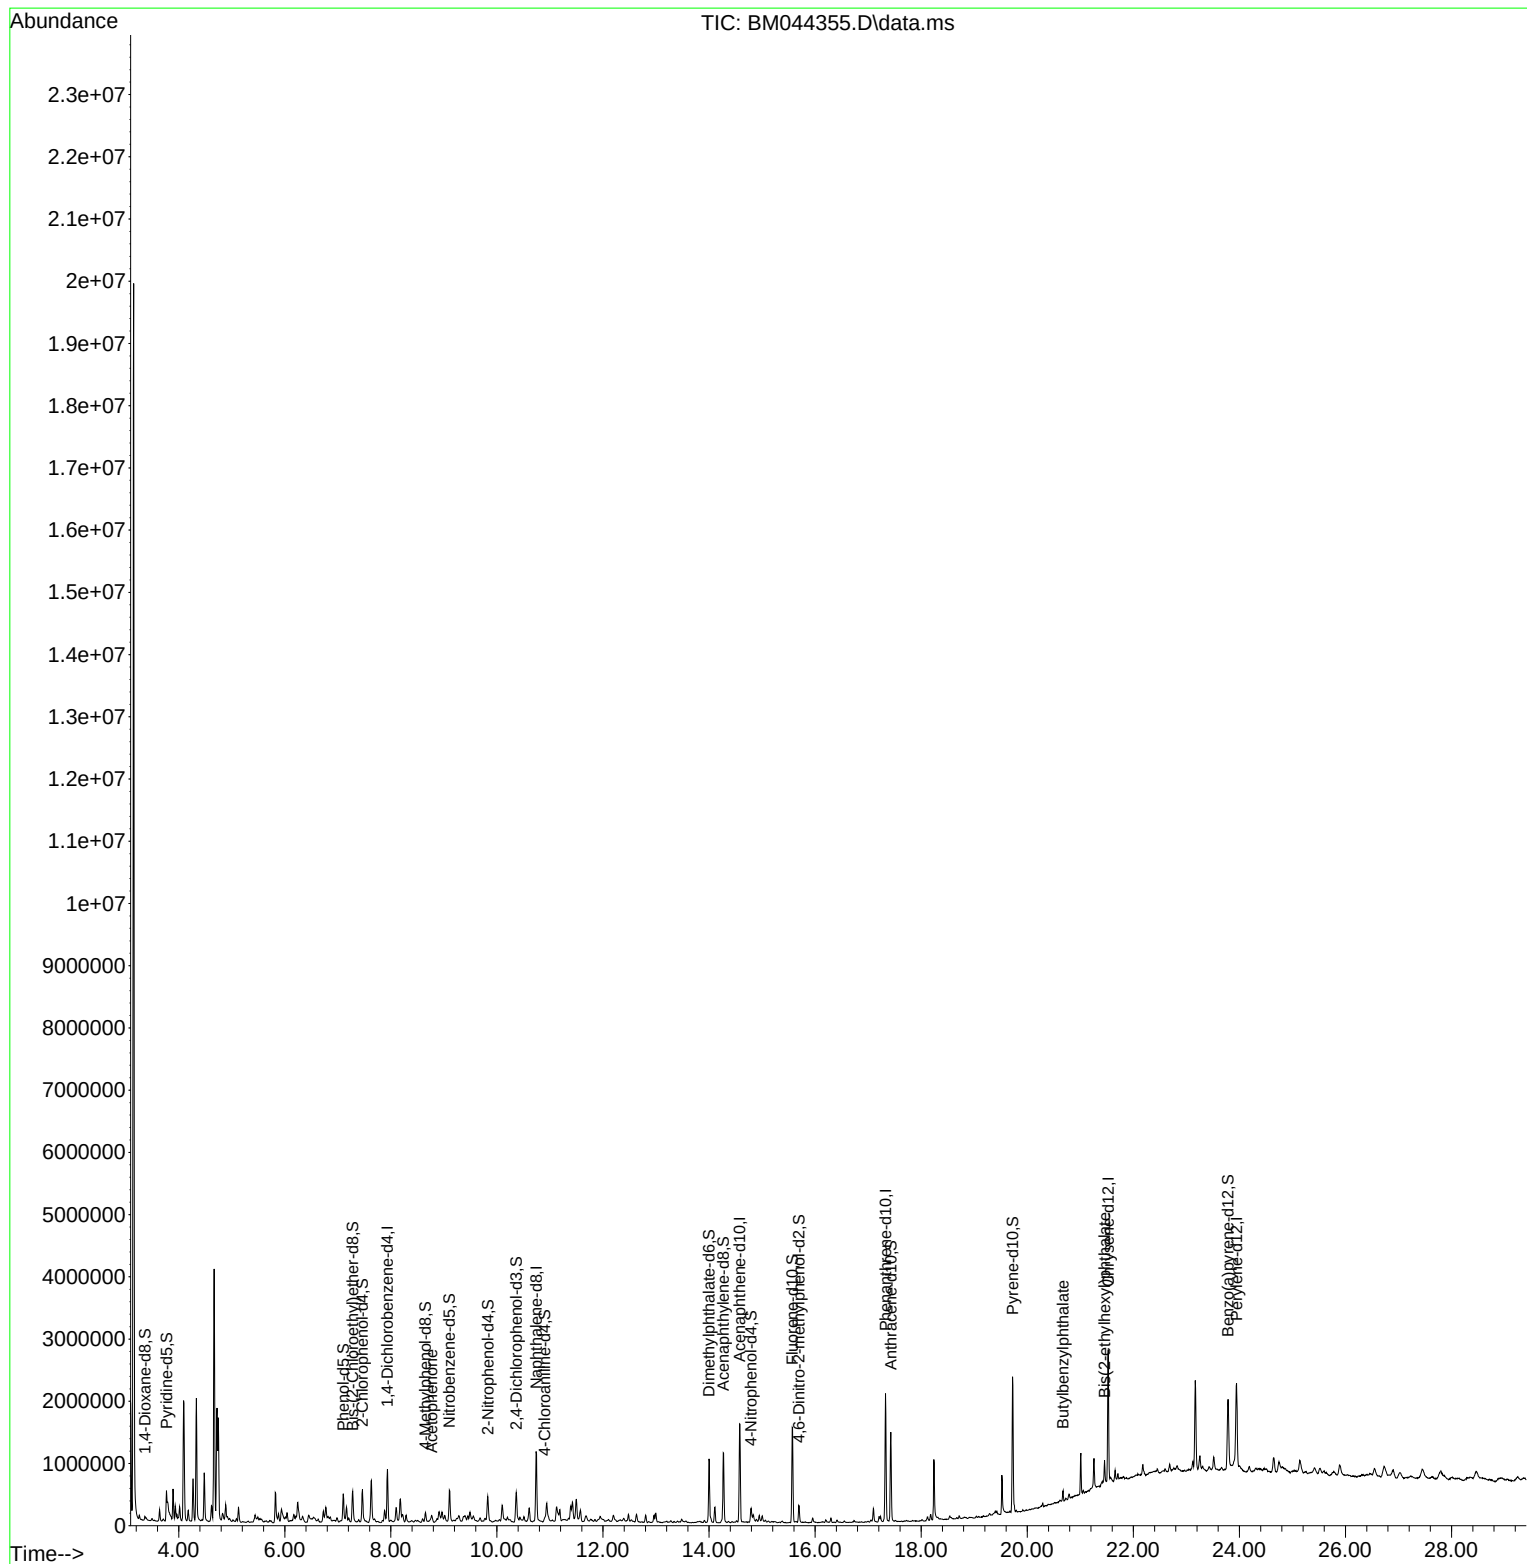


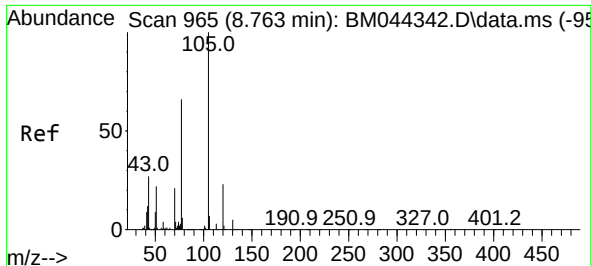

#16
Acetophenone
Concen: 1.450 ng/ul
RT: 8.769 min Scan# 965
Delta R.T. 0.006 min
Lab File: BM044355.D
Acq: 27 Feb 2024 05:41




Instrument :
BNA_M
ClientSampleId :
BH9S1


Tgt Ion:105 Resp: 38522
Ion Ratio Lower Upper
105 100
77 75.8 61.2 91.8
51 28.8 21.1 31.7

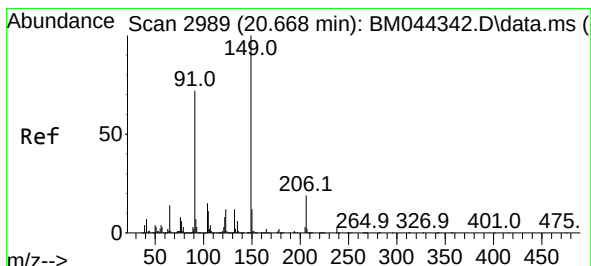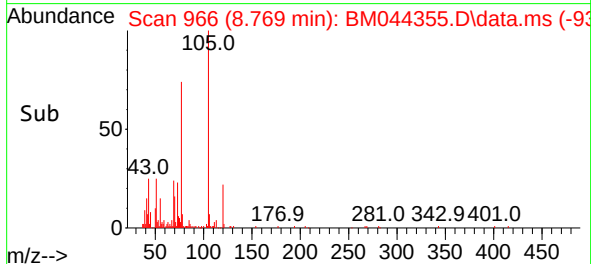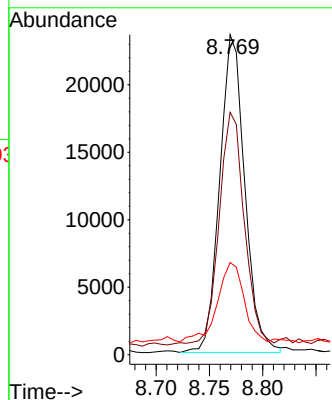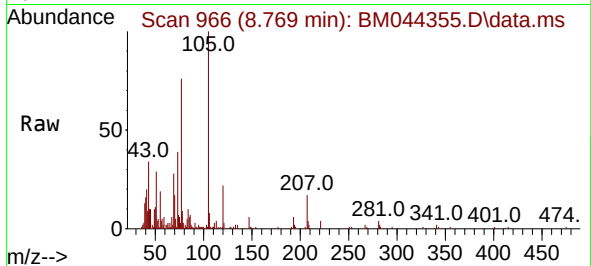

#83
Butylbenzylphthalate
Concen: 1.366 ng/ul
RT: 20.674 min Scan# 2990
Delta R.T. 0.006 min
Lab File: BM044355.D
Acq: 27 Feb 2024 05:41

Tgt Ion:149 Resp: 45510
Ion Ratio Lower Upper
149 100
91 72.1 58.1 87.1
206 19.2 15.0 22.4

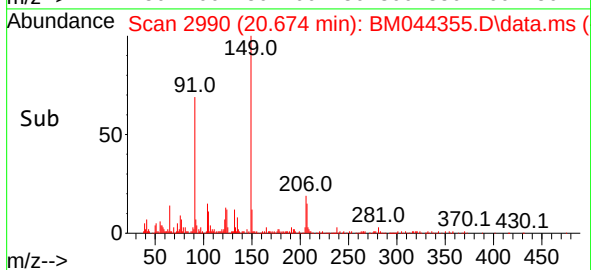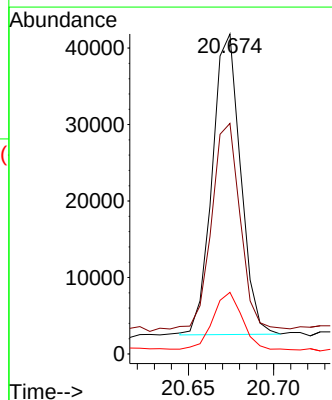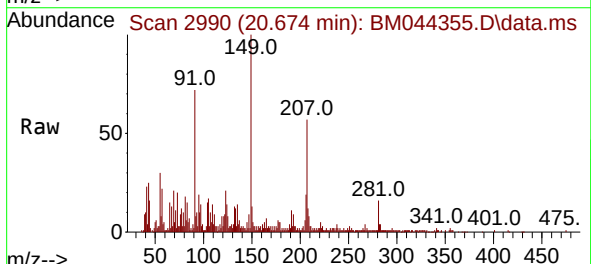

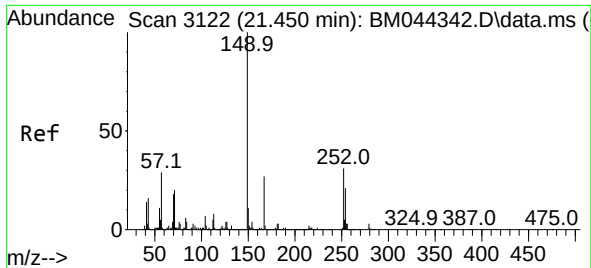

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 2.127 ng/ul
 RT: 21.457 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: BM044355.D
 Acq: 27 Feb 2024 05:41

Instrument :
 BNA_M
 ClientSampleId :
 BH9S1

Tgt Ion:149 Resp: 108466
 Ion Ratio Lower Upper
 149 100
 167 26.5 22.1 33.1
 279 4.2 2.4 3.6#

