

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044361.D
 Acq On : 27 Feb 2024 11:37
 Operator : MA/JU
 Sample : P1517-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH9R9

Quant Time: Feb 27 22:34:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 27 00:07:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	221322	20.000	ng/u1	0.00
20) Naphthalene-d8	10.739	136	965524	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.574	164	560160	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.327	188	1146826	20.000	ng/u1	0.00
79) Chrysene-d12	21.521	240	978547	20.000	ng/u1	0.00
88) Perylene-d12	23.939	264	1028595	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	19354	2.759	ng/uL	0.00
4) Pyridine-d5	3.781	84	349364	18.237	ng/u1	0.00
7) Phenol-d5	7.098	99	314031	14.811	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	215089	15.666	ng/u1	0.00
11) 2-Chlorophenol-d4	7.463	132	257792	16.144	ng/u1	0.00
15) 4-Methylphenol-d8	8.651	113	96201	5.997	ng/u1	0.00
21) Nitrobenzene-d5	9.104	128	128065	16.313	ng/u1	0.00
24) 2-Nitrophenol-d4	9.828	143	139034	17.359	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.363	165	213330	15.099	ng/u1	0.00
31) 4-Chloroaniline-d4	10.898	131	81886	3.451	ng/u1	0.02
46) Dimethylphthalate-d6	13.998	166	742041	17.176	ng/u1	0.00
49) Acenaphthylene-d8	14.269	160	829211	16.682	ng/u1	0.00
54) 4-Nitrophenol-d4	14.786	143	95619	11.123	ng/u1	0.01
60) Fluorene-d10	15.568	176	656194	17.945	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.698	200	72314	10.162	ng/u1	0.00
73) Anthracene-d10	17.427	188	876596	16.031	ng/u1	0.00
81) Pyrene-d10	19.721	212	1171152	19.894	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.780	264	883523	16.763	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.456	149	104340	2.049	ng/u1	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044361.D
Acq On : 27 Feb 2024 11:37
Operator : MA/JU
Sample : P1517-01
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH9R9

Quant Time: Feb 27 22:34:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 27 00:07:53 2024
Response via : Initial Calibration

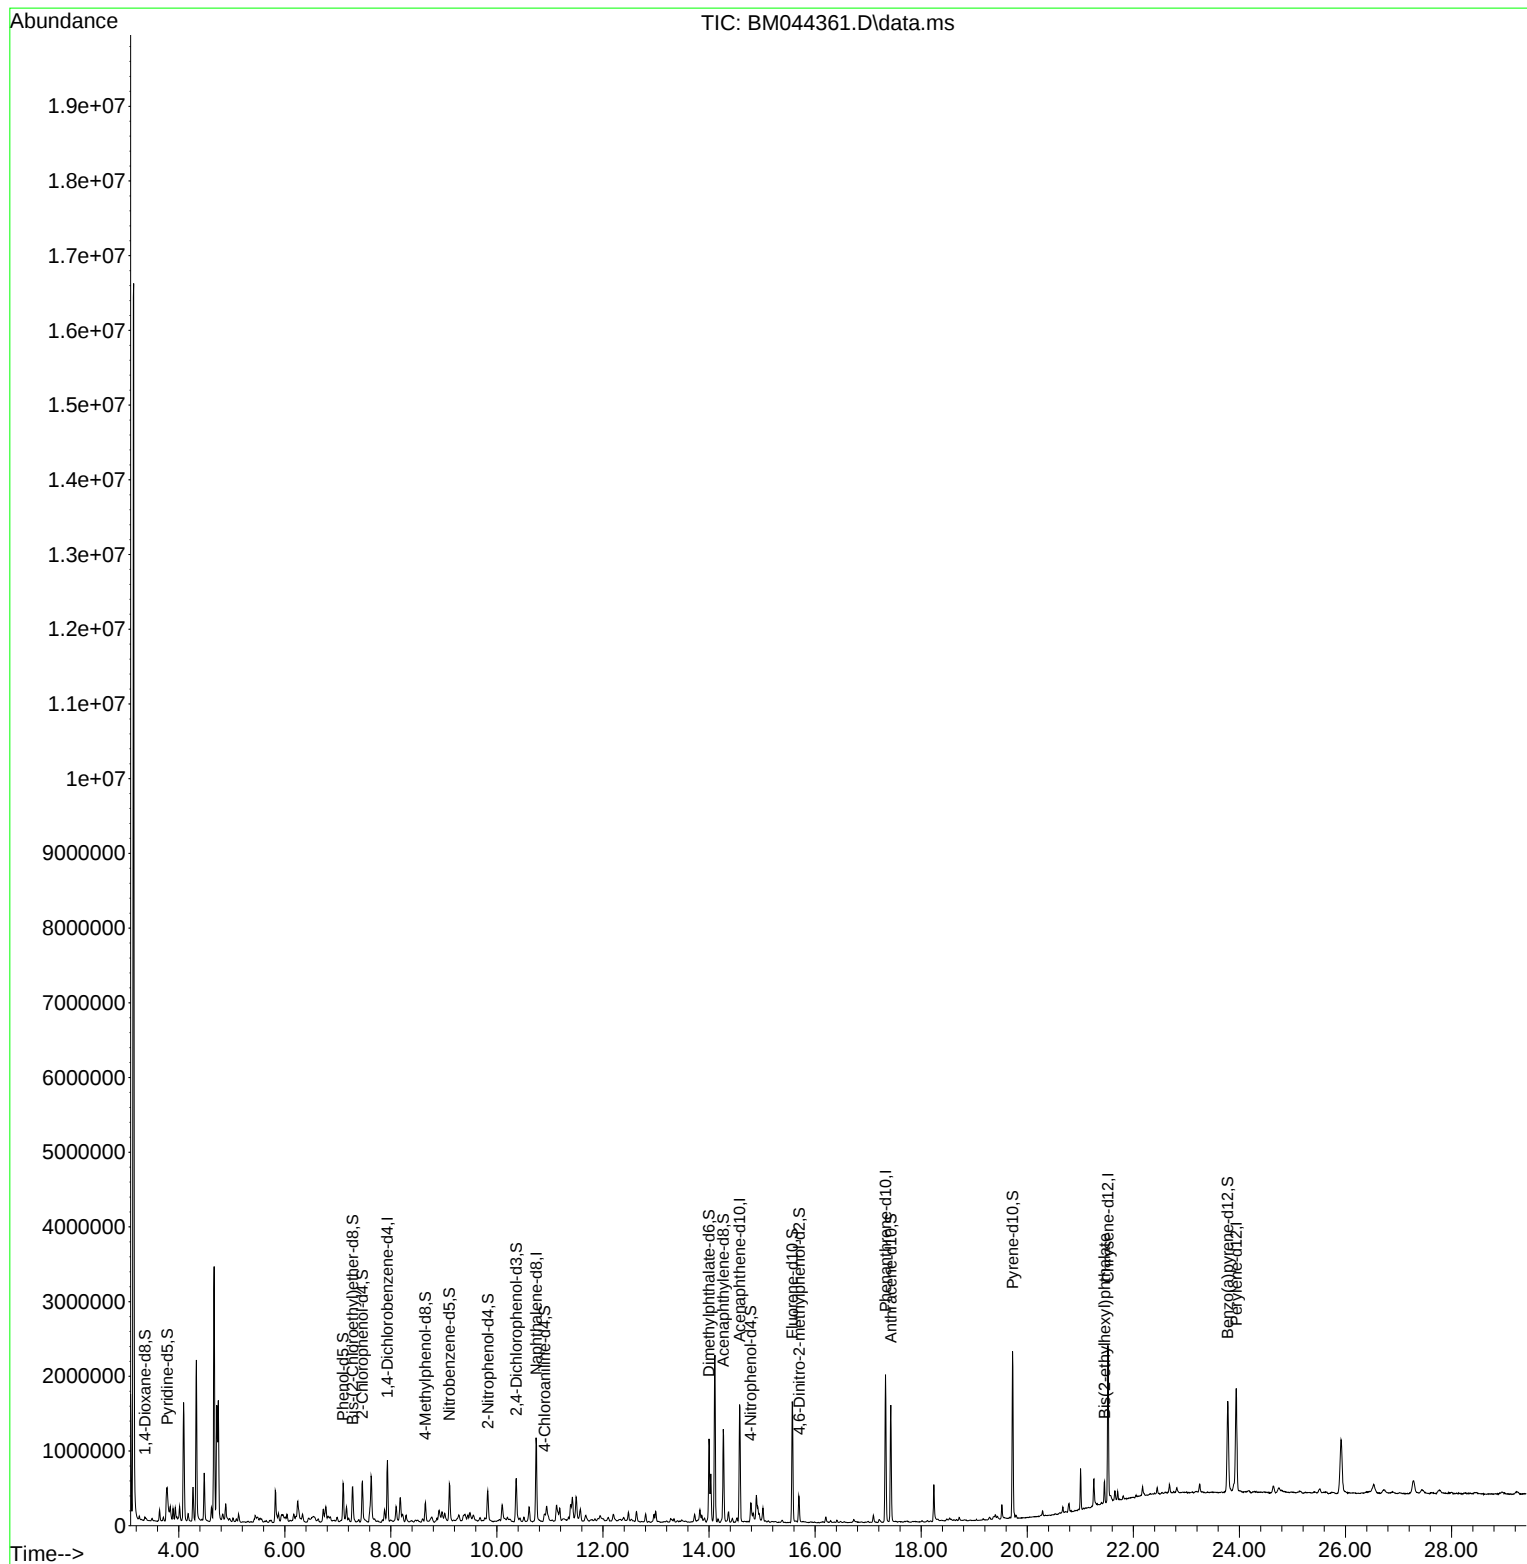

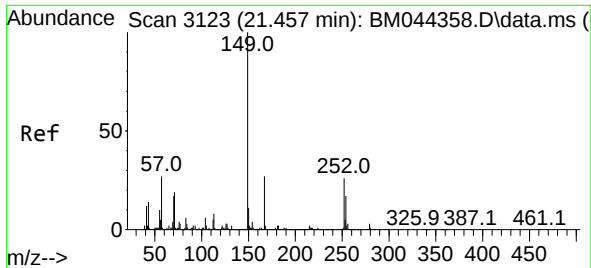

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 2.049 ng/ul
 RT: 21.456 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: BM044361.D
 Acq: 27 Feb 2024 11:37

Instrument :
 BNA_M
 ClientSampleId :
 BH9R9

Tgt Ion:149 Resp: 104340
 Ion Ratio Lower Upper
 149 100
 167 27.3 22.1 33.1
 279 3.6 2.4 3.6

