

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044359.D
 Acq On : 27 Feb 2024 10:24
 Operator : MA/JU
 Sample : PB159204BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK204

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044359.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.357	43	46	53	rVB	84726	111930	2.19%	0.193%
2	3.775	114	117	134	rBV	965130	1513382	29.62%	2.606%
3	4.099	169	172	179	rVB	17331	25512	0.50%	0.044%
4	7.093	674	681	694	rBV	1061468	1688621	33.04%	2.908%
5	7.269	705	711	724	rBV	881498	1423954	27.87%	2.452%
6	7.457	736	743	754	rBV	1060650	1704181	33.35%	2.934%
7	7.928	815	823	833	rBV	839119	1332421	26.07%	2.294%
8	8.640	937	944	956	rBV	1221533	2058264	40.28%	3.544%
9	9.098	1014	1022	1032	rBV	944767	1608183	31.47%	2.769%
10	9.822	1137	1145	1159	rBV	782848	1318053	25.79%	2.270%
11	10.357	1228	1236	1246	rBV	1154409	1989204	38.93%	3.425%
12	10.733	1291	1300	1308	rVB	1148543	1955568	38.27%	3.367%
13	10.886	1318	1326	1340	rBV	1142222	2100028	41.10%	3.616%
14	12.328	1565	1571	1576	rBV	21955	33958	0.66%	0.058%
15	13.480	1763	1767	1772	rVB2	17740	26299	0.51%	0.045%
16	13.551	1776	1779	1785	rVB7	3749	6248	0.12%	0.011%
17	13.998	1846	1855	1866	rVV	1943814	2764060	54.09%	4.759%
18	14.269	1894	1901	1915	rBV	2395460	3552968	69.53%	6.118%
19	14.574	1944	1953	1965	rBV	1658287	2481427	48.56%	4.273%
20	14.786	1981	1989	2013	rBV	555875	1321255	25.86%	2.275%
21	15.368	2083	2088	2091	rBV6	3518	5674	0.11%	0.010%
22	15.568	2111	2122	2136	rBV	3004491	4307361	84.29%	7.417%
23	15.692	2137	2143	2159	rVV	896661	1254330	24.55%	2.160%
24	15.810	2159	2163	2169	rVB4	14991	25871	0.51%	0.045%
25	15.986	2187	2193	2198	rVV6	4898	7737	0.15%	0.013%
26	16.027	2198	2200	2206	rVB6	3247	5925	0.12%	0.010%
27	16.092	2206	2211	2212	rBV4	4293	5447	0.11%	0.009%
28	16.139	2215	2219	2223	rVB7	4419	6192	0.12%	0.011%
29	16.357	2252	2256	2261	rBV5	10634	15795	0.31%	0.027%
30	17.004	2363	2366	2371	rVB7	5718	6681	0.13%	0.012%
31	17.115	2377	2385	2387	rBV7	5165	10722	0.21%	0.018%
32	17.327	2414	2421	2431	rBV	2045686	2841192	55.60%	4.892%
33	17.427	2431	2438	2461	rVB2	3233790	4622014	90.45%	7.959%
34	17.880	2510	2515	2516	rBV5	4043	5478	0.11%	0.009%
35	18.233	2571	2575	2579	rBV5	19584	29250	0.57%	0.050%
36	18.504	2617	2621	2628	rBV9	3447	7342	0.14%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044359.D
Acq On : 27 Feb 2024 10:24
Operator : MA/JU
Sample : PB159204BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK204

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	19.286	2750	2754	2761	rVB2	38185	56921	1.11%	0.098%
38	19.356	2762	2766	2771	rBV	35206	52108	1.02%	0.090%
39	19.521	2791	2794	2797	rBV5	16390	22765	0.45%	0.039%
40	19.674	2817	2820	2823	rBV4	13920	18468	0.36%	0.032%
41	19.727	2823	2829	2838	rVV	3750450	5110143	100.00%	8.799%
42	21.527	3130	3135	3142	rBV	2175754	2842728	55.63%	4.895%
43	23.786	3512	3519	3532	rVB2	2375226	4880274	95.50%	8.403%
44	23.944	3539	3546	3557	rVB	1384261	2920010	57.14%	5.028%




Sum of corrected areas: 58075944

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044359.D
Acq On : 27 Feb 2024 10:24
Operator : MA/JU
Sample : PB159204BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

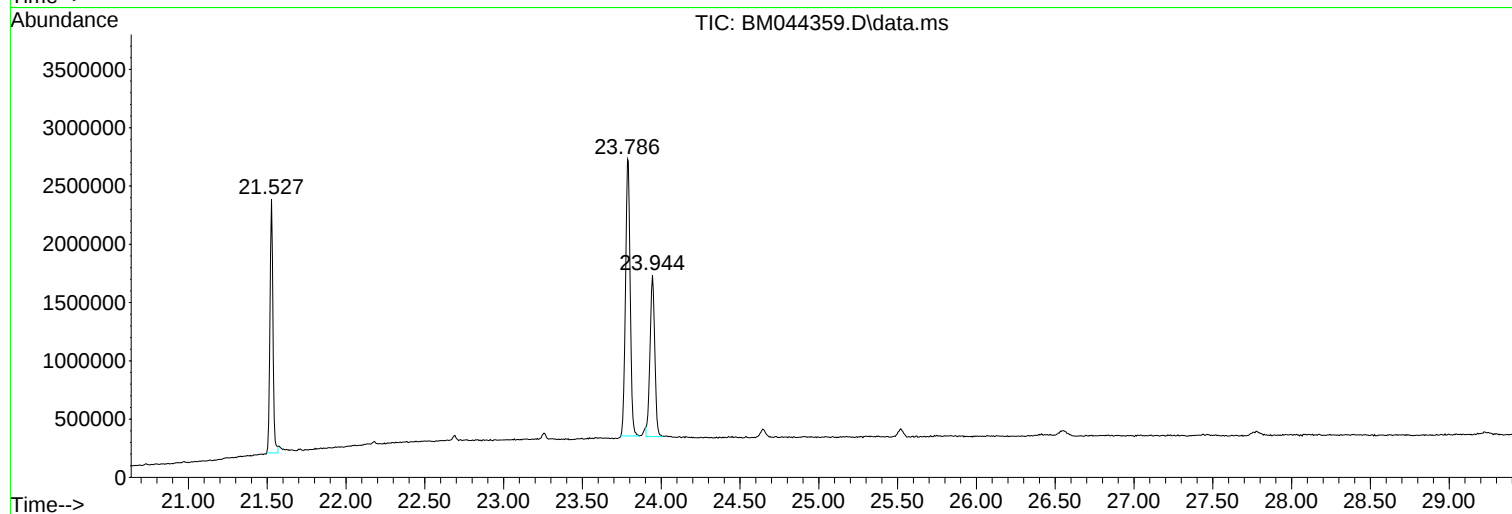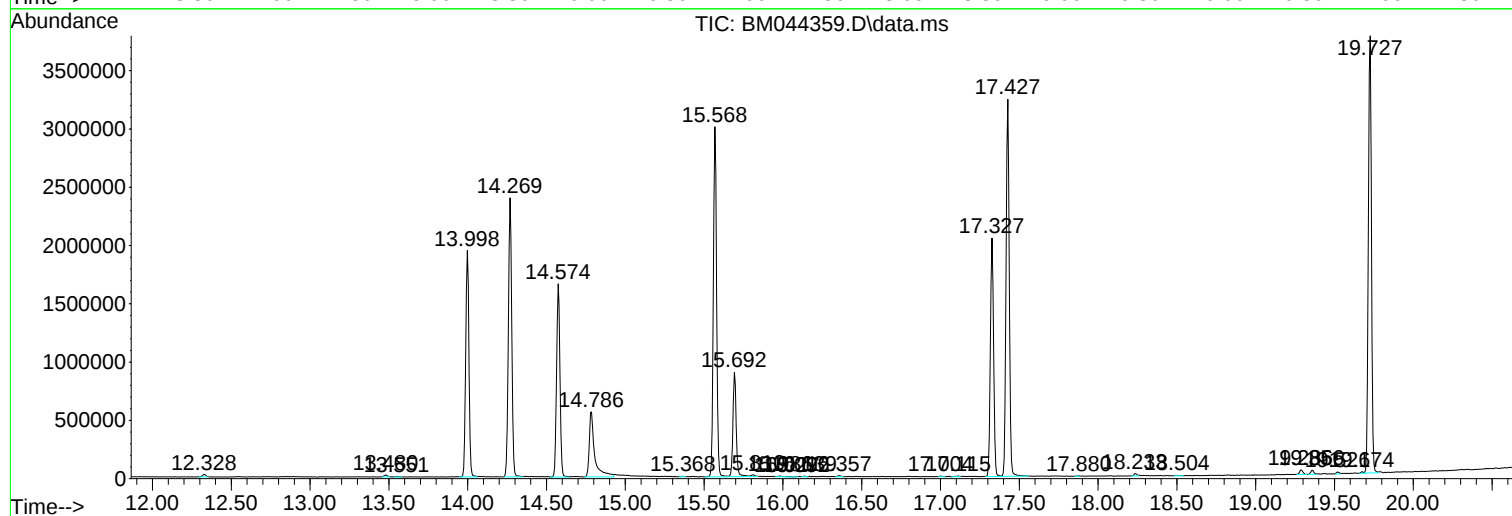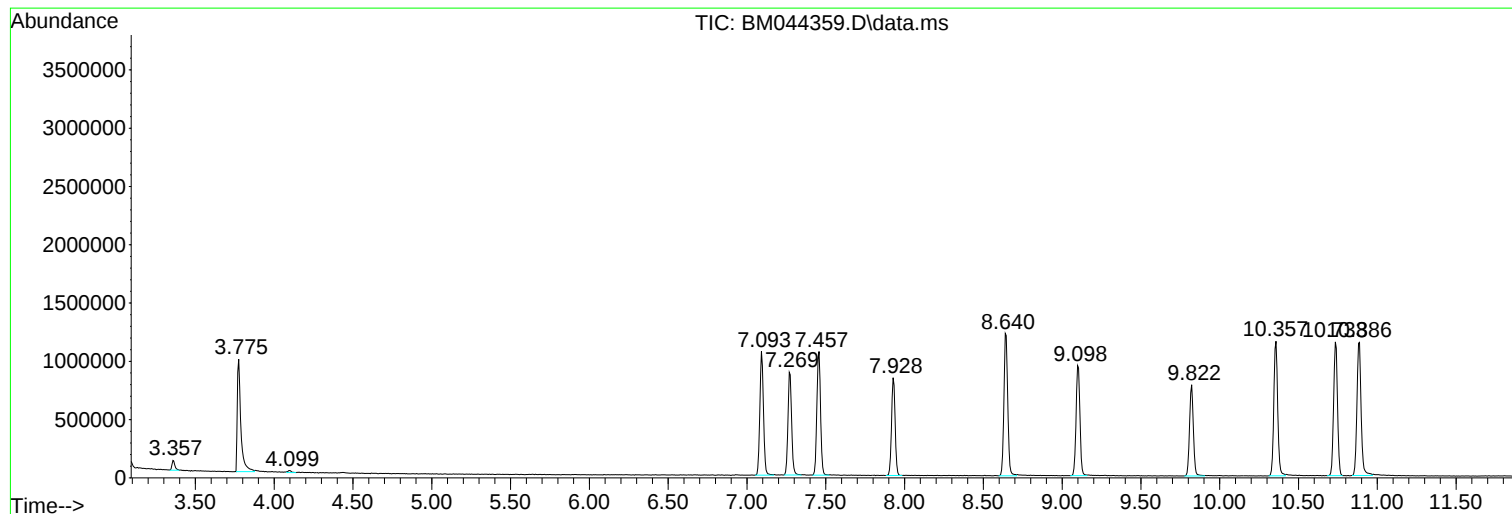

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044359.D
Acq On : 27 Feb 2024 10:24
Operator : MA/JU
Sample : PB159204BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044359.D
Acq On : 27 Feb 2024 10:24
Operator : MA/JU
Sample : PB159204BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK204

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------