

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044377.D
 Acq On : 27 Feb 2024 21:59
 Operator : MA/JU
 Sample : PB159256BL
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK256

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044377.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	43	47	56	rVB	86322	112291	2.27%	0.198%
2	3.781	115	118	135	rBV	994408	1548029	31.27%	2.731%
3	4.104	170	173	178	rVB	19401	26323	0.53%	0.046%
4	4.522	242	244	249	rVB6	5748	6854	0.14%	0.012%
5	7.104	676	683	696	rBV	1049984	1642917	33.19%	2.899%
6	7.281	707	713	730	rVB	856580	1385910	27.99%	2.445%
7	7.469	738	745	758	rVB	1014068	1646336	33.26%	2.905%
8	7.939	818	825	835	rVB	836392	1313955	26.54%	2.318%
9	8.651	937	946	964	rBV	1212932	2012847	40.66%	3.551%
10	9.110	1017	1024	1036	rBV	914947	1538388	31.07%	2.714%
11	9.833	1139	1147	1161	rBV	746423	1276271	25.78%	2.252%
12	10.363	1230	1237	1256	rBV	1089040	1964230	39.68%	3.466%
13	10.745	1294	1302	1310	rBV	1172754	1953867	39.47%	3.447%
14	10.892	1320	1327	1345	rBV	1120893	2069559	41.80%	3.651%
15	12.339	1566	1573	1580	rVB	20918	39378	0.80%	0.069%
16	13.486	1762	1768	1775	rBV2	24893	39309	0.79%	0.069%
17	14.004	1850	1856	1873	rBV	1977522	2762849	55.81%	4.875%
18	14.274	1892	1902	1914	rBV	2329042	3516985	71.04%	6.205%
19	14.580	1947	1954	1963	rBV	1721213	2513875	50.78%	4.435%
20	14.792	1982	1990	2008	rBV	499241	1197215	24.18%	2.112%
21	14.992	2022	2024	2032	rVB10	7908	18851	0.38%	0.033%
22	15.574	2116	2123	2133	rBV	2926835	4237496	85.60%	7.476%
23	15.698	2137	2144	2159	rVV	801004	1136434	22.96%	2.005%
24	15.815	2161	2164	2168	rVB4	16804	22018	0.44%	0.039%
25	16.145	2217	2220	2224	rVB6	4192	5592	0.11%	0.010%
26	16.362	2254	2257	2262	rVV5	9101	11464	0.23%	0.020%
27	17.009	2362	2367	2370	rBV6	5260	7824	0.16%	0.014%
28	17.115	2381	2385	2391	rVB5	5794	8329	0.17%	0.015%
29	17.333	2415	2422	2431	rBV	1954122	2851800	57.60%	5.032%
30	17.433	2432	2439	2450	rVV	3080954	4511892	91.14%	7.961%
31	18.239	2573	2576	2580	rBV6	7399	11121	0.22%	0.020%
32	19.292	2750	2755	2759	rBV2	34218	46222	0.93%	0.082%
33	19.362	2763	2767	2774	rVB	31487	43320	0.88%	0.076%
34	19.527	2792	2795	2796	rBV3	6670	6962	0.14%	0.012%
35	19.680	2818	2821	2822	rBV3	10347	9356	0.19%	0.017%
36	19.727	2823	2829	2838	rVV	3672914	4950613	100.00%	8.735%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044377.D
Acq On : 27 Feb 2024 21:59
Operator : MA/JU
Sample : PB159256BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK256

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	21.527	3130	3135	3143	rBV	2103594	2696721	54.47%	4.758%
38	23.791	3512	3520	3534	rBV	2356916	4688865	94.71%	8.273%
39	23.944	3540	3546	3557	rVB	1353716	2845847	57.48%	5.021%




Sum of corrected areas: 56678115

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044377.D
Acq On : 27 Feb 2024 21:59
Operator : MA/JU
Sample : PB159256BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK256

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

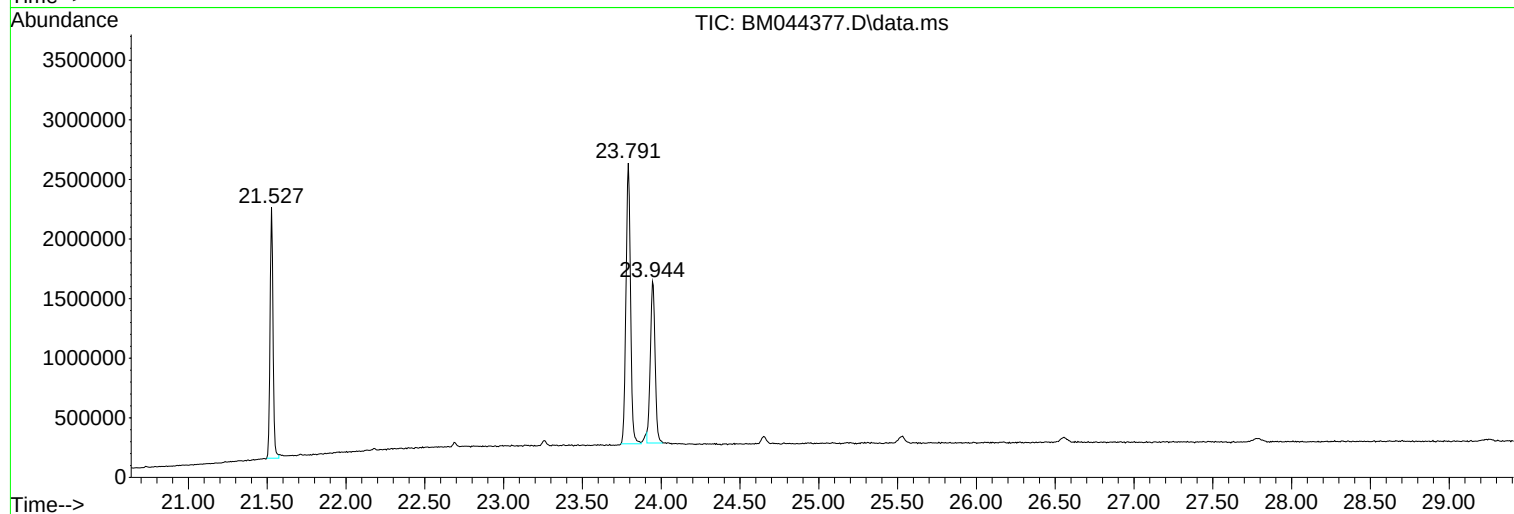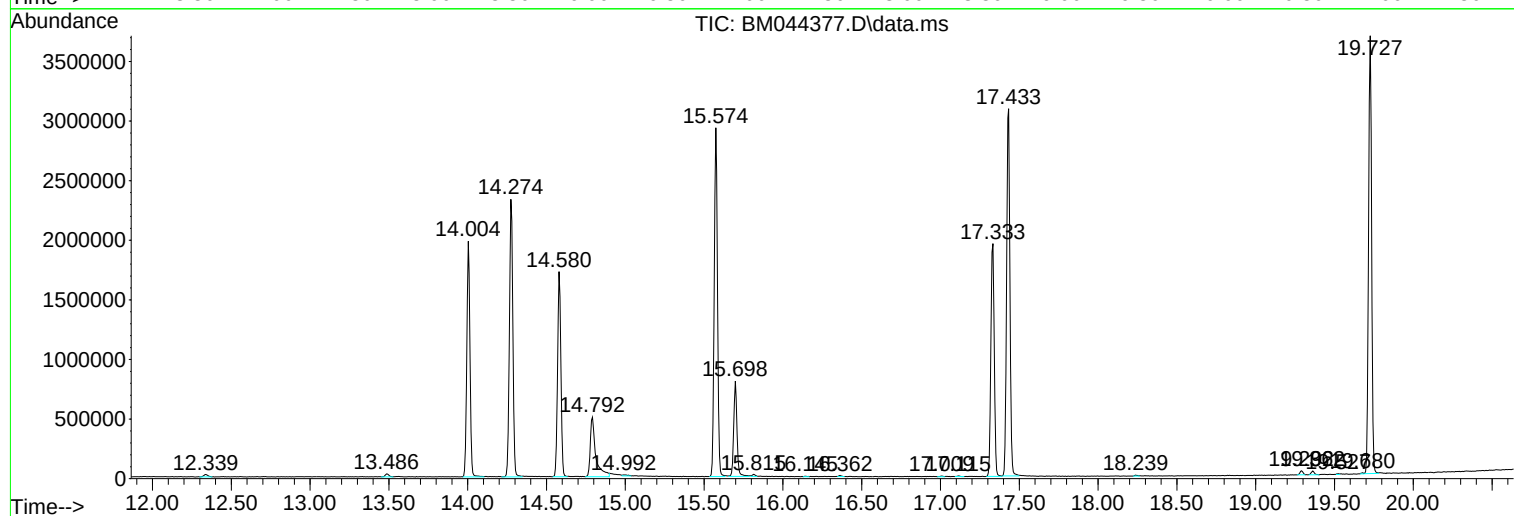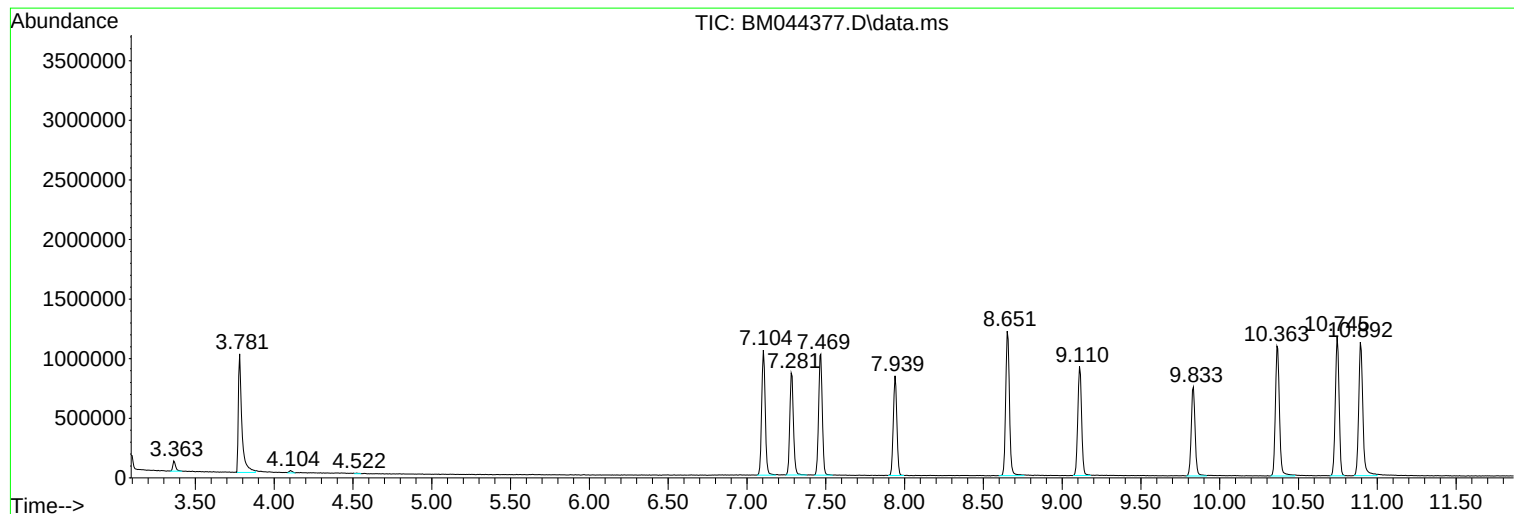

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044377.D
Acq On : 27 Feb 2024 21:59
Operator : MA/JU
Sample : PB159256BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK256

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044377.D
Acq On : 27 Feb 2024 21:59
Operator : MA/JU
Sample : PB159256BL
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK256

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------