

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044380.D
 Acq On : 27 Feb 2024 23:49
 Operator : MA/JU
 Sample : P1498-18
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AC2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044380.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	37	41	46	rBV	721690	924764	14.76%	1.643%
2	3.399	51	53	61	rVB2	38263	57944	0.92%	0.103%
3	3.787	116	119	131	rBV	184084	328647	5.25%	0.584%
4	4.104	170	173	178	rVB2	18774	24342	0.39%	0.043%
5	4.628	258	262	268	rVB2	45140	60164	0.96%	0.107%
6	5.587	421	425	430	rVB	35609	49493	0.79%	0.088%
7	7.104	677	683	694	rVB	207315	336165	5.37%	0.597%
8	7.281	707	713	725	rBV	945653	1494700	23.86%	2.656%
9	7.463	738	744	754	rVV	816308	1307665	20.87%	2.323%
10	7.551	758	759	766	rVB6	7270	7539	0.12%	0.013%
11	7.940	818	825	833	rBV	704452	1104093	17.62%	1.962%
12	8.651	939	946	956	rBV	573566	944824	15.08%	1.679%
13	9.110	1013	1024	1035	rBV	1007476	1697404	27.09%	3.016%
14	9.504	1087	1091	1095	rVB5	6437	10627	0.17%	0.019%
15	9.828	1138	1146	1160	rBV	780164	1330771	21.24%	2.364%
16	10.363	1230	1237	1257	rBV	1098077	1906410	30.43%	3.387%
17	10.745	1292	1302	1312	rBV	1006313	1675216	26.74%	2.976%
18	10.892	1319	1327	1351	rBV	936500	1750566	27.94%	3.110%
19	12.339	1566	1573	1580	rVB2	21037	36990	0.59%	0.066%
20	13.410	1752	1755	1761	rVB4	6445	11276	0.18%	0.020%
21	13.486	1761	1768	1773	rBV2	27489	45253	0.72%	0.080%
22	14.004	1849	1856	1867	rBV	2226092	3088948	49.30%	5.488%
23	14.274	1893	1902	1917	rBV	2602550	3887029	62.04%	6.906%
24	14.580	1946	1954	1962	rBV	1499552	2152451	34.35%	3.824%
25	14.798	1985	1991	2007	rBV2	60541	204563	3.26%	0.363%
26	15.004	2021	2026	2033	rVB8	12573	23994	0.38%	0.043%
27	15.380	2088	2090	2096	rVB4	5955	7662	0.12%	0.014%
28	15.574	2116	2123	2134	rBV	3391346	4816383	76.87%	8.557%
29	15.698	2138	2144	2156	rVV	1062345	1505457	24.03%	2.675%
30	15.810	2160	2163	2170	rVB4	16994	27947	0.45%	0.050%
31	16.298	2244	2246	2252	rVB6	4620	7676	0.12%	0.014%
32	16.363	2252	2257	2261	rBV6	12754	22086	0.35%	0.039%
33	16.880	2341	2345	2351	rVB7	6720	8986	0.14%	0.016%
34	17.010	2362	2367	2370	rBV6	5838	8472	0.14%	0.015%
35	17.327	2415	2421	2432	rBV	1646056	2449546	39.10%	4.352%
36	17.433	2432	2439	2458	rVV	3776449	5586883	89.17%	9.926%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044380.D
Acq On : 27 Feb 2024 23:49
Operator : MA/JU
Sample : P1498-18
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	18.009	2533	2537	2544	rVB9	16405	23160	0.37%	0.041%
38	18.239	2570	2576	2587	rBV2	89109	152931	2.44%	0.272%
39	18.562	2629	2631	2639	rVB8	5969	8479	0.14%	0.015%
40	18.721	2654	2658	2664	rBV7	13169	23574	0.38%	0.042%
41	19.286	2750	2754	2760	rBV2	46853	66692	1.06%	0.118%
42	19.362	2762	2767	2771	rBV	41854	64476	1.03%	0.115%
43	19.439	2777	2780	2782	rBV4	7014	8224	0.13%	0.015%
44	19.521	2790	2794	2800	rBV4	40974	52953	0.85%	0.094%
45	19.674	2817	2820	2823	rBV2	23895	27853	0.44%	0.049%
46	19.727	2823	2829	2838	rVV	4700721	6265598	100.00%	11.132%
47	21.256	3086	3089	3096	rBV3	70834	102985	1.64%	0.183%
48	21.527	3129	3135	3144	rBV	1753100	2374150	37.89%	4.218%
49	23.786	3512	3519	3533	rVB2	2872602	5783383	92.30%	10.276%
50	23.944	3539	3546	3555	rVB	1163245	2425392	38.71%	4.309%




Sum of corrected areas: 56282786

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044380.D
Acq On : 27 Feb 2024 23:49
Operator : MA/JU
Sample : P1498-18
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

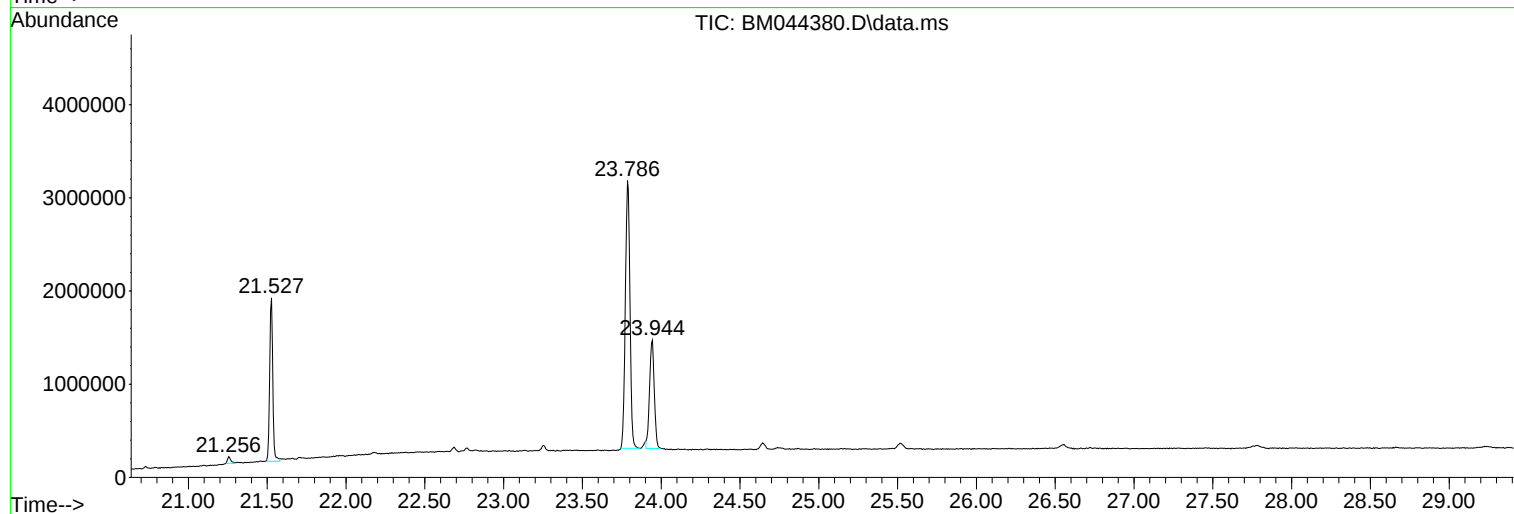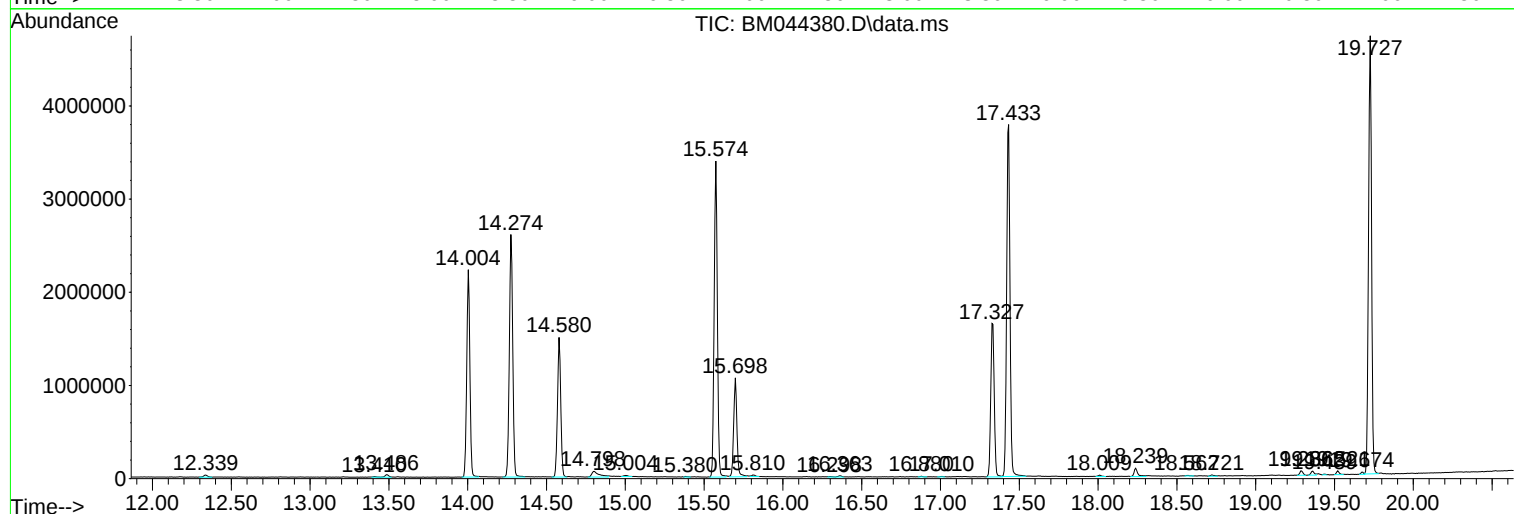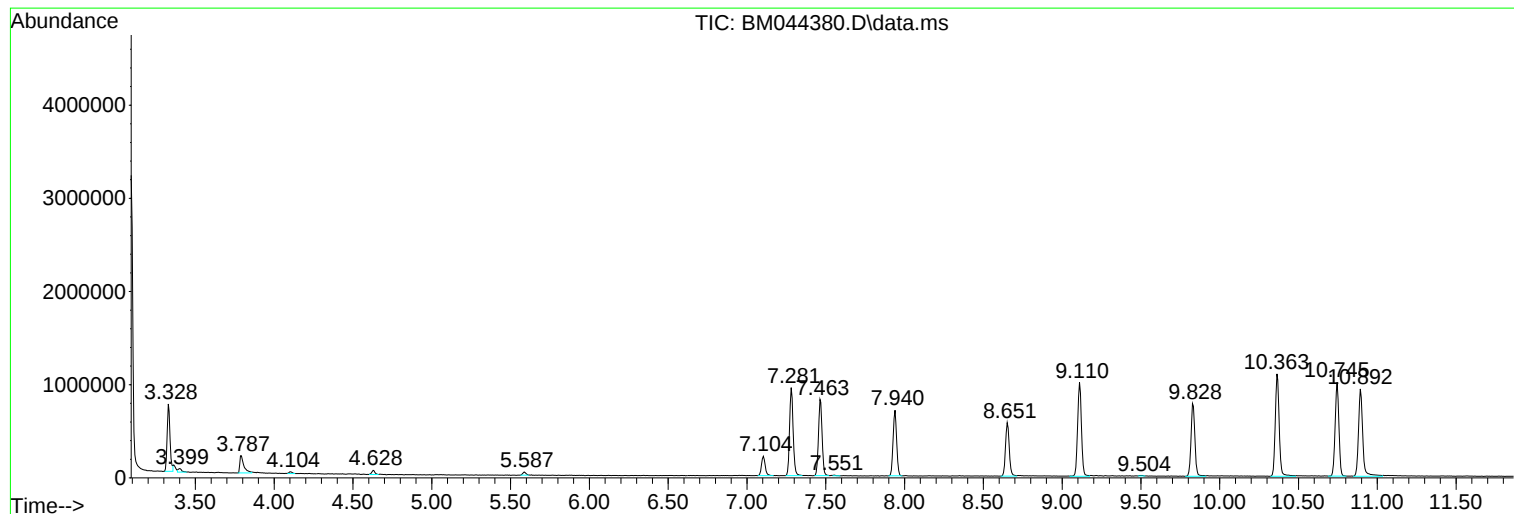

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044380.D
Acq On : 27 Feb 2024 23:49
Operator : MA/JU
Sample : P1498-18
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044380.D
Acq On : 27 Feb 2024 23:49
Operator : MA/JU
Sample : P1498-18
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AC2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------