

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044381.D
 Acq On : 28 Feb 2024 00:25
 Operator : MA/JU
 Sample : P1498-19
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044381.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.328	38	41	45	rBV	48546	63540	0.99%	0.116%
2	3.363	45	47	51	rVB	49596	57754	0.90%	0.105%
3	3.787	116	119	142	rBV	276816	497160	7.75%	0.904%
4	4.104	169	173	178	rVB	20183	27885	0.43%	0.051%
5	4.628	257	262	268	rVB	59455	85271	1.33%	0.155%
6	5.593	421	426	431	rBV	28396	42788	0.67%	0.078%
7	7.104	677	683	692	rBV	221104	355012	5.53%	0.646%
8	7.281	707	713	722	rBV	957501	1511289	23.55%	2.749%
9	7.469	737	745	755	rBV	847112	1364765	21.27%	2.483%
10	7.545	755	758	765	rVB8	6529	13445	0.21%	0.024%
11	7.940	819	825	835	rVB	635919	994609	15.50%	1.809%
12	8.651	940	946	956	rBV	614440	1023534	15.95%	1.862%
13	9.110	1016	1024	1034	rBV	1019288	1706270	26.59%	3.104%
14	9.834	1137	1147	1160	rBV	783012	1345051	20.96%	2.447%
15	10.363	1230	1237	1259	rBV	1064847	1910742	29.78%	3.476%
16	10.745	1294	1302	1312	rVB	865940	1464686	22.83%	2.665%
17	10.892	1318	1327	1354	rBV	1043464	1960306	30.55%	3.566%
18	12.339	1568	1573	1580	rVB	20214	35761	0.56%	0.065%
19	13.486	1762	1768	1773	rVV3	25992	42490	0.66%	0.077%
20	14.004	1849	1856	1864	rBV	2253813	3135993	48.88%	5.705%
21	14.274	1895	1902	1913	rBV2	2614999	3873129	60.36%	7.046%
22	14.580	1947	1954	1962	rBV	1246617	1870359	29.15%	3.403%
23	14.804	1985	1992	2013	rBV3	58428	228439	3.56%	0.416%
24	15.386	2086	2091	2095	rBV5	4676	9310	0.15%	0.017%
25	15.574	2114	2123	2135	rBV	3489797	4972411	77.50%	9.046%
26	15.698	2138	2144	2159	rVV	1087948	1553987	24.22%	2.827%
27	15.810	2160	2163	2172	rVB5	17184	35684	0.56%	0.065%
28	16.357	2252	2256	2262	rVB6	10912	17272	0.27%	0.031%
29	17.010	2363	2367	2372	rVB8	6342	9444	0.15%	0.017%
30	17.333	2415	2422	2432	rBV	1438664	2101702	32.76%	3.824%
31	17.433	2432	2439	2452	rBV	3919486	5758773	89.75%	10.477%
32	18.009	2533	2537	2541	rBV6	11343	14477	0.23%	0.026%
33	18.239	2570	2576	2582	rBV3	32313	52403	0.82%	0.095%
34	19.292	2750	2755	2761	rVB3	46318	64825	1.01%	0.118%
35	19.362	2762	2767	2771	rBV	44848	66659	1.04%	0.121%
36	19.521	2790	2794	2799	rBV5	26818	35794	0.56%	0.065%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044381.D
Acq On : 28 Feb 2024 00:25
Operator : MA/JU
Sample : P1498-19
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	19.680	2817	2821	2823	rBV3	20629	26078	0.41%	0.047%
38	19.727	2823	2829	2838	rVV	4738316	6416212	100.00%	11.673%
39	20.292	2923	2925	2930	rVB5	11898	12210	0.19%	0.022%
40	20.733	2997	3000	3004	rBV4	16908	23638	0.37%	0.043%
41	21.527	3130	3135	3141	rBV	1506476	1981359	30.88%	3.605%
42	23.791	3512	3520	3532	rBV2	2982880	6073135	94.65%	11.049%
43	23.944	3540	3546	3558	rVB	1020969	2132169	33.23%	3.879%




Sum of corrected areas: 54967820

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044381.D
Acq On : 28 Feb 2024 00:25
Operator : MA/JU
Sample : P1498-19
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

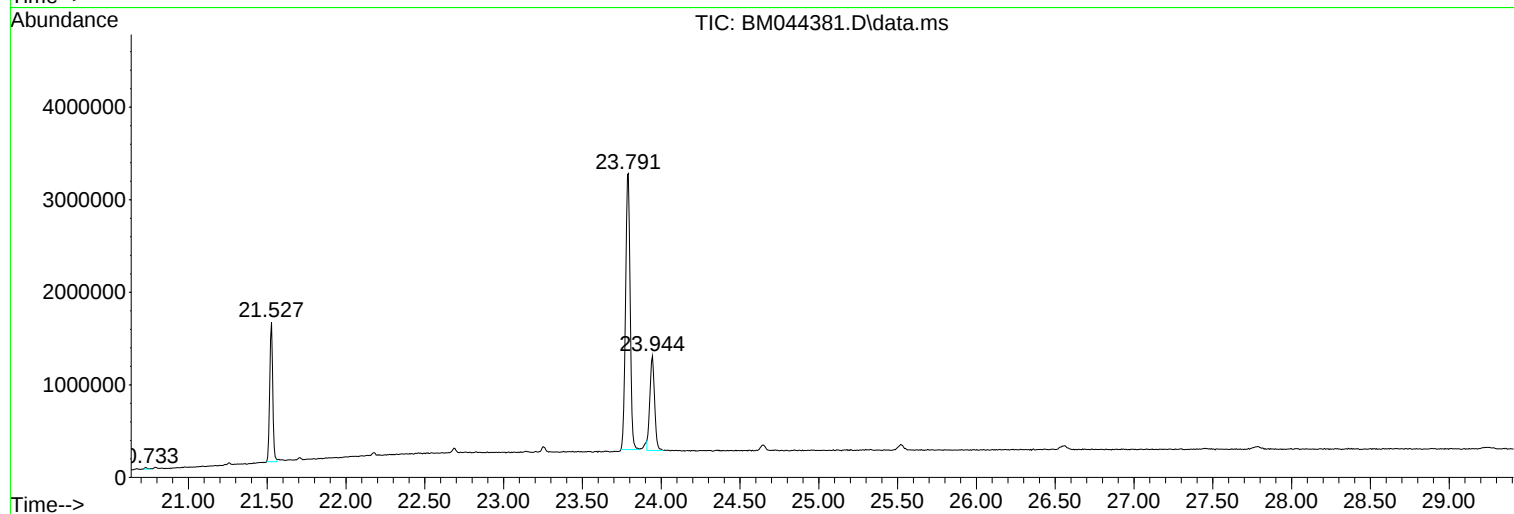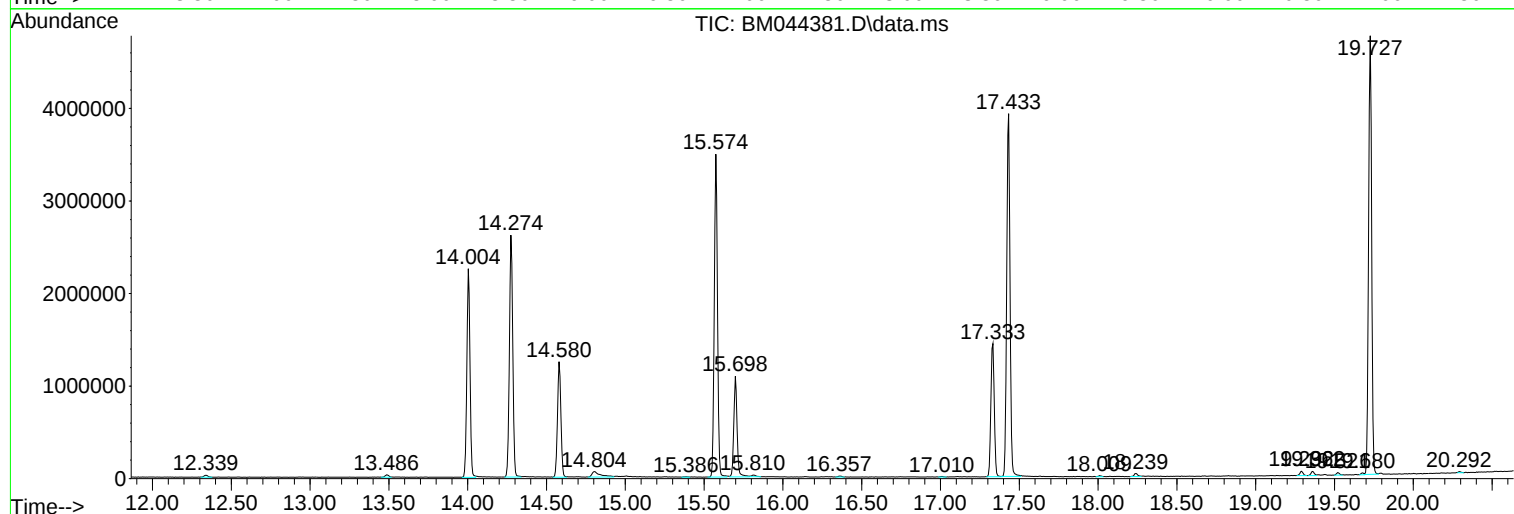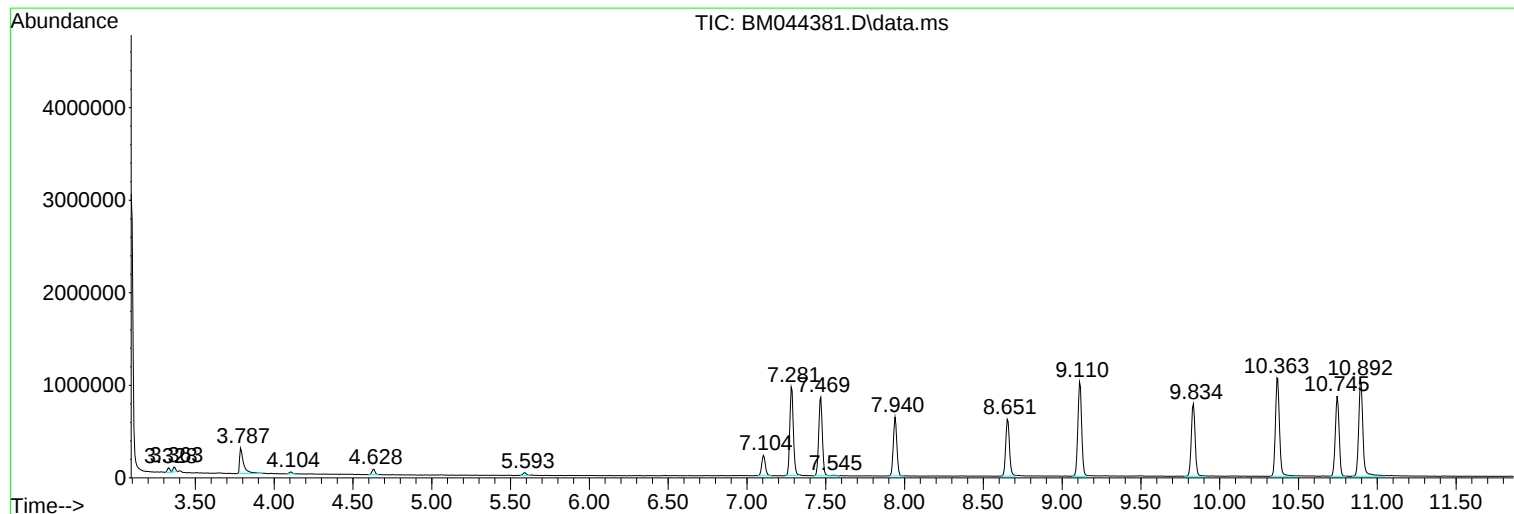

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044381.D
Acq On : 28 Feb 2024 00:25
Operator : MA/JU
Sample : P1498-19
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044381.D
Acq On : 28 Feb 2024 00:25
Operator : MA/JU
Sample : P1498-19
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------