

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044382.D
 Acq On : 28 Feb 2024 01:02
 Operator : MA/JU
 Sample : P1508-06
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH405

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044382.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	44	47	53	rBV	48645	63150	1.00%	0.117%
2	3.651	93	96	100	rBV5	6804	10470	0.17%	0.019%
3	3.787	116	119	133	rBV	221198	405315	6.42%	0.750%
4	4.104	170	173	180	rVB4	15970	24825	0.39%	0.046%
5	7.104	677	683	692	rBV	208942	336210	5.32%	0.622%
6	7.287	707	714	723	rBV	854520	1405331	22.25%	2.602%
7	7.469	738	745	755	rBV	807925	1259164	19.94%	2.331%
8	7.939	818	825	835	rBV	659261	1052623	16.67%	1.949%
9	8.657	939	947	956	rBV	573280	969548	15.35%	1.795%
10	9.110	1016	1024	1038	rBV	937657	1593241	25.22%	2.950%
11	9.216	1038	1042	1048	rVB6	8972	17124	0.27%	0.032%
12	9.833	1138	1147	1160	rBV	728988	1241203	19.65%	2.298%
13	10.369	1230	1238	1254	rBV	1014413	1790184	28.34%	3.314%
14	10.745	1294	1302	1311	rVB	929211	1584599	25.09%	2.934%
15	10.892	1319	1327	1350	rBV	875642	1697214	26.87%	3.142%
16	12.339	1567	1573	1582	rVB2	21339	39611	0.63%	0.073%
17	13.492	1764	1769	1774	rVB3	18234	30311	0.48%	0.056%
18	14.004	1850	1856	1869	rBV	2156167	3071854	48.63%	5.687%
19	14.274	1894	1902	1910	rBV	2434066	3698721	58.56%	6.848%
20	14.580	1948	1954	1964	rBV	1403204	2054015	32.52%	3.803%
21	14.804	1983	1992	2006	rBV2	55680	196829	3.12%	0.364%
22	15.386	2085	2091	2095	rBV6	5079	9479	0.15%	0.018%
23	15.574	2115	2123	2138	rBV	3376921	4892755	77.46%	9.059%
24	15.698	2138	2144	2160	rVV	1022869	1475174	23.36%	2.731%
25	15.810	2160	2163	2169	rVB5	15314	27877	0.44%	0.052%
26	16.362	2252	2257	2262	rVB8	10598	16890	0.27%	0.031%
27	17.333	2415	2422	2432	rBV	1591320	2338980	37.03%	4.331%
28	17.433	2432	2439	2457	rVV	3993860	5735887	90.81%	10.620%
29	17.645	2469	2475	2477	rVB6	5014	9270	0.15%	0.017%
30	18.239	2572	2576	2581	rBV5	21455	30703	0.49%	0.057%
31	18.821	2672	2675	2680	rBV7	4559	7657	0.12%	0.014%
32	19.292	2750	2755	2760	rBV2	43978	63101	1.00%	0.117%
33	19.362	2762	2767	2772	rBV	41087	57576	0.91%	0.107%
34	19.521	2790	2794	2799	rBV5	22215	31886	0.50%	0.059%
35	19.680	2817	2821	2823	rBV2	19279	23609	0.37%	0.044%
36	19.727	2823	2829	2839	rVV	4877526	6316186	100.00%	11.694%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044382.D
Acq On : 28 Feb 2024 01:02
Operator : MA/JU
Sample : P1508-06
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH405

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	21.527	3130	3135	3145	rBV	1674919	2231644	35.33%	4.132%
38	23.785	3512	3519	3532	rBV2	2916692	5912760	93.61%	10.947%
39	23.944	3540	3546	3556	rVB	1106220	2288302	36.23%	4.237%




Sum of corrected areas: 54011278

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044382.D
Acq On : 28 Feb 2024 01:02
Operator : MA/JU
Sample : P1508-06
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH405

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

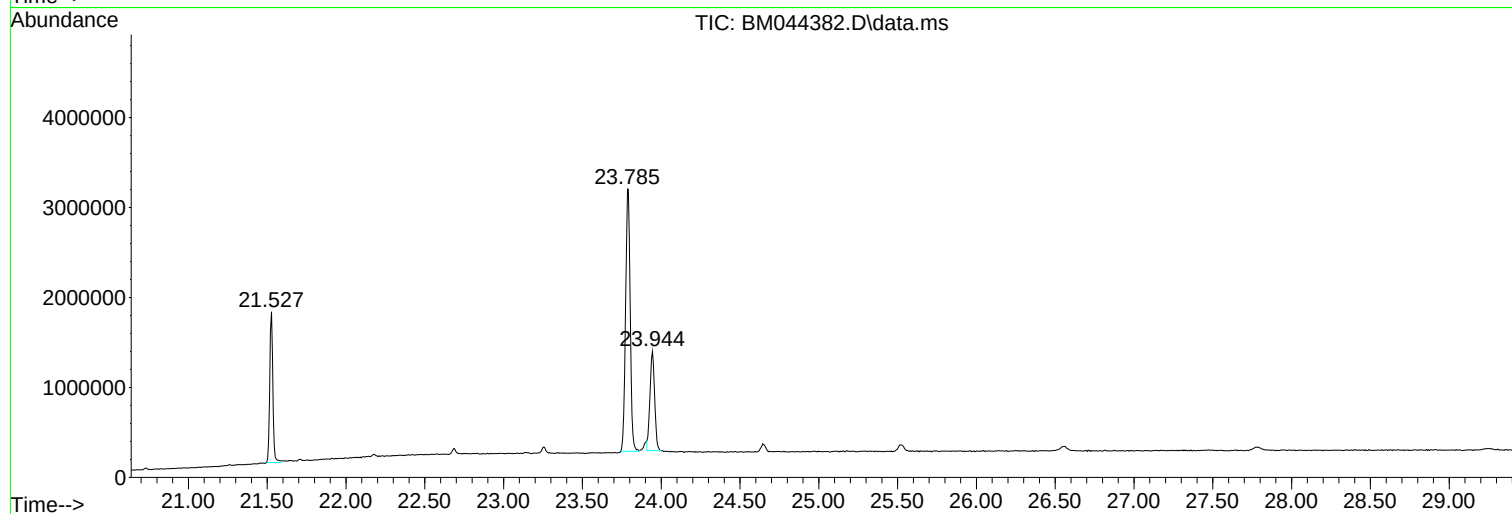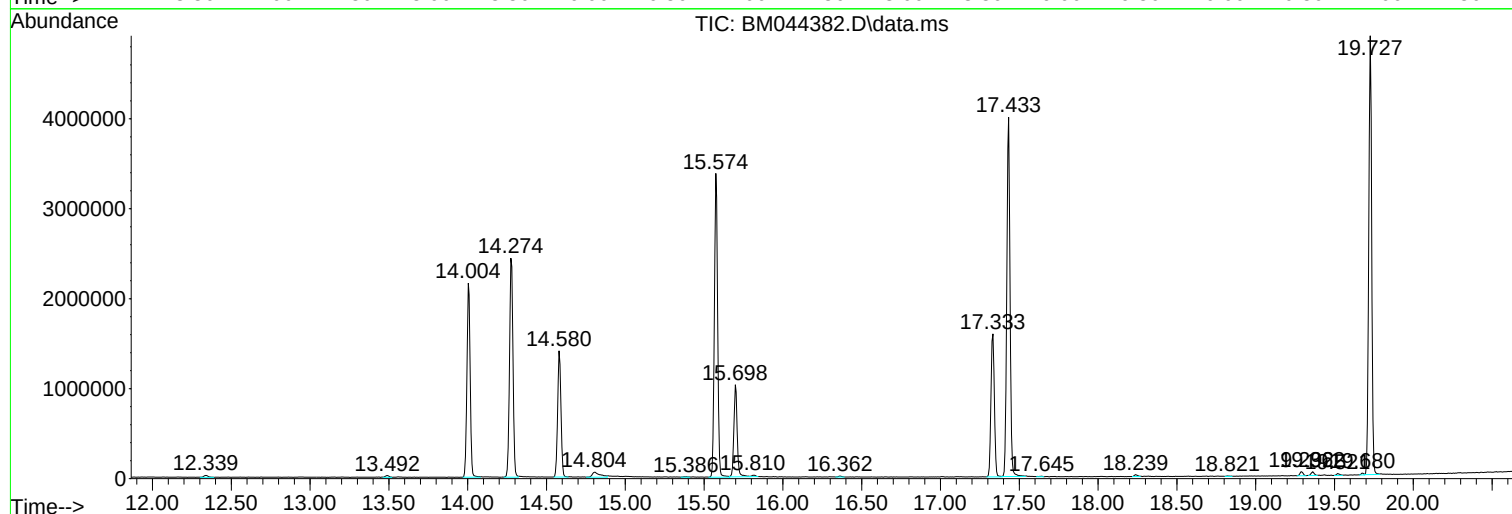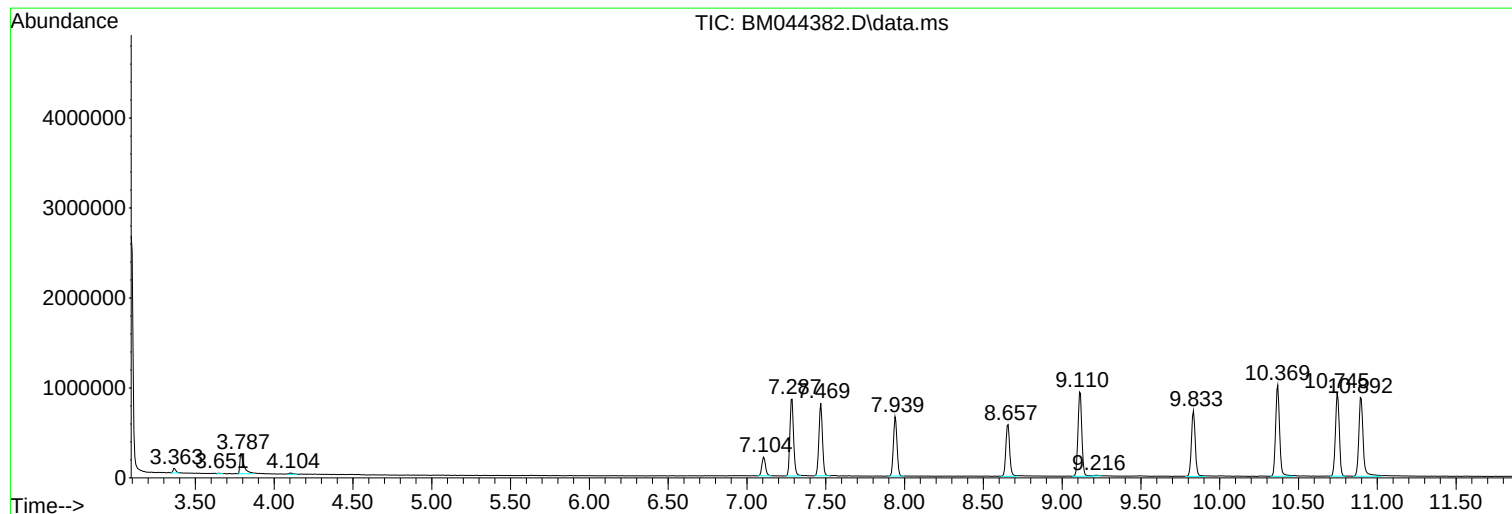

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044382.D
Acq On : 28 Feb 2024 01:02
Operator : MA/JU
Sample : P1508-06
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH405

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044382.D
Acq On : 28 Feb 2024 01:02
Operator : MA/JU
Sample : P1508-06
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH405

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc