

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044383.D
 Acq On : 28 Feb 2024 01:38
 Operator : MA/JU
 Sample : P1508-07
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH406

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044383.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	44	47	52	rVB	55824	66655	1.04%	0.116%
2	3.787	116	119	142	rBV	326436	569078	8.92%	0.987%
3	4.104	170	173	178	rVB3	15976	19939	0.31%	0.035%
4	7.104	677	683	691	rBV	233230	378567	5.93%	0.656%
5	7.281	707	713	724	rBV	1009731	1632208	25.59%	2.830%
6	7.469	738	745	753	rBV	923866	1446979	22.68%	2.509%
7	7.940	818	825	835	rBV	707896	1110884	17.41%	1.926%
8	8.651	938	946	958	rBV	652414	1099288	17.23%	1.906%
9	9.116	1015	1025	1037	rBV	1079828	1854769	29.07%	3.216%
10	9.216	1040	1042	1048	rVB3	14511	22146	0.35%	0.038%
11	9.498	1086	1090	1097	rVB6	5844	10993	0.17%	0.019%
12	9.834	1139	1147	1158	rBV	865899	1434884	22.49%	2.488%
13	10.369	1229	1238	1256	rBV	1188442	2071534	32.47%	3.592%
14	10.545	1263	1268	1282	rBV2	42928	101589	1.59%	0.176%
15	10.745	1295	1302	1314	rVB	995253	1670681	26.19%	2.897%
16	10.892	1317	1327	1347	rBV	1075601	1992621	31.24%	3.455%
17	11.575	1438	1443	1449	rVB10	6373	11960	0.19%	0.021%
18	12.339	1567	1573	1580	rBV	23879	46293	0.73%	0.080%
19	12.945	1671	1676	1680	rBV7	5129	9173	0.14%	0.016%
20	13.410	1753	1755	1760	rVB5	5688	7702	0.12%	0.013%
21	13.492	1763	1769	1773	rVV4	13799	21036	0.33%	0.036%
22	13.557	1776	1780	1784	rBV6	4454	8425	0.13%	0.015%
23	14.004	1849	1856	1866	rBV	2217629	3238542	50.77%	5.615%
24	14.274	1893	1902	1913	rBV	2779121	4166376	65.31%	7.224%
25	14.580	1948	1954	1963	rBV	1461566	2136582	33.49%	3.705%
26	14.804	1985	1992	2014	rBV3	56044	215346	3.38%	0.373%
27	14.998	2020	2025	2036	rVB3	6978	22576	0.35%	0.039%
28	15.392	2087	2092	2094	rBV5	6485	9891	0.16%	0.017%
29	15.574	2115	2123	2137	rBV	3552763	5193939	81.42%	9.006%
30	15.698	2138	2144	2154	rVV	1041022	1439127	22.56%	2.495%
31	15.816	2161	2164	2170	rVB2	18675	24999	0.39%	0.043%
32	16.363	2254	2257	2262	rVB5	11043	15350	0.24%	0.027%
33	17.110	2378	2384	2386	rBV7	4588	6488	0.10%	0.011%
34	17.333	2415	2422	2431	rBV	1665846	2425872	38.03%	4.206%
35	17.433	2432	2439	2452	rBV	3980089	5778757	90.59%	10.020%
36	18.021	2534	2539	2543	rVB7	4339	8193	0.13%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044383.D
 Acq On : 28 Feb 2024 01:38
 Operator : MA/JU
 Sample : P1508-07
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH406

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

37	18.239	2565	2576	2583	rBV2	50163	81768	1.28%	0.142%
38	18.568	2630	2632	2640	rVB7	4349	7222	0.11%	0.013%
39	19.292	2749	2755	2760	rBV2	49759	72540	1.14%	0.126%
40	19.362	2763	2767	2772	rVV	44601	63264	0.99%	0.110%
41	19.439	2776	2780	2783	rVV5	8456	11801	0.18%	0.020%
42	19.521	2790	2794	2799	rBV6	23382	31746	0.50%	0.055%
43	19.680	2817	2821	2823	rBV3	20874	26595	0.42%	0.046%
44	19.727	2823	2829	2838	rVV	4765905	6379301	100.00%	11.061%
45	21.256	3086	3089	3095	rBV5	32359	45755	0.72%	0.079%
46	21.527	3129	3135	3146	rBV	1690562	2318699	36.35%	4.021%
47	23.791	3512	3520	3533	rBV	2943428	5968662	93.56%	10.349%
48	23.944	3540	3546	3559	rVB	1163667	2394868	37.54%	4.153%




Sum of corrected areas: 57671663

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044383.D
Acq On : 28 Feb 2024 01:38
Operator : MA/JU
Sample : P1508-07
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH406

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

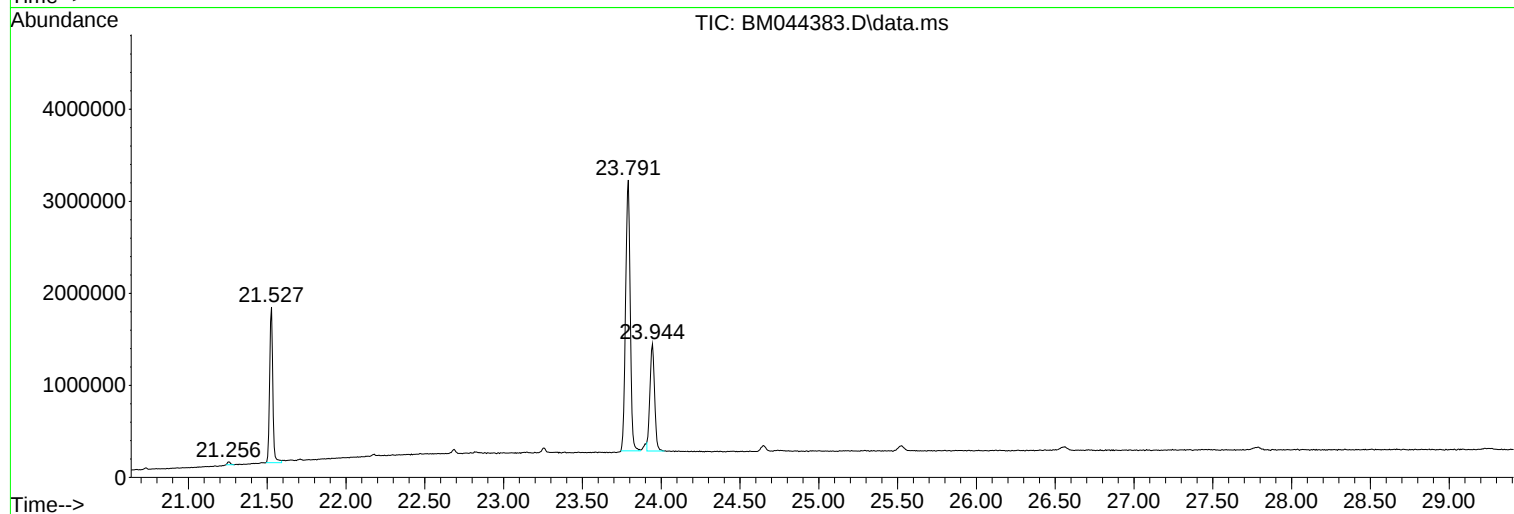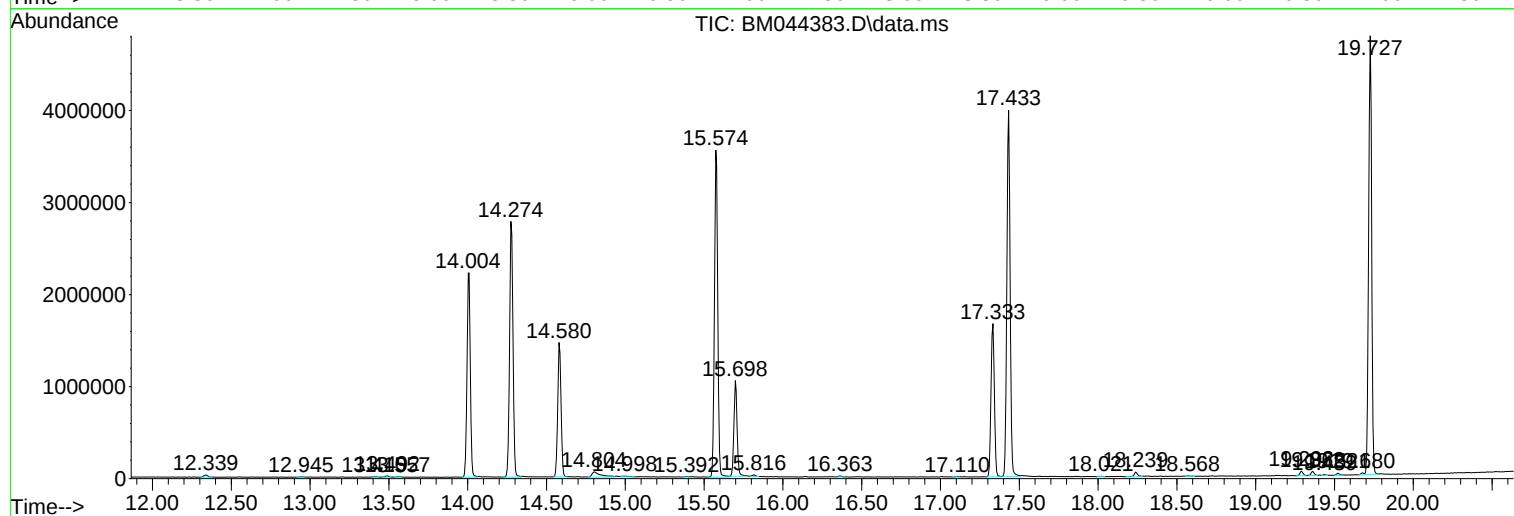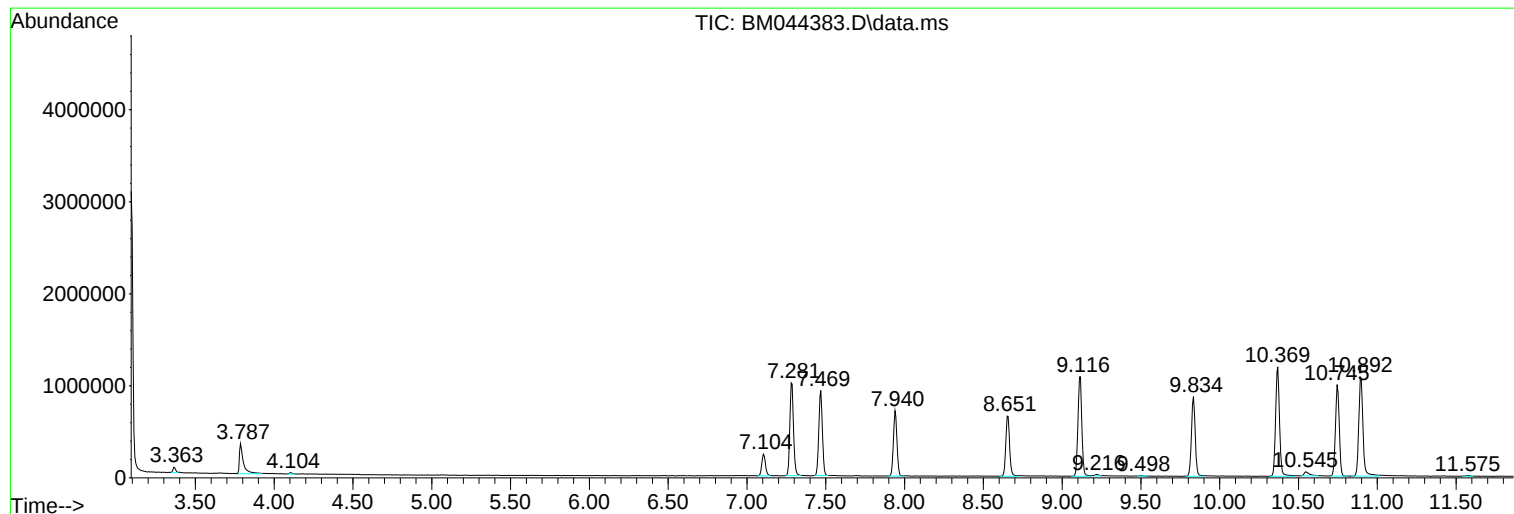

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044383.D
Acq On : 28 Feb 2024 01:38
Operator : MA/JU
Sample : P1508-07
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH406

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044383.D
Acq On : 28 Feb 2024 01:38
Operator : MA/JU
Sample : P1508-07
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH406

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------