

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044384.D
 Acq On : 28 Feb 2024 02:15
 Operator : MA/JU
 Sample : P1508-08
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH408

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044384.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	44	47	56	rBV	53304	72738	1.01%	0.119%
2	3.787	115	119	133	rBV	378436	630790	8.80%	1.033%
3	4.105	171	173	178	rVB2	13416	16310	0.23%	0.027%
4	5.646	430	435	442	rVB9	4655	10445	0.15%	0.017%
5	7.104	676	683	696	rBV	244529	400287	5.59%	0.656%
6	7.281	707	713	728	rBV	1040596	1648375	23.00%	2.701%
7	7.469	738	745	753	rBV	908101	1461968	20.40%	2.395%
8	7.557	756	760	762	rVB5	5496	7708	0.11%	0.013%
9	7.940	817	825	833	rBV	648417	1027162	14.33%	1.683%
10	8.651	939	946	958	rBV	695965	1154172	16.10%	1.891%
11	9.110	1015	1024	1036	rBV	1136556	1884523	26.29%	3.088%
12	9.834	1137	1147	1155	rBV	876122	1476080	20.60%	2.418%
13	10.363	1229	1237	1251	rBV	1223174	2146023	29.94%	3.516%
14	10.745	1294	1302	1309	rVB	927810	1540827	21.50%	2.524%
15	10.892	1319	1327	1339	rBV	1211836	2175406	30.35%	3.564%
16	11.569	1436	1442	1446	rBV9	5336	10329	0.14%	0.017%
17	12.339	1567	1573	1579	rBV	26340	45901	0.64%	0.075%
18	13.486	1762	1768	1775	rBV2	28078	48118	0.67%	0.079%
19	14.004	1849	1856	1869	rBV	2567761	3555284	49.61%	5.825%
20	14.274	1893	1902	1918	rBV	2953264	4417048	61.63%	7.237%
21	14.580	1946	1954	1968	rBV	1390501	2022505	28.22%	3.314%
22	14.804	1985	1992	2007	rBV2	69457	236586	3.30%	0.388%
23	15.386	2086	2091	2094	rBV4	5997	8754	0.12%	0.014%
24	15.574	2116	2123	2138	rBV	3897238	5562127	77.61%	9.113%
25	15.698	2138	2144	2158	rVV	1254707	1739153	24.27%	2.849%
26	15.816	2159	2164	2175	rVB2	21944	46849	0.65%	0.077%
27	16.357	2253	2256	2264	rVB5	13761	22596	0.32%	0.037%
28	17.004	2363	2366	2371	rVB6	5800	8384	0.12%	0.014%
29	17.151	2387	2391	2396	rVB8	10971	14427	0.20%	0.024%
30	17.327	2415	2421	2432	rBV	1590178	2315404	32.31%	3.793%
31	17.433	2432	2439	2454	rVV	4328179	6410980	89.45%	10.503%
32	18.239	2572	2576	2582	rBV2	36709	50002	0.70%	0.082%
33	19.292	2750	2755	2760	rVB2	56230	79187	1.10%	0.130%
34	19.362	2762	2767	2771	rBV	49246	65797	0.92%	0.108%
35	19.439	2776	2780	2784	rVV7	7986	11881	0.17%	0.019%
36	19.521	2790	2794	2799	rBV3	35206	51366	0.72%	0.084%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044384.D
Acq On : 28 Feb 2024 02:15
Operator : MA/JU
Sample : P1508-08
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH408

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	19.674	2817	2820	2823	rBV2	22210	26677	0.37%	0.044%
38	19.727	2823	2829	2838	rVV	5300532	7166930	100.00%	11.742%
39	21.527	3129	3135	3144	rBV	1600460	2233903	31.17%	3.660%
40	23.791	3511	3520	3533	rBV2	3345817	6918100	96.53%	11.334%
41	23.944	3539	3546	3555	rVB	1110342	2316057	32.32%	3.795%




Sum of corrected areas: 61037159

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044384.D
Acq On : 28 Feb 2024 02:15
Operator : MA/JU
Sample : P1508-08
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH408

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

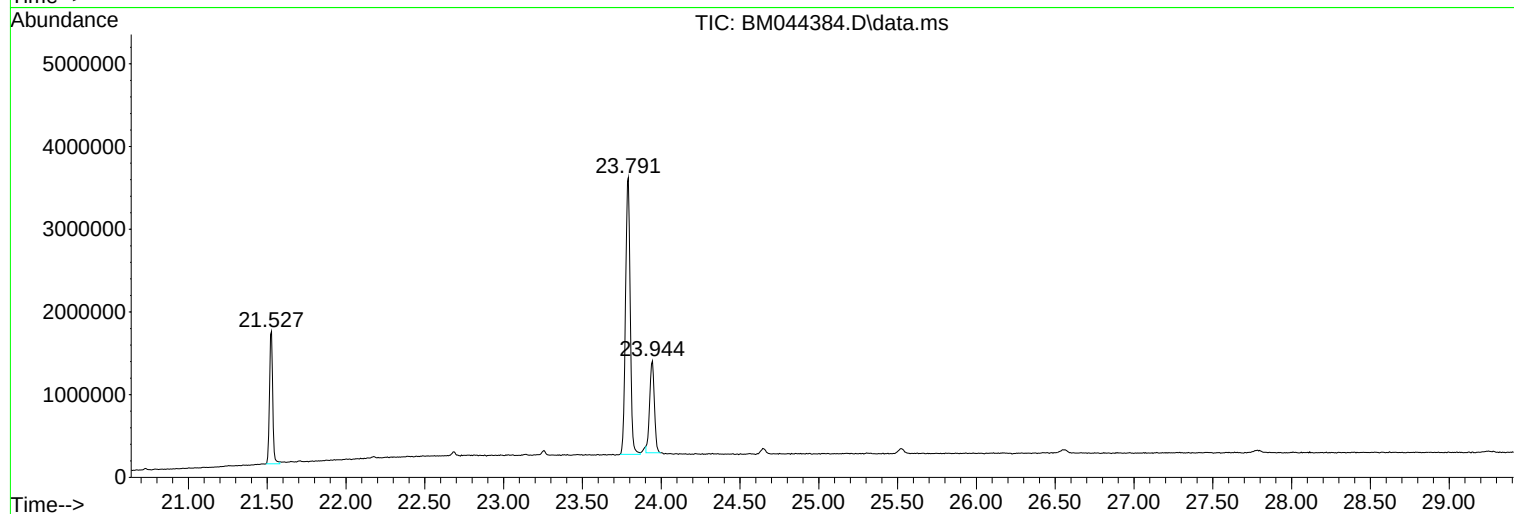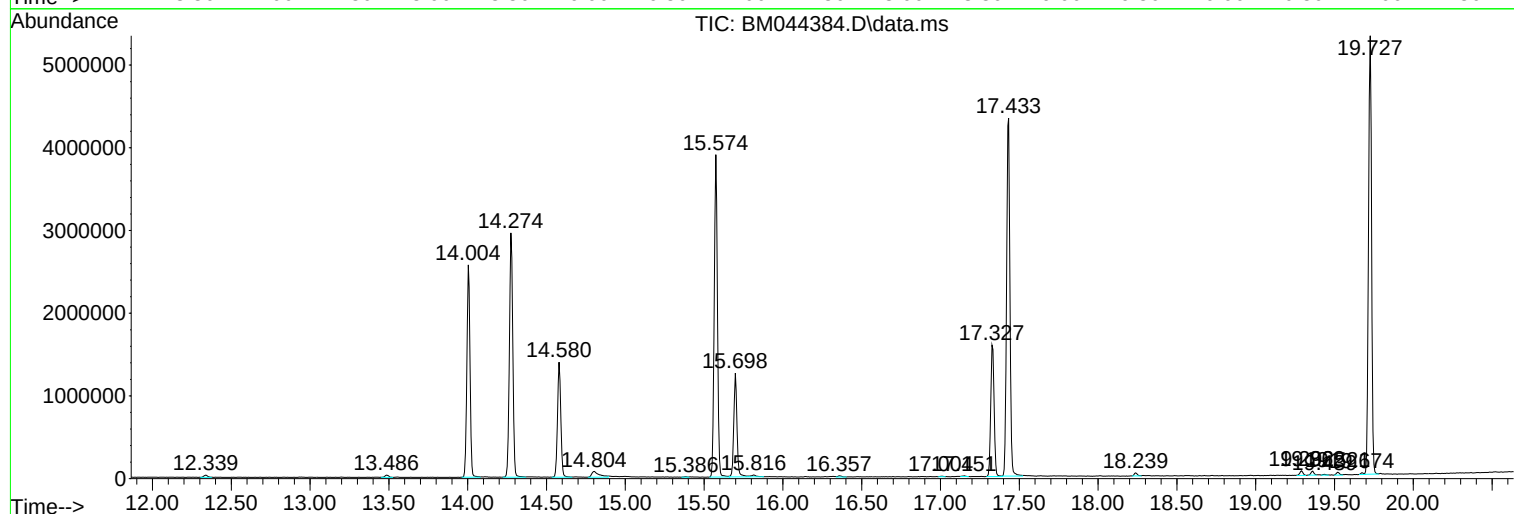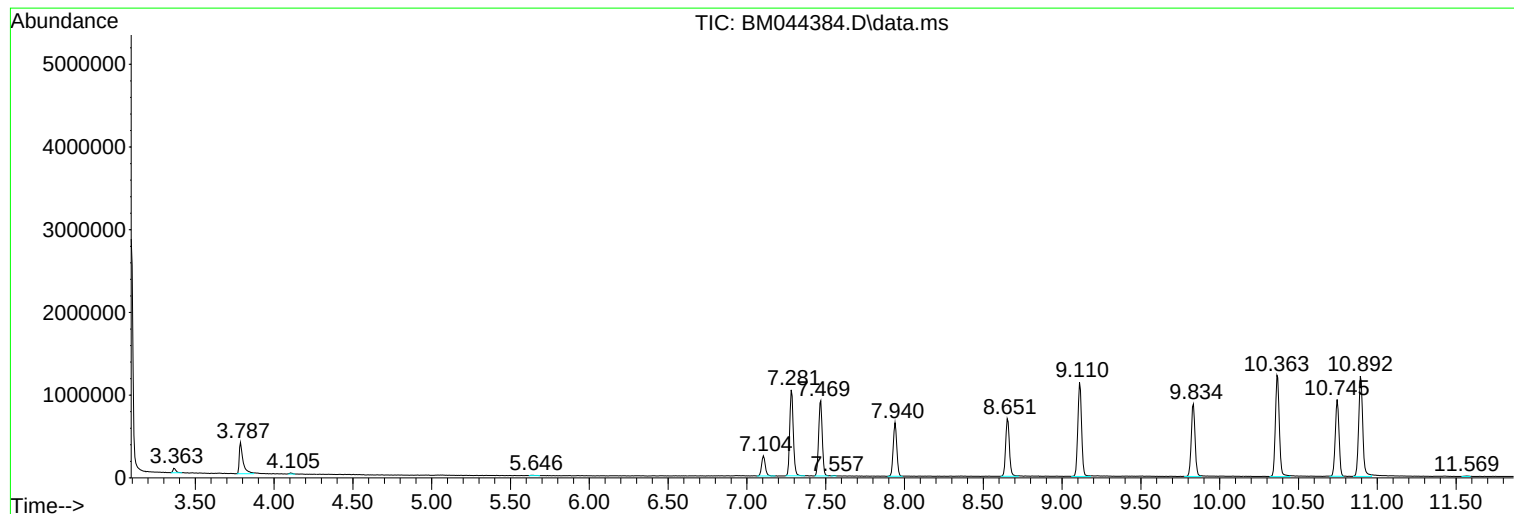

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044384.D
Acq On : 28 Feb 2024 02:15
Operator : MA/JU
Sample : P1508-08
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH408

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044384.D
Acq On : 28 Feb 2024 02:15
Operator : MA/JU
Sample : P1508-08
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH408

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc