

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044385.D
 Acq On : 28 Feb 2024 02:51
 Operator : MA/JU
 Sample : P1526-02
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E10A5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044385.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	44	47	54	rVB	43671	56731	0.88%	0.106%
2	3.793	117	120	132	rBV	107805	207798	3.23%	0.387%
3	4.634	257	263	270	rVB	170159	244501	3.80%	0.456%
4	7.104	678	683	692	rBV	211800	347047	5.40%	0.647%
5	7.286	707	714	730	rVB	875072	1425938	22.18%	2.658%
6	7.469	737	745	757	rBV	821112	1305509	20.31%	2.434%
7	7.939	819	825	834	rBV	612988	983676	15.30%	1.834%
8	8.657	940	947	959	rBV	610261	1013047	15.76%	1.889%
9	9.116	1017	1025	1035	rBV	932720	1610578	25.05%	3.003%
10	9.833	1139	1147	1160	rBV	766618	1275905	19.85%	2.379%
11	10.369	1231	1238	1248	rBV	1052814	1808637	28.14%	3.372%
12	10.745	1295	1302	1312	rVB	873438	1484192	23.09%	2.767%
13	10.898	1320	1328	1342	rBV	629679	1204893	18.74%	2.246%
14	12.339	1569	1573	1580	rVB4	21971	37284	0.58%	0.070%
15	13.415	1753	1756	1763	rBV7	5716	9637	0.15%	0.018%
16	13.492	1763	1769	1777	rVB2	18993	31582	0.49%	0.059%
17	14.004	1848	1856	1871	rBV	2108377	3045693	47.38%	5.678%
18	14.274	1895	1902	1916	rBV	2516928	3792246	58.99%	7.070%
19	14.580	1946	1954	1964	rBV	1256989	1904612	29.63%	3.551%
20	14.804	1986	1992	2009	rBV2	57084	208727	3.25%	0.389%
21	15.004	2022	2026	2035	rVB2	7647	19655	0.31%	0.037%
22	15.574	2116	2123	2131	rBV	3311442	4764741	74.12%	8.883%
23	15.698	2138	2144	2159	rBV	1019766	1461826	22.74%	2.725%
24	15.815	2161	2164	2171	rVB4	14286	23370	0.36%	0.044%
25	16.362	2254	2257	2262	rVB4	11870	16066	0.25%	0.030%
26	16.745	2316	2322	2325	rBV7	6108	8939	0.14%	0.017%
27	17.121	2380	2386	2393	rBV9	4455	11435	0.18%	0.021%
28	17.333	2415	2422	2432	rBV	1502485	2135570	33.22%	3.981%
29	17.433	2432	2439	2456	rBV	4116919	5876862	91.42%	10.956%
30	18.015	2534	2538	2541	rBV6	5351	7973	0.12%	0.015%
31	18.109	2552	2554	2559	rBV5	4242	7003	0.11%	0.013%
32	18.239	2570	2576	2584	rBV2	83717	124856	1.94%	0.233%
33	18.715	2654	2657	2661	rBV4	4549	6756	0.11%	0.013%
34	19.292	2749	2755	2761	rBV2	49021	75958	1.18%	0.142%
35	19.362	2763	2767	2772	rBV	42424	65202	1.01%	0.122%
36	19.521	2790	2794	2798	rBV4	35174	44440	0.69%	0.083%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044385.D
Acq On : 28 Feb 2024 02:51
Operator : MA/JU
Sample : P1526-02
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	19.674	2817	2820	2823	rBV4	18686	23599	0.37%	0.044%
38	19.727	2823	2829	2838	rVV	4787066	6428410	100.00%	11.985%
39	19.968	2867	2870	2876	rVB2	23837	26122	0.41%	0.049%
40	20.727	2997	2999	3003	rVB4	20189	19051	0.30%	0.036%
41	21.256	3086	3089	3095	rBV3	56036	75212	1.17%	0.140%
42	21.527	3129	3135	3147	rBV	1478367	2084163	32.42%	3.886%
43	23.791	3511	3520	3532	rBV	3020868	6193167	96.34%	11.546%
44	23.944	3540	3546	3557	rVB	1030312	2140142	33.29%	3.990%




Sum of corrected areas: 53638751

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044385.D
Acq On : 28 Feb 2024 02:51
Operator : MA/JU
Sample : P1526-02
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

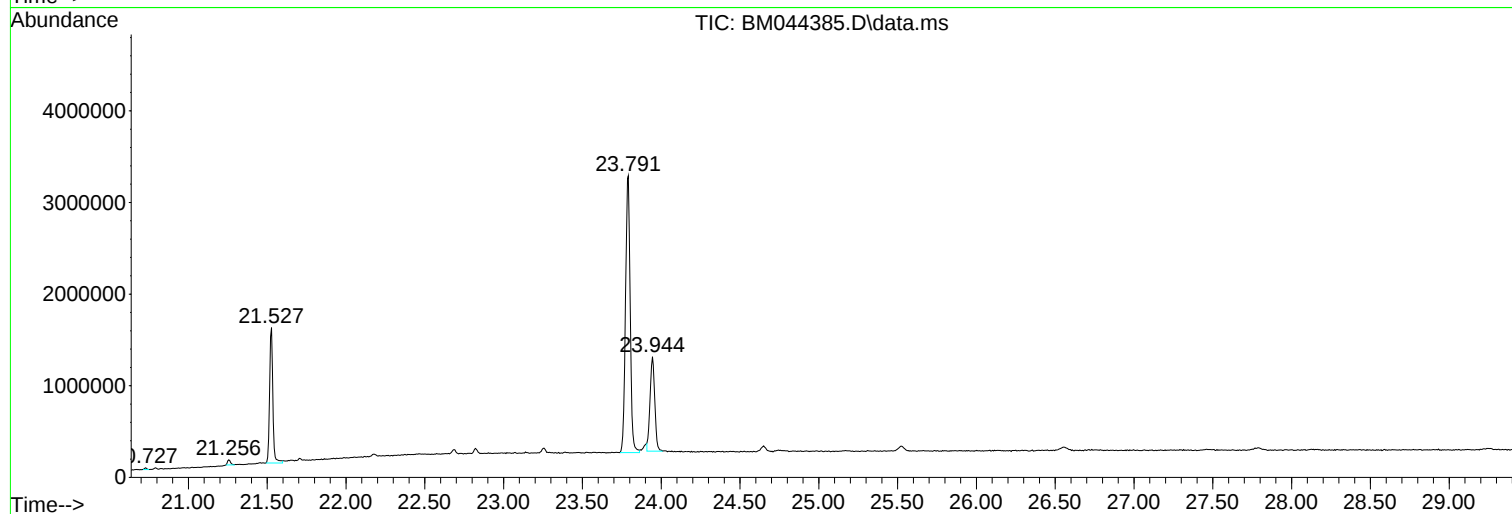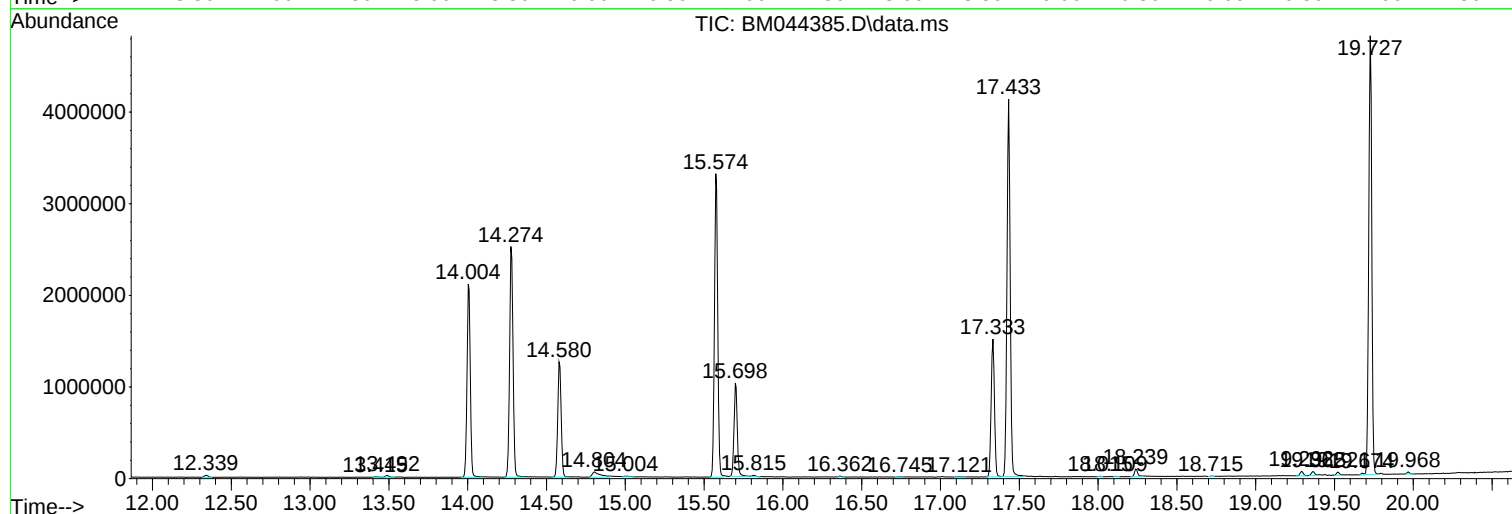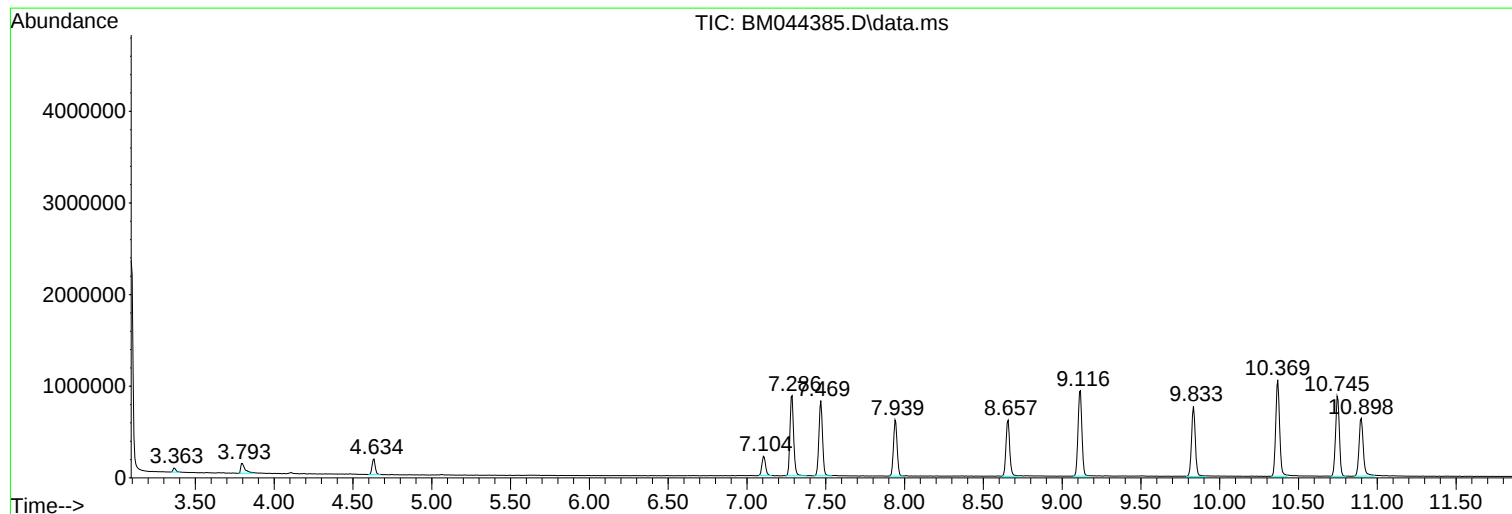

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044385.D
Acq On : 28 Feb 2024 02:51
Operator : MA/JU
Sample : P1526-02
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044385.D
Acq On : 28 Feb 2024 02:51
Operator : MA/JU
Sample : P1526-02
Misc :
ALS Vial : 66 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------