

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044387.D
 Acq On : 28 Feb 2024 04:04
 Operator : MA/JU
 Sample : P1501-16
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E10A3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044387.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	44	48	53	rVB	53073	65953	0.99%	0.112%
2	3.787	116	119	147	rVB	302652	541180	8.10%	0.921%
3	4.105	170	173	178	rVB2	20328	25672	0.38%	0.044%
4	4.493	235	239	246	rVB5	13543	23397	0.35%	0.040%
5	5.440	395	400	406	rVB6	8782	13803	0.21%	0.023%
6	5.593	421	426	431	rBV	25500	35923	0.54%	0.061%
7	5.875	471	474	479	rBV6	4202	7916	0.12%	0.013%
8	5.999	491	495	501	rBV8	5533	8212	0.12%	0.014%
9	6.940	648	655	665	rBV2	16710	35540	0.53%	0.060%
10	7.110	678	684	694	rVB	219251	353444	5.29%	0.601%
11	7.287	708	714	729	rVB	961996	1501650	22.48%	2.555%
12	7.469	737	745	756	rVV	849881	1348290	20.18%	2.294%
13	7.551	756	759	764	rVB6	6447	10303	0.15%	0.018%
14	7.946	819	826	834	rBV	624585	996558	14.92%	1.695%
15	8.010	834	837	842	rVB6	5329	7579	0.11%	0.013%
16	8.210	864	871	874	rBV5	4285	8480	0.13%	0.014%
17	8.522	919	924	929	rBV6	12221	23689	0.35%	0.040%
18	8.575	929	933	938	rVB5	10284	17323	0.26%	0.029%
19	8.657	940	947	956	rBV	645471	1031327	15.44%	1.755%
20	9.116	1017	1025	1036	rBV	1029040	1719427	25.74%	2.925%
21	9.216	1040	1042	1046	rVB5	6556	7034	0.11%	0.012%
22	9.275	1049	1052	1053	rBV3	7589	7491	0.11%	0.013%
23	9.834	1139	1147	1161	rBV	795458	1354684	20.28%	2.305%
24	10.069	1183	1187	1193	rVB7	10084	19542	0.29%	0.033%
25	10.369	1229	1238	1249	rBV	1152315	1973774	29.54%	3.358%
26	10.557	1263	1270	1275	rBV9	10878	26364	0.39%	0.045%
27	10.751	1295	1303	1311	rVB	897247	1519333	22.74%	2.585%
28	10.898	1319	1328	1341	rBV	1010359	1812255	27.13%	3.083%
29	11.551	1434	1439	1446	rBV3	15881	28529	0.43%	0.049%
30	12.339	1568	1573	1579	rBV	25082	43259	0.65%	0.074%
31	12.392	1579	1582	1591	rVV	29460	65222	0.98%	0.111%
32	12.557	1604	1610	1617	rVB	5335	12824	0.19%	0.022%
33	12.804	1647	1652	1660	rVV3	17317	27100	0.41%	0.046%
34	12.881	1660	1665	1668	rVB6	4375	8846	0.13%	0.015%
35	12.951	1668	1677	1680	rBV10	5132	13586	0.20%	0.023%
36	13.033	1686	1691	1692	rBV5	8173	11553	0.17%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044387.D
Acq On : 28 Feb 2024 04:04
Operator : MA/JU
Sample : P1501-16
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	13.057	1693	1695	1704	rVB	16194	27271	0.41%	0.046%
38	13.204	1716	1720	1726	rVB8	8740	16652	0.25%	0.028%
39	13.433	1750	1759	1763	rBV4	13318	26357	0.39%	0.045%
40	13.492	1763	1769	1776	rBV2	25134	42072	0.63%	0.072%
41	13.580	1776	1784	1791	rBV5	34824	67713	1.01%	0.115%
42	13.780	1813	1818	1826	rBV10	6037	12794	0.19%	0.022%
43	13.957	1842	1848	1850	rBV7	6060	10721	0.16%	0.018%
44	14.010	1850	1857	1866	rVV	2497483	3396622	50.84%	5.779%
45	14.116	1872	1875	1881	rVB8	8156	13354	0.20%	0.023%
46	14.280	1894	1903	1913	rBV	2777827	4121789	61.70%	7.012%
47	14.357	1913	1916	1924	rVB9	7560	17965	0.27%	0.031%
48	14.586	1947	1955	1961	rBV	1300200	1984763	29.71%	3.377%
49	14.633	1961	1963	1969	rVB6	23645	31055	0.46%	0.053%
50	14.798	1986	1991	2003	rBV2	90413	239836	3.59%	0.408%
51	14.992	2022	2024	2031	rVB8	7294	14529	0.22%	0.025%
52	15.386	2087	2091	2094	rBV5	6060	8952	0.13%	0.015%
53	15.580	2116	2124	2138	rBV	3655604	5336684	79.88%	9.079%
54	15.698	2138	2144	2157	rVV	1095908	1621424	24.27%	2.758%
55	15.816	2161	2164	2170	rVB3	16896	28057	0.42%	0.048%
56	15.904	2175	2179	2184	rVB3	15723	22779	0.34%	0.039%
57	15.980	2184	2192	2198	rBV2	56460	98614	1.48%	0.168%
58	16.151	2216	2221	2224	rVB7	5598	6863	0.10%	0.012%
59	16.239	2231	2236	2239	rBV3	8861	12131	0.18%	0.021%
60	16.363	2253	2257	2262	rVB6	14276	21089	0.32%	0.036%
61	16.527	2282	2285	2289	rVB5	5826	6802	0.10%	0.012%
62	16.739	2319	2321	2327	rVB7	5256	6802	0.10%	0.012%
63	16.839	2333	2338	2351	rBV	50999	87111	1.30%	0.148%
64	17.016	2364	2368	2372	rVB6	7280	10671	0.16%	0.018%
65	17.333	2416	2422	2432	rBV	1604600	2271156	34.00%	3.864%
66	17.433	2432	2439	2452	rVV	4246450	5942520	88.95%	10.110%
67	17.533	2454	2456	2462	rVV6	18470	34296	0.51%	0.058%
68	17.604	2465	2468	2477	rVB9	13226	27027	0.40%	0.046%
69	18.010	2533	2537	2541	rVB7	11795	16789	0.25%	0.029%
70	18.239	2570	2576	2583	rBV	84968	126273	1.89%	0.215%
71	18.327	2587	2591	2593	rVB3	6734	9162	0.14%	0.016%
72	18.451	2606	2612	2616	rBV8	4446	9257	0.14%	0.016%
73	18.727	2657	2659	2664	rVB6	7041	7007	0.10%	0.012%
74	18.980	2699	2702	2707	rBV6	7682	12671	0.19%	0.022%
75	19.292	2751	2755	2761	rVB2	52719	71264	1.07%	0.121%
76	19.362	2761	2767	2772	rBV	48120	76686	1.15%	0.130%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044387.D
Acq On : 28 Feb 2024 04:04
Operator : MA/JU
Sample : P1501-16
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

77	19.521	2790	2794	2799	rBV4	41866	54587	0.82%	0.093%
78	19.680	2817	2821	2823	rBV4	20454	26992	0.40%	0.046%
79	19.727	2823	2829	2838	rVV	5054938	6680598	100.00%	11.365%
80	21.256	3087	3089	3097	rVB5	47950	64446	0.96%	0.110%
81	21.527	3130	3135	3144	rBV	1758458	2276296	34.07%	3.873%
82	23.792	3512	3520	3532	rBV	3351217	6597864	98.76%	11.225%
83	23.944	3540	3546	3557	rVB	1160378	2476794	37.07%	4.214%




Sum of corrected areas: 58780219

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044387.D
Acq On : 28 Feb 2024 04:04
Operator : MA/JU
Sample : P1501-16
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

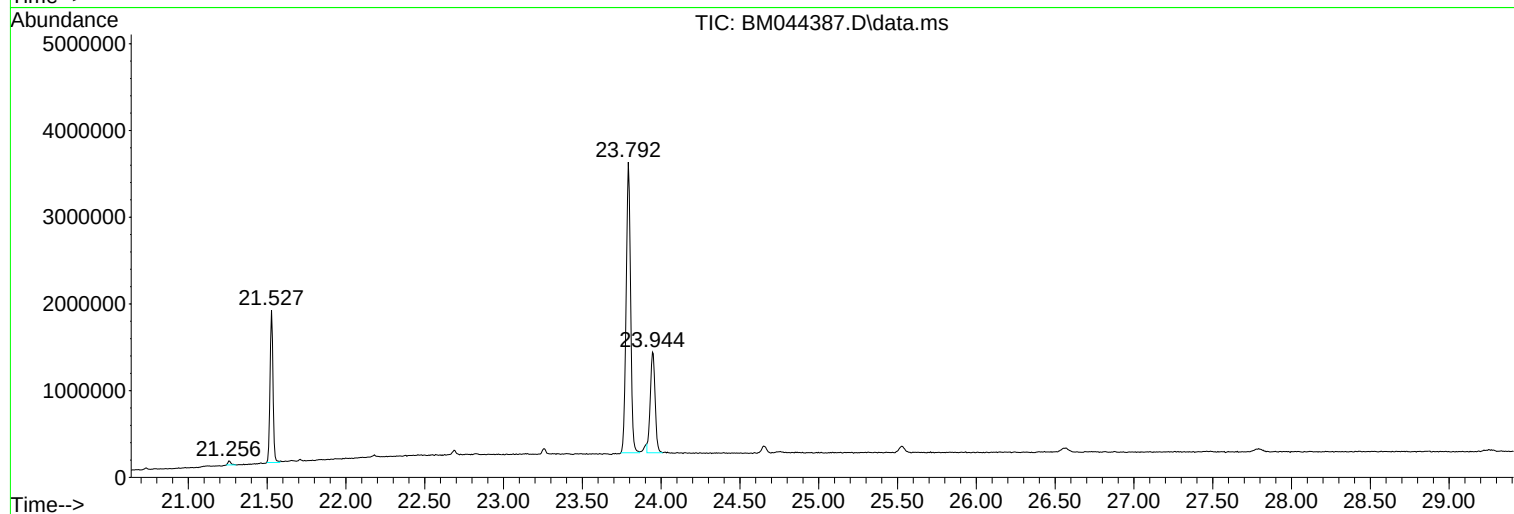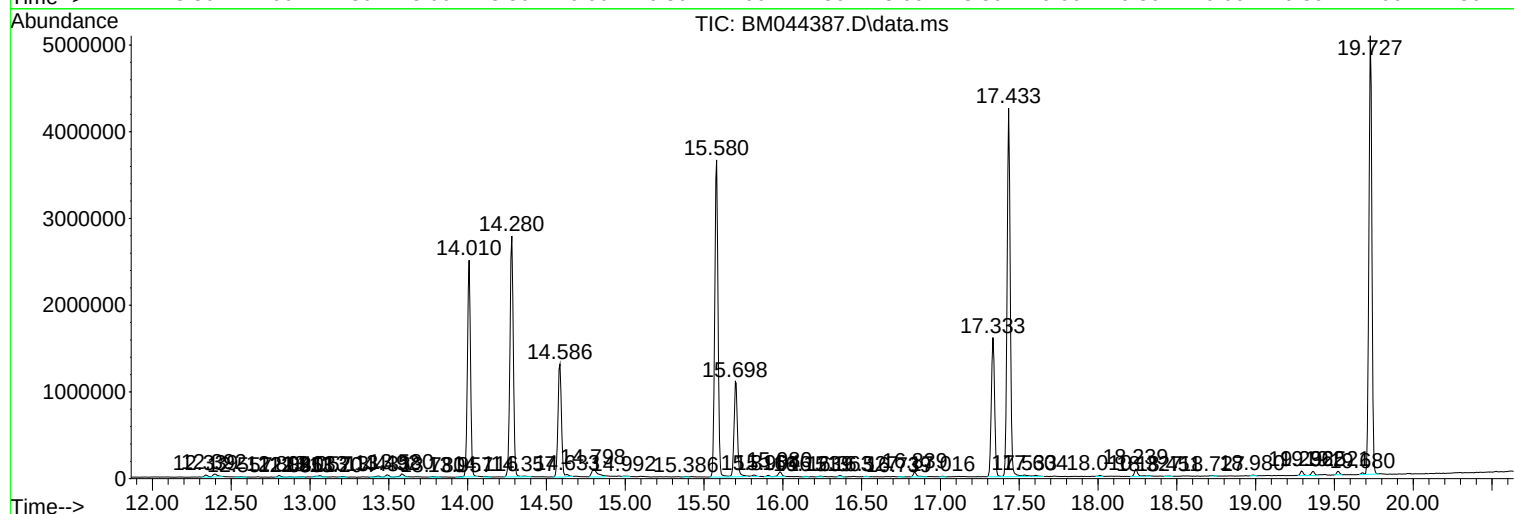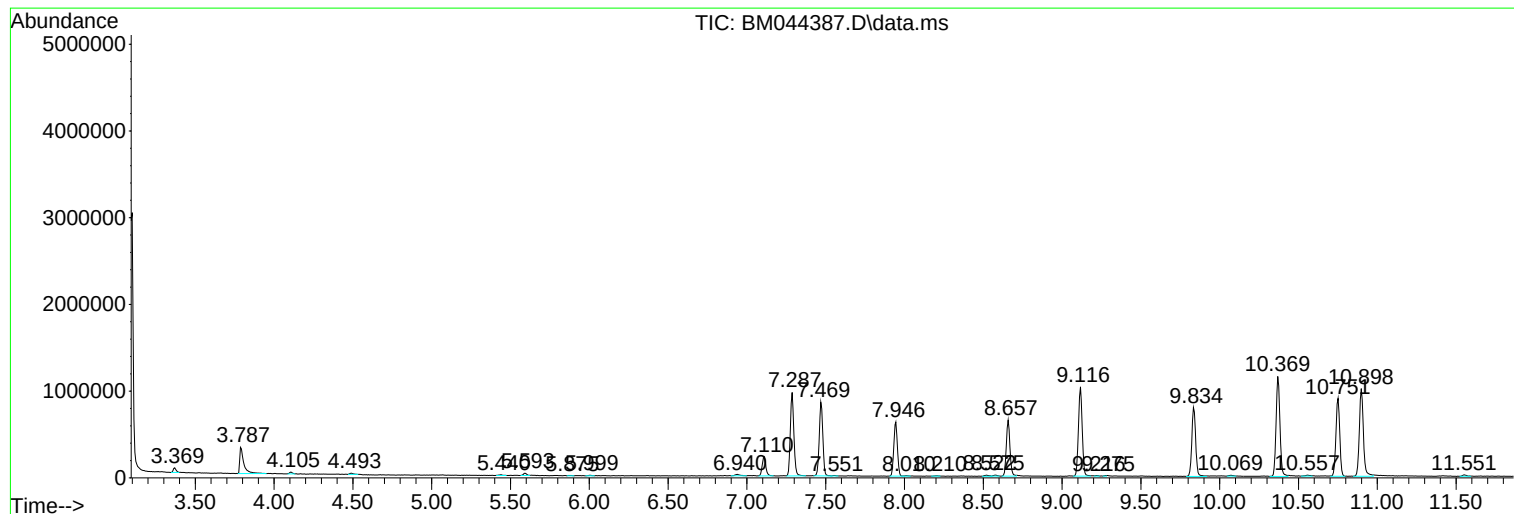

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044387.D
Acq On : 28 Feb 2024 04:04
Operator : MA/JU
Sample : P1501-16
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044387.D
Acq On : 28 Feb 2024 04:04
Operator : MA/JU
Sample : P1501-16
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E10A3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------