

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044392.D
 Acq On : 28 Feb 2024 07:43
 Operator : MA/JU
 Sample : PB159253BL
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK253

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044392.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	44	47	54	rBV	81185	113487	2.50%	0.217%
2	3.781	115	118	136	rBV	959653	1510601	33.22%	2.888%
3	4.110	170	174	179	rVB3	15649	22192	0.49%	0.042%
4	7.110	677	684	695	rBV	994219	1558337	34.27%	2.979%
5	7.287	708	714	728	rVB	866443	1337526	29.42%	2.557%
6	7.469	738	745	754	rBV	1028284	1595126	35.08%	3.050%
7	7.945	819	826	835	rVB	791736	1243414	27.35%	2.377%
8	8.657	937	947	957	rBV	1165152	1892483	41.62%	3.618%
9	9.116	1015	1025	1041	rBV	888266	1502505	33.04%	2.873%
10	9.833	1140	1147	1158	rBV	702595	1196775	26.32%	2.288%
11	10.369	1230	1238	1255	rBV	1066545	1827861	40.20%	3.495%
12	10.751	1295	1303	1313	rVB	1064374	1809834	39.80%	3.460%
13	10.898	1320	1328	1356	rBV	1049794	1971506	43.36%	3.769%
14	12.345	1567	1574	1581	rVB2	19365	35838	0.79%	0.069%
15	13.492	1763	1769	1773	rBV2	20860	32506	0.71%	0.062%
16	14.010	1850	1857	1866	rBV	1797314	2510376	55.21%	4.800%
17	14.280	1894	1903	1912	rBV	2152979	3218653	70.79%	6.154%
18	14.586	1948	1955	1965	rVV	1504790	2237874	49.22%	4.279%
19	14.792	1984	1990	2010	rBV	414427	1065569	23.44%	2.037%
20	15.580	2116	2124	2137	rBV	2662569	3878584	85.30%	7.415%
21	15.704	2139	2145	2160	rVV	704584	1029956	22.65%	1.969%
22	15.815	2161	2164	2170	rVB4	12612	21491	0.47%	0.041%
23	16.368	2253	2258	2264	rVB8	9752	16822	0.37%	0.032%
24	17.121	2382	2386	2392	rBV5	4769	8336	0.18%	0.016%
25	17.333	2415	2422	2431	rBV	1811882	2540791	55.88%	4.858%
26	17.433	2432	2439	2455	rVV	2951459	4126479	90.75%	7.889%
27	17.580	2462	2464	2469	rVB5	3868	4965	0.11%	0.009%
28	18.251	2573	2578	2581	rBV5	7939	13191	0.29%	0.025%
29	19.292	2751	2755	2760	rBV2	32360	45092	0.99%	0.086%
30	19.362	2762	2767	2772	rBV	30238	48868	1.07%	0.093%
31	19.521	2792	2794	2797	rBV4	4760	5673	0.12%	0.011%
32	19.680	2819	2821	2823	rBV2	6948	6795	0.15%	0.013%
33	19.727	2823	2829	2840	rVV	3262404	4546864	100.00%	8.693%
34	21.533	3130	3136	3146	rBV	1742251	2439360	53.65%	4.664%
35	23.791	3513	3520	3532	rBV2	2108592	4290871	94.37%	8.204%
36	23.950	3541	3547	3563	rVB	1211629	2598272	57.14%	4.968%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044392.D
Acq On : 28 Feb 2024 07:43
Operator : MA/JU
Sample : PB159253BL
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK253

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 52304873

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044392.D
Acq On : 28 Feb 2024 07:43
Operator : MA/JU
Sample : PB159253BL
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK253

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

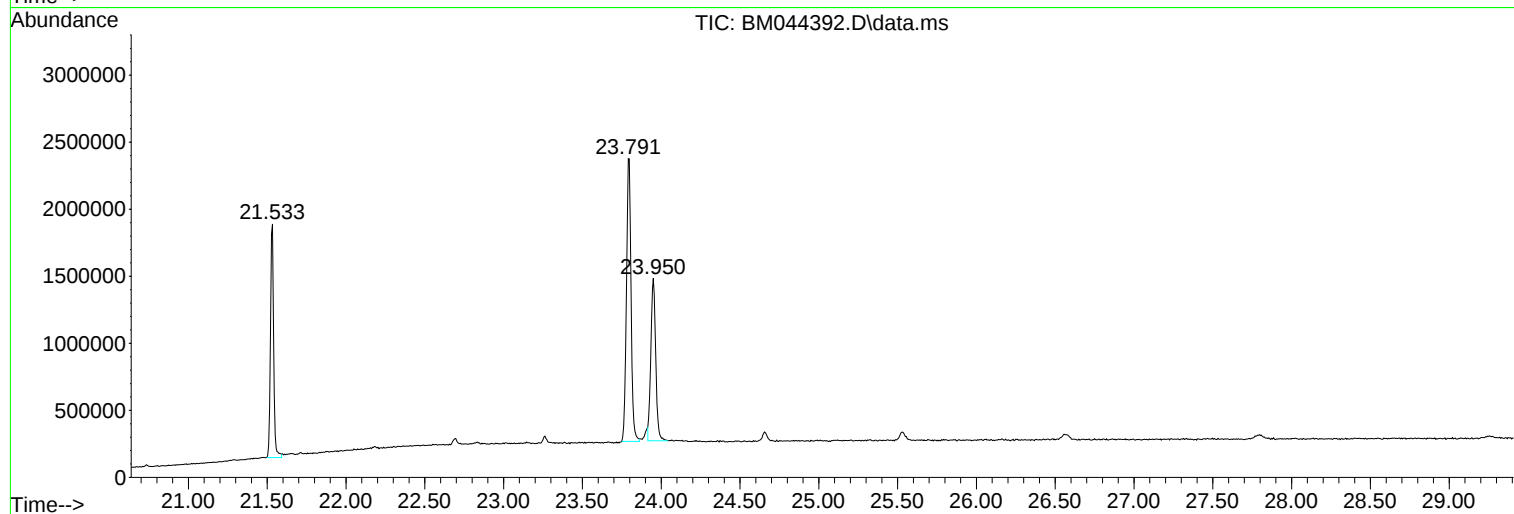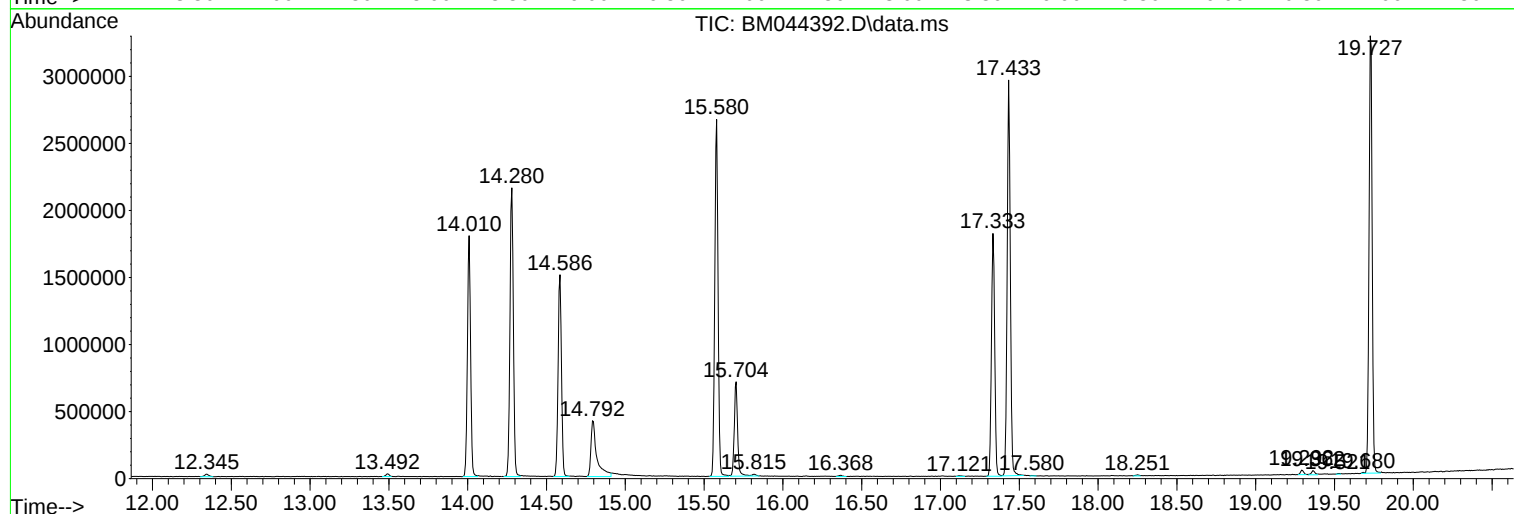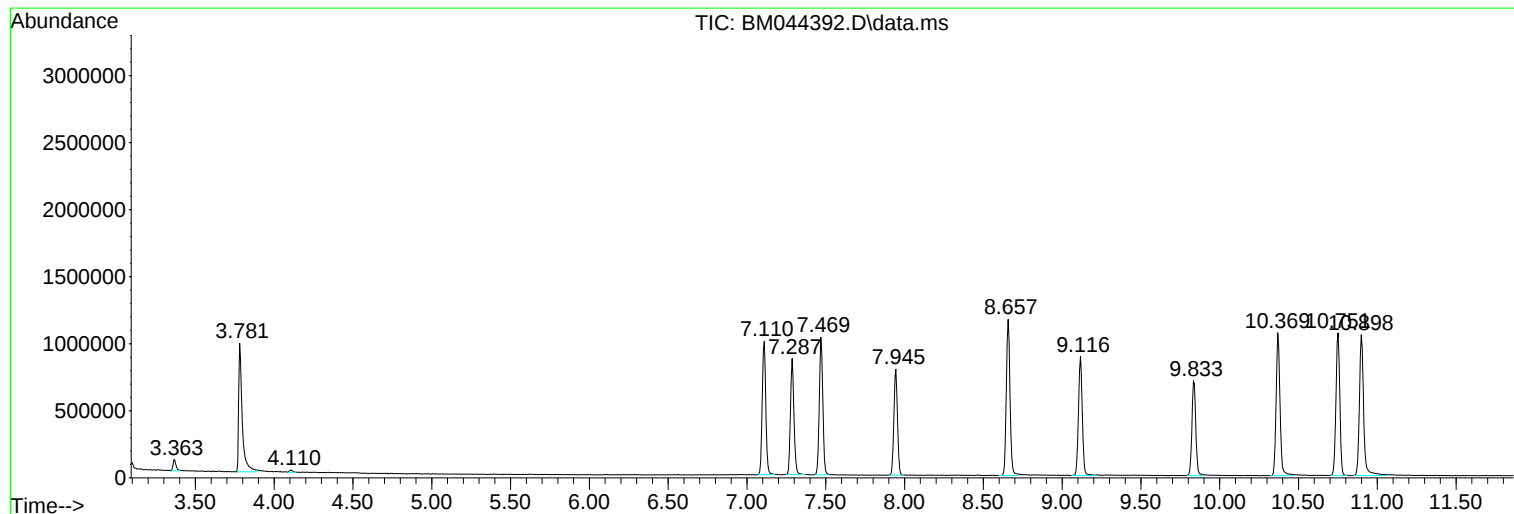

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044392.D
Acq On : 28 Feb 2024 07:43
Operator : MA/JU
Sample : PB159253BL
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK253

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044392.D
Acq On : 28 Feb 2024 07:43
Operator : MA/JU
Sample : PB159253BL
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK253

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc