

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044394.D
 Acq On : 28 Feb 2024 08:55
 Operator : MA/JU
 Sample : P1508-04
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH402

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	44	48	52	rBV	60090	75181	1.10%	0.124%
2	3.799	117	121	138	rBV	101296	206324	3.01%	0.340%
3	4.110	170	174	180	rVB2	14973	21470	0.31%	0.035%
4	7.110	677	684	694	rVV	256447	423556	6.17%	0.697%
5	7.287	708	714	724	rBV	1179149	1838963	26.80%	3.027%
6	7.469	738	745	755	rBV	1035143	1644588	23.97%	2.707%
7	7.945	819	826	833	rBV	715436	1110103	16.18%	1.827%
8	8.657	941	947	957	rBV	760716	1224903	17.85%	2.016%
9	9.116	1017	1025	1034	rBV	1248234	2088976	30.45%	3.439%
10	9.281	1051	1053	1059	rVB7	4239	6931	0.10%	0.011%
11	9.839	1139	1148	1161	rBV	963695	1662990	24.24%	2.737%
12	10.369	1230	1238	1253	rBV	1358129	2342790	34.15%	3.856%
13	10.751	1295	1303	1311	rBV	997518	1661957	24.22%	2.736%
14	10.898	1321	1328	1351	rBV	858656	1582409	23.06%	2.605%
15	12.345	1566	1574	1579	rBV2	27987	48801	0.71%	0.080%
16	13.492	1763	1769	1775	rBV4	13889	23374	0.34%	0.038%
17	14.010	1850	1857	1867	rBV	2629061	3650559	53.21%	6.009%
18	14.280	1895	1903	1915	rBV2	3049306	4548666	66.30%	7.487%
19	14.586	1947	1955	1963	rBV	1462260	2143206	31.24%	3.528%
20	14.810	1986	1993	2015	rBV3	58021	235109	3.43%	0.387%
21	15.580	2116	2124	2138	rBV	4030166	5647997	82.32%	9.297%
22	15.704	2138	2145	2160	rVV	1150335	1648078	24.02%	2.713%
23	15.816	2160	2164	2172	rVB3	20576	41358	0.60%	0.068%
24	16.145	2214	2220	2226	rBV7	4109	7305	0.11%	0.012%
25	16.363	2254	2257	2262	rVB3	11707	17812	0.26%	0.029%
26	17.015	2363	2368	2372	rVB4	6780	7965	0.12%	0.013%
27	17.110	2380	2384	2387	rBV6	7276	10472	0.15%	0.017%
28	17.333	2416	2422	2432	rBV	1690671	2401231	35.00%	3.953%
29	17.433	2432	2439	2461	rVV	4167195	6164194	89.84%	10.147%
30	18.245	2572	2577	2582	rBV3	33963	50812	0.74%	0.084%
31	19.298	2751	2756	2760	rBV3	49806	68066	0.99%	0.112%
32	19.368	2762	2768	2775	rVV	45333	72087	1.05%	0.119%
33	19.439	2777	2780	2785	rVB7	7543	13753	0.20%	0.023%
34	19.527	2791	2795	2801	rBV6	23629	35056	0.51%	0.058%
35	19.680	2818	2821	2823	rBV3	18907	20407	0.30%	0.034%
36	19.733	2823	2830	2838	rVV	5079454	6861004	100.00%	11.294%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044394.D
Acq On : 28 Feb 2024 08:55
Operator : MA/JU
Sample : P1508-04
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH402

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	20.733	2998	3000	3005	rBV6	14418	17591	0.26%	0.029%
38	21.462	3121	3124	3128	rBV	52115	61027	0.89%	0.100%
39	21.533	3130	3136	3146	rBV	1662565	2295629	33.46%	3.779%
40	23.797	3513	3521	3535	rBV2	3111142	6401674	93.31%	10.537%
41	23.950	3541	3547	3561	rVB	1116800	2367096	34.50%	3.896%




Sum of corrected areas: 60751470

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044394.D
Acq On : 28 Feb 2024 08:55
Operator : MA/JU
Sample : P1508-04
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH402

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

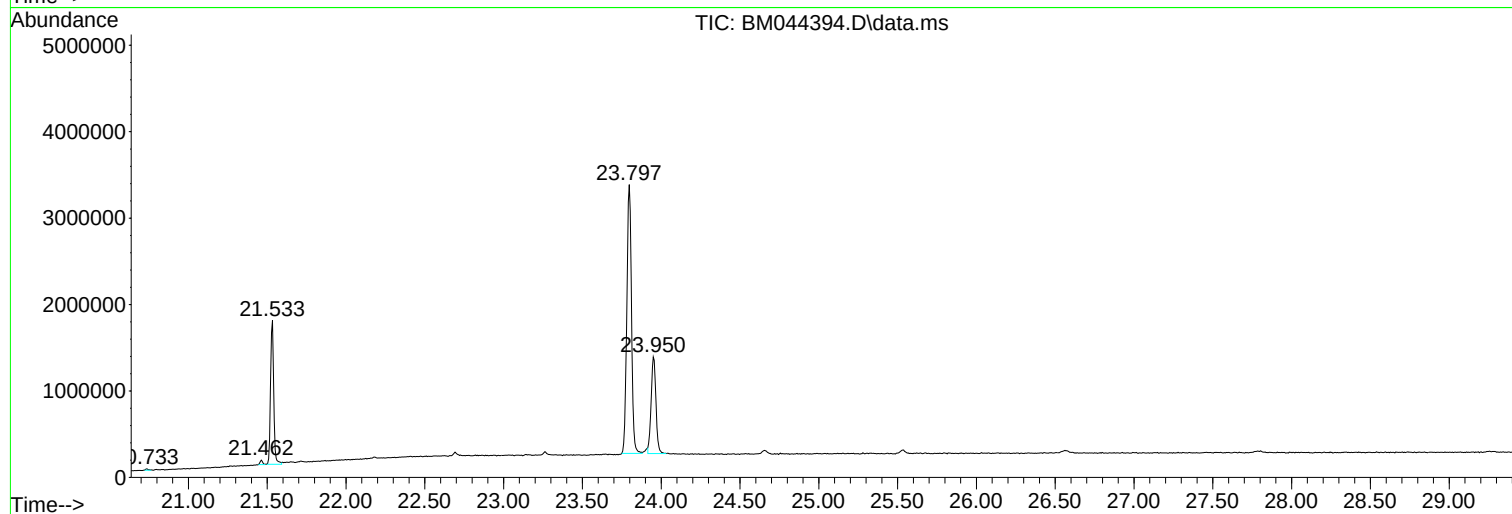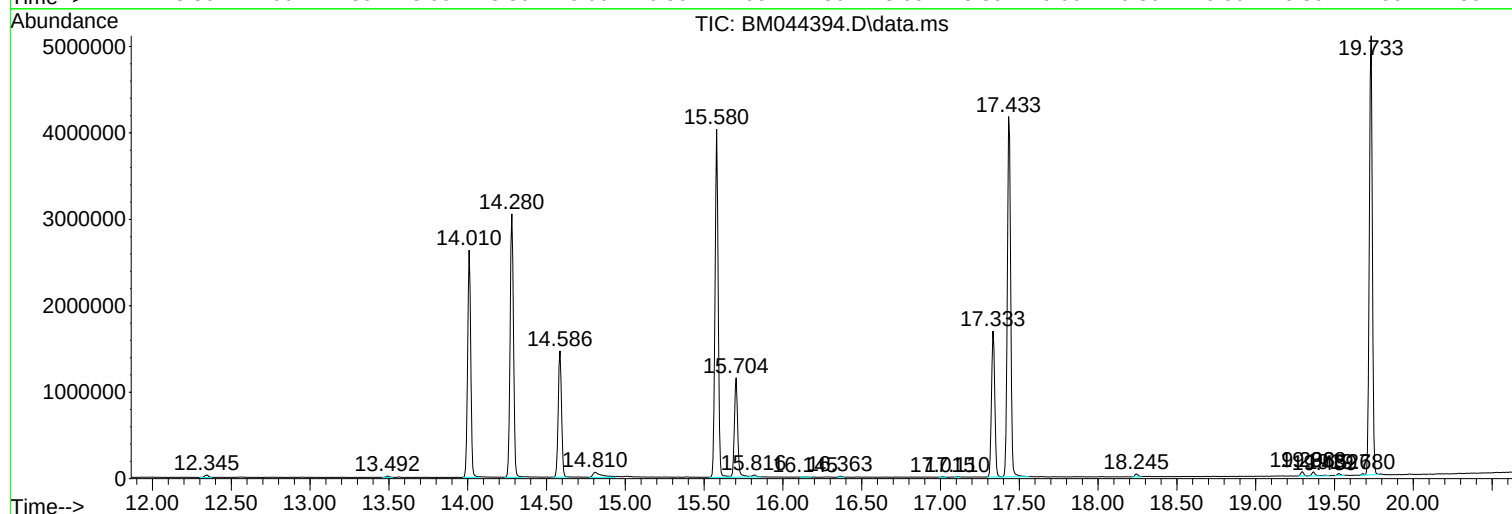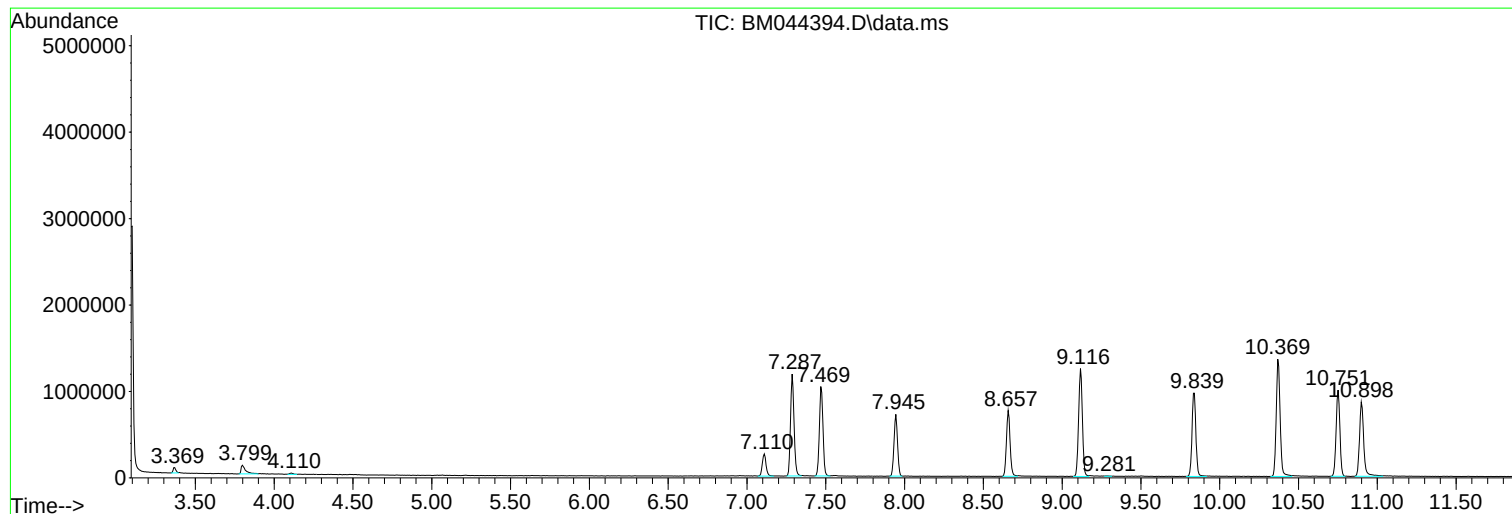

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044394.D
Acq On : 28 Feb 2024 08:55
Operator : MA/JU
Sample : P1508-04
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH402

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044394.D
Acq On : 28 Feb 2024 08:55
Operator : MA/JU
Sample : P1508-04
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH402

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc