

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044396.D
 Acq On : 28 Feb 2024 10:09
 Operator : MA/JU
 Sample : P1508-09
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH409

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044396.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	44	47	56	rVB	56896	81301	1.25%	0.142%
2	3.793	116	120	135	rBV	221309	404930	6.21%	0.707%
3	4.105	171	173	177	rVB2	13982	17453	0.27%	0.030%
4	7.110	677	684	693	rBV	223748	368821	5.66%	0.644%
5	7.287	707	714	730	rBV	994127	1586434	24.34%	2.771%
6	7.469	738	745	755	rBV	898650	1404200	21.54%	2.452%
7	7.557	758	760	765	rVB6	6208	7353	0.11%	0.013%
8	7.945	819	826	833	rBV	692093	1081335	16.59%	1.888%
9	8.657	940	947	958	rBV	655363	1066607	16.36%	1.863%
10	9.116	1017	1025	1037	rBV	1090455	1789353	27.45%	3.125%
11	9.504	1087	1091	1096	rVB7	5161	8372	0.13%	0.015%
12	9.834	1140	1147	1162	rBV	829504	1402746	21.52%	2.450%
13	10.369	1231	1238	1257	rBV	1161626	2011929	30.87%	3.514%
14	10.751	1296	1303	1311	rBV	964200	1623969	24.91%	2.836%
15	10.898	1320	1328	1345	rBV	1013592	1883664	28.90%	3.290%
16	11.575	1439	1443	1451	rBV10	5172	10716	0.16%	0.019%
17	12.180	1542	1546	1552	rVB7	4146	7194	0.11%	0.013%
18	12.345	1569	1574	1582	rVB	23369	43263	0.66%	0.076%
19	12.951	1672	1677	1680	rBV5	7881	11919	0.18%	0.021%
20	13.204	1716	1720	1726	rVB8	5324	9128	0.14%	0.016%
21	13.416	1753	1756	1763	rVB7	7254	11406	0.17%	0.020%
22	13.492	1763	1769	1775	rBV2	24502	39358	0.60%	0.069%
23	14.010	1849	1857	1871	rBV	2366833	3294797	50.55%	5.754%
24	14.280	1896	1903	1920	rBV	2818854	4084401	62.66%	7.133%
25	14.586	1948	1955	1964	rBV	1407011	2078394	31.88%	3.630%
26	14.810	1986	1993	2005	rBV2	54186	181963	2.79%	0.318%
27	15.004	2021	2026	2036	rVB2	8421	22619	0.35%	0.040%
28	15.386	2086	2091	2095	rBV	20388	29529	0.45%	0.052%
29	15.580	2117	2124	2138	rBV	3546304	5216730	80.03%	9.110%
30	15.704	2138	2145	2156	rVV	1078733	1539787	23.62%	2.689%
31	15.821	2161	2165	2171	rVB2	18184	30889	0.47%	0.054%
32	16.151	2215	2221	2224	rBV6	5604	9083	0.14%	0.016%
33	16.368	2254	2258	2262	rVB6	10845	15046	0.23%	0.026%
34	16.751	2318	2323	2329	rBV8	4696	8276	0.13%	0.014%
35	17.015	2365	2368	2371	rVB5	5649	7124	0.11%	0.012%
36	17.333	2415	2422	2432	rBV	1627023	2324999	35.67%	4.060%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044396.D
 Acq On : 28 Feb 2024 10:09
 Operator : MA/JU
 Sample : P1508-09
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH409

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

37	17.433	2432	2439	2461	rVV	4156728	5960006	91.43%	10.409%
38	17.633	2470	2473	2481	rBV6	6116	10624	0.16%	0.019%
39	18.021	2535	2539	2543	rVB6	5937	8283	0.13%	0.014%
40	18.245	2572	2577	2582	rBV	79031	114729	1.76%	0.200%
41	19.292	2751	2755	2761	rBV3	47073	66470	1.02%	0.116%
42	19.362	2763	2767	2772	rVV	39676	54492	0.84%	0.095%
43	19.439	2777	2780	2784	rVB6	6480	10530	0.16%	0.018%
44	19.527	2791	2795	2801	rBV4	32869	43849	0.67%	0.077%
45	19.680	2818	2821	2824	rBV4	21404	23140	0.35%	0.040%
46	19.733	2824	2830	2839	rVV	4841576	6518474	100.00%	11.384%
47	20.733	2998	3000	3003	rBV3	18847	18468	0.28%	0.032%
48	21.262	3087	3090	3099	rBV4	57476	93896	1.44%	0.164%
49	21.533	3131	3136	3146	rBV	1639561	2164597	33.21%	3.780%
50	23.797	3513	3521	3533	rBV2	3030162	6162274	94.54%	10.762%
51	23.950	3541	3547	3559	rVB	1077201	2295724	35.22%	4.009%




Sum of corrected areas: 57260644

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044396.D
Acq On : 28 Feb 2024 10:09
Operator : MA/JU
Sample : P1508-09
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH409

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

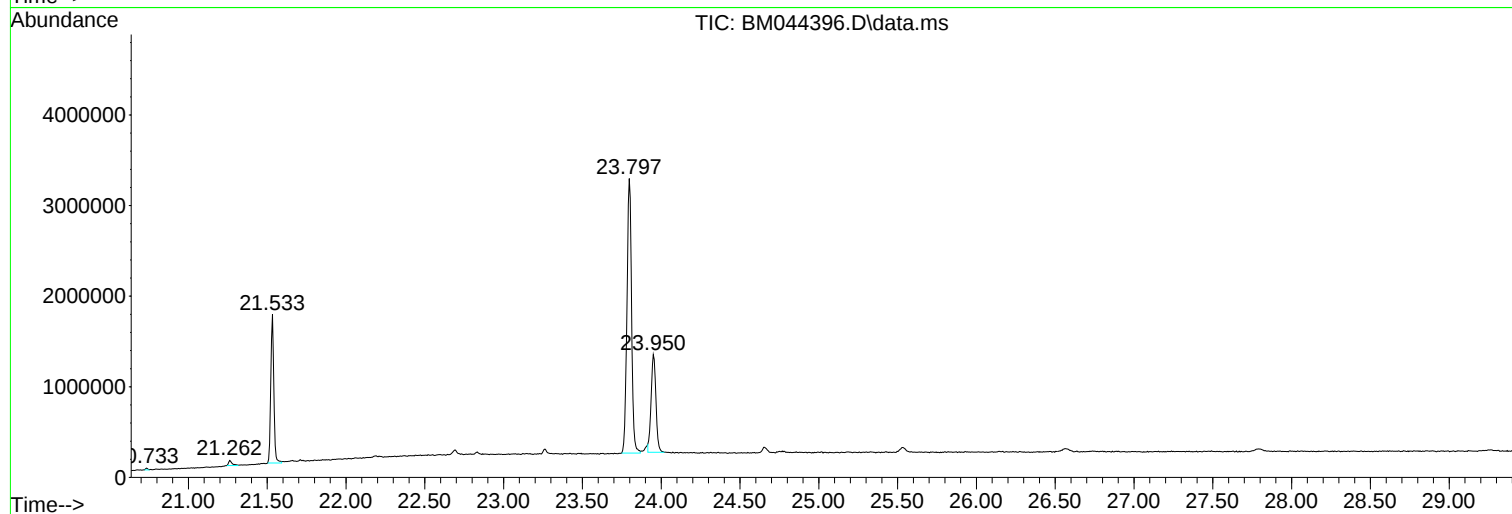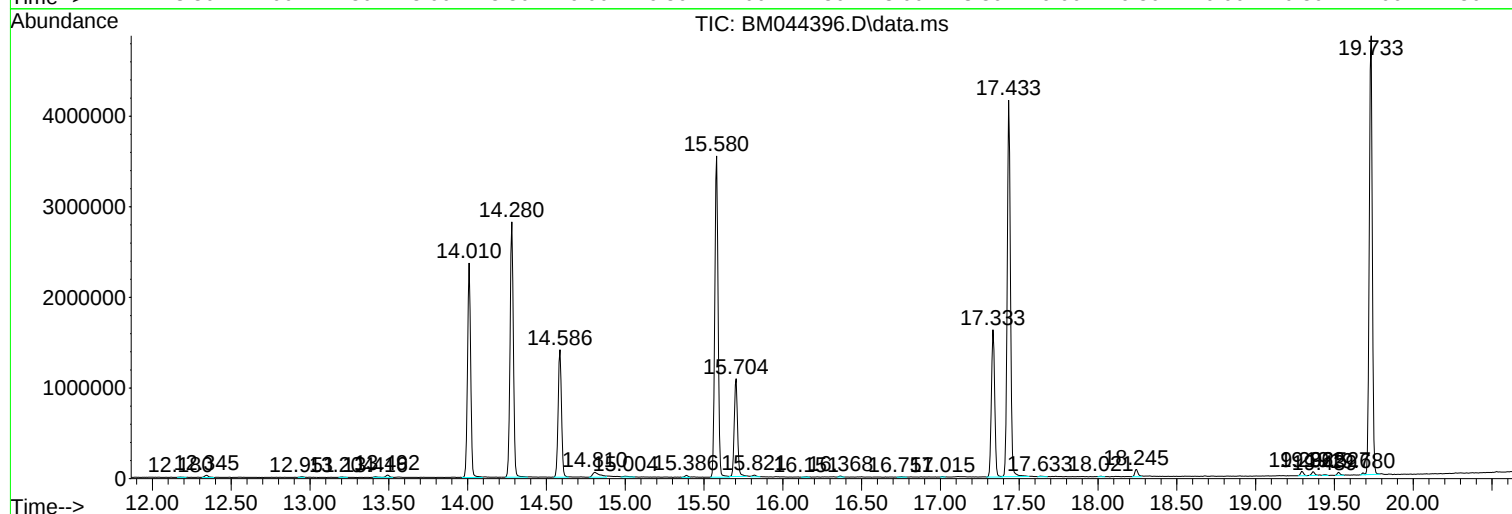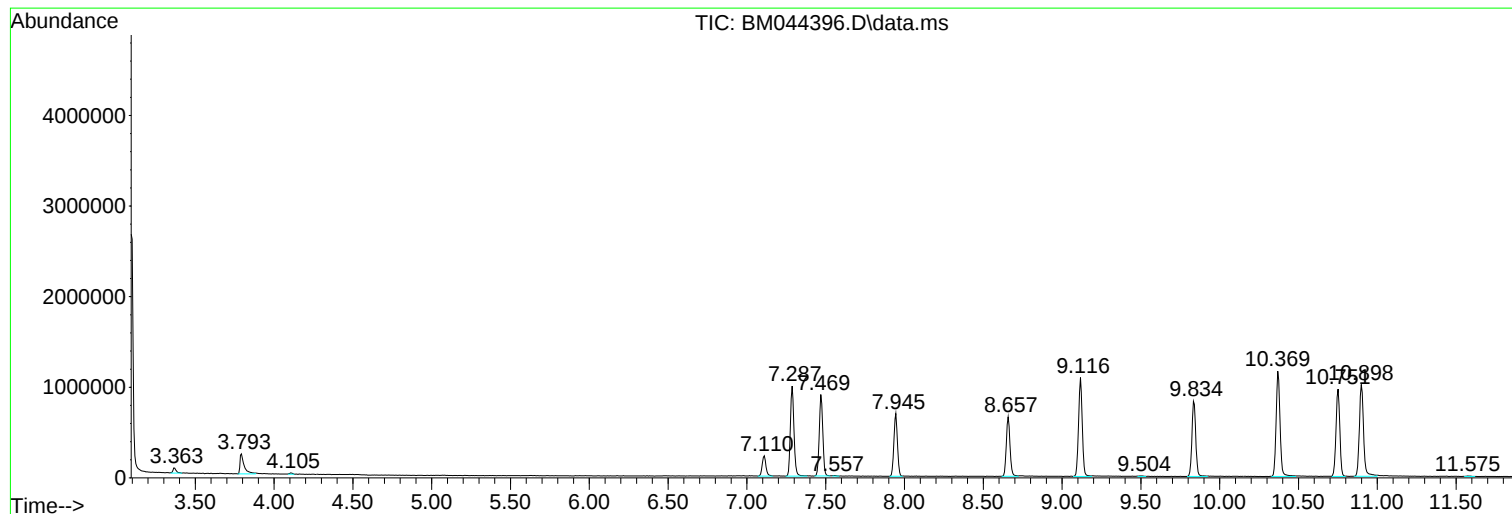

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044396.D
Acq On : 28 Feb 2024 10:09
Operator : MA/JU
Sample : P1508-09
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH409

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044396.D
Acq On : 28 Feb 2024 10:09
Operator : MA/JU
Sample : P1508-09
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH409

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc