

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044397.D
 Acq On : 28 Feb 2024 10:45
 Operator : MA/JU
 Sample : P1508-10
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH412

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044397.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	44	48	55	rVB	57532	77529	1.04%	0.119%
2	3.787	116	119	138	rBV	365961	635896	8.50%	0.974%
3	4.110	171	174	177	rVB	17214	20963	0.28%	0.032%
4	7.110	676	684	692	rBV	257327	423699	5.66%	0.649%
5	7.287	707	714	729	rBV	1098753	1732272	23.15%	2.652%
6	7.469	737	745	753	rBV	966081	1530024	20.45%	2.342%
7	7.945	819	826	834	rBV	723167	1151033	15.38%	1.762%
8	8.657	940	947	957	rBV	737150	1187039	15.86%	1.817%
9	9.116	1017	1025	1038	rBV	1197372	1969521	26.32%	3.015%
10	9.228	1040	1044	1049	rVB5	12624	22300	0.30%	0.034%
11	9.504	1087	1091	1095	rBV6	7097	10361	0.14%	0.016%
12	9.551	1095	1099	1103	rVV4	8390	11055	0.15%	0.017%
13	9.839	1139	1148	1157	rBV	907415	1568672	20.96%	2.402%
14	10.369	1228	1238	1247	rBV	1301837	2213179	29.57%	3.388%
15	10.751	1295	1303	1310	rBV	1067927	1771687	23.67%	2.712%
16	10.898	1321	1328	1342	rBV	1237745	2212822	29.57%	3.388%
17	11.586	1441	1445	1449	rVB7	7846	11859	0.16%	0.018%
18	12.186	1542	1547	1550	rVB7	6331	10189	0.14%	0.016%
19	12.339	1566	1573	1581	rBV2	26362	50203	0.67%	0.077%
20	13.416	1752	1756	1761	rBV4	10235	15655	0.21%	0.024%
21	13.492	1764	1769	1775	rVB3	17715	27205	0.36%	0.042%
22	14.010	1850	1857	1867	rBV	2582267	3619168	48.36%	5.541%
23	14.280	1896	1903	1911	rBV	3082097	4564700	61.00%	6.988%
24	14.486	1935	1938	1945	rVB5	15627	26743	0.36%	0.041%
25	14.586	1948	1955	1964	rBV	1527134	2295694	30.68%	3.515%
26	14.804	1986	1992	2004	rBV2	72498	221601	2.96%	0.339%
27	15.104	2039	2043	2048	rBV8	5252	7492	0.10%	0.011%
28	15.392	2085	2092	2094	rBV7	5514	9504	0.13%	0.015%
29	15.439	2094	2100	2108	rVB2	26170	42464	0.57%	0.065%
30	15.580	2116	2124	2132	rBV	4013910	5752821	76.87%	8.807%
31	15.704	2138	2145	2158	rBV	1257688	1777822	23.76%	2.722%
32	15.821	2162	2165	2168	rBV2	14295	20291	0.27%	0.031%
33	16.304	2241	2247	2254	rBV	37002	61744	0.83%	0.095%
34	16.368	2254	2258	2264	rVB4	15724	24748	0.33%	0.038%
35	16.815	2331	2334	2339	rVB7	6429	8326	0.11%	0.013%
36	17.015	2364	2368	2372	rVB6	6515	10208	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044397.D
 Acq On : 28 Feb 2024 10:45
 Operator : MA/JU
 Sample : P1508-10
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH412

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

37	17.104	2378	2383	2387	rBV2	38954	53914	0.72%	0.083%
38	17.151	2387	2391	2402	rVB9	12246	21328	0.29%	0.033%
39	17.333	2415	2422	2432	rBV	1848728	2639249	35.27%	4.040%
40	17.433	2432	2439	2451	rVV2	4578216	6680546	89.27%	10.227%
41	17.633	2471	2473	2479	rVB6	8624	13518	0.18%	0.021%
42	17.845	2506	2509	2514	rBV	31584	40484	0.54%	0.062%
43	18.015	2536	2538	2543	rVB5	7513	11868	0.16%	0.018%
44	18.245	2572	2577	2584	rBV	91646	140213	1.87%	0.215%
45	18.545	2624	2628	2631	rBV2	27356	34511	0.46%	0.053%
46	18.686	2648	2652	2654	rVB5	7440	9775	0.13%	0.015%
47	19.180	2732	2736	2741	rVB3	20115	27840	0.37%	0.043%
48	19.292	2751	2755	2760	rBV3	54313	81150	1.08%	0.124%
49	19.368	2763	2768	2772	rBV	50308	67842	0.91%	0.104%
50	19.439	2778	2780	2784	rVB5	9715	8636	0.12%	0.013%
51	19.527	2791	2795	2805	rBV5	36605	65142	0.87%	0.100%
52	19.680	2818	2821	2824	rBV2	26785	31124	0.42%	0.048%
53	19.733	2824	2830	2838	rVV	5591532	7483491	100.00%	11.457%
54	20.733	2998	3000	3006	rVB6	23595	26329	0.35%	0.040%
55	21.262	3086	3090	3095	rBV4	70867	117775	1.57%	0.180%
56	21.533	3130	3136	3149	rBV	1958932	2613711	34.93%	4.001%
57	23.797	3513	3521	3532	rBV2	3654247	7289061	97.40%	11.159%
58	23.950	3541	3547	3560	rVB	1312466	2766509	36.97%	4.235%




Sum of corrected areas: 65320505

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044397.D
Acq On : 28 Feb 2024 10:45
Operator : MA/JU
Sample : P1508-10
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH412

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

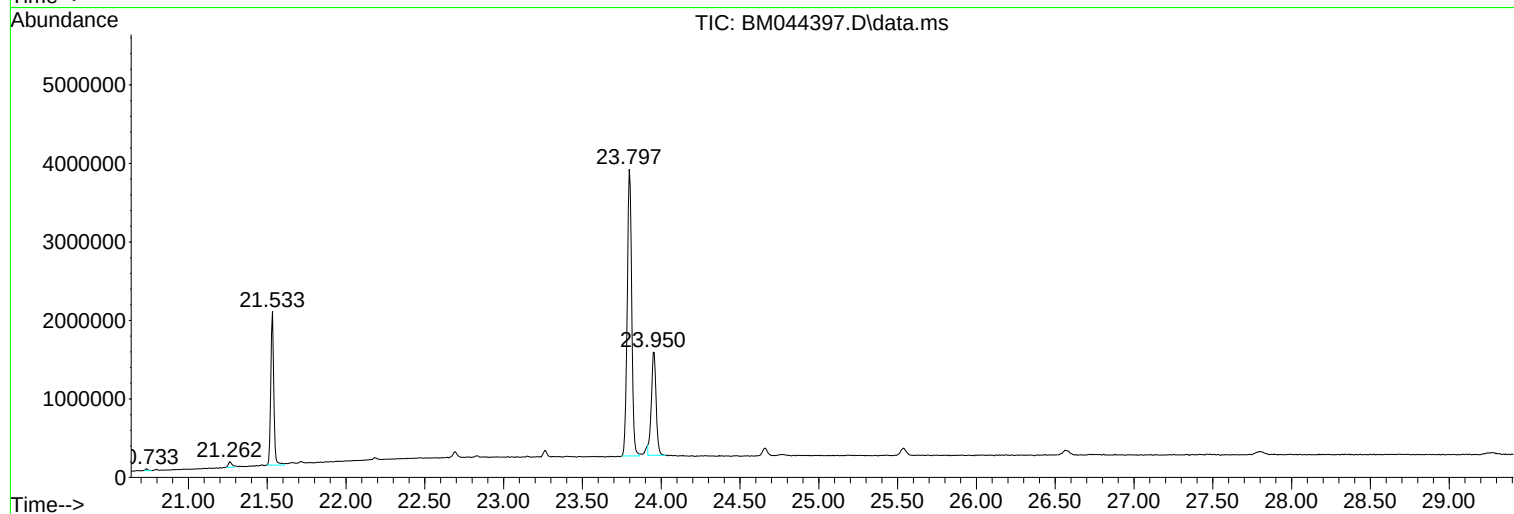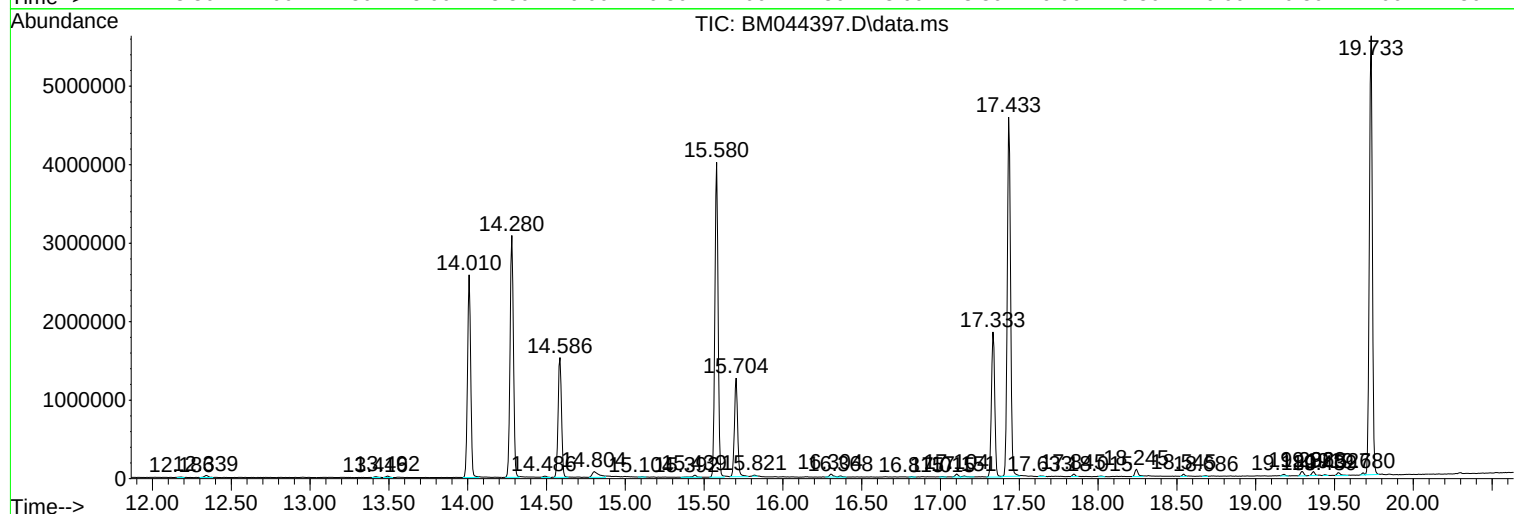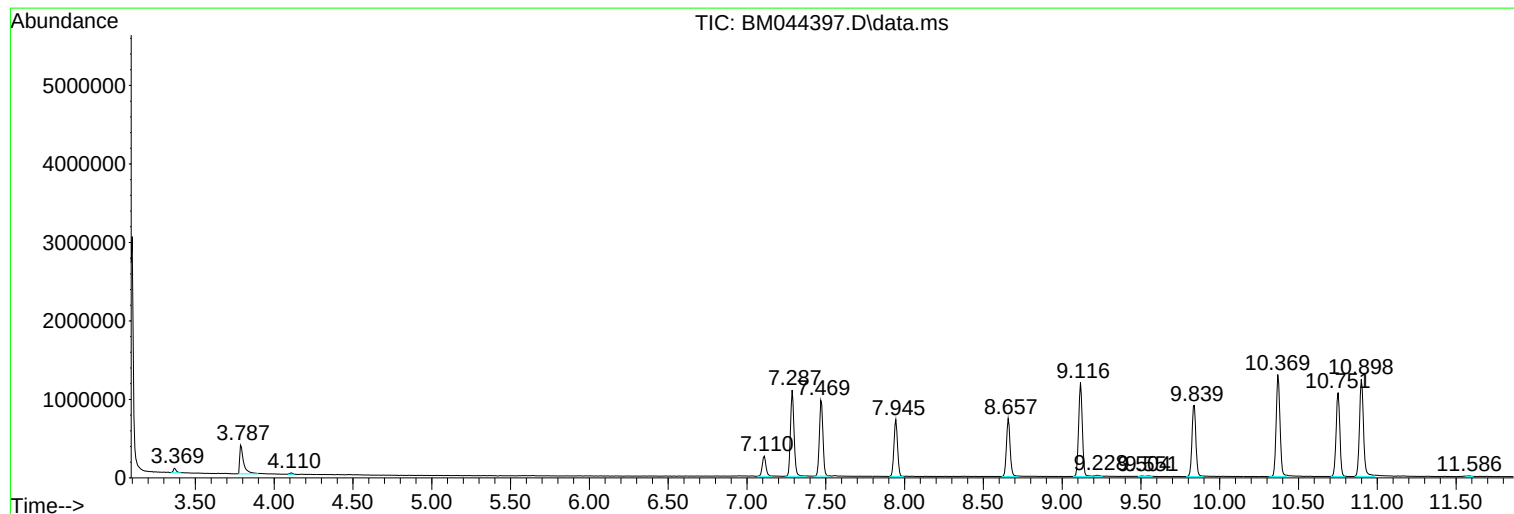

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044397.D
Acq On : 28 Feb 2024 10:45
Operator : MA/JU
Sample : P1508-10
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH412

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044397.D
Acq On : 28 Feb 2024 10:45
Operator : MA/JU
Sample : P1508-10
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH412

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------