

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
 Data File : BM044398.D
 Acq On : 28 Feb 2024 11:22
 Operator : MA/JU
 Sample : P1508-01
 Misc :
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3Z5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044398.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	44	48	55	rVB	58412	82324	1.19%	0.136%
2	3.787	116	119	141	rBV	310858	560972	8.14%	0.924%
3	4.110	171	174	179	rVB	13665	18128	0.26%	0.030%
4	7.110	677	684	693	rBV	224472	376190	5.46%	0.620%
5	7.287	707	714	727	rBV	1012393	1609637	23.35%	2.651%
6	7.469	738	745	754	rBV	902702	1428729	20.73%	2.353%
7	7.945	818	826	834	rBV	720859	1145021	16.61%	1.886%
8	8.657	940	947	959	rBV	672318	1102031	15.99%	1.815%
9	9.116	1016	1025	1034	rBV	1114389	1839254	26.68%	3.030%
10	9.228	1038	1044	1049	rVV7	8253	15552	0.23%	0.026%
11	9.833	1140	1147	1163	rBV	865480	1440983	20.90%	2.374%
12	10.369	1229	1238	1257	rBV	1221280	2086513	30.27%	3.437%
13	10.751	1290	1303	1312	rBV	1036562	1752512	25.42%	2.887%
14	10.898	1320	1328	1342	rBV	1118881	2012923	29.20%	3.316%
15	12.345	1568	1574	1581	rVB	23479	40810	0.59%	0.067%
16	13.492	1764	1769	1776	rBV	24074	39406	0.57%	0.065%
17	14.010	1850	1857	1874	rBV	2425654	3372717	48.92%	5.556%
18	14.280	1895	1903	1914	rBV	2860969	4244352	61.57%	6.991%
19	14.586	1947	1955	1966	rBV	1520719	2281204	33.09%	3.758%
20	14.810	1987	1993	2008	rBV2	51623	183705	2.66%	0.303%
21	15.580	2116	2124	2138	rBV	3712244	5368882	77.88%	8.844%
22	15.704	2138	2145	2160	rVV	1082543	1588845	23.05%	2.617%
23	15.821	2160	2165	2169	rVB4	17882	29078	0.42%	0.048%
24	16.368	2252	2258	2262	rBV6	10337	16608	0.24%	0.027%
25	17.333	2415	2422	2430	rBV	1840112	2577438	37.39%	4.246%
26	17.433	2432	2439	2454	rBV	4408791	6229097	90.36%	10.261%
27	18.021	2532	2539	2542	rVB8	3963	7351	0.11%	0.012%
28	18.239	2572	2576	2583	rBV5	22721	36520	0.53%	0.060%
29	19.239	2740	2746	2749	rBV6	4840	10580	0.15%	0.017%
30	19.292	2751	2755	2761	rBV2	50890	73745	1.07%	0.121%
31	19.362	2763	2767	2773	rVV	42347	62812	0.91%	0.103%
32	19.439	2778	2780	2785	rVB6	7187	10907	0.16%	0.018%
33	19.527	2791	2795	2800	rBV6	15976	23120	0.34%	0.038%
34	19.680	2818	2821	2823	rBV	21314	22719	0.33%	0.037%
35	19.733	2823	2830	2838	rVB	4975729	6893746	100.00%	11.355%
36	20.733	2998	3000	3005	rVB5	16689	18089	0.26%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044398.D
Acq On : 28 Feb 2024 11:22
Operator : MA/JU
Sample : P1508-01
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3Z5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Title : SVOA CALIBRATION

37	21.533	3130	3136	3148	rBV	1901796	2578980	37.41%	4.248%
38	23.797	3513	3521	3534	rBV2	3353221	6809487	98.78%	11.217%
39	23.950	3541	3547	3562	rVB	1294542	2717917	39.43%	4.477%




Sum of corrected areas: 60708884

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044398.D
Acq On : 28 Feb 2024 11:22
Operator : MA/JU
Sample : P1508-01
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3Z5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

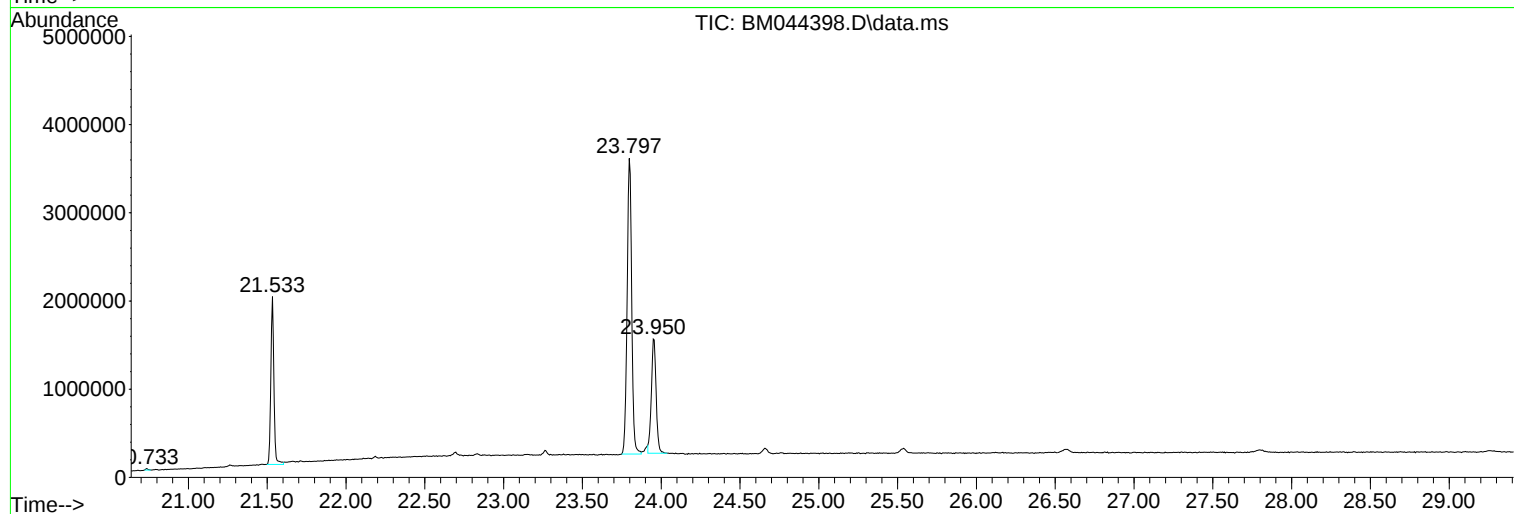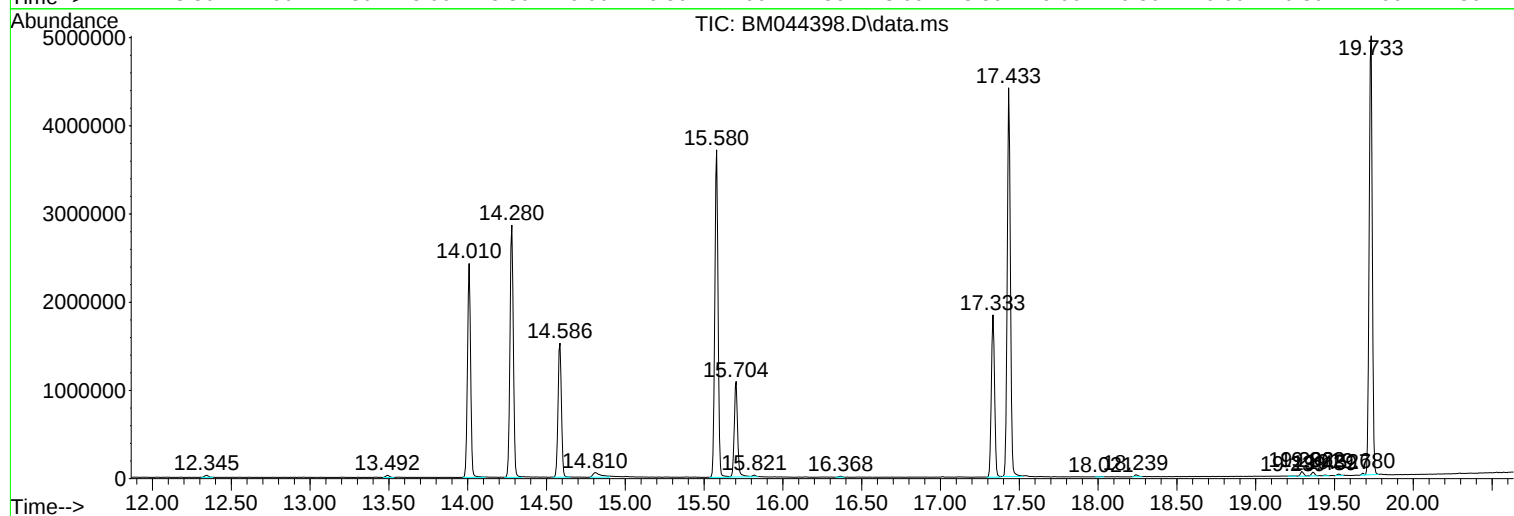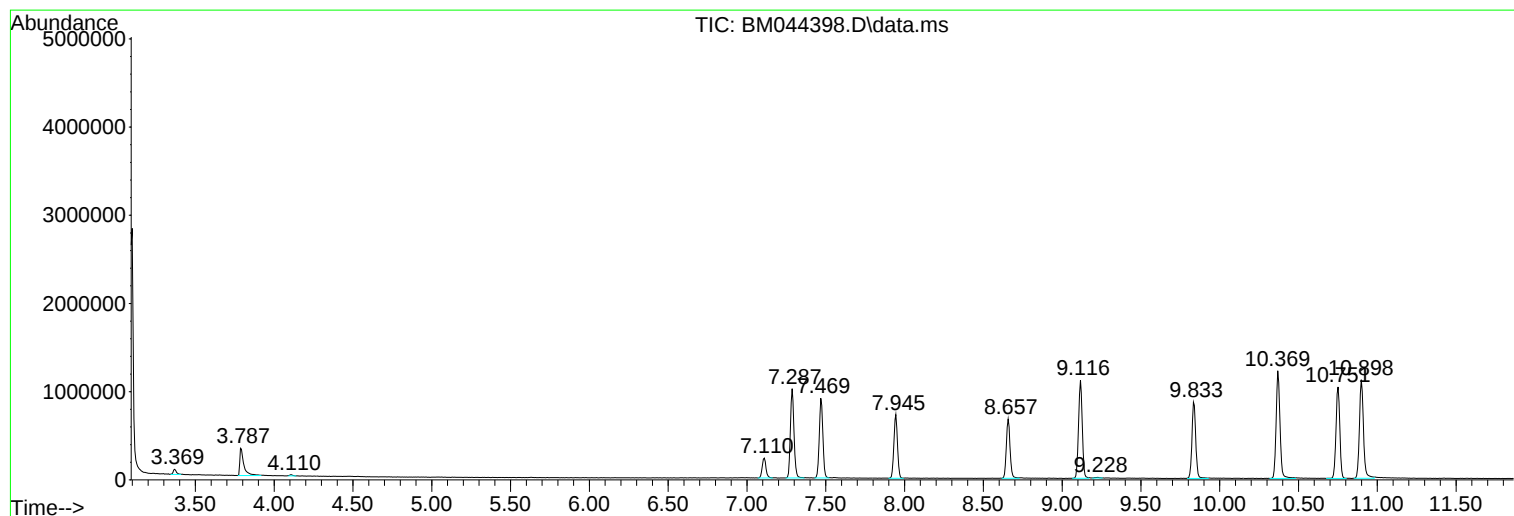

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044398.D
Acq On : 28 Feb 2024 11:22
Operator : MA/JU
Sample : P1508-01
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3Z5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022624\
Data File : BM044398.D
Acq On : 28 Feb 2024 11:22
Operator : MA/JU
Sample : P1508-01
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3Z5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022324.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc