


Data Path : Z:\HPCHEM1\BNA_M\Data\BM022715\
 Data File : BM000610.D
 Acq On : 27 Feb 2015 17:23
 Operator : TP/IZ
 Sample : DFTPP29
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP29

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM01.2-EPA-SIM-BM022715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 27 23:02:43 2015

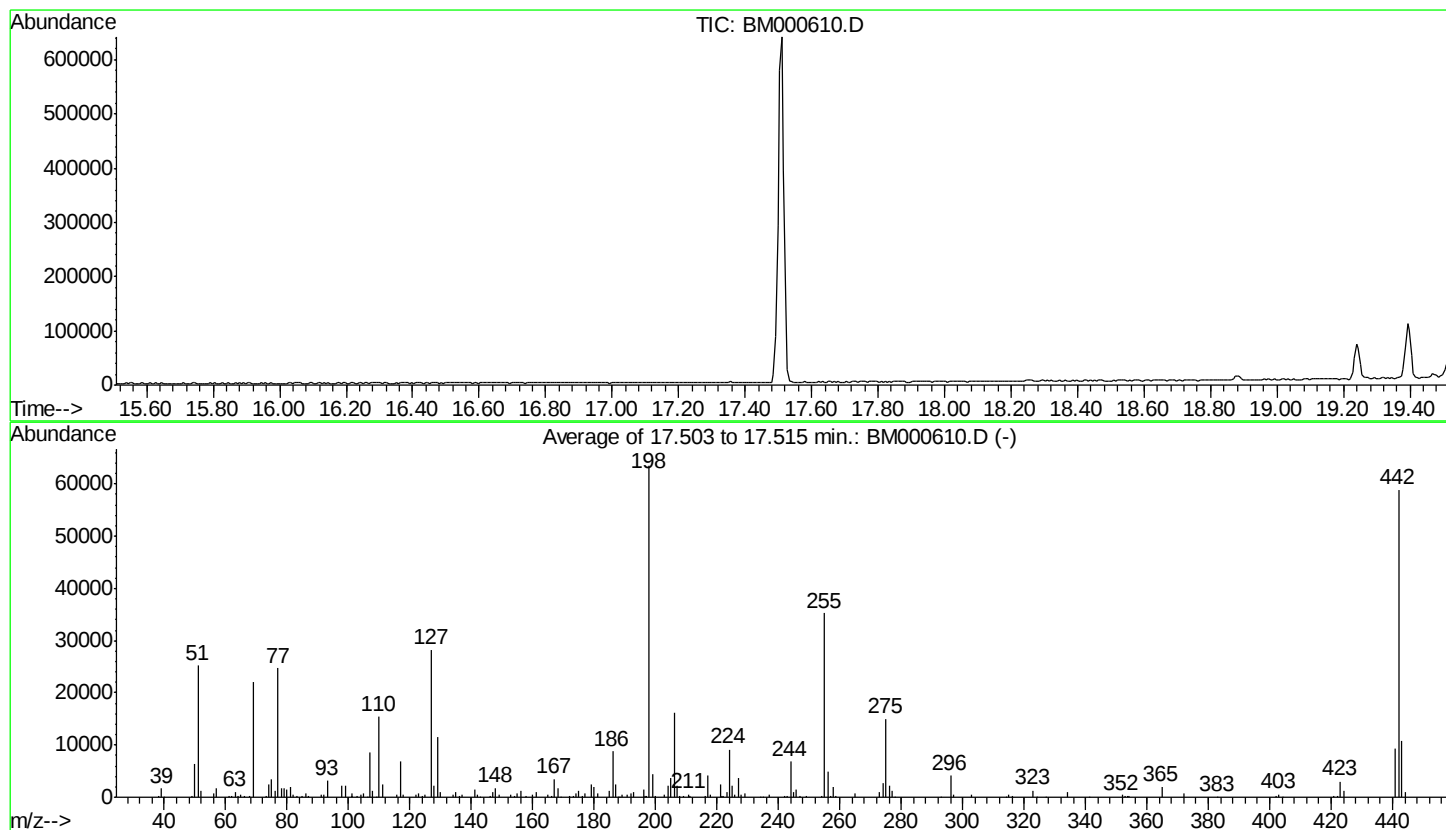

AutoFind: Scans 2519, 2520, 2521; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.8	25252	PASS
68	69	0.00	2	1.6	356	PASS
69	198	0.00	100	34.6	21979	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.5	28269	PASS
197	198	0.00	1	0.4	255	PASS
198	198	100	100	100.0	63520	PASS
199	198	5	9	6.8	4320	PASS
275	198	10	60	23.6	14997	PASS
365	198	1	100	3.1	1989	PASS
441	443	0.01	100	86.5	9303	PASS
442	198	50	100	92.8	58933	PASS
443	442	15	24	18.2	10753	PASS

m/z	Abundance
38.00	502.0
39.10	2097.0
40.10	532.0
44.00	2332.0
49.00	321.0
50.00	8119.0
51.10	31536.0
52.10	1495.0
56.00	1076.0
57.00	1993.0
61.00	499.0
62.10	389.0
63.00	1192.0
64.00	342.0
65.10	669.0
65.90	333.0
67.90	462.0
69.00	26672.0
73.00	785.0
74.10	3468.0
75.00	4095.0
76.10	1444.0
77.10	30320.0
78.10	2335.0
79.00	2379.0
80.00	1733.0
81.00	2795.0
82.00	629.0
83.00	455.0
85.00	465.0
86.00	629.0
86.90	485.0
90.90	448.0
92.10	779.0
93.00	3742.0
98.00	2723.0
99.00	2578.0
101.00	1086.0
103.00	336.0
104.00	827.0
104.90	1036.0
107.00	10079.0
108.00	1499.0
110.00	18912.0
111.00	2811.0
115.90	438.0
117.00	7711.0
118.00	541.0
122.00	707.0
123.00	832.0
123.90	616.0
125.00	466.0
127.10	32888.0
128.00	2463.0
129.00	12504.0
130.00	934.0
133.90	631.0
135.00	1133.0
136.10	470.0
136.90	645.0
141.00	1679.0
142.00	507.0
142.90	335.0
146.00	382.0
147.00	1181.0
148.00	1959.0
149.00	645.0
153.00	527.0
155.00	946.0
156.10	1499.0
160.10	774.0
161.10	917.0
164.90	599.0
166.10	688.0
167.00	3482.0
168.00	2145.0
168.90	335.0
173.00	433.0
174.00	678.0
175.10	1396.0
176.00	518.0
177.10	650.0
179.00	2581.0
180.00	2508.0
181.00	756.0
184.90	1326.0
186.00	9135.0
187.00	2756.0
187.90	365.0
188.90	647.0
190.90	562.0

Instrument :
BNA_M
ClientSampleId :
DFTPP29

192.00	806.0
193.10	1138.0
196.00	1270.0
196.70	442.0
197.10	353.0
198.00	68664.0
199.00	5070.0
200.10	472.0
202.90	528.0
204.10	2402.0
205.10	4205.0
206.10	17224.0
207.10	3826.0
208.00	1341.0
209.00	454.0
210.80	635.0
211.10	602.0
216.00	386.0
217.00	4207.0
217.90	492.0
221.10	2533.0
221.70	775.0
223.10	1054.0
224.00	9643.0
225.00	2127.0
226.00	566.0
227.00	4021.0
228.00	595.0
228.90	878.0
233.90	318.0
235.00	379.0
237.00	492.0
242.00	418.0
243.00	353.0
244.10	7076.0
245.00	772.0
245.90	1385.0
254.20	416.0
255.00	35040.0
256.00	5110.0
256.90	426.0
258.00	2011.0
258.80	384.0
265.00	656.0
273.00	1160.0
274.00	2264.0
275.00	15822.0
276.10	1857.0
276.90	1158.0
277.80	393.0
292.90	323.0
296.00	4566.0
296.80	409.0
303.10	448.0
315.00	381.0
316.00	402.0
323.00	1406.0
327.00	301.0
334.10	815.0
351.90	472.0
354.00	347.0
364.90	1512.0
372.10	639.0
383.00	338.0
402.90	410.0
423.00	2946.0
424.00	1051.0
441.00	7376.0
442.00	47416.0
443.10	8162.0
444.00	773.0

Instrument :
BNA_M
ClientSampleId :
DFTPP29

m/z	Abundance
38.00	404.0
39.00	1934.0
40.00	454.0
44.10	1925.0
48.90	342.0
50.10	7068.0
51.10	28952.0
52.10	1387.0
56.00	881.0
57.10	2269.0
61.10	416.0
62.00	430.0
63.00	1149.0
64.90	530.0
68.00	607.0
69.00	25648.0
73.10	649.0
74.10	2656.0
75.00	3740.0
76.00	1397.0
77.10	28896.0
78.10	1928.0
79.00	1830.0
80.00	1719.0
81.00	2120.0
82.10	384.0
83.10	581.0
85.00	516.0
85.90	1062.0
86.90	332.0
91.00	530.0
91.90	534.0
93.00	3710.0
98.00	2666.0
99.00	2658.0
101.00	1167.0
102.90	605.0
103.90	986.0
104.90	568.0
106.10	324.0
107.00	9928.0
108.00	1430.0
109.00	366.0
110.00	17464.0
111.00	2929.0
115.90	723.0
117.00	7780.0
118.00	753.0
122.00	664.0
123.00	1129.0
123.90	449.0
124.90	594.0
127.00	32184.0
128.00	2347.0
129.00	13702.0
130.00	1082.0
134.00	443.0
135.00	1209.0
136.00	460.0
136.90	558.0
141.00	1657.0
141.80	436.0
146.00	374.0
147.10	1090.0
148.00	2232.0
149.00	544.0
153.00	610.0
153.90	631.0
155.00	940.0
156.00	1646.0
158.00	520.0
160.00	631.0
160.90	1007.0
165.00	678.0
166.00	378.0
167.00	4207.0
168.10	2037.0
171.90	374.0
173.10	324.0
174.00	852.0
175.10	1567.0
177.10	694.0
178.90	2787.0
180.00	2205.0
181.00	645.0
185.00	1337.0
186.00	10463.0
187.10	3080.0
188.10	387.0
188.90	668.0
190.90	445.0

Instrument :
BNA_M
ClientSampleId :
DFTPP29

192.00	1118.0
192.90	1255.0
196.00	1848.0
196.80	324.0
197.10	389.0
198.00	75576.0
199.00	4738.0
200.10	557.0
202.90	331.0
204.10	2793.0
205.10	4175.0
206.10	19392.0
207.10	4167.0
208.00	974.0
208.90	473.0
210.90	1023.0
216.10	490.0
217.00	5012.0
218.00	829.0
221.00	3048.0
221.90	596.0
223.00	974.0
224.10	10279.0
225.00	2899.0
225.90	359.0
227.00	4279.0
228.00	725.0
229.00	897.0
237.00	444.0
241.80	337.0
243.00	431.0
244.10	7619.0
245.10	1081.0
246.00	1566.0
246.90	424.0
248.90	451.0
254.00	460.0
255.00	42712.0
256.00	6249.0
257.00	553.0
258.00	1967.0
258.90	400.0
265.00	1266.0
272.90	1246.0
274.00	3113.0
275.00	18152.0
276.00	2991.0
277.00	1581.0
296.00	5275.0
296.90	609.0
303.00	438.0
314.10	354.0
314.80	464.0
323.00	1606.0
334.00	1416.0
341.00	320.0
352.00	483.0
353.00	433.0
353.80	354.0
365.00	2448.0
372.10	837.0
401.90	384.0
402.90	714.0
404.00	312.0
420.90	499.0
422.00	576.0
423.00	3678.0
423.90	1345.0
441.00	11468.0
442.10	72672.0
443.10	13855.0
443.90	1214.0

Instrument :
BNA_M
ClientSampleId :
DFTPP29

m/z	Abundance
39.00	1075.0
40.00	522.0
44.00	2058.0
50.10	3707.0
51.10	15268.0
52.10	718.0
55.90	407.0
57.00	890.0
63.00	653.0
63.90	304.0
66.00	302.0
69.00	13618.0
73.00	594.0
74.00	1171.0
75.00	2208.0
76.10	713.0
77.10	14942.0
78.00	960.0
79.00	1083.0
80.00	734.0
81.00	1317.0
81.90	323.0
86.00	526.0
91.10	310.0
92.00	355.0
92.90	1950.0
98.00	1510.0
99.10	1159.0
101.20	520.0
104.90	557.0
107.00	5868.0
108.00	661.0
110.00	9811.0
111.00	1478.0
117.00	4871.0
122.10	439.0
123.00	612.0
124.90	302.0
127.00	19736.0
128.00	1559.0
129.00	8610.0
130.00	629.0
134.00	428.0
135.00	906.0
137.00	581.0
140.90	1105.0
141.90	361.0
147.10	742.0
148.00	1009.0
149.00	447.0
153.10	357.0
154.90	444.0
156.00	850.0
159.90	314.0
160.90	738.0
164.90	509.0
167.00	2716.0
168.10	1128.0
171.90	310.0
173.10	340.0
173.90	356.0
175.00	993.0
177.10	717.0
179.00	2004.0
180.00	1274.0
180.90	604.0
184.90	772.0
186.10	6575.0
187.00	1667.0
189.00	441.0
190.90	373.0
191.90	557.0
193.00	800.0
196.00	1094.0
198.00	46320.0
198.90	3154.0
202.90	321.0
204.00	1615.0
205.00	2951.0
206.00	11885.0
207.10	3142.0
208.00	550.0
211.10	486.0
217.00	3658.0
218.00	348.0
221.10	1755.0
222.00	333.0
223.00	896.0
224.10	7567.0
225.00	1389.0
226.00	323.0

Instrument :
BNA_M
ClientSampleId :
DFTPP29

226.90	2669.0
228.00	467.0
228.90	622.0
237.00	343.0
244.10	5799.0
245.10	807.0
246.00	1214.0
255.10	28016.0
256.00	3038.0
258.10	1682.0
265.00	640.0
272.90	536.0
274.00	2604.0
275.00	11018.0
276.00	1604.0
276.90	994.0
296.00	2657.0
297.00	418.0
303.00	481.0
314.90	435.0
323.00	962.0
324.10	355.0
333.90	606.0
352.00	393.0
354.10	550.0
365.00	2007.0
371.90	747.0
401.90	371.0
403.00	462.0
421.00	438.0
423.00	2601.0
424.00	1135.0
441.00	9065.0
442.00	56712.0
443.00	10242.0
444.10	977.0

Instrument :
BNA_M
ClientSampleId :
DFTPP29

Scan 2513 (17.468 min): BM000610.D
DFTPP29

m/z	Abundance
39.90	481.0
44.10	2659.0
73.10	419.0
207.00	1570.0
208.10	594.0

Instrument :
BNA_M
ClientSampleId :
DFTPP29