

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022717\
 Data File : BM009036.D
 Acq On : 27 Feb 2017 19:21
 Operator : SJ/MA
 Sample : I1943-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DABR5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.358	41	46	54	rVB2	51326	77384	1.64%	0.188%
2	7.045	668	673	681	rVB	149880	239625	5.07%	0.582%
3	7.228	696	704	712	rBV	586305	904890	19.16%	2.198%
4	7.422	729	737	745	rBV	575945	940213	19.91%	2.284%
5	7.898	811	818	826	rVB	712074	1128096	23.88%	2.740%
6	8.592	929	936	945	rBV	415463	672924	14.25%	1.635%
7	9.057	1008	1015	1022	rBV	725455	1225653	25.95%	2.977%
8	9.781	1130	1138	1146	rBV	586889	978351	20.71%	2.376%
9	10.310	1221	1228	1237	rBV	825256	1346839	28.52%	3.271%
10	10.698	1286	1294	1302	rVB	859398	1460007	30.91%	3.546%
11	13.939	1836	1845	1854	rBV	1561813	2182644	46.21%	5.302%
12	14.227	1886	1894	1902	rBV	1611254	2344022	49.63%	5.694%
13	14.533	1940	1946	1954	rBV2	1157863	1829843	38.74%	4.445%
14	14.721	1972	1978	1986	rBV2	106535	186624	3.95%	0.453%
15	15.527	2109	2115	2124	rVB	2316948	3234664	68.49%	7.857%
16	15.639	2128	2134	2143	rBV	823158	1150218	24.35%	2.794%
17	17.280	2407	2413	2420	rBV	1594013	2227691	47.17%	5.411%
18	17.380	2423	2430	2442	rVV	2842069	3975020	84.16%	9.655%
19	19.427	2774	2778	2784	rBV6	45794	64993	1.38%	0.158%
20	19.556	2796	2800	2806	rBV3	27782	56545	1.20%	0.137%
21	19.668	2813	2819	2828	rBV	3584916	4723071	100.00%	11.472%
22	21.450	3117	3122	3129	rBV	2319947	2812734	59.55%	6.832%
23	23.644	3488	3495	3505	rVB	2479582	4717300	99.88%	11.458%
24	23.791	3514	3520	3530	rVB2	1360216	2690632	56.97%	6.535%


Sum of corrected areas: 41169983

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022717\
Data File : BM009036.D
Acq On : 27 Feb 2017 19:21
Operator : SJ/MA
Sample : I1943-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DABR5

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM022317.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

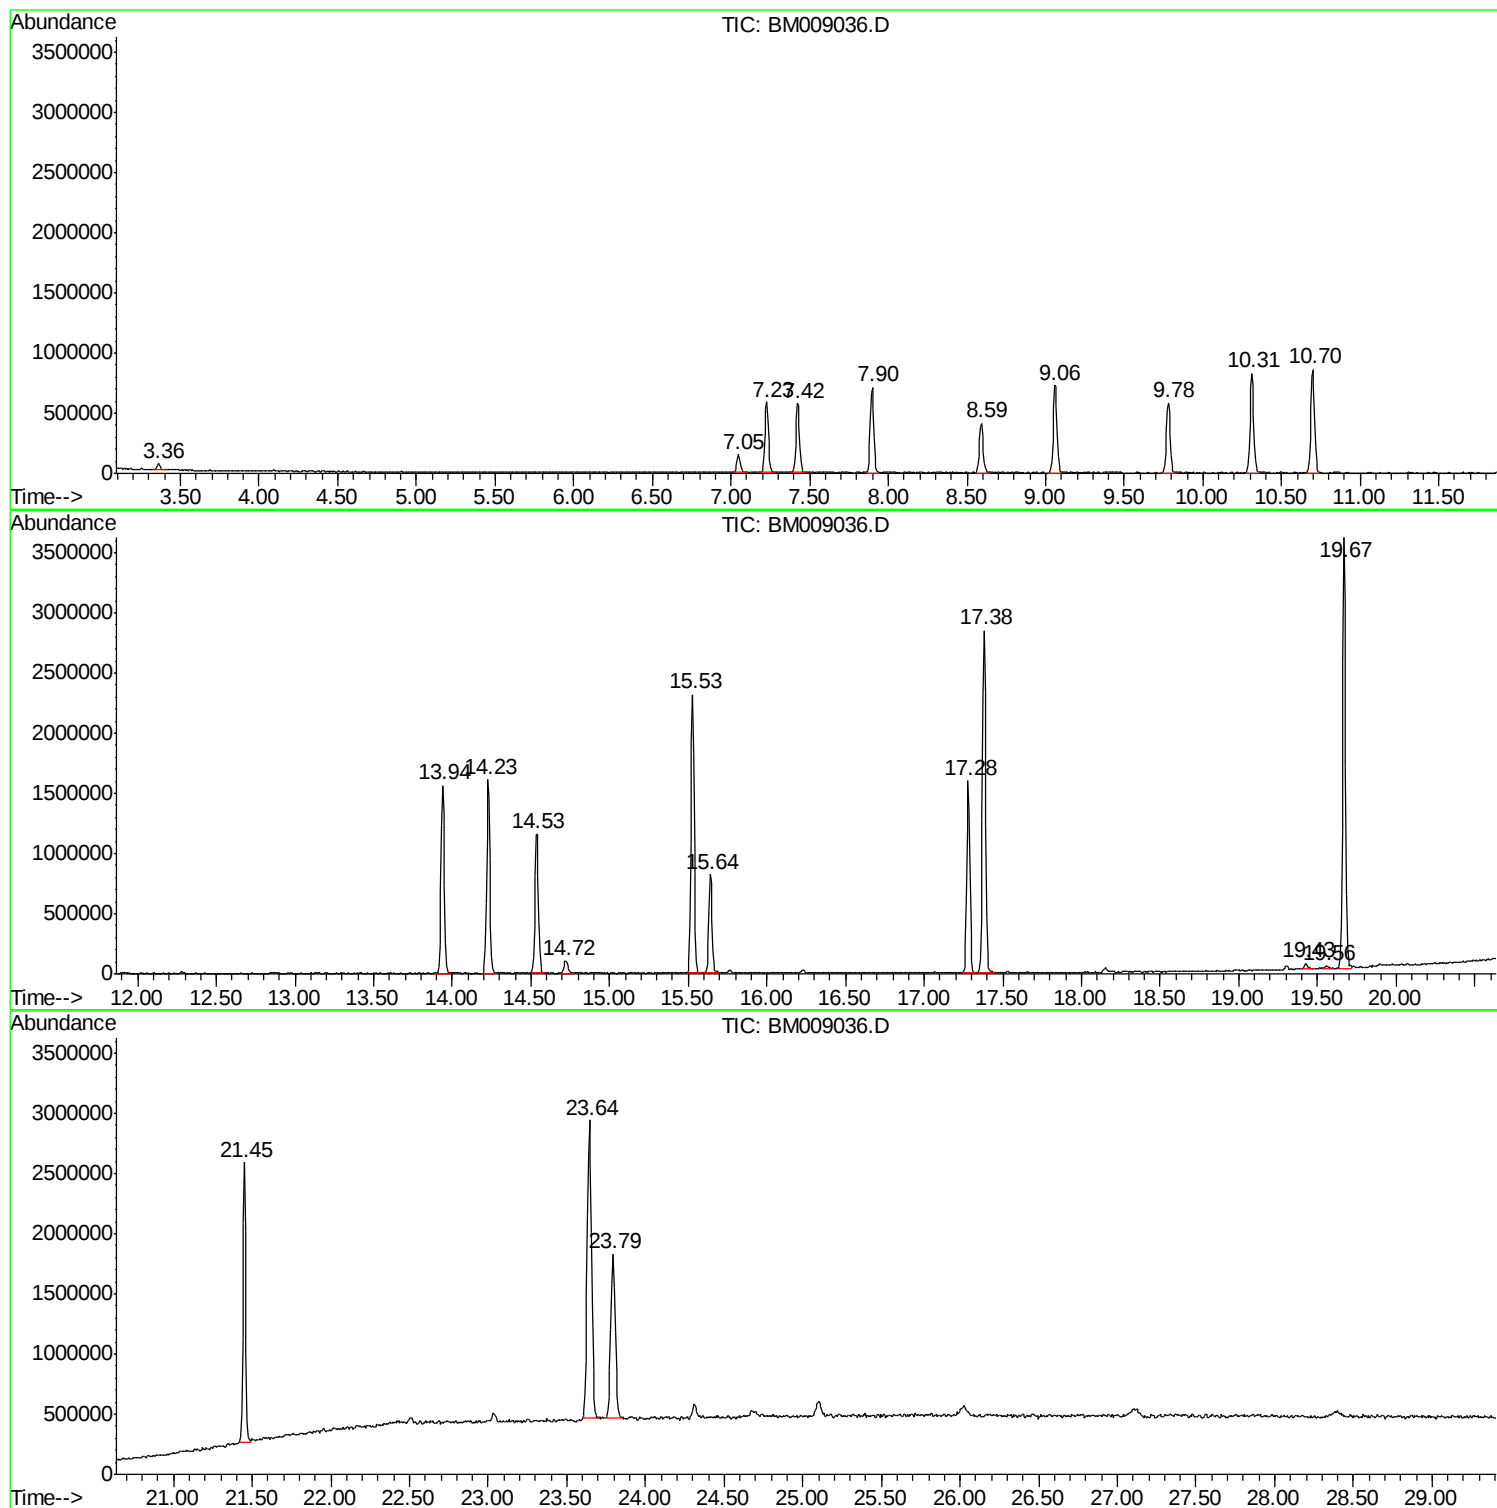

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022717\
Data File : BM009036.D
Acq On : 27 Feb 2017 19:21
Operator : SJ/MA
Sample : I1943-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DABR5

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022717\
Data File : BM009036.D
Acq On : 27 Feb 2017 19:21
Operator : SJ/MA
Sample : I1943-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DABR5

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022317.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc