

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022718\
 Data File : BM014389.D
 Acq On : 27 Feb 2018 19:02
 Operator : SJ/JU
 Sample : J1631-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Feb 28 00:47:08 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 28 00:45:45 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	108773	20.00	ng/ul	0.00
18) Naphthalene-d8	10.29	136	447510	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.18	164	260407	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.94	188	518944	20.00	ng/ul	0.00
75) Chrysene-d12	21.16	240	503174	20.00	ng/ul	0.00
83) Perylene-d12	23.34	264	494908	20.00	ng/ul	0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.10	96	7809	3.07	ng/uL	0.00
5) Phenol-d5	6.73	99	169574	18.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.87	67	101983	18.33	ng/ul	0.00
9) 2-Chlorophenol-d4	7.06	132	141466	20.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.25	113	138213	17.18	ng/ul	0.01
19) Nitrobenzene-d5	8.68	128	73900	22.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.40	143	83603	24.42	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.94	165	159039	22.43	ng/ul	0.01
29) 4-Chloroaniline-d4	10.46	131	114694	16.42	ng/ul	0.00
43) Dimethylphthalate-d6	13.60	166	530195	24.65	ng/ul	0.00
46) Acenaphthylene-d8	13.87	160	658692	24.84	ng/ul	0.01
51) 4-Nitrophenol-d4	14.46	143	53983	18.18	ng/ul	0.03
57) Fluorene-d10	15.19	176	445257	23.11	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	8964	2.88	ng/ul	0.01
70) Anthracene-d10	17.04	188	668407	26.70	ng/ul	0.00
76) Pyrene-d10	19.35	212	673316	25.94	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.20	264	619261	25.71	ng/ul	0.02

Target Compounds

					Ovalue
4) Benzaldehyde	6.69	77	4171	1.113 ng/ul	86
6) Phenol	6.76	94	26967	2.795 ng/ul	90
14) Acetophenone	8.36	105	21432	1.544 ng/ul	85
28) Naphthalene	10.34	128	68791	2.993 ng/ul	96
34) 2-Methylnaphthalene	11.97	142	24014	1.373 ng/ul	92
44) Dimethylphthalate	13.65	163	233312	11.002 ng/ul	100
47) Acenaphthylene	13.90	152	111923	4.465 ng/ul	97
49) Acenaphthene	14.25	153	41291	2.340 ng/ul	90
53) Dibenzofuran	14.59	168	45826	1.732 ng/ul	100
58) Fluorene	15.24	166	60223	2.636 ng/ul#	97
69) Phenanthrene	16.99	178	1320689	44.171 ng/ul	99
71) Anthracene	17.08	178	246667	8.203 ng/ul	97
72) Carbazole	17.36	167	109697	4.339 ng/ul	98
74) Fluoranthene	19.02	202	2313829	64.773 ng/ul#	95
77) Pyrene	19.39	202	2129587	63.685 ng/ul#	92
80) Benzo(a)anthracene	21.14	228	1082123	34.459 ng/ul	96
82) Chrysene	21.20	228	1119305	38.208 ng/ul	98
85) Benzo(b)fluoranthene	22.70	252	1397288	42.166 ng/ul#	98
86) Benzo(k)fluoranthene	22.70	252	1397288	44.349 ng/ul#	96
88) Benzo(a)pyrene	23.25	252	1004296	33.915 ng/ul#	97
89) Indeno(1,2,3-cd)pyrene	25.51	276	672648	23.409 ng/ul#	96
90) Dibenz(a,h)anthracene	25.51	278	180416	7.556 ng/ul#	82
91) Benzo(g,h,i)perylene	26.17	276	494415	21.240 ng/ul#	95

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022718\
Data File : BM014389.D
Acq On : 27 Feb 2018 19:02
Operator : SJ/JU
Sample : J1631-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Feb 28 00:47:08 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 28 00:45:45 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022718\
Data File : BM014389.D
Acq On : 27 Feb 2018 19:02
Operator : SJ/JU
Sample : J1631-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Feb 28 00:47:08 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 28 00:45:45 2018
Response via : Initial Calibration

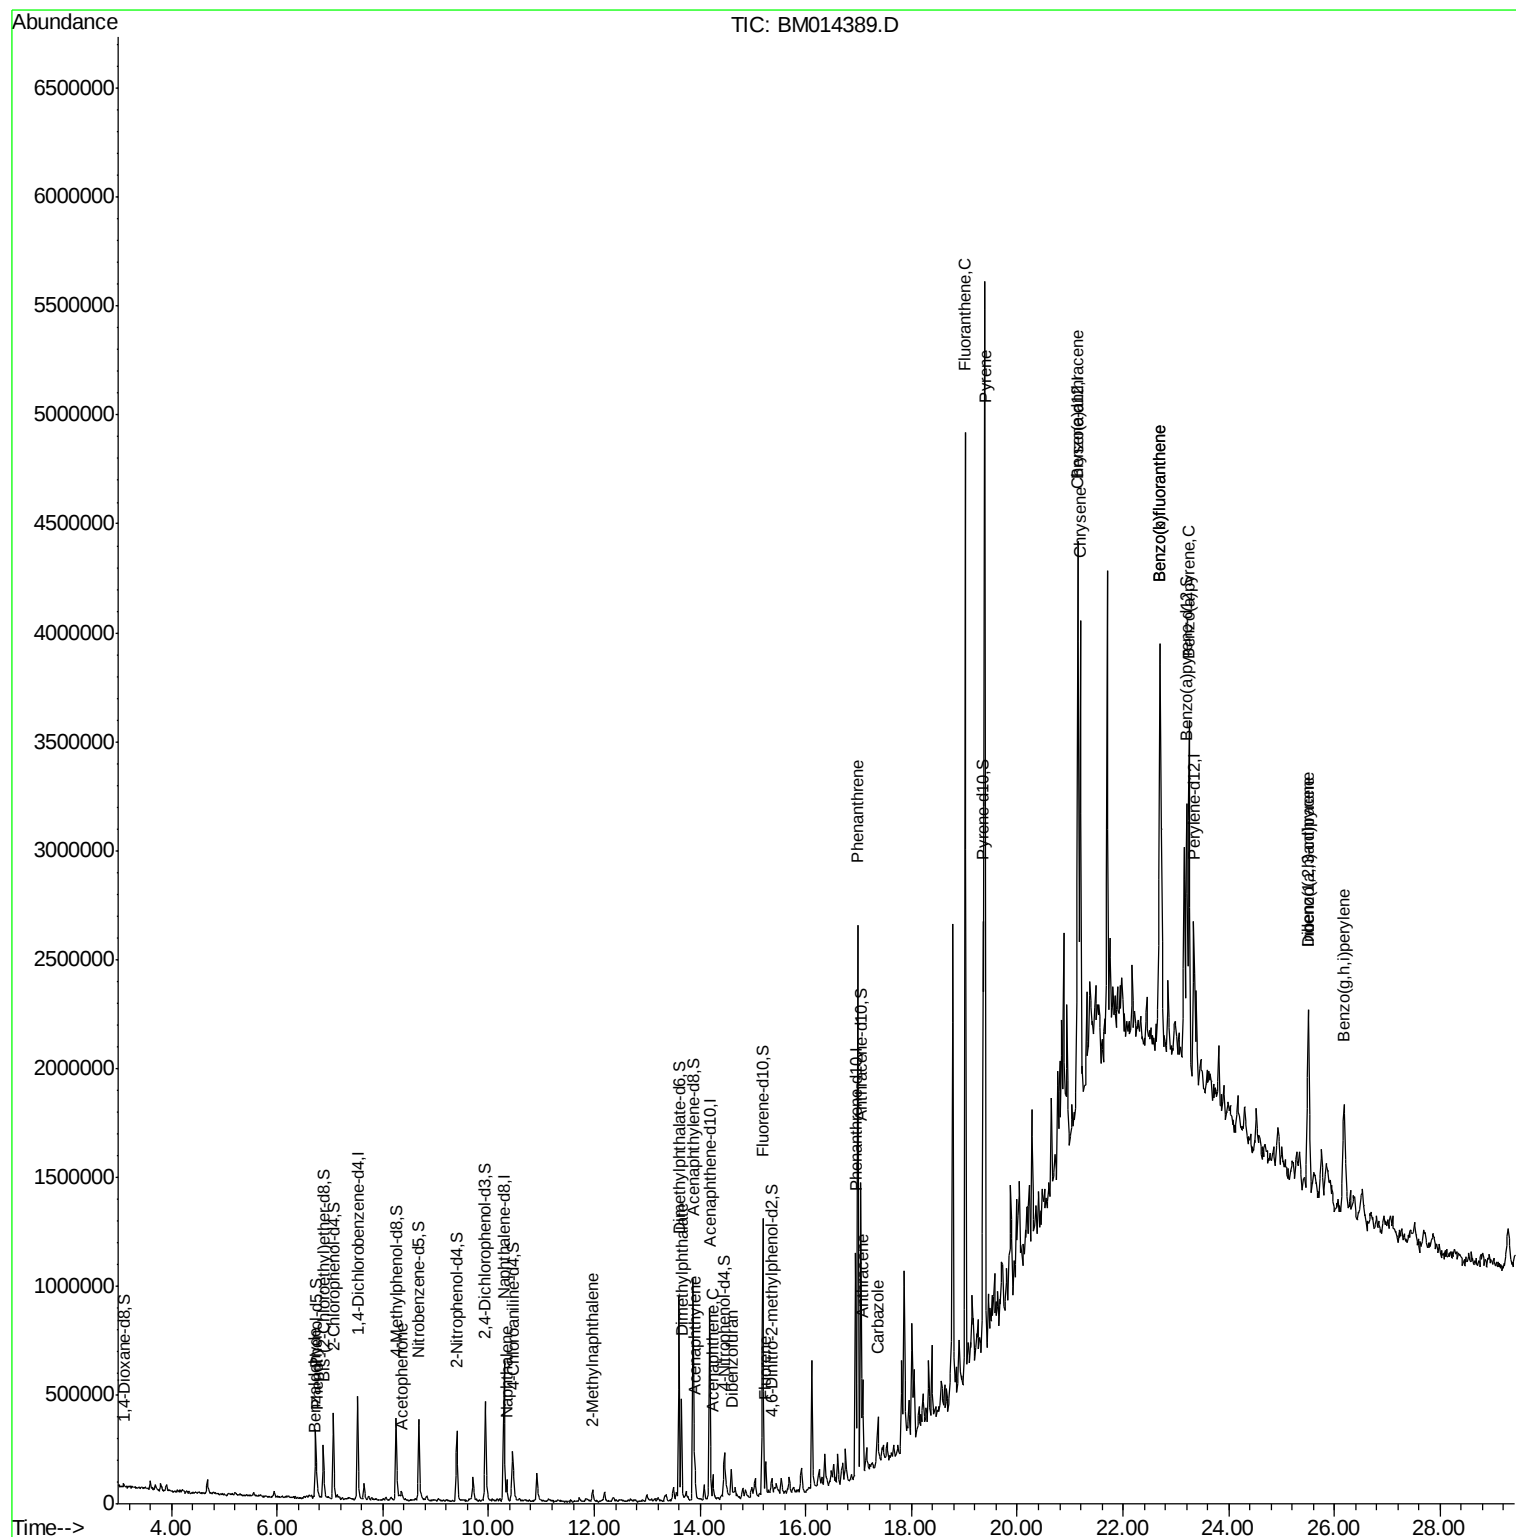

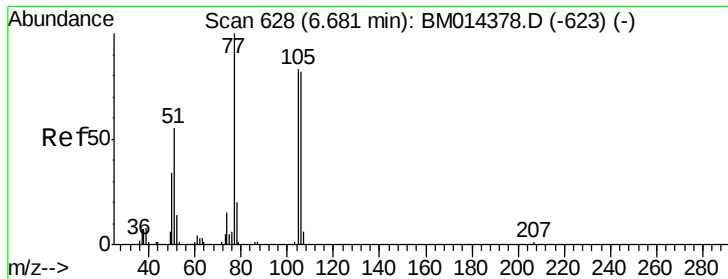

#4

Benzaldehyde

Concen: 1.113 ng/ul

RT: 6.69 min Scan# 630

Delta R.T. 0.01 min

Lab File: BM014389.D

Acq: 27 Feb 2018 19:02

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 77 Resp: 4171

Ion Ratio Lower Upper

77 100

105 67.9 66.1 99.1




106 96.0 67.8 101.6

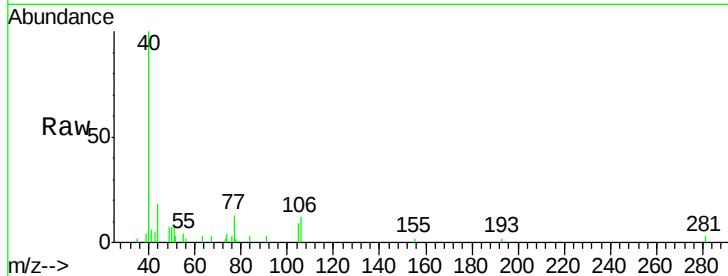

Abundance Ion 77.00 (76.70 to 77.70): BM014378.D (-623) (-)

Ion 105.00 (104.70 to 105.70): BM014378.D (-623) (-)

Ion 106.00 (105.70 to 106.70): BM014378.D (-623) (-)

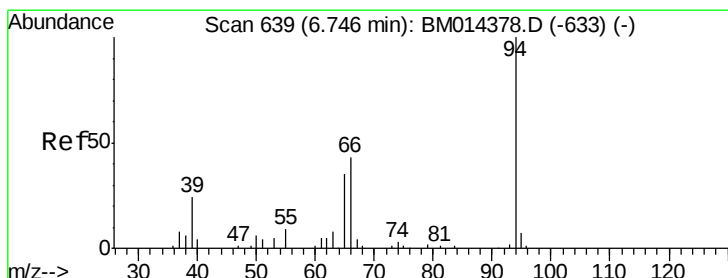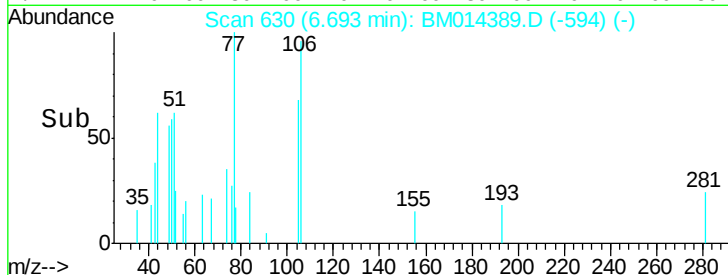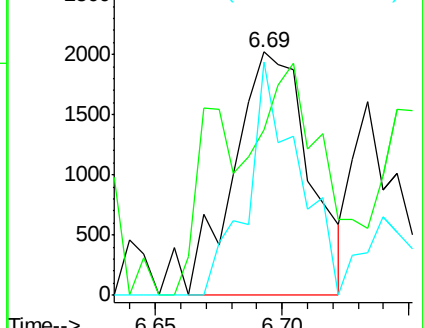

#6

Phenol

Concen: 2.795 ng/ul

RT: 6.76 min Scan# 641

Delta R.T. 0.01 min

Lab File: BM014389.D

Acq: 27 Feb 2018 19:02


Tgt Ion: 94 Resp: 26967

Ion Ratio Lower Upper

94 100

65 39.9 28.2 42.4



66 50.5 47.2 70.8

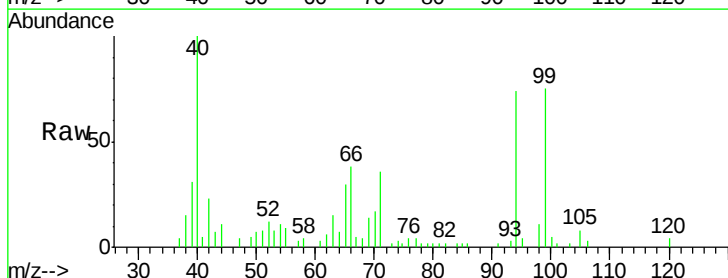


Abundance Ion 94.00 (93.70 to 94.70): BM014378.D (-633) (-)

Ion 65.00 (64.70 to 65.70): BM014378.D (-633) (-)

Ion 66.00 (65.70 to 66.70): BM014378.D (-633) (-)



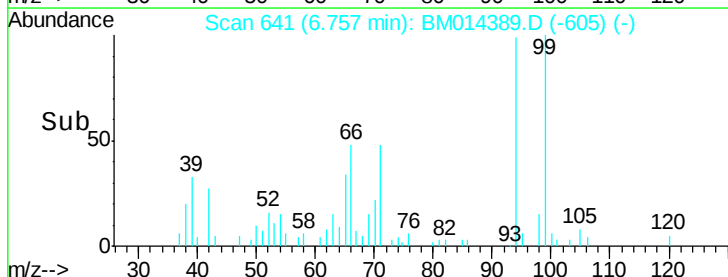
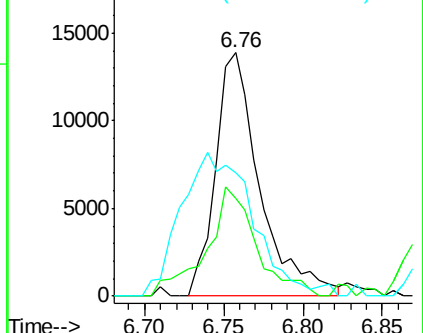




#14
Acetophenone
Concen: 1.544 ng/ul
RT: 8.36 min Scan# 913
Delta R.T. 0.01 min
Lab File: BM014389.D
Acq: 27 Feb 2018 19:02




Instrument :
BNA_M
ClientSampled :


Tot Ion:105 Resp: 21432
Ion Ratio Lower Upper
105 100
77 75.6 74.2 111.4
51 31.6 23.4 35.2

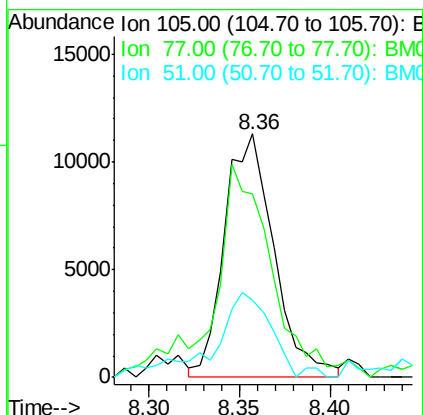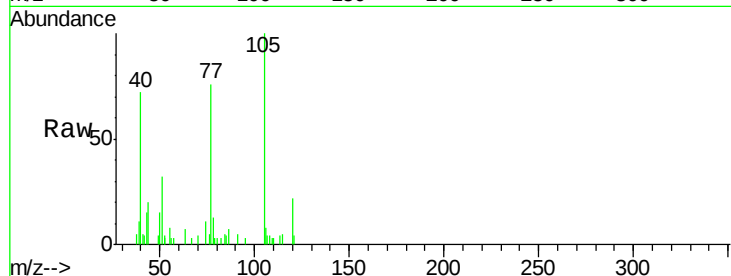

#28
Naphthalene
Concen: 2.993 ng/ul
RT: 10.34 min Scan# 1250
Delta R.T. -0.00 min
Lab File: BM014389.D
Acq: 27 Feb 2018 19:02

Tgt Ion:128 Resp: 68791
Ion Ratio Lower Upper
128 100
129 8.9 8.8 13.2
127 12.3 10.6 16.0

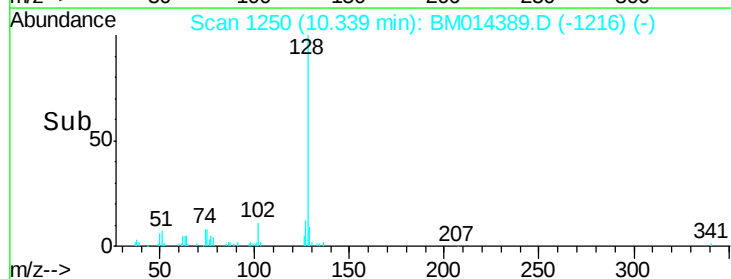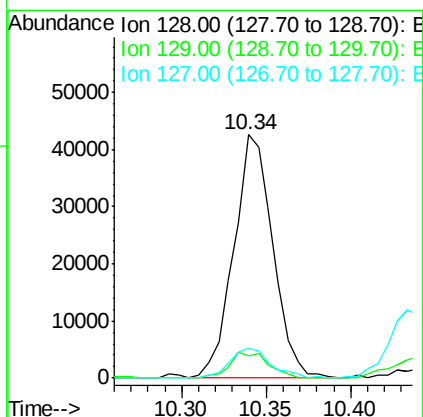







#34
 2-Methylnaphthalene
 Concen: 1.373 ng/ul
 RT: 11.97 min Scan# 1527
 Delta R.T. 0.01 min
 Lab File: BM014389.D
 Acq: 27 Feb 2018 19:02

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:142 Resp: 24014
 Ion Ratio Lower Upper
 142 100
 141 85.3 74.1 111.1

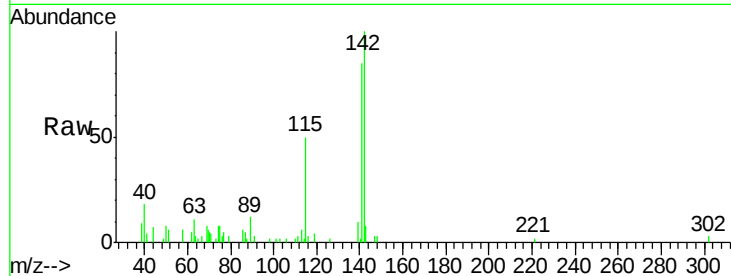


Abundance Ion 142.00 (141.70 to 142.70): E
 Ion 141.00 (140.70 to 141.70): E


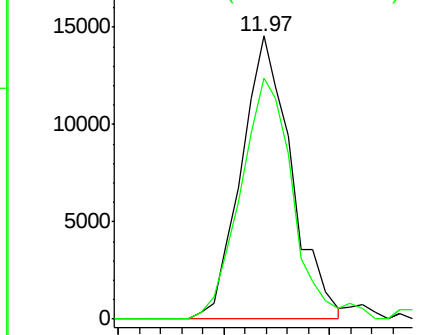



#44
 Dimethylphthalate
 Concen: 11.002 ng/ul
 RT: 13.65 min Scan# 1813
 Delta R.T. 0.01 min
 Lab File: BM014389.D
 Acq: 27 Feb 2018 19:02

Tgt Ion:163 Resp: 233312
 Ion Ratio Lower Upper
 163 100
 194 4.0 3.5 5.3
 164 10.3 8.2 12.4

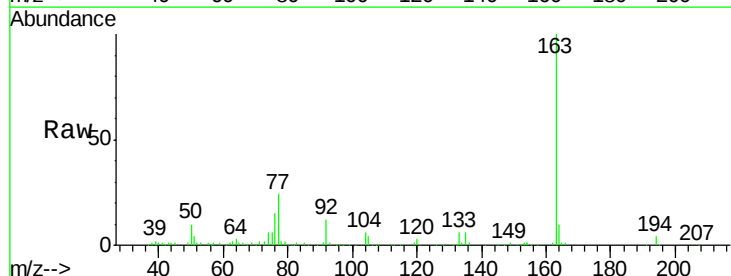

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

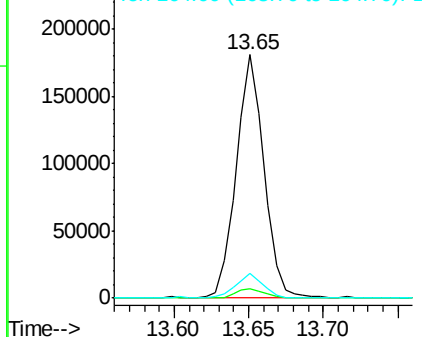



#47

Acenaphthylene

Concen: 4.465 ng/ul

RT: 13.90 min Scan# 1856

Delta R.T. 0.01 min

Lab File: BM014389.D

Acq: 27 Feb 2018 19:02

Instrument :

BNA_M

ClientSampleId :


Tot Ion:152 Resp: 111923

Ion Ratio Lower Upper




152 100

151 19.9 16.3 24.5

153 10.8 10.2 15.4

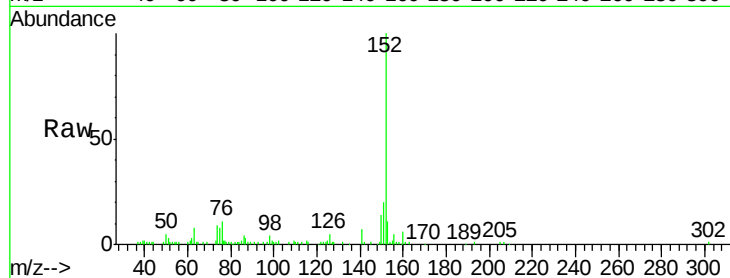

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E
Ion 153.00 (152.70 to 153.70): E

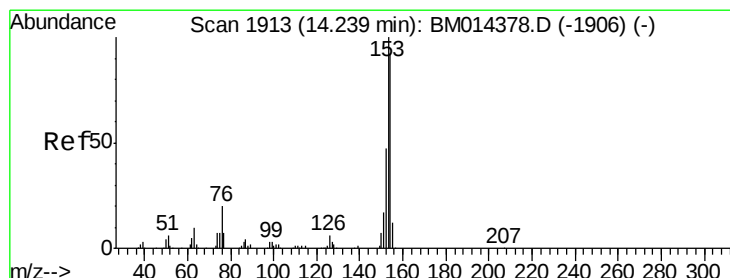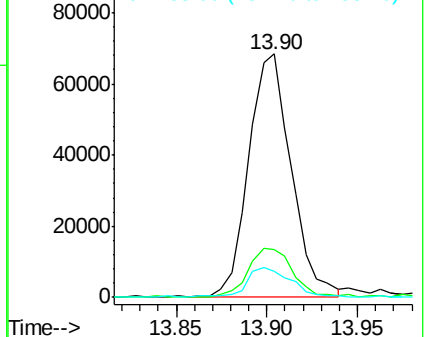

#49

Acenaphthene

Concen: 2.340 ng/ul

RT: 14.25 min Scan# 1914

Delta R.T. 0.01 min

Lab File: BM014389.D

Acq: 27 Feb 2018 19:02


Tgt Ion:153 Resp: 41291

Ion Ratio Lower Upper



153 100


152 48.3 37.6 56.4

154 74.9 70.4 105.6

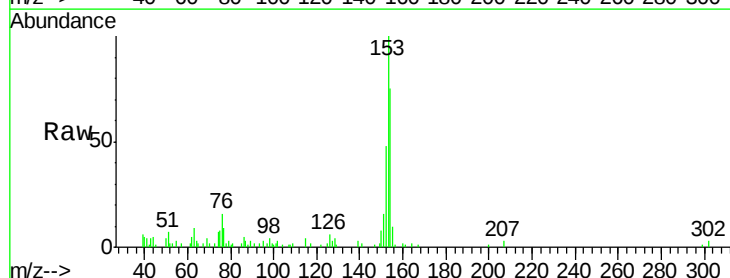

Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E




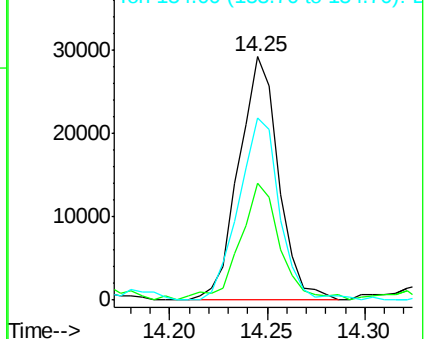




#53
Dibenzenofuran
Concen: 1.732 ng/ul
RT: 14.59 min Scan# 1973
Delta R.T. 0.01 min
Lab File: BM014389.D
Acq: 27 Feb 2018 19:02




Instrument :
BNA_M
ClientSampleId :


Tot Ion:168 Resp: 45826
Ion Ratio Lower Upper
168 100
139 38.5 30.8 46.2

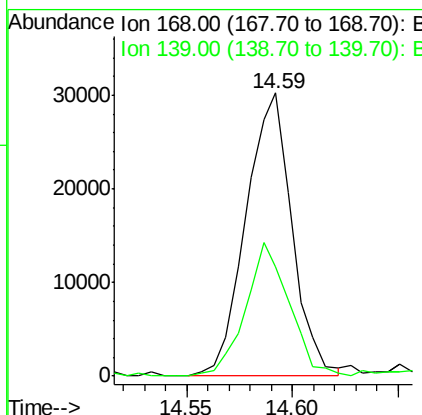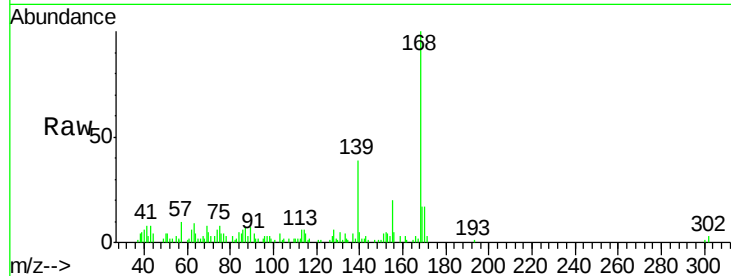

#58
Fluorene
Concen: 2.636 ng/ul
RT: 15.24 min Scan# 2083
Delta R.T. 0.01 min
Lab File: BM014389.D
Acq: 27 Feb 2018 19:02

Tgt Ion:166 Resp: 60223
Ion Ratio Lower Upper
166 100
165 99.1 77.9 116.9
167 17.8 10.6 16.0#

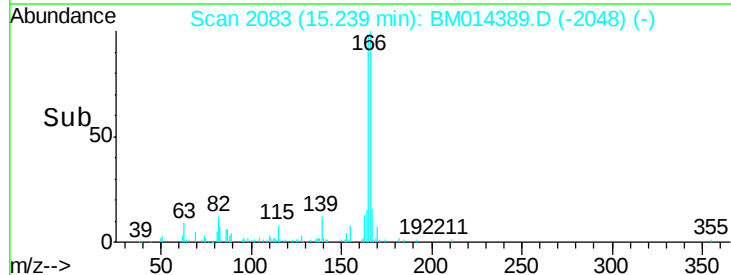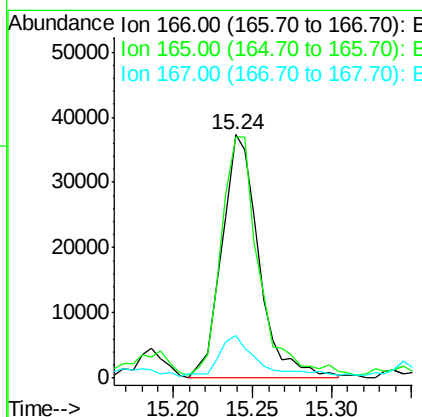



#69

Phenanthrene

Concen: 44.171 ng/ul

RT: 16.99 min Scan# 2380

Delta R.T. 0.01 min

Lab File: BM014389.D

Acq: 27 Feb 2018 19:02


Instrument :

BNA_M

ClientSampled :

Tot Ion:178 Resp: 1320689




Ion	Ratio	Lower	Upper
178	100		
179	15.1	12.6	19.0
176	19.2	14.9	22.3

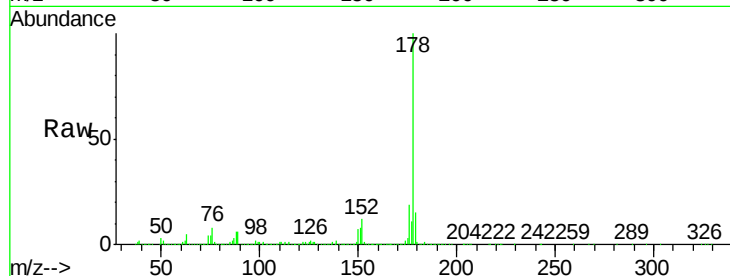

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

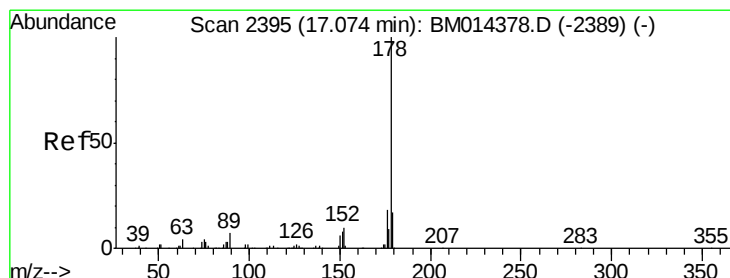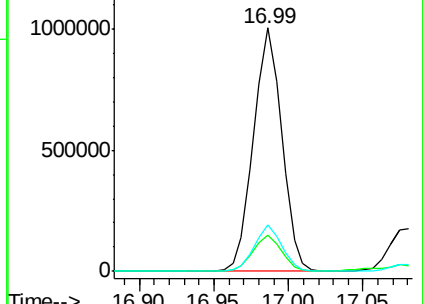

#71

Anthracene

Concen: 8.203 ng/ul

RT: 17.08 min Scan# 2396


Delta R.T. 0.01 min

Lab File: BM014389.D

Acq: 27 Feb 2018 19:02

Tgt Ion:178 Resp: 246667



Ion	Ratio	Lower	Upper
178	100		
179	14.0	11.7	17.5
176	16.3	14.6	21.8

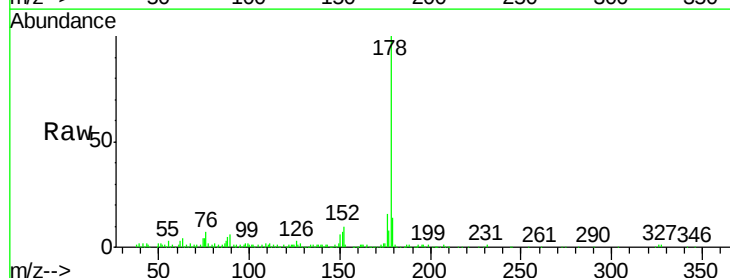


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E



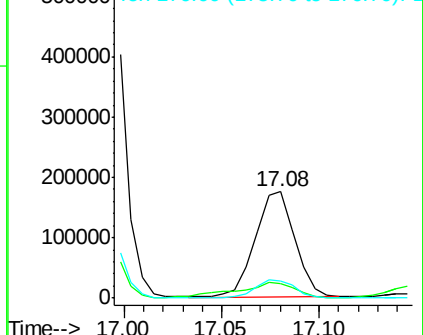





#72
 Carbazole
 Concen: 4.339 ng/ul
 RT: 17.36 min Scan# 2444
 Delta R.T. 0.01 min
 Lab File: BM014389.D
 Acq: 27 Feb 2018 19:02




Instrument :
 BNA_M
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
167	100		
166	21.1	17.1	25.7
139	14.2	10.0	15.0

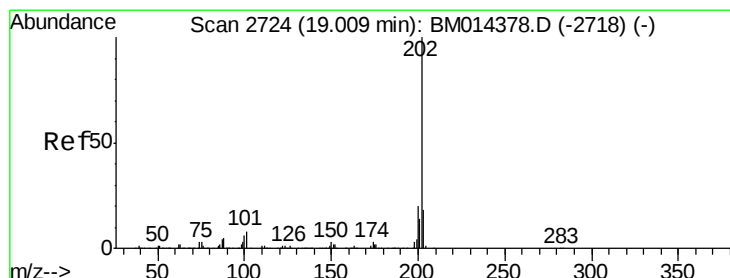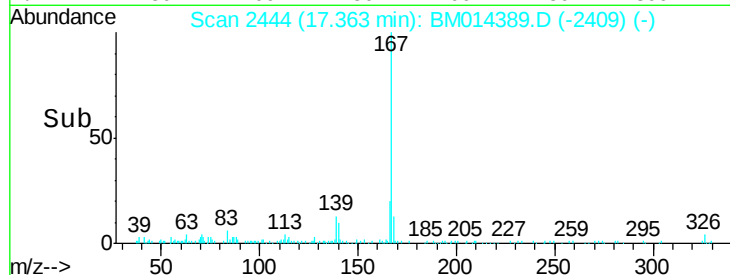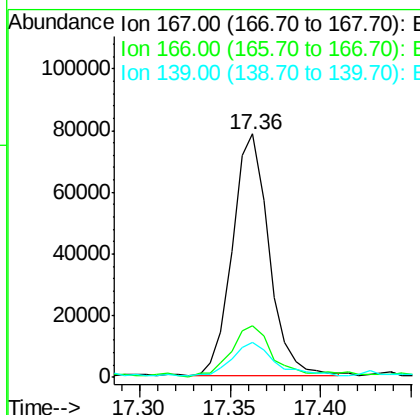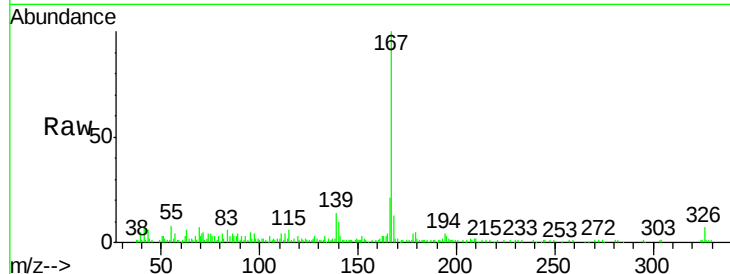

#74
 Fluoranthene
 Concen: 64.773 ng/ul
 RT: 19.02 min Scan# 2726
 Delta R.T. 0.01 min
 Lab File: BM014389.D
 Acq: 27 Feb 2018 19:02

Tgt Ion	Ratio	Lower	Upper
202	100		
101	7.8	4.6	7.0#
100	5.8	3.4	5.2#

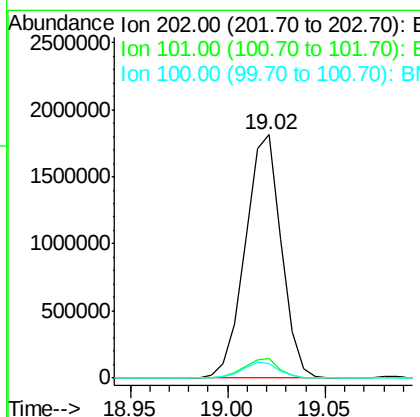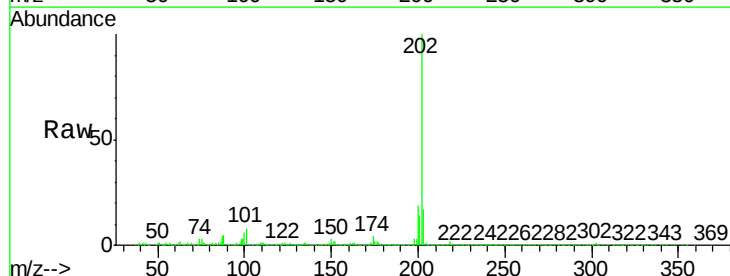



#77

Pvrene

Concen: 63.685 ng/ul

RT: 19.39 min Scan# 2788

Delta R.T. 0.01 min

Lab File: BM014389.D

Acq: 27 Feb 2018 19:02

Instrument :

BNA_M

ClientSampleId :


Tot Ion:202 Resp: 2129587

Ion Ratio Lower Upper

202 100

101 9.7 5.1 7.7#




100 8.0 4.9 7.3#



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

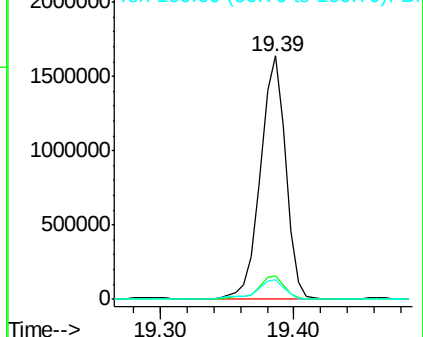

#80

Benzo(a)anthracene

Concen: 34.459 ng/ul

RT: 21.14 min Scan# 3087

Delta R.T. 0.01 min

Lab File: BM014389.D

Acq: 27 Feb 2018 19:02


Tgt Ion:228 Resp: 1082123

Ion Ratio Lower Upper

228 100

229 21.5 15.4 23.0



226 28.4 21.4 32.0




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

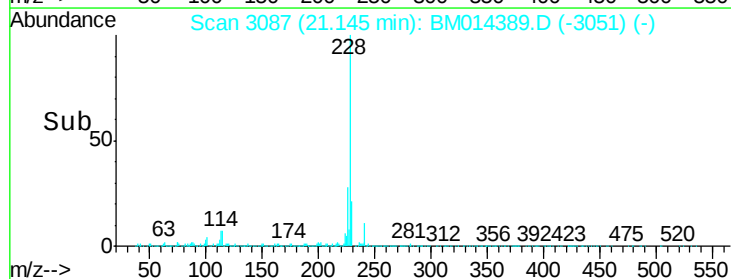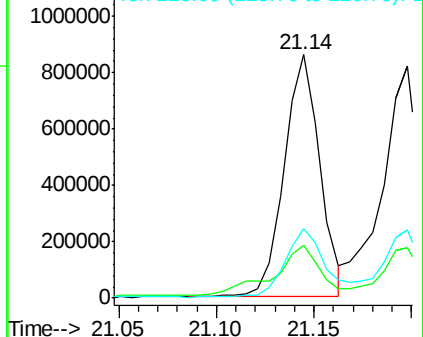

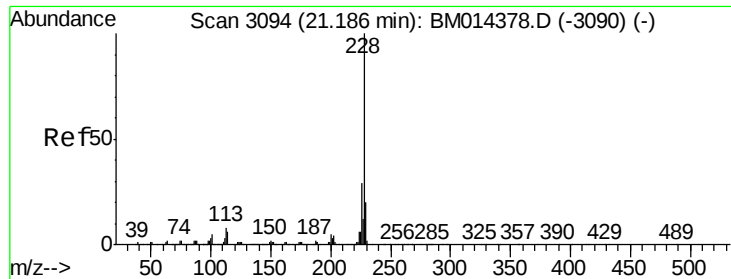

#82

Chrysene

Concen: 38.208 ng/ul

RT: 21.20 min Scan# 3096

Delta R.T. 0.01 min

Lab File: BM014389.D

Acq: 27 Feb 2018 19:02


Instrument :

BNA_M

ClientSampleId :

Tot Ion:228 Resp: 1119305

Ion	Ratio	Lower	Upper
228	100		
226	29.4	23.4	35.2
229	22.0	15.5	23.3



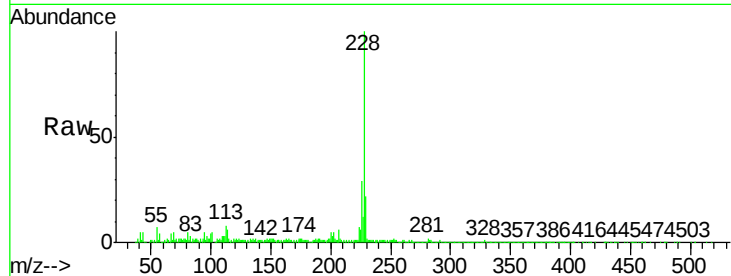


Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

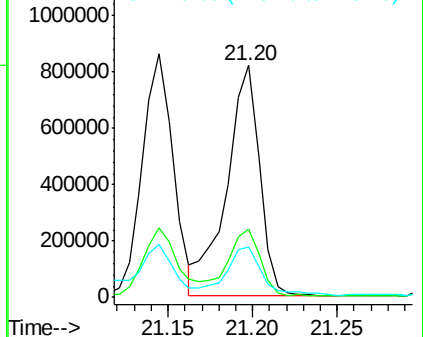

#85

Benzo(b)fluoranthene

Concen: 42.166 ng/ul

RT: 22.70 min Scan# 3351


Delta R.T. 0.02 min

Lab File: BM014389.D

Acq: 27 Feb 2018 19:02

Tgt Ion:252 Resp: 1397288

Ion	Ratio	Lower	Upper
252	100		
253	22.7	17.9	26.9
125	8.0	3.6	5.4






Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E



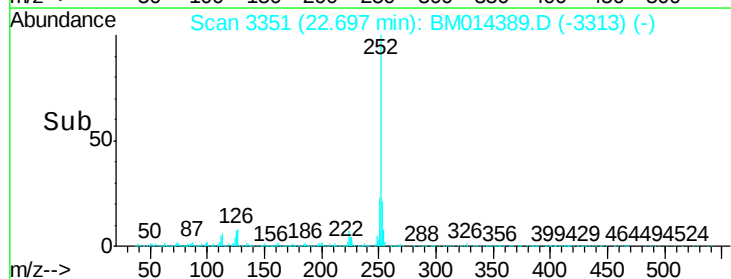
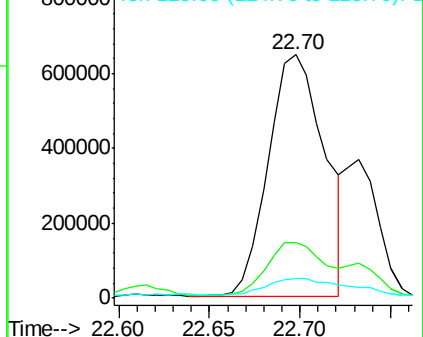




#86
Benzo(k)fluoranthene
Concen: 44.349 ng/ul
RT: 22.70 min Scan# 3351
Delta R.T. -0.02 min
Lab File: BM014389.D
Acq: 27 Feb 2018 19:02




Instrument :
BNA_M
ClientSampleId :


Tot Ion:252 Resp: 1397288
Ion Ratio Lower Upper
252 100
253 22.7 17.1 25.7
125 8.0 3.4 5.2#

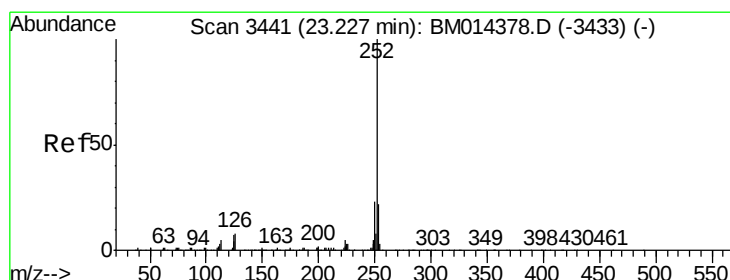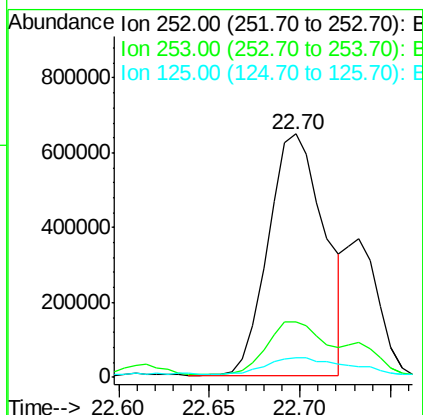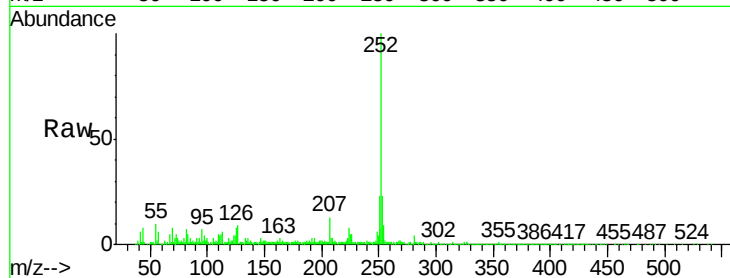

#88
Benzo(a)pyrene
Concen: 33.915 ng/ul
RT: 23.25 min Scan# 3445
Delta R.T. 0.02 min
Lab File: BM014389.D
Acq: 27 Feb 2018 19:02

Tgt Ion:252 Resp: 1004296
Ion Ratio Lower Upper
252 100
253 23.5 18.2 27.2
125 8.2 4.0 6.0#

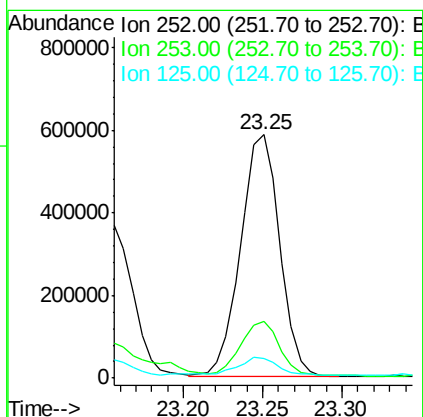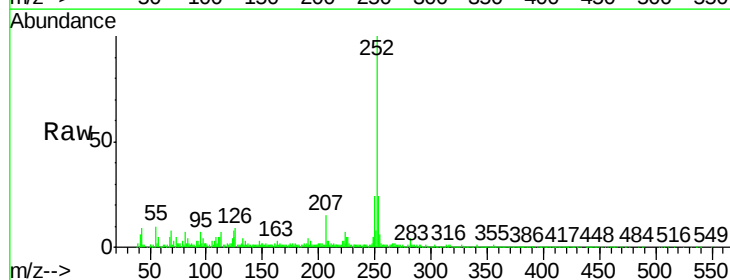




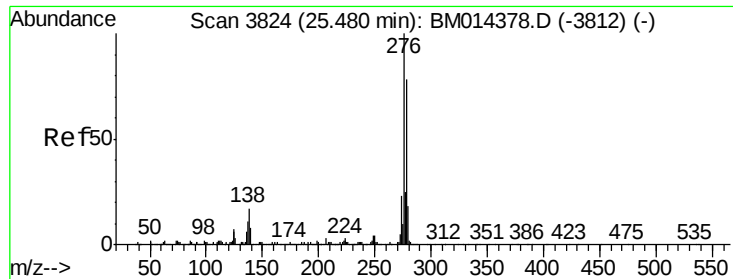


#89

Indeno(1,2,3-cd)pyrene
Concen: 23.409 ng/ul
RT: 25.51 min Scan# 3829
Delta R.T. 0.03 min
Lab File: BM014389.D
Acq: 27 Feb 2018 19:02

Instrument :
BNA_M
ClientSampleId :




Tot Ion	Ratio	Lower	Upper
276	100		
138	14.2	9.3	13.9#
277	26.4	19.9	29.9

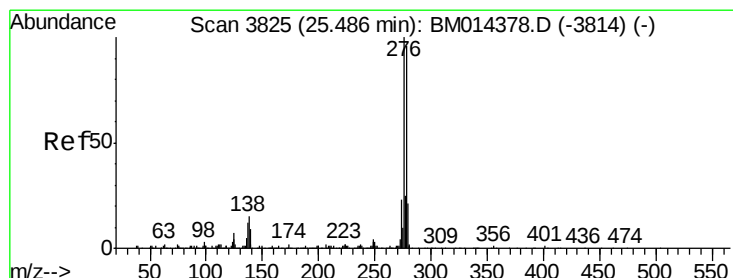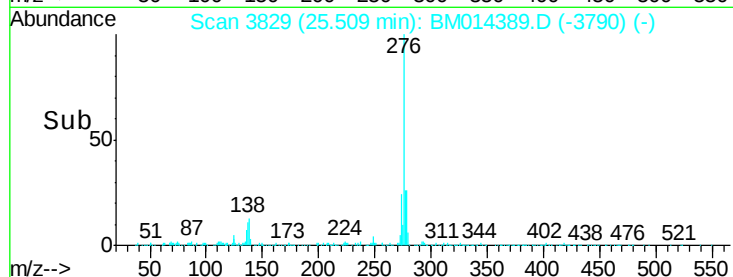
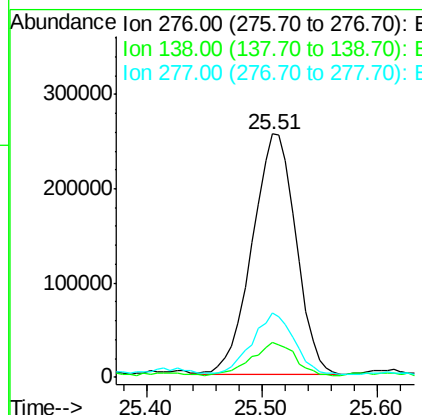
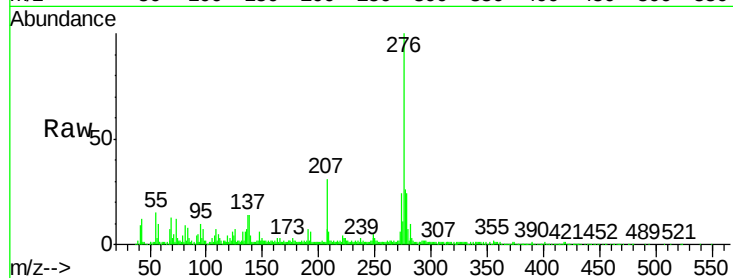


#90

Dibenzo(a,h)anthracene
Concen: 7.556 ng/ul
RT: 25.51 min Scan# 3829
Delta R.T. 0.02 min
Lab File: BM014389.D
Acq: 27 Feb 2018 19:02

Tgt Ion	Ratio	Lower	Upper
278	100		
139	21.5	5.8	8.8#
279	28.5	18.6	27.8#

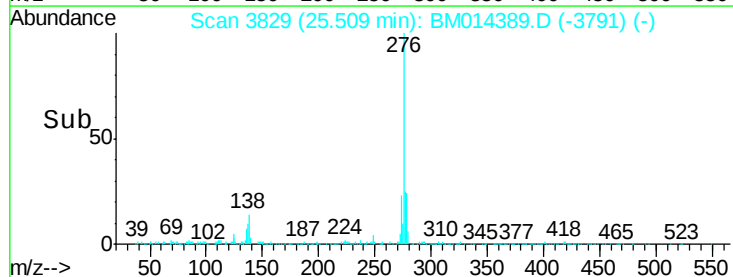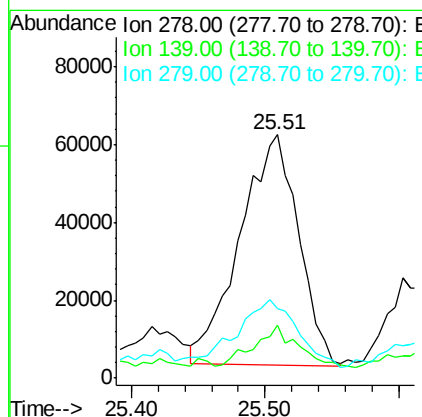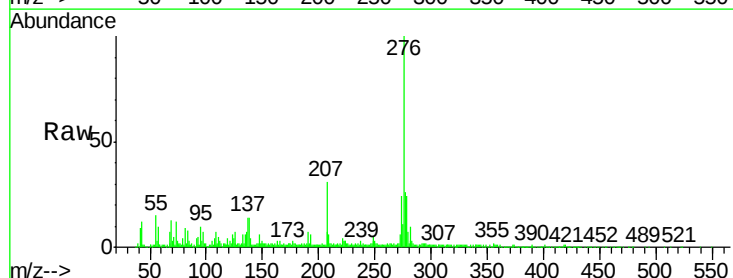

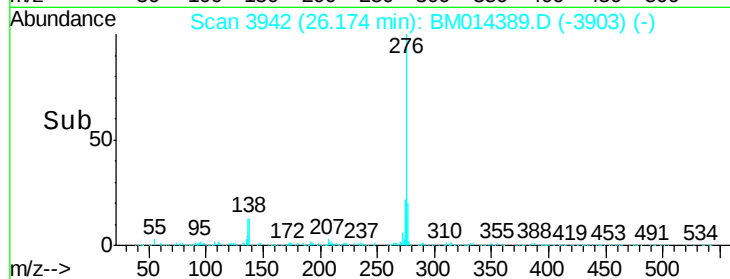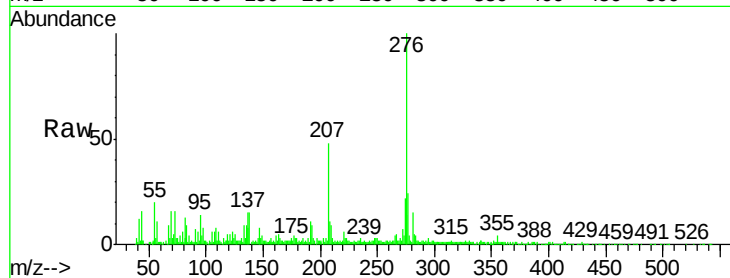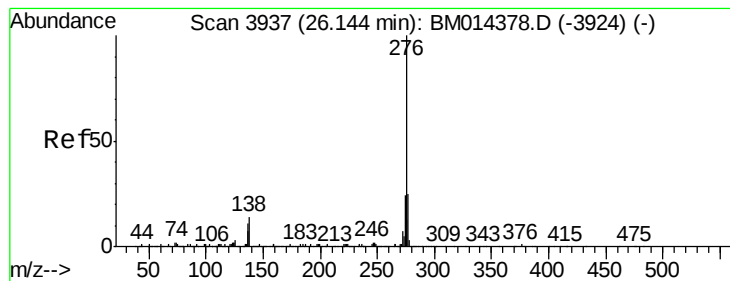

#91

Benzo(a,h,i)perylene

Concen: 21.240 ng/ul

RT: 26.17 min Scan# 3942

Delta R.T. 0.03 min

Lab File: BM014389.D

Acq: 27 Feb 2018 19:02

Instrument :

BNA_M

ClientSampleId :

Tot Ion:276 Resp: 494415

Ion Ratio Lower Upper

276 100

138 14.9 8.5 12.7#

277 24.1 18.6 28.0

