


Data Path : Z:\HPCHEM1\BNA M\Data\BM022718\
Data File : BM014389.D
Acq On : 27 Feb 2018 19:02
Operator : SJ/JU
Sample : J1631-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BE609

Manual Integrations
APPROVED

Sohil
2/28/2018 1:59:22 PM

Quant Time: Feb 28 01:56:15 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 28 00:45:45 2018
Response via : Initial Calibration

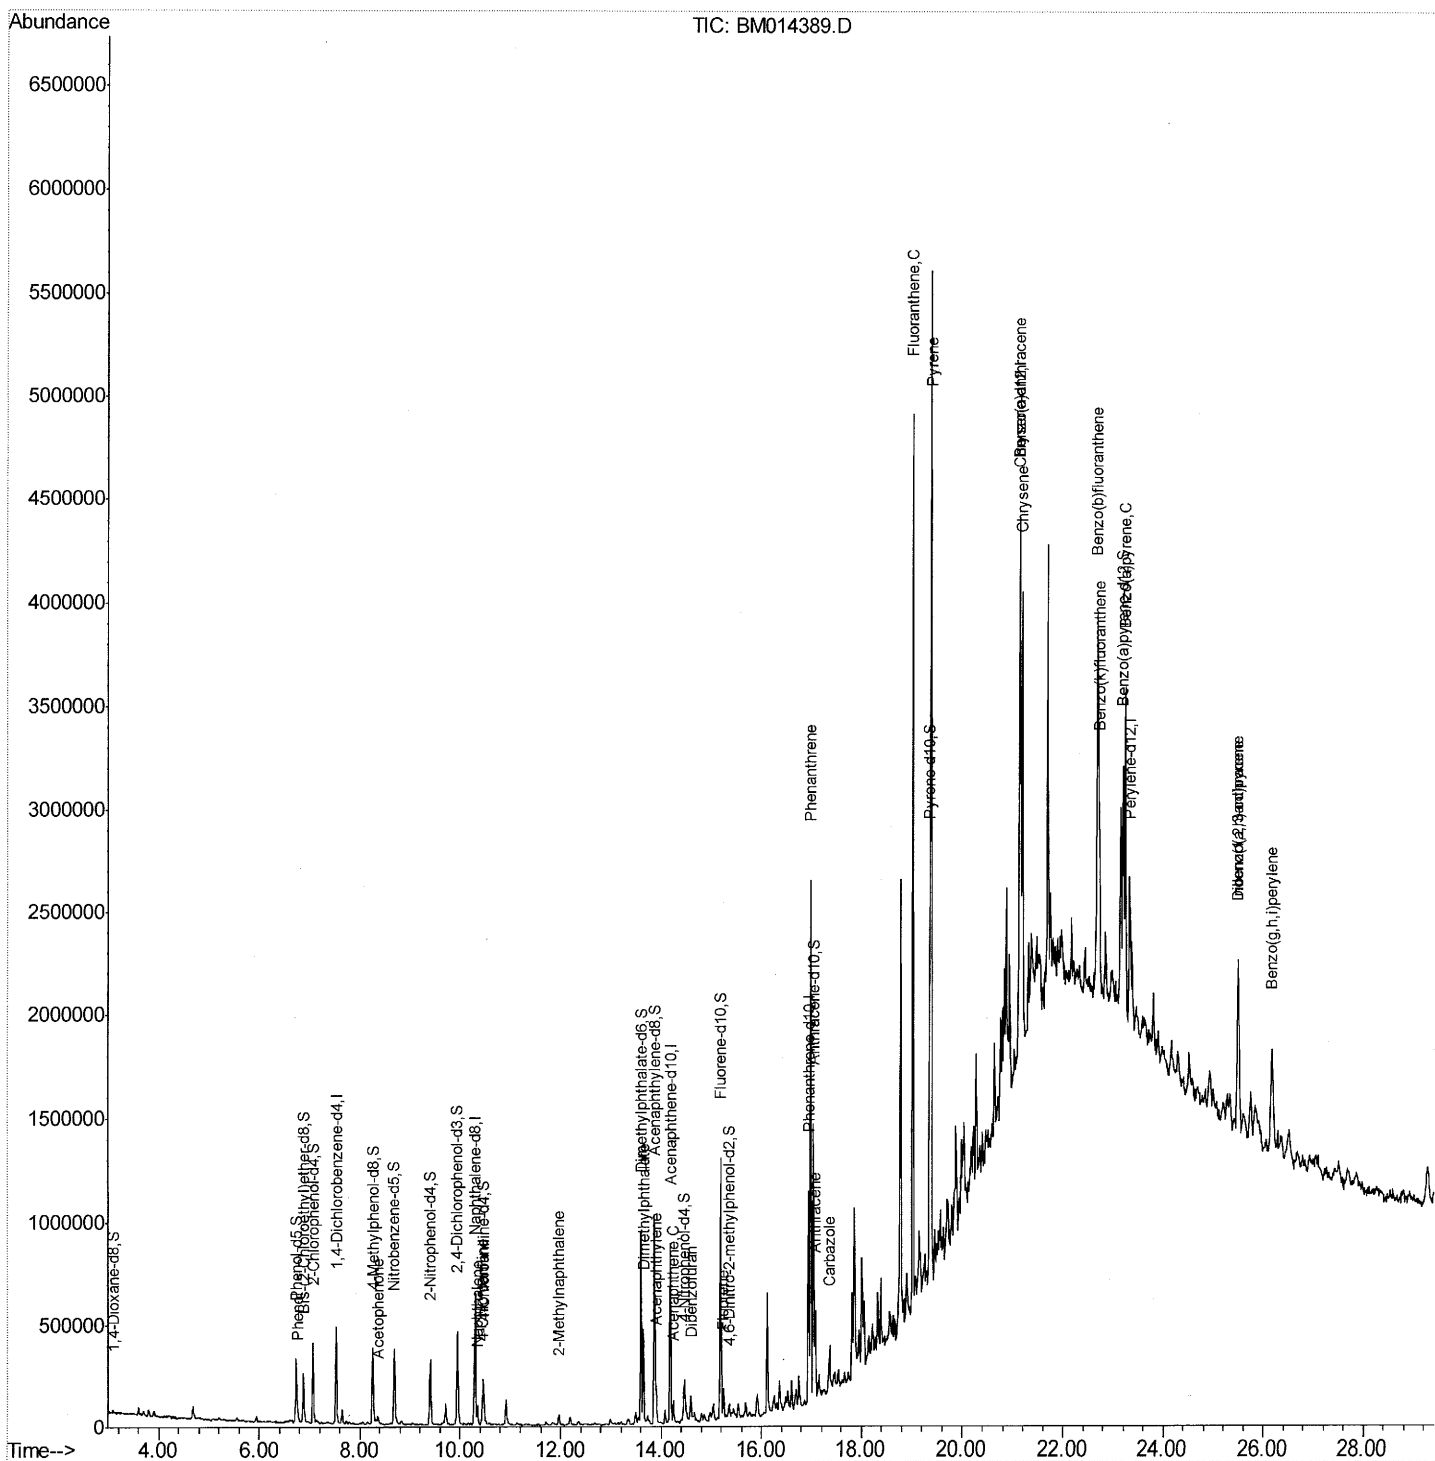

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM022718\
Data File : BM014389.D
Acq On : 27 Feb 2018 19:02
Operator : SJ/JU
Sample : J1631-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BE609

Manual Integrations
APPROVED

Sohil
2/28/2018 1:59:22 PM

Quant Time: Feb 28 00:47:08 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 28 00:45:45 2018
Response via : Initial Calibration

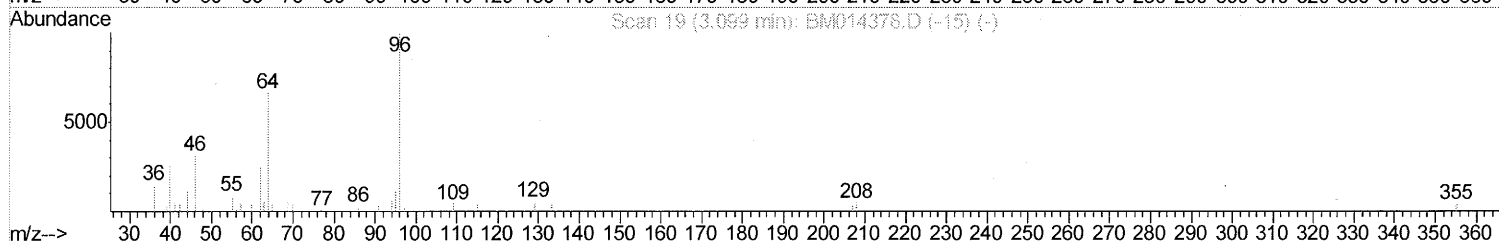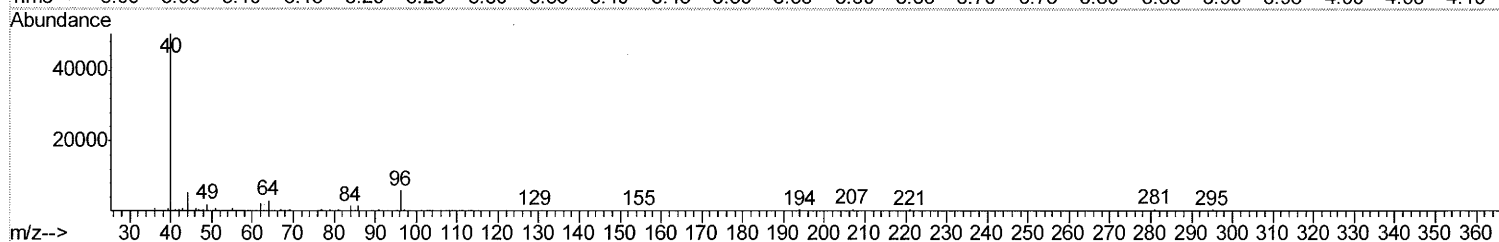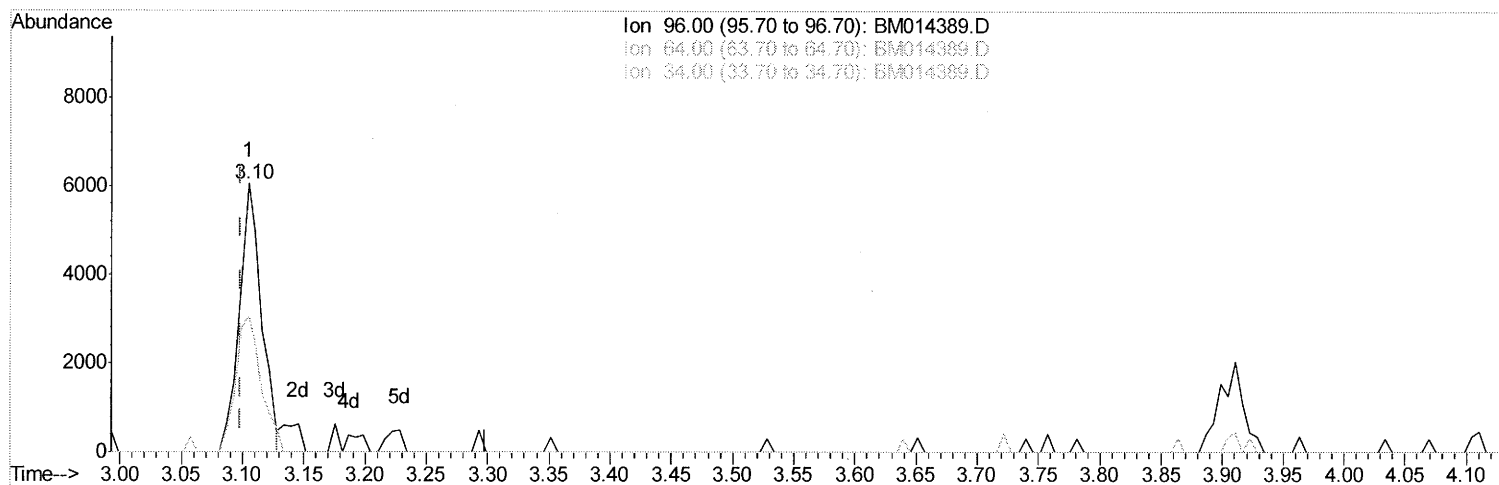

TIC: BM014389.D

(3) 1,4-Dioxane-d8 (S)

3.105min (+0.006) 3.07ng/uL

response 7809

Ion	Exp%	Act%
96.00	100	100
64.00	74.90	58.18#
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM022718\
Data File : BM014389.D
Acq On : 27 Feb 2018 19:02
Operator : SJ/JU
Sample : J1631-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BE609

Manual Integrations
APPROVED

Sohil
2/28/2018 1:59:22 PM

Quant Time: Feb 28 00:47:08 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 28 00:45:45 2018
Response via : Initial Calibration

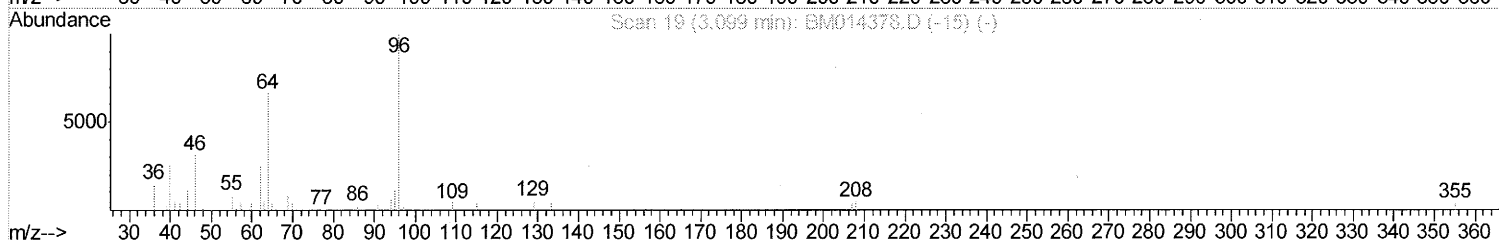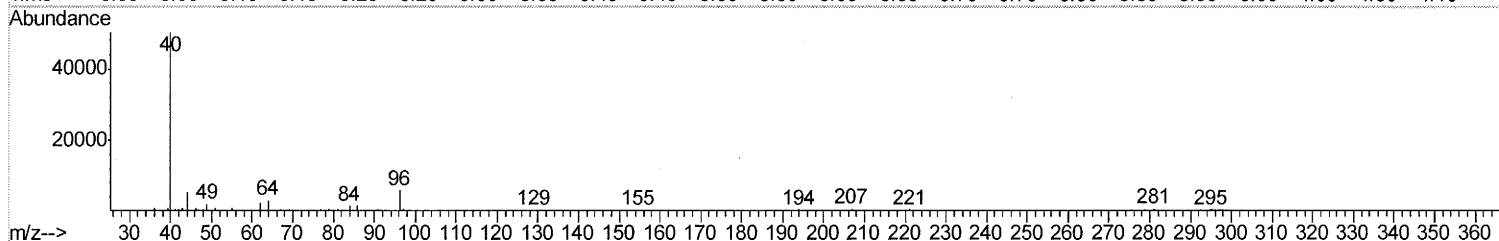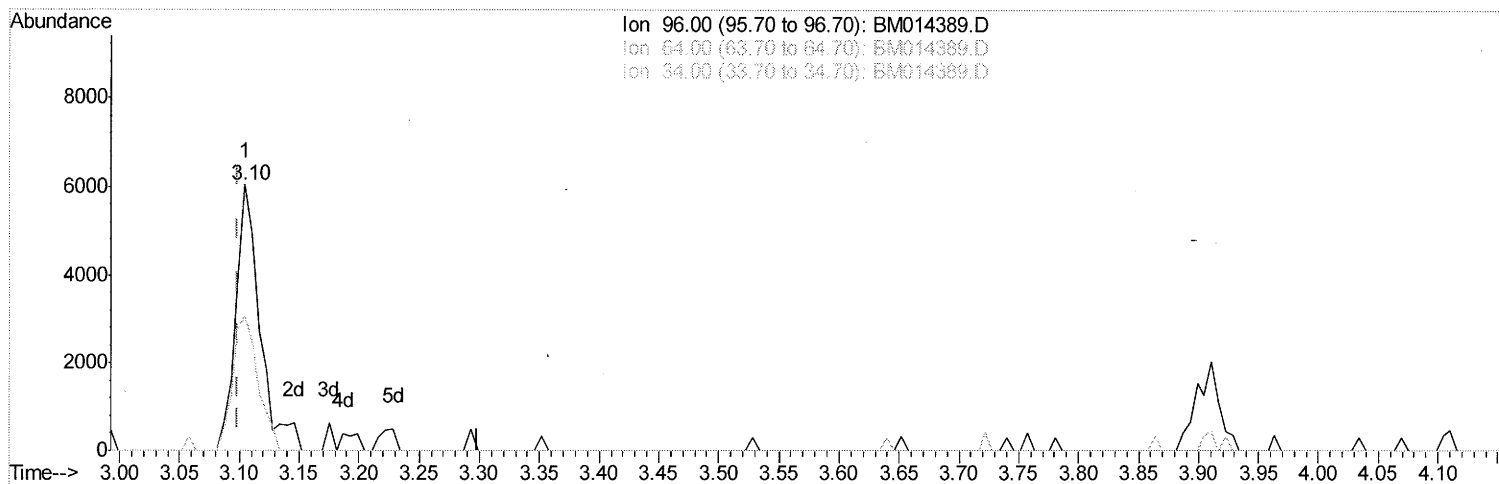

TIC: BM014389.D

(3) 1,4-Dioxane-d8 (S)

3.105min (+0.006) 3.32ng/uL m

response 8440

Ion	Exp%	Act%
96.00	100	100
64.00	74.90	53.83#
34.00	0.00	0.00
0.00	0.00	0.00

SJ 2/28/18

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM022718\
Data File : BM014389.D
Acq On : 27 Feb 2018 19:02
Operator : SJ/JU
Sample : J1631-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BE609

Manual Integrations
APPROVED

Sohil
2/28/2018 1:59:22 PM

Quant Time: Feb 28 01:52:21 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 28 00:45:45 2018
Response via : Initial Calibration

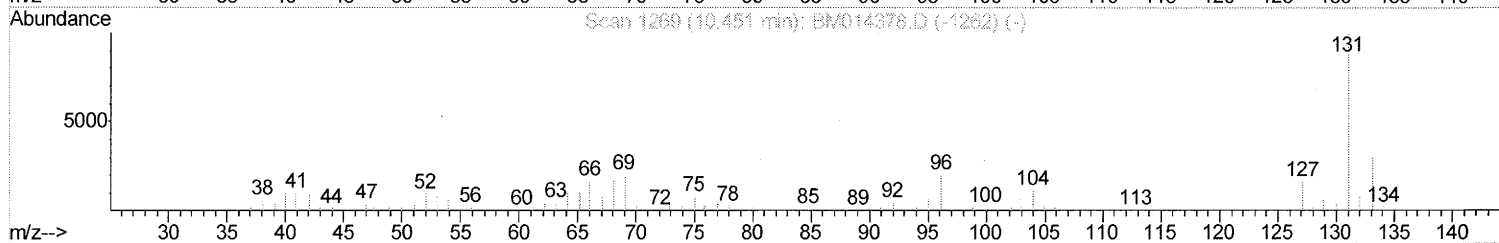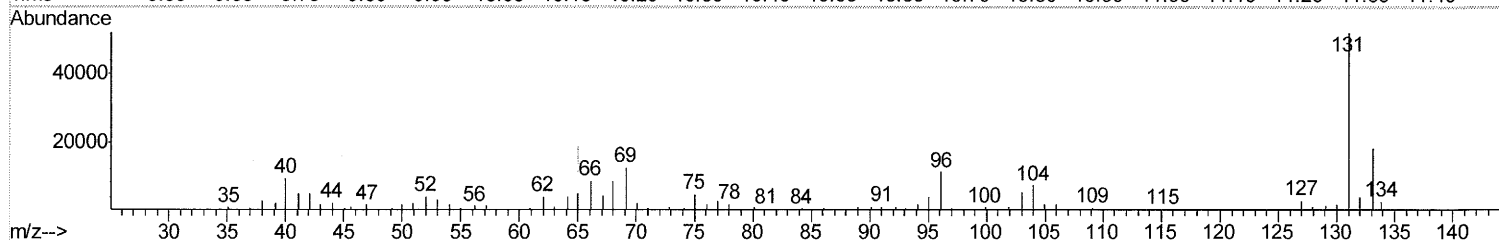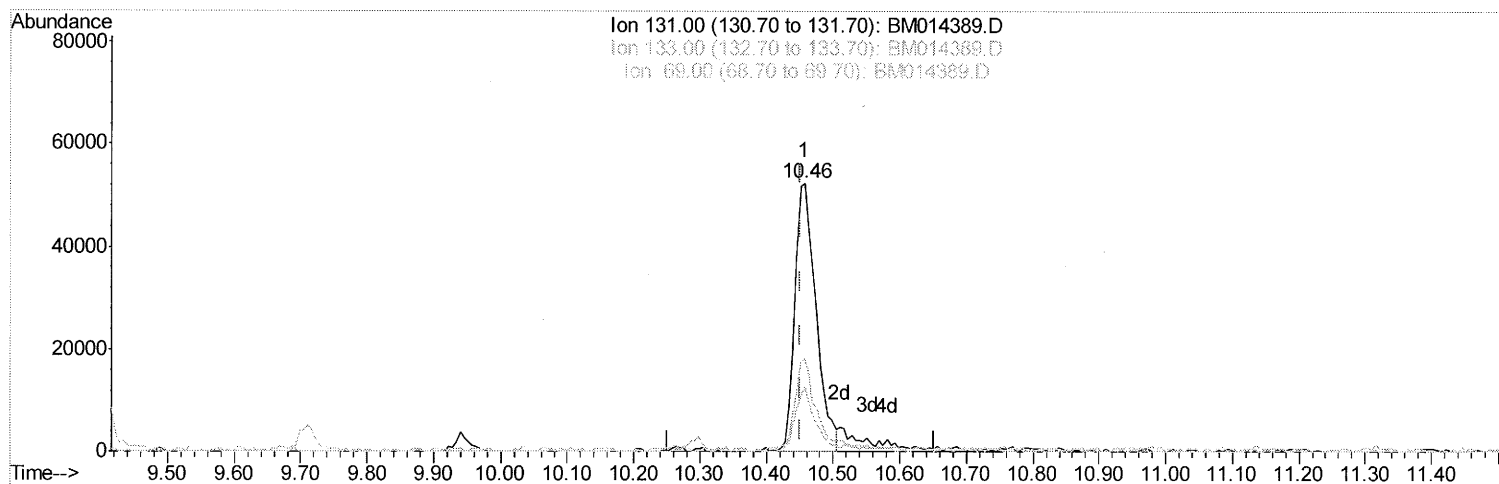

TIC: BM014389.D

(29) 4-Chloroaniline-d4 (S)

10.457min (+0.006) 16.42ng/ul

response 114694

Ion	Exp%	Act%
131.00	100	100
133.00	31.40	34.51
69.00	24.30	24.03
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM022718\
Data File : BM014389.D
Acq On : 27 Feb 2018 19:02
Operator : SJ/JU
Sample : J1631-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BE609

Manual Integrations
APPROVED

Sohil
2/28/2018 1:59:22 PM

Quant Time: Feb 28 01:52:21 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 28 00:45:45 2018
Response via : Initial Calibration

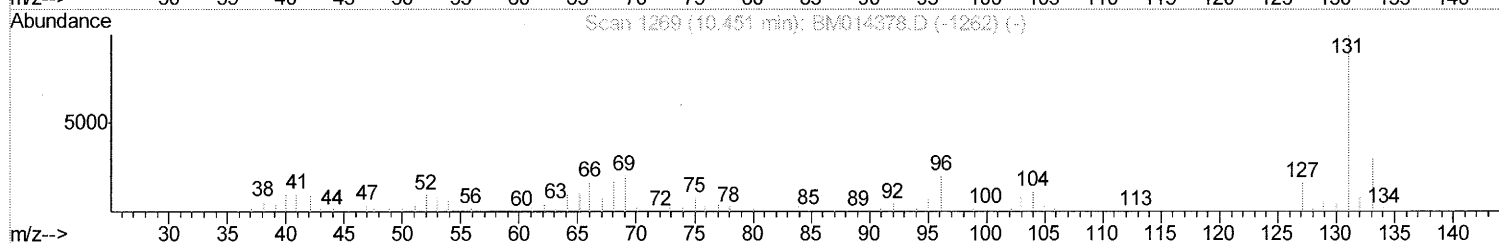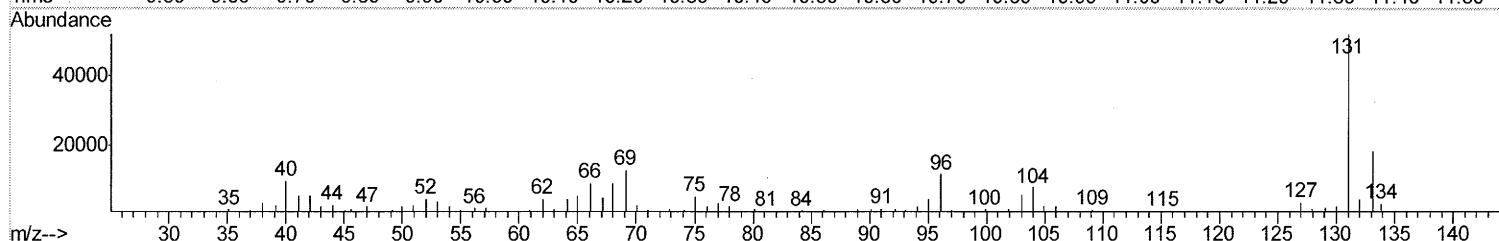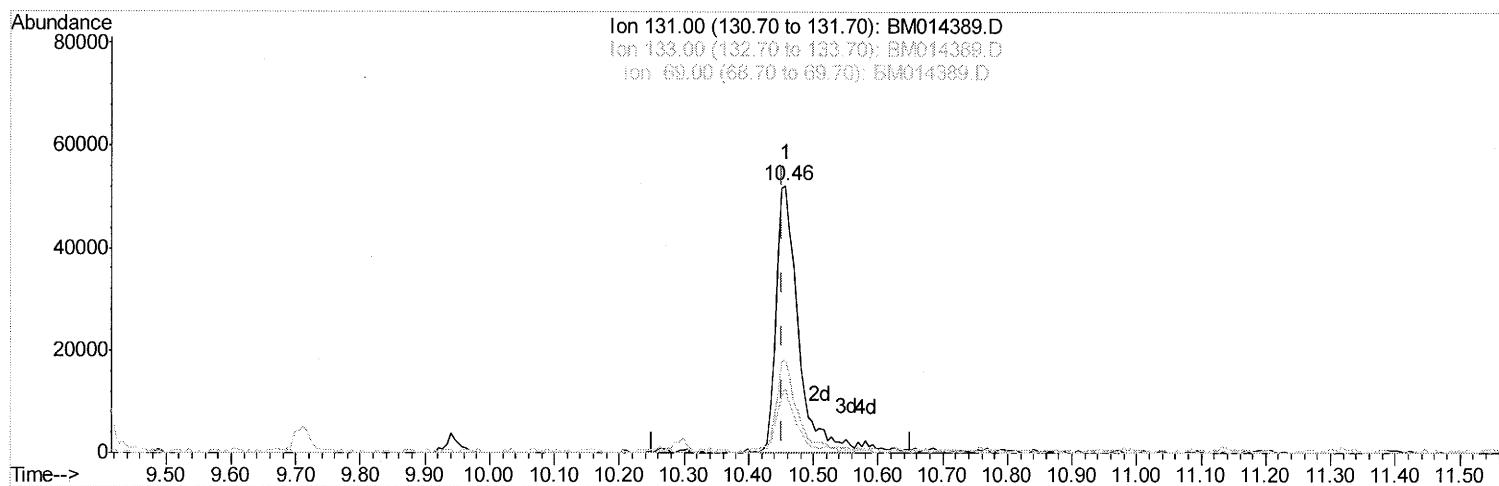

TIC: BM014389.D

(29) 4-Chloroaniline-d4 (S)

10.457min (+0.006) 17.74ng/ul m

response 123931

Ion	Exp%	Act%
131.00	100	100
133.00	31.40	34.51
69.00	24.30	24.03
0.00	0.00	0.00

not 28/28

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM022718\
Data File : BM014389.D
Acq On : 27 Feb 2018 19:02
Operator : SJ/JU
Sample : J1631-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE609

Manual Integrations
APPROVED

Sohil
2/28/2018 1:59:22 PM

Quant Time: Feb 28 01:53:14 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 28 00:45:45 2018
Response via : Initial Calibration

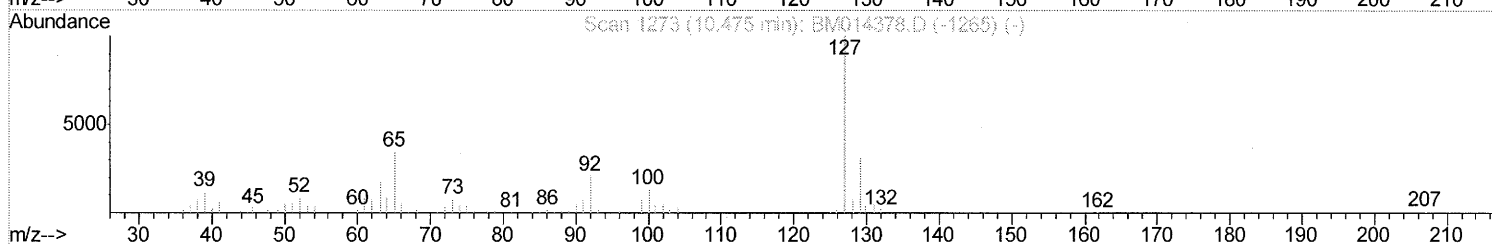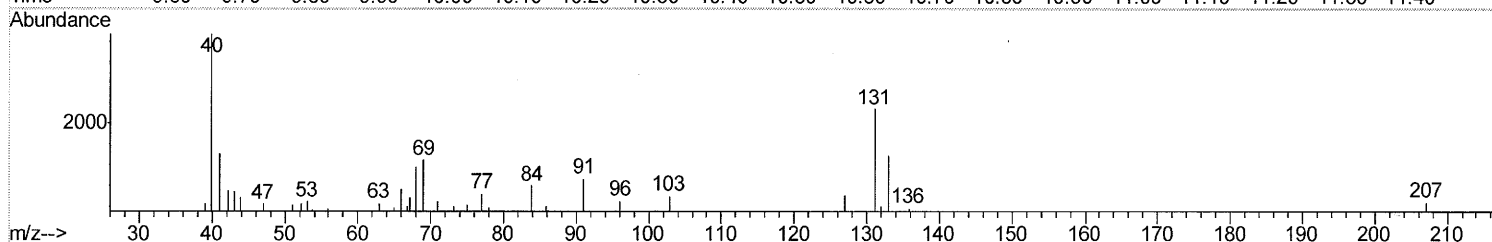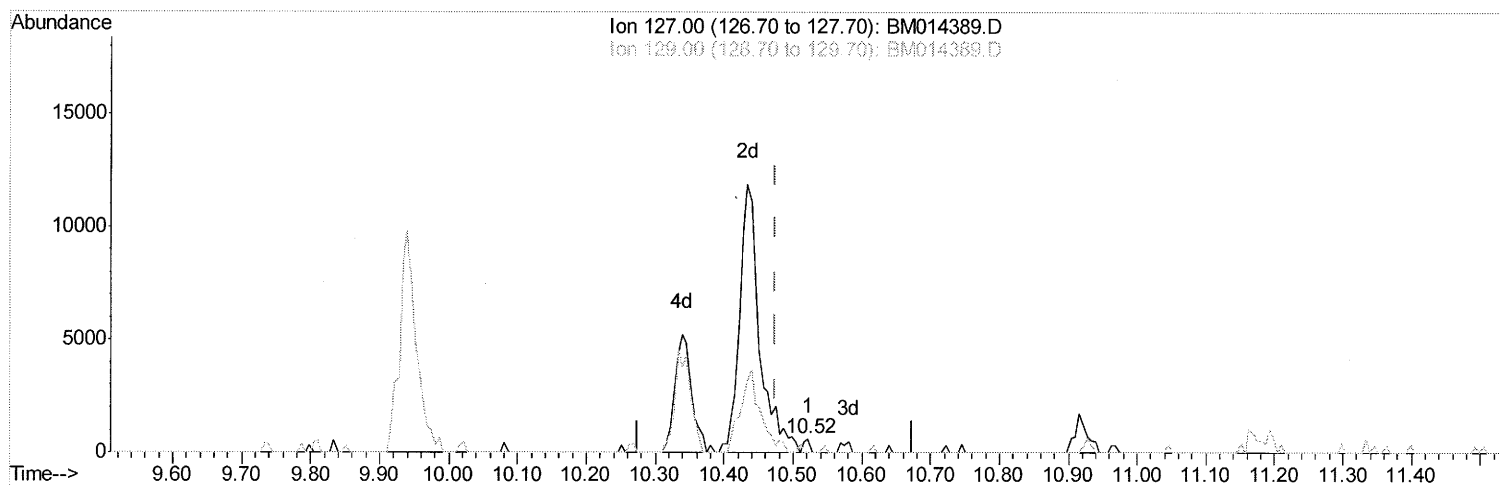

TIC: BM014389.D

(30) 4-Chloroaniline

10.522min (+0.047) 0.05ng/ul

response 386

Ion	Exp%	Act%
127.00	100	100
129.00	35.50	0.00#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM022718\
Data File : BM014389.D
Acq On : 27 Feb 2018 19:02
Operator : SJ/JU
Sample : J1631-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BE609

Manual Integrations
APPROVED

Sohil
2/28/2018 1:59:22 PM

Quant Time: Feb 28 01:53:14 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 28 00:45:45 2018
Response via : Initial Calibration

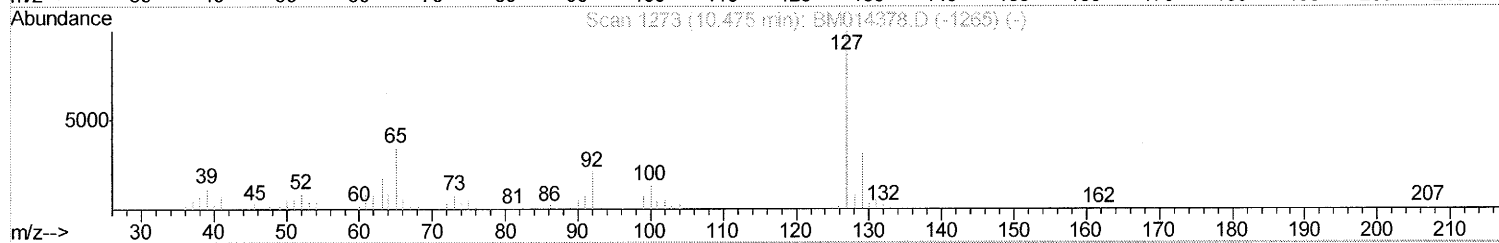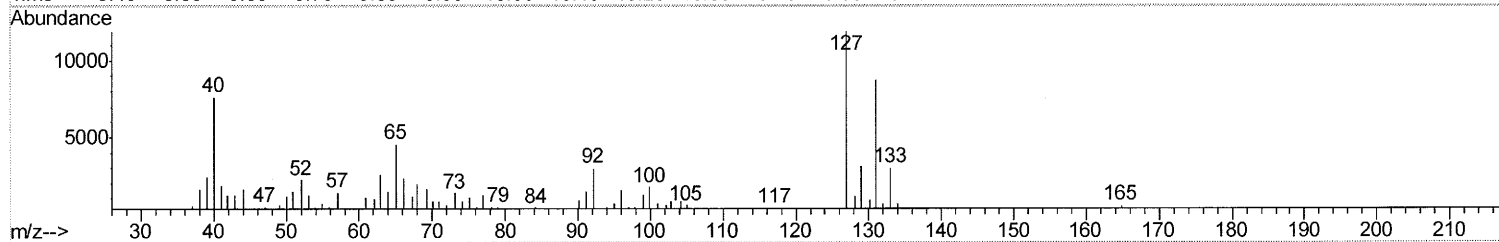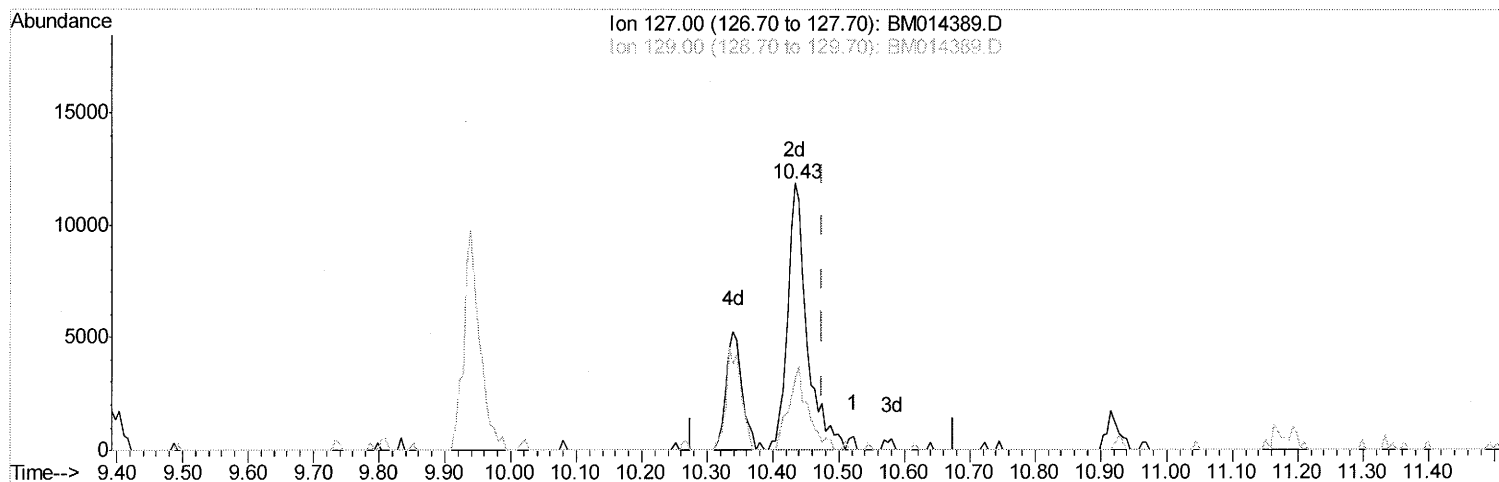

TIC: BM014389.D

(30) 4-Chloroaniline

10.434min (-0.041) 3.42ng/ul m

response 24329

Ion	Exp%	Act%
127.00	100	100
129.00	35.50	26.38#
0.00	0.00	0.00
0.00	0.00	0.00

Handwritten signature

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM022718\
Data File : BM014389.D
Acq On : 27 Feb 2018 19:02
Operator : SJ/JU
Sample : J1631-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE609

Manual Integrations
APPROVED

Sohil
2/28/2018 1:59:22 PM

Quant Time: Feb 28 01:53:14 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 28 00:45:45 2018
Response via : Initial Calibration

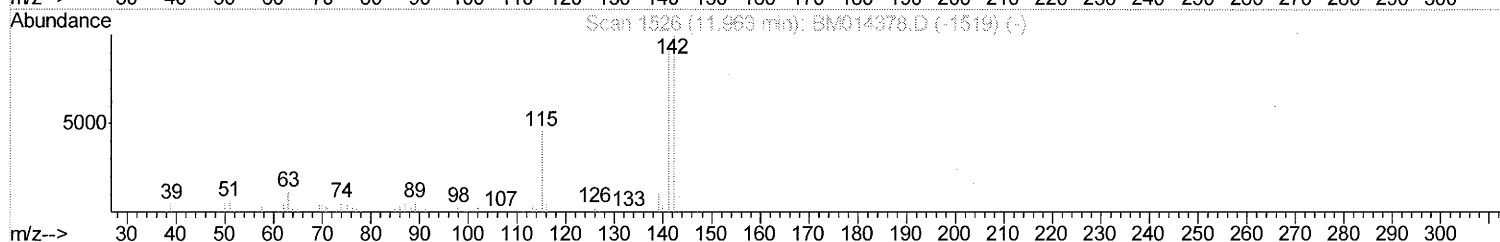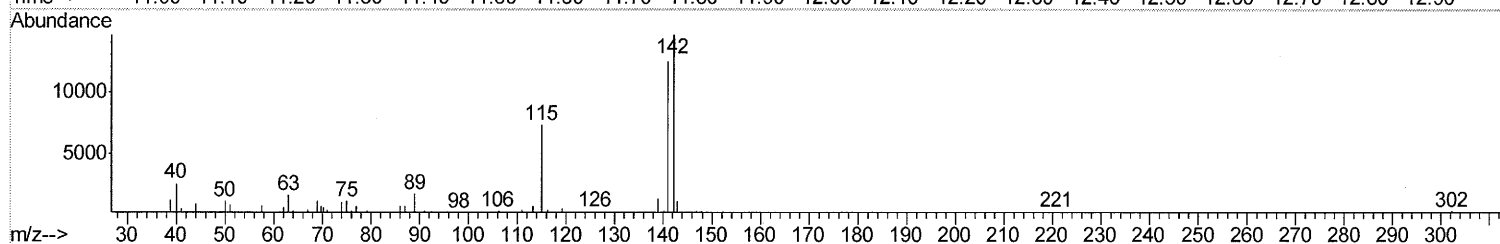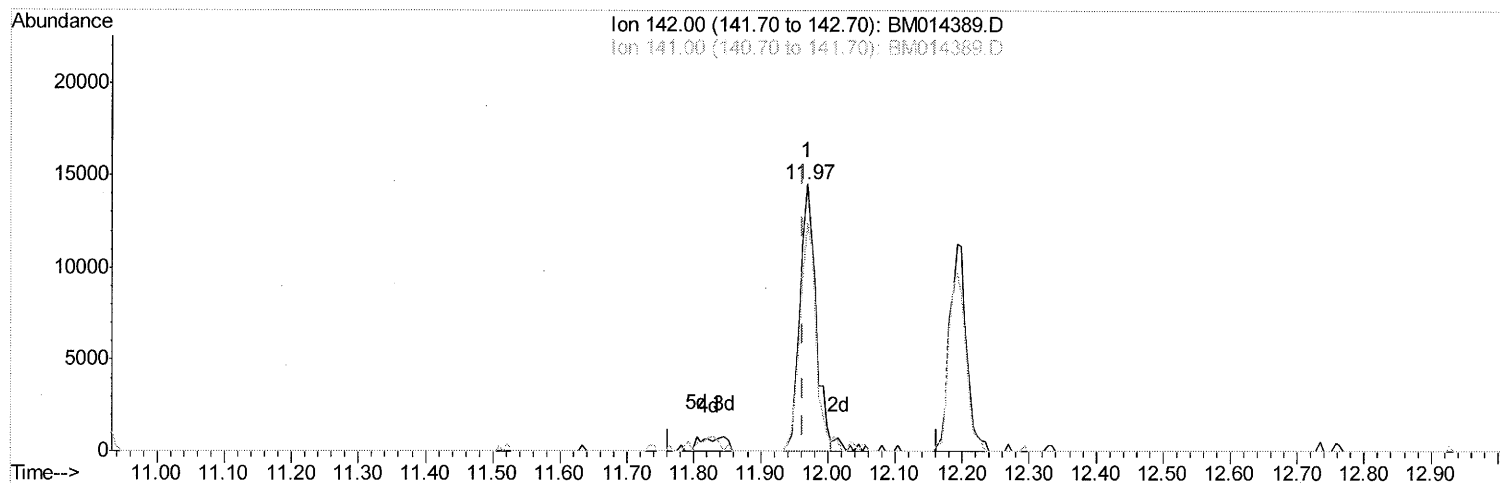

TIC: BM014389.D

(34) 2-Methylnaphthalene

11.969min (+0.006) 1.37ng/ul

response 24014

Ion	Exp%	Act%
142.00	100	100
141.00	92.60	85.34
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM022718\
 Data File : BM014389.D
 Acq On : 27 Feb 2018 19:02
 Operator : SJ/JU
 Sample : J1631-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BE609

Manual Integrations
 APPROVED

Sohil
 2/28/2018 1:59:22 PM

Quant Time: Feb 28 01:53:14 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 28 00:45:45 2018
 Response via : Initial Calibration

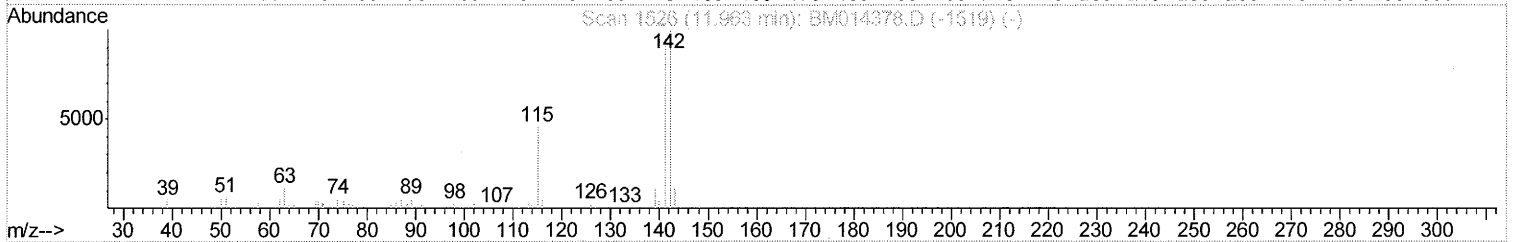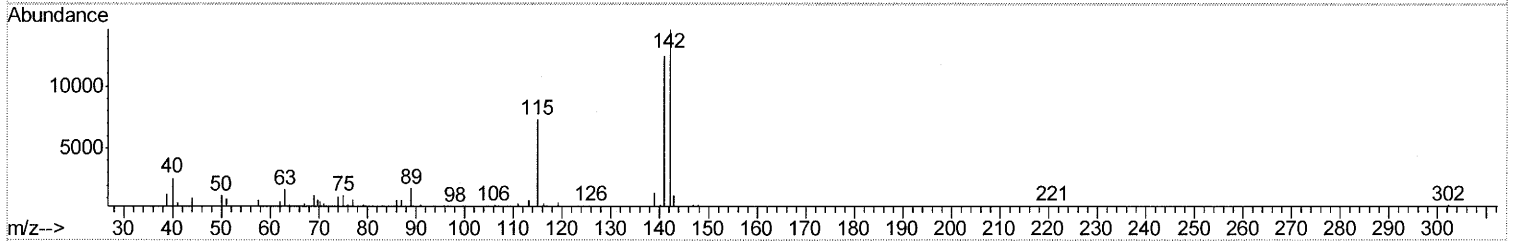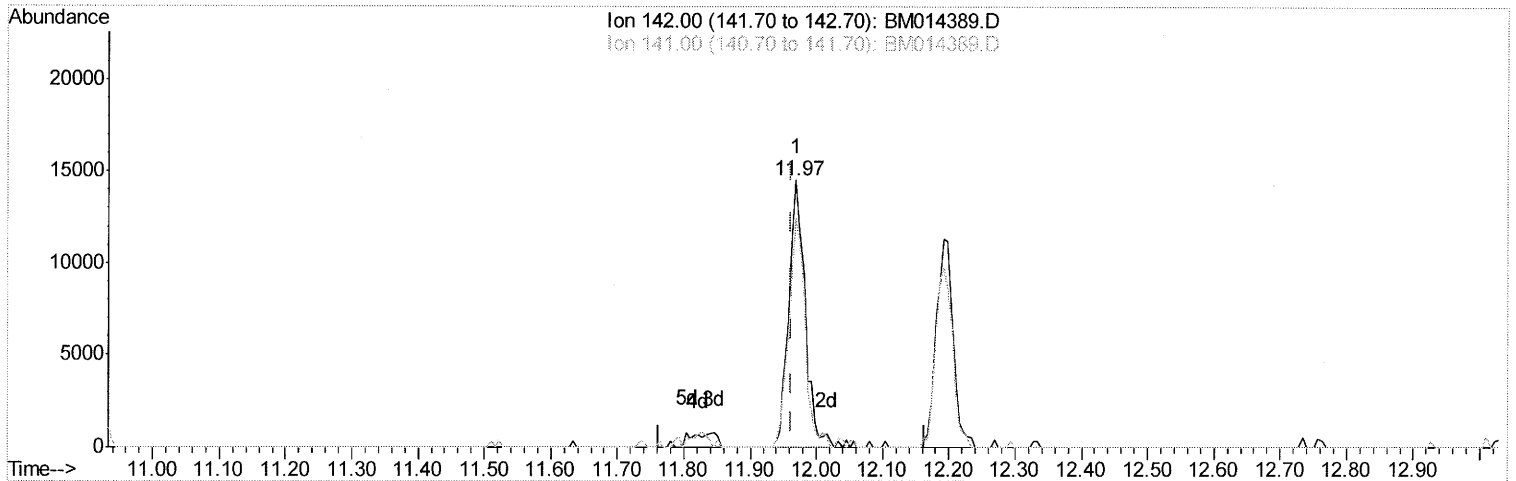

TIC: BM014389.D

(34) 2-Methylnaphthalene

11.969min (+0.006) 1.41ng/ul m

response 24615

Ion	Exp%	Act%
142.00	100	100
141.00	92.60	85.34
0.00	0.00	0.00
0.00	0.00	0.00

per 2/28/18

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM022718\
Data File : BM014389.D
Acq On : 27 Feb 2018 19:02
Operator : SJ/JU
Sample : J1631-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BE609

Manual Integrations
APPROVED

Sohil
2/28/2018 1:59:22 PM

Quant Time: Feb 28 01:53:14 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 28 00:45:45 2018
Response via : Initial Calibration

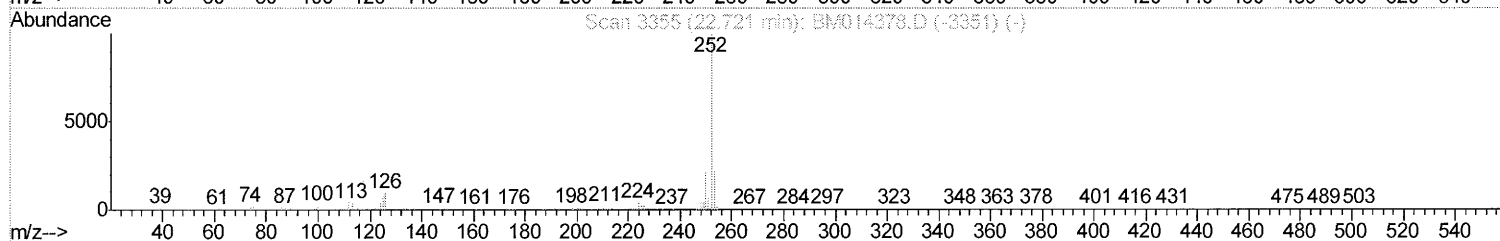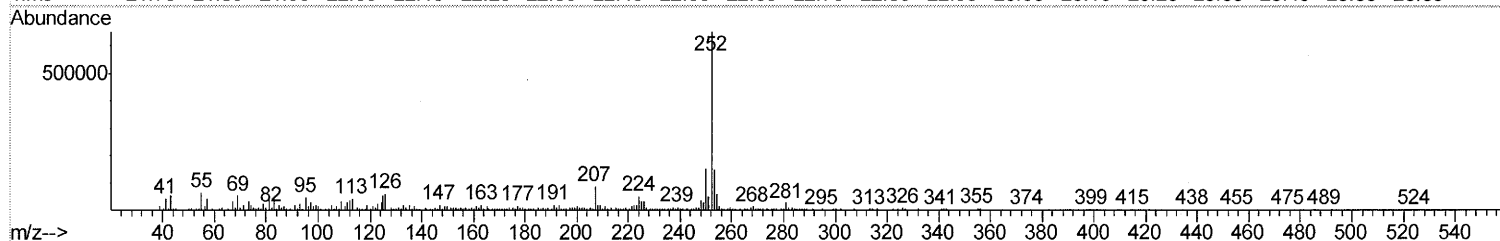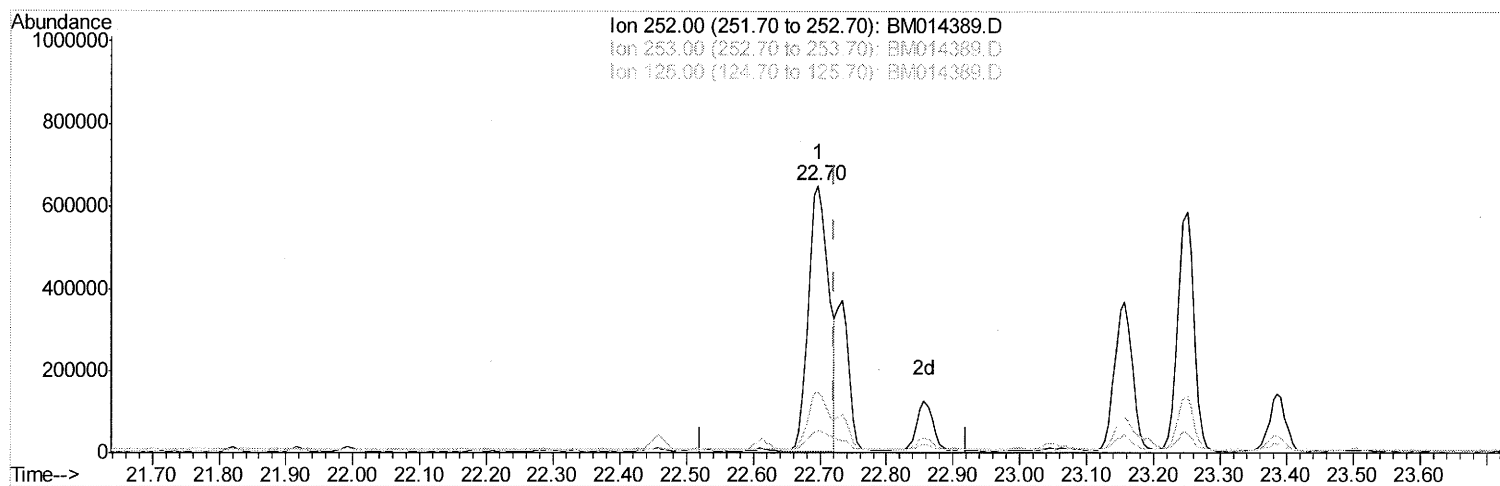

TIC: BM014389.D

(86) Benzo(k)fluoranthene

22.697min (-0.024) 44.35ng/ul

response 1397288

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	22.65
125.00	4.30	8.05#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA M\Data\BM022718\
Data File : BM014389.D
Acq On : 27 Feb 2018 19:02
Operator : SJ/JU
Sample : J1631-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BE609

Manual Integrations
APPROVED

Sohil
2/28/2018 1:59:22 PM

Quant Time: Feb 28 01:53:14 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 28 00:45:45 2018
Response via : Initial Calibration

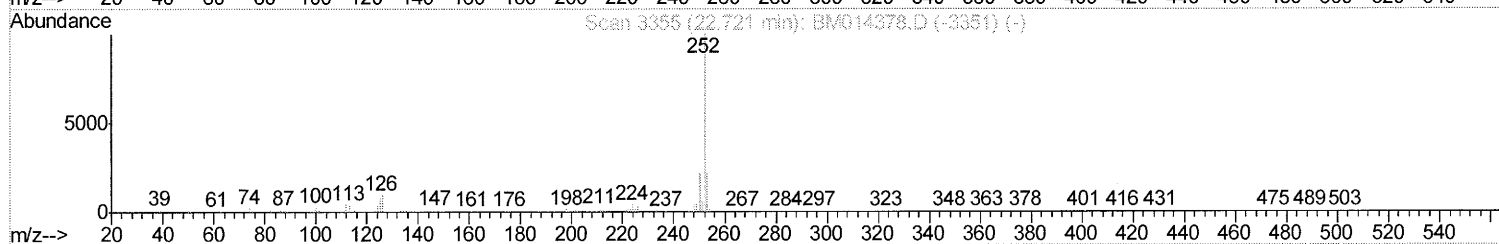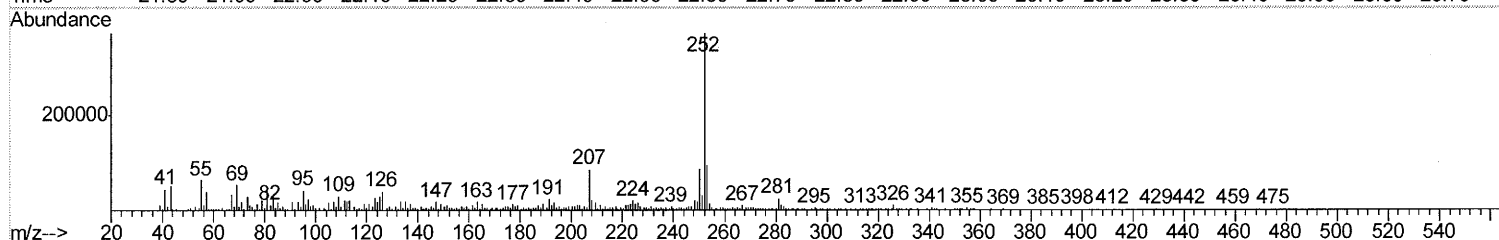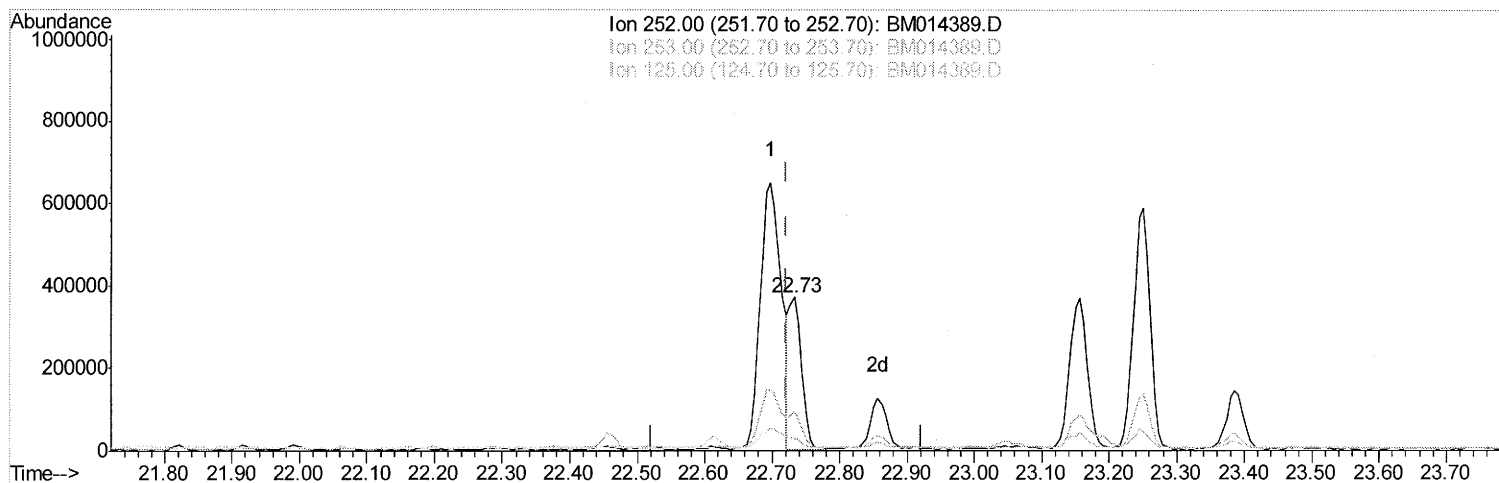

TIC: BM014389.D

(86) Benzo(k)fluoranthene

22.733min (+0.012) 14.82ng/ul m

response 466822

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	25.39
125.00	4.30	7.77#
0.00	0.00	0.00

per 2/28/18

Data Path : Z:\HPCHEM1\BNA M\Data\BM022718\
 Data File : BM014389.D
 Acq On : 27 Feb 2018 19:02
 Operator : SJ/JU
 Sample : J1631-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 BE609

Manual Integrations
 APPROVED

Sohil
 2/28/2018 1:59:22 PM

Quant Time: Feb 28 01:56:15 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 28 00:45:45 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.52	152	108773	20.00	ng/ul	0.00
18) Naphthalene-d8	10.29	136	447510	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.18	164	260407	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.94	188	518944	20.00	ng/ul	0.00
75) Chrysene-d12	21.16	240	503174	20.00	ng/ul	0.00
83) Perylene-d12	23.34	264	494908	20.00	ng/ul	0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.10	96	8440m	3.32	ng/ul	0.00
5) Phenol-d5	6.73	99	169574	18.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.87	67	101983	18.33	ng/ul	0.00
9) 2-Chlorophenol-d4	7.06	132	141466	20.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.25	113	138213	17.18	ng/ul	0.01
19) Nitrobenzene-d5	8.68	128	73900	22.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.40	143	83603	24.42	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.94	165	159039	22.43	ng/ul	0.01
29) 4-Chloroaniline-d4	10.46	131	123931m	17.74	ng/ul	0.00
43) Dimethylphthalate-d6	13.60	166	530195	24.65	ng/ul	0.00
46) Acenaphthylene-d8	13.87	160	658692	24.84	ng/ul	0.01
51) 4-Nitrophenol-d4	14.46	143	53983	18.18	ng/ul	0.03
57) Fluorene-d10	15.19	176	445257	23.11	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.35	200	8964	2.88	ng/ul	0.01
70) Anthracene-d10	17.04	188	668407	26.70	ng/ul	0.00
76) Pyrene-d10	19.35	212	673316	25.94	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.20	264	619261	25.71	ng/ul	0.02

Target Compounds

					Ovalue
6) Phenol	6.76	94	26967	2.795	ng/ul 90
14) Acetophenone	8.36	105	21432	1.544	ng/ul 85
28) Naphthalene	10.34	128	68791	2.993	ng/ul 96
30) 4-Chloroaniline	10.43	127	24329m	3.415	ng/ul
34) 2-Methylnaphthalene	11.97	142	24615m	1.407	ng/ul
44) Dimethylphthalate	13.65	163	233312	11.002	ng/ul 100
47) Acenaphthylene	13.90	152	111923	4.465	ng/ul 97
49) Acenaphthene	14.25	153	41291	2.340	ng/ul 90
53) Dibenzofuran	14.59	168	45826	1.732	ng/ul 100
58) Fluorene	15.24	166	60223	2.636	ng/ul# 97
69) Phenanthrene	16.99	178	1320689	44.171	ng/ul 99
71) Anthracene	17.08	178	246667	8.203	ng/ul 97
72) Carbazole	17.36	167	109697	4.339	ng/ul 98
74) Fluoranthene	19.02	202	2313829	64.773	ng/ul# 95
77) Pyrene	19.39	202	2129587	63.685	ng/ul# 92
80) Benzo(a)anthracene	21.14	228	1082123	34.459	ng/ul 96
82) Chrysene	21.20	228	1119305	38.208	ng/ul 98
85) Benzo(b)fluoranthene	22.70	252	1397288	42.166	ng/ul# 98
86) Benzo(k)fluoranthene	22.73	252	466822m	14.817	ng/ul
88) Benzo(a)pyrene	23.25	252	1004296	33.915	ng/ul# 97
89) Indeno(1,2,3-cd)pyrene	25.51	276	672648	23.409	ng/ul# 96
90) Dibenzo(a,h)anthracene	25.51	278	180416	7.556	ng/ul# 82
91) Benzo(g,h,i)perylene	26.17	276	494415	21.240	ng/ul# 95

Data Path : Z:\HPCHEM1\BNA M\Data\BM022718\
Data File : BM014389.D
Acq On : 27 Feb 2018 19:02
Operator : SJ/JU
Sample : J1631-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BE609

Manual Integrations
APPROVED

Sohil
2/28/2018 1:59:22 PM

Quant Time: Feb 28 01:56:15 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 28 00:45:45 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed