

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022718\  
 Data File : BM014388.D  
 Acq On : 27 Feb 2018 18:26  
 Operator : SJ/JU  
 Sample : J1631-10  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 BE5Z1

Manual Integrations  
 APPROVED

Sohil  
 2/28/2018 1:59:19 PM

Quant Time: Feb 28 01:35:34 2018  
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Wed Feb 28 00:45:45 2018  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 7.52  | 152  | 106534   | 20.00 | ng/ul | 0.00     |
| 18) Naphthalene-d8        | 10.29 | 136  | 453752   | 20.00 | ng/ul | 0.00     |
| 35) Acenaphthene-d10      | 14.18 | 164  | 255362   | 20.00 | ng/ul | 0.00     |
| 61) Phenanthrene-d10      | 16.94 | 188  | 519589   | 20.00 | ng/ul | 0.00     |
| 75) Chrysene-d12          | 21.16 | 240  | 511403   | 20.00 | ng/ul | 0.01     |
| 83) Perylene-d12          | 23.34 | 264  | 488274   | 20.00 | ng/ul | 0.02     |

## System Monitoring Compounds

|                                |       |     |         |       |       |      |
|--------------------------------|-------|-----|---------|-------|-------|------|
| 3) 1,4-Dioxane-d8              | 3.10  | 96  | 16359m  | 6.57  | ng/uL | 0.00 |
| 5) Phenol-d5                   | 6.73  | 99  | 282200  | 31.34 | ng/ul | 0.00 |
| 7) Bis-(2-Chloroethyl)ether-d  | 6.87  | 67  | 185228  | 33.98 | ng/ul | 0.00 |
| 9) 2-Chlorophenol-d4           | 7.06  | 132 | 243653  | 35.29 | ng/ul | 0.00 |
| 13) 4-Methylphenol-d8          | 8.25  | 113 | 200233  | 25.42 | ng/ul | 0.01 |
| 19) Nitrobenzene-d5            | 8.68  | 128 | 125583  | 37.45 | ng/ul | 0.00 |
| 22) 2-Nitrophenol-d4           | 9.40  | 143 | 130159  | 37.50 | ng/ul | 0.00 |
| 26) 2,4-Dichlorophenol-d3      | 9.94  | 165 | 241159  | 33.55 | ng/ul | 0.01 |
| 29) 4-Chloroaniline-d4         | 10.46 | 131 | 137866  | 19.47 | ng/ul | 0.00 |
| 43) Dimethylphthalate-d6       | 13.60 | 166 | 768643  | 36.45 | ng/ul | 0.00 |
| 46) Acenaphthylene-d8          | 13.87 | 160 | 975974  | 37.53 | ng/ul | 0.01 |
| 51) 4-Nitrophenol-d4           | 14.45 | 143 | 72758   | 24.99 | ng/ul | 0.02 |
| 57) Fluorene-d10               | 15.19 | 176 | 644823  | 34.13 | ng/ul | 0.00 |
| 62) 4,6-Dinitro-2-methylphenol | 15.36 | 200 | 16307   | 5.23  | ng/ul | 0.02 |
| 70) Anthracene-d10             | 17.04 | 188 | 955853  | 38.13 | ng/ul | 0.00 |
| 76) Pyrene-d10                 | 19.36 | 212 | 1002734 | 38.02 | ng/ul | 0.01 |
| 87) Benzo(a)pyrene-d12         | 23.21 | 264 | 907302  | 38.18 | ng/ul | 0.02 |

## Target Compounds

|                            |       |     |         |         | Ovalue |    |
|----------------------------|-------|-----|---------|---------|--------|----|
| 6) Phenol                  | 6.76  | 94  | 39618   | 4.193   | ng/ul  | 92 |
| 14) Acetophenone           | 8.35  | 105 | 24354   | 1.792   | ng/ul# | 95 |
| 28) Naphthalene            | 10.34 | 128 | 169237  | 7.262   | ng/ul  | 99 |
| 34) 2-Methylnaphthalene    | 11.97 | 142 | 35207   | 1.985   | ng/ul  | 98 |
| 44) Dimethylphthalate      | 13.65 | 163 | 448779  | 21.581  | ng/ul  | 97 |
| 47) Acenaphthylene         | 13.90 | 152 | 135305  | 5.505   | ng/ul  | 97 |
| 49) Acenaphthene           | 14.24 | 153 | 83515   | 4.826   | ng/ul  | 96 |
| 53) Dibenzofuran           | 14.59 | 168 | 92064   | 3.548   | ng/ul  | 90 |
| 56) Diethylphthalate       | 15.02 | 149 | 37898   | 1.635   | ng/ul# | 84 |
| 58) Fluorene               | 15.24 | 166 | 119775  | 5.346   | ng/ul# | 97 |
| 69) Phenanthrene           | 16.99 | 178 | 2531911 | 84.576  | ng/ul  | 99 |
| 71) Anthracene             | 17.07 | 178 | 522847  | 17.366  | ng/ul  | 98 |
| 72) Carbazole              | 17.36 | 167 | 224044  | 8.850   | ng/ul  | 98 |
| 74) Fluoranthene           | 19.02 | 202 | 4144001 | 115.863 | ng/ul# | 93 |
| 77) Pyrene                 | 19.39 | 202 | 3652275 | 107.463 | ng/ul# | 91 |
| 80) Benzo(a)anthracene     | 21.14 | 228 | 2036044 | 63.792  | ng/ul  | 99 |
| 82) Chrysene               | 21.20 | 228 | 1838395 | 61.745  | ng/ul  | 98 |
| 85) Benzo(b)fluoranthene   | 22.70 | 252 | 2458811 | 75.207  | ng/ul# | 97 |
| 86) Benzo(k)fluoranthene   | 22.74 | 252 | 773307m | 24.878  | ng/ul  |    |
| 88) Benzo(a)pyrene         | 23.26 | 252 | 1756089 | 60.108  | ng/ul# | 98 |
| 89) Indeno(1,2,3-cd)pyrene | 25.53 | 276 | 1146284 | 40.434  | ng/ul# | 98 |
| 90) Dibenz(a,h)anthracene  | 25.52 | 278 | 338905  | 14.387  | ng/ul# | 83 |
| 91) Benzo(g,h,i)perylene   | 26.20 | 276 | 868685  | 37.825  | ng/ul# | 93 |

Data Path : Z:\HPCHEM1\BNA M\DATA\BM022718\  
Data File : BM014388.D  
Acq On : 27 Feb 2018 18:26  
Operator : SJ/JU  
Sample : J1631-10  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
BE5Z1

Manual Integrations  
APPROVED

Sohil  
2/28/2018 1:59:19 PM

Quant Time: Feb 28 01:35:34 2018  
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Feb 28 00:45:45 2018  
Response via : Initial Calibration

| Internal Standards | R.T. | QIon | Response | Conc | Units | Dev(Min) |
|--------------------|------|------|----------|------|-------|----------|
|--------------------|------|------|----------|------|-------|----------|

|       |  |  |  |  |  |  |
|-------|--|--|--|--|--|--|
| ----- |  |  |  |  |  |  |
| ----- |  |  |  |  |  |  |

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM022718\  
Data File : BM014388.D  
Acq On : 27 Feb 2018 18:26  
Operator : SJ/JU  
Sample : J1631-10  
Misc :  
ALS Vial : 12 Sample Multiplier: 1


Instrument :  
BNA\_M  
ClientSampleID :  
BE5Z1

Quant Time: Feb 28 01:35:34 2018  
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM021418.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Wed Feb 28 00:45:45 2018  
Response via : Initial Calibration

Manual Integrations  
APPROVED

Sohil  
2/28/2018 1:59:19 PM

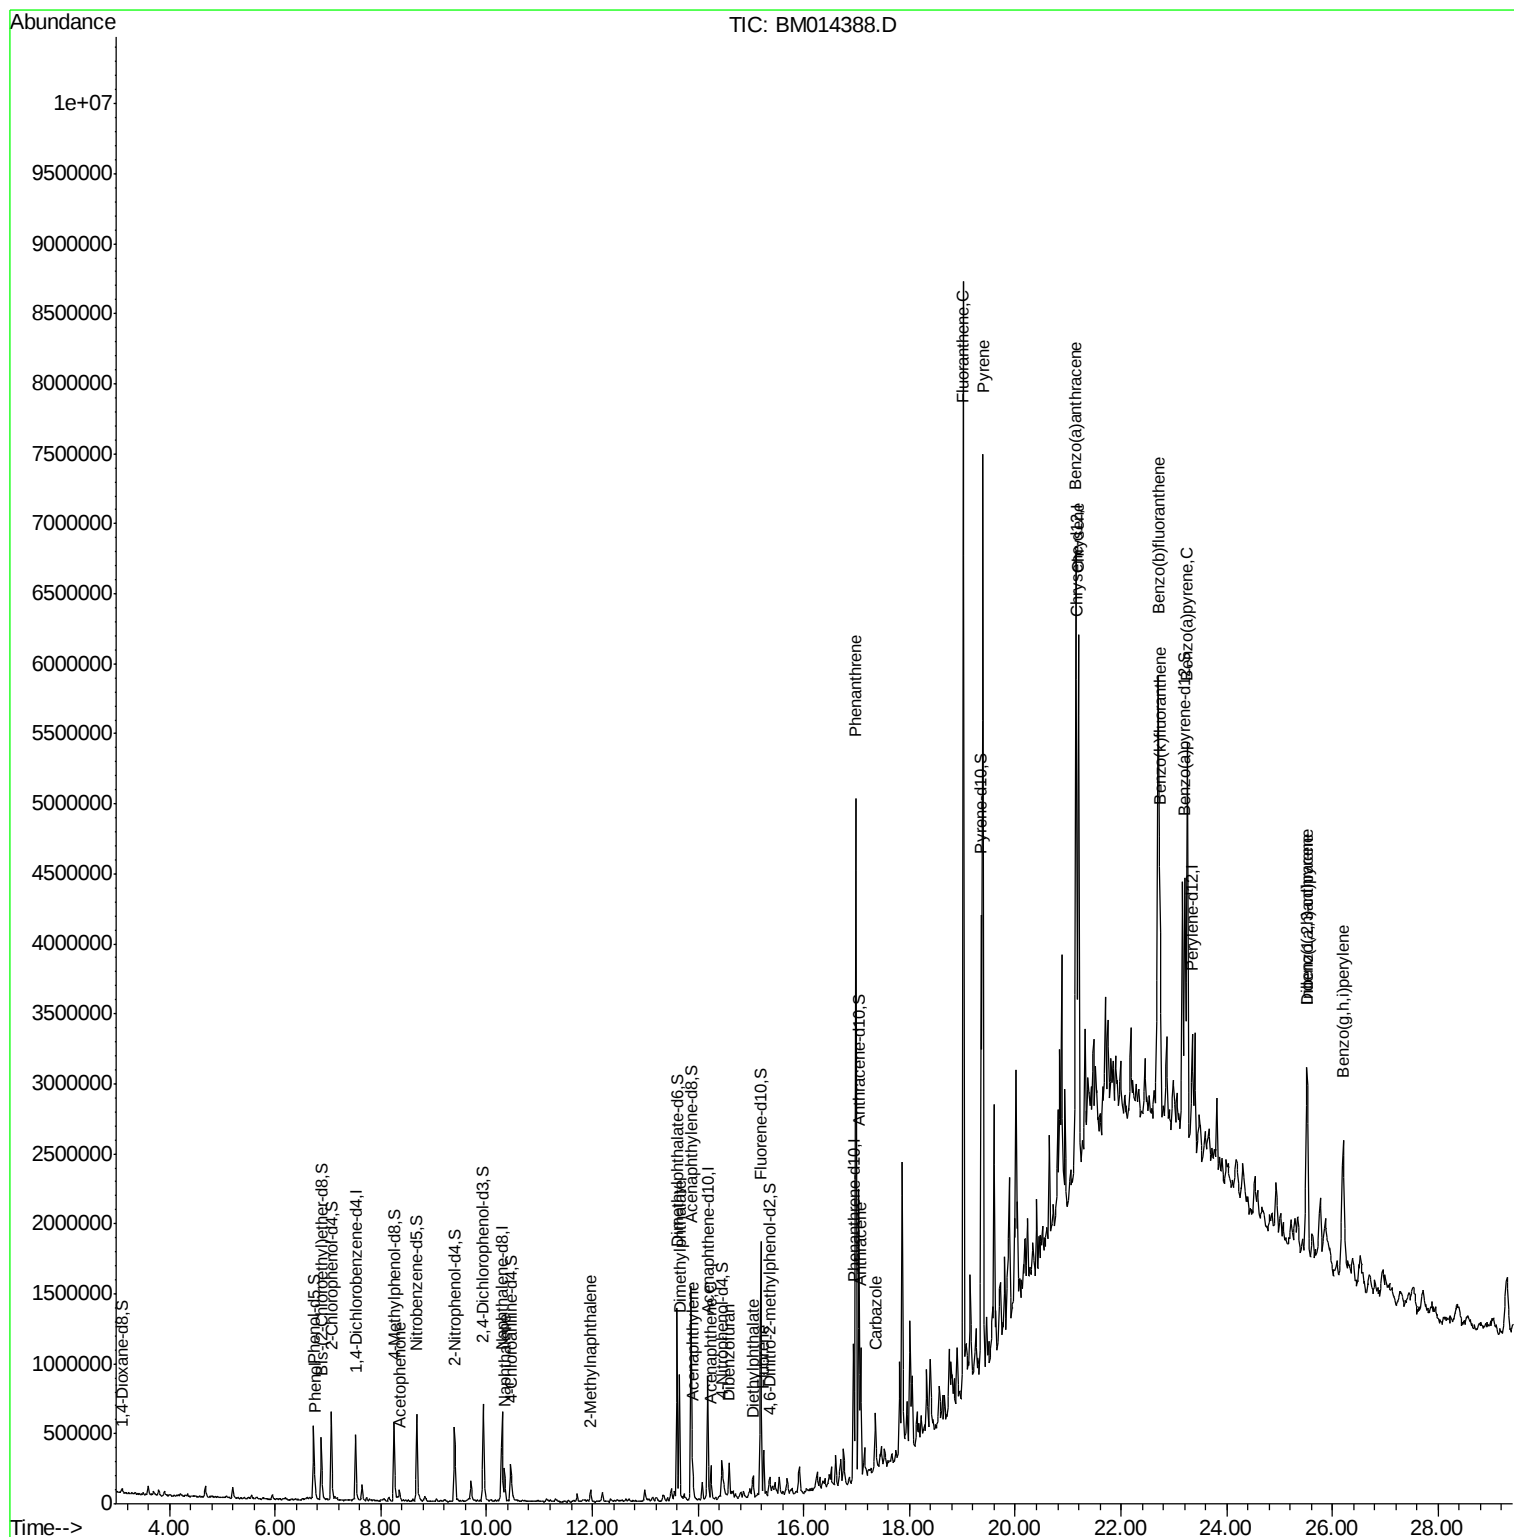

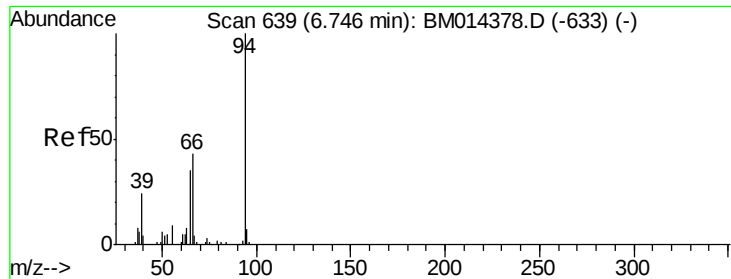

#6

Phenol





Concen: 4.193 ng/ul  
 RT: 6.76 min Scan# 641  
 Delta R.T. 0.01 min  
 Lab File: BM014388.D  
 Acq: 27 Feb 2018 18:26

Instrument :  
 BNA\_M  
 ClientSampled :  
 BE5Z1

| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 94      | 100   |       |       |
| 65      | 36.0  | 28.2  | 42.4  |
| 66      | 67.5  | 47.2  | 70.8  |

Manual Integrations  
 APPROVED

Sohil  
 2/28/2018 1:59:19 PM


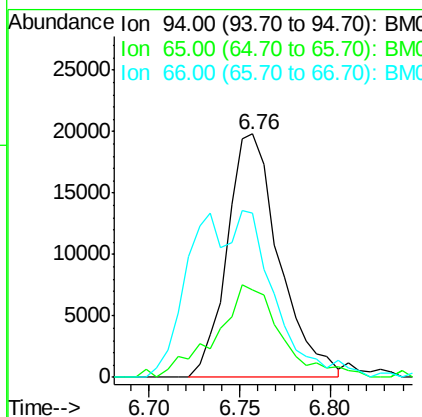
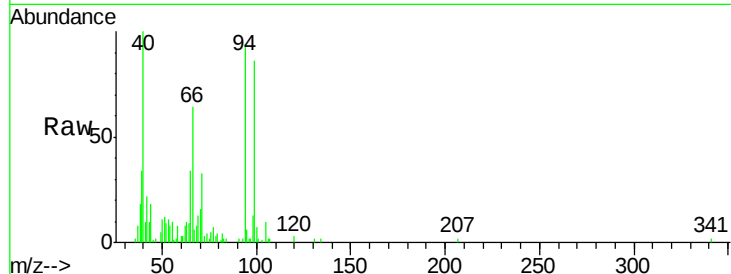



#14

Acetophenone

Concen: 1.792 ng/ul  
 RT: 8.35 min Scan# 912  
 Delta R.T. 0.01 min  
 Lab File: BM014388.D  
 Acq: 27 Feb 2018 18:26

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 105     | 100   |       |       |
| 77      | 91.4  | 74.2  | 111.4 |
| 51      | 38.0  | 23.4  | 35.2  |

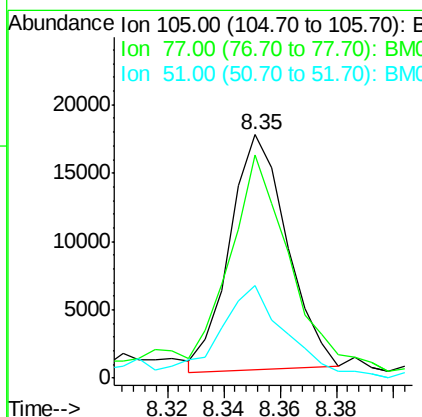

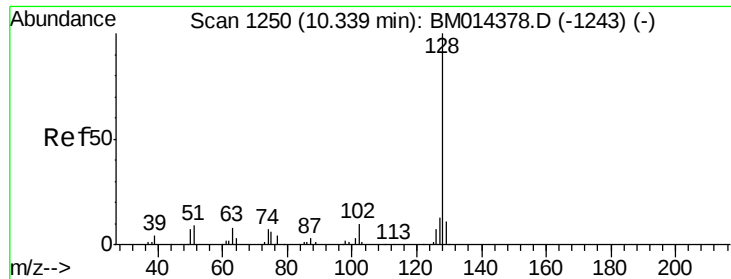





#28  
Naphthalene  
Concen: 7.262 ng/ul  
RT: 10.34 min Scan# 1250  
Delta R.T. -0.00 min  
Lab File: BM014388.D  
Acq: 27 Feb 2018 18:26

Instrument :  
BNA\_M  
ClientSampled :  
BE5Z1

| Tot Ion | Ratio | Resp   | Lower | Upper |
|---------|-------|--------|-------|-------|
| 128     | 100   | 169237 |       |       |
| 129     | 11.0  |        | 8.8   | 13.2  |
| 127     | 12.5  |        | 10.6  | 16.0  |




Manual Integrations  
APPROVED


Sohil  
2/28/2018 1:59:19 PM

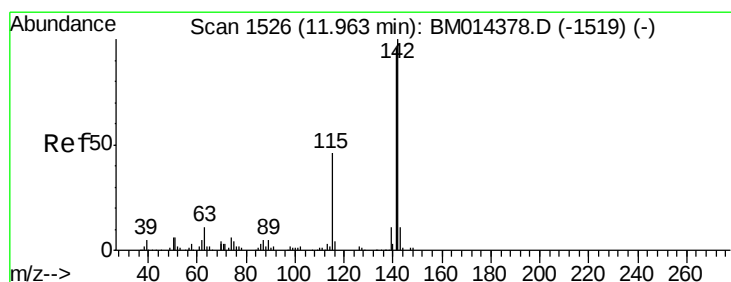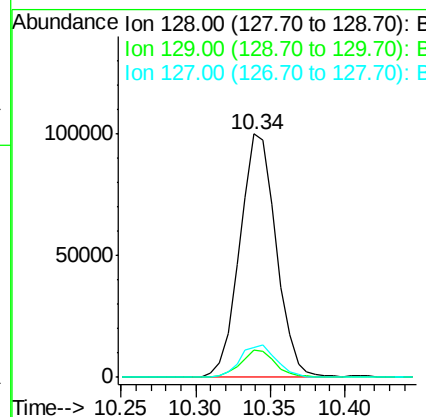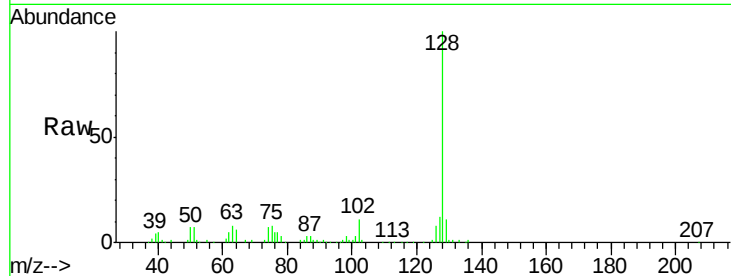

#34  
2-Methylnaphthalene  
Concen: 1.985 ng/ul  
RT: 11.97 min Scan# 1527  
Delta R.T. 0.01 min  
Lab File: BM014388.D  
Acq: 27 Feb 2018 18:26

| Tgt Ion | Ratio | Resp  | Lower | Upper |
|---------|-------|-------|-------|-------|
| 142     | 100   | 35207 |       |       |
| 141     | 90.5  |       | 74.1  | 111.1 |

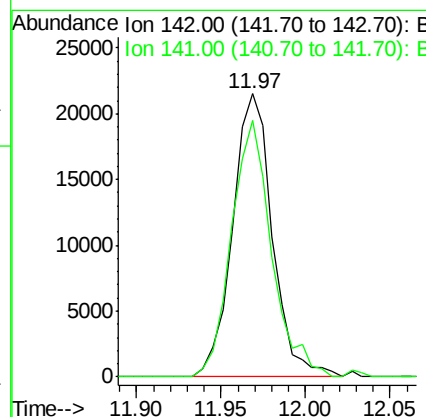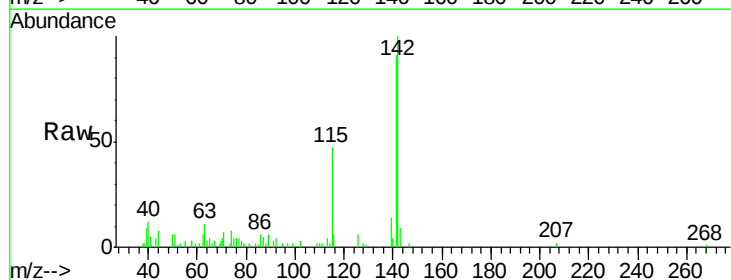

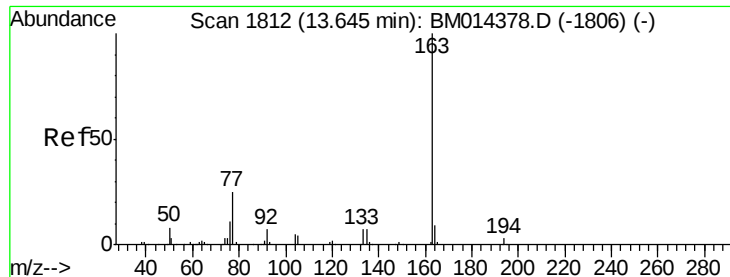





#44  
Dimethylphthalate  
Concen: 21.581 ng/ul  
RT: 13.65 min Scan# 1813  
Delta R.T. 0.01 min  
Lab File: BM014388.D  
Acq: 27 Feb 2018 18:26

Instrument :  
BNA\_M  
ClientSampleId :  
BE5Z1

| Tot Ion | Ratio | Resp   | Lower | Upper |
|---------|-------|--------|-------|-------|
| 163     | 100   | 448779 |       |       |
| 194     | 3.9   |        | 3.5   | 5.3   |
| 164     | 8.7   |        | 8.2   | 12.4  |




Manual Integrations  
APPROVED


Sohil  
2/28/2018 1:59:19 PM

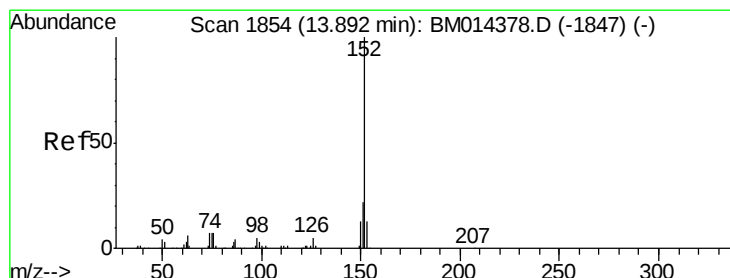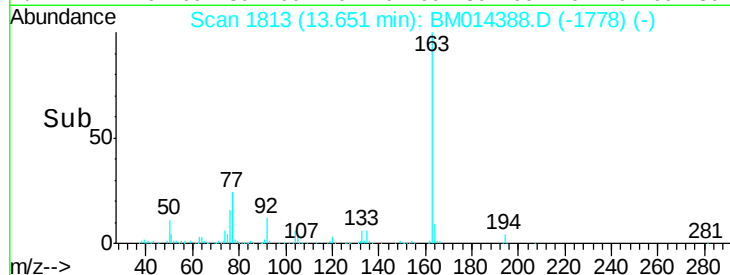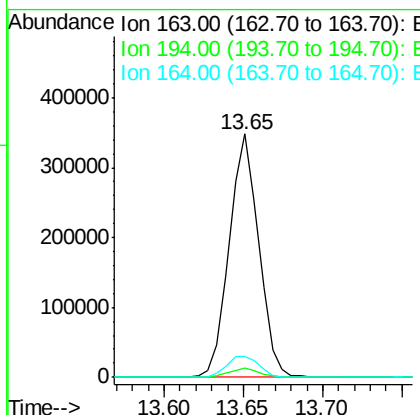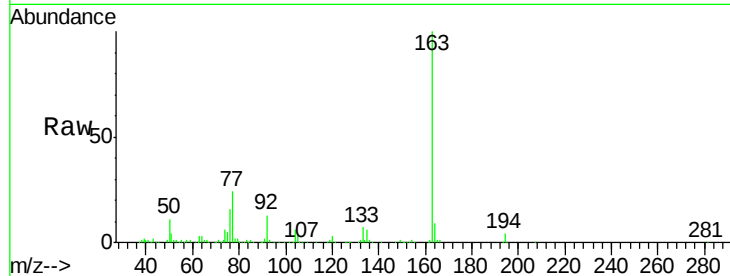

#47  
Acenaphthylene  
Concen: 5.505 ng/ul  
RT: 13.90 min Scan# 1856  
Delta R.T. 0.01 min  
Lab File: BM014388.D  
Acq: 27 Feb 2018 18:26

| Tgt Ion | Ratio | Resp   | Lower | Upper |
|---------|-------|--------|-------|-------|
| 152     | 100   | 135305 |       |       |
| 151     | 19.4  |        | 16.3  | 24.5  |
| 153     | 14.5  |        | 10.2  | 15.4  |

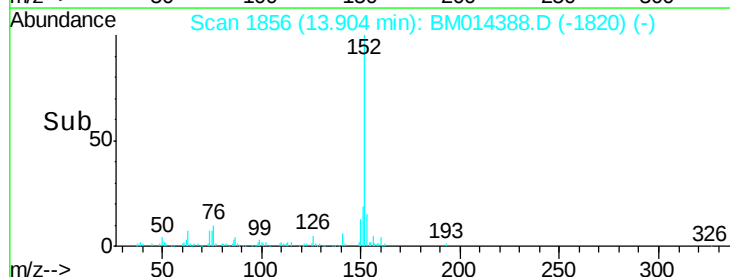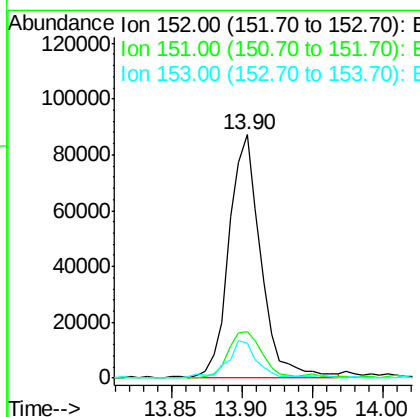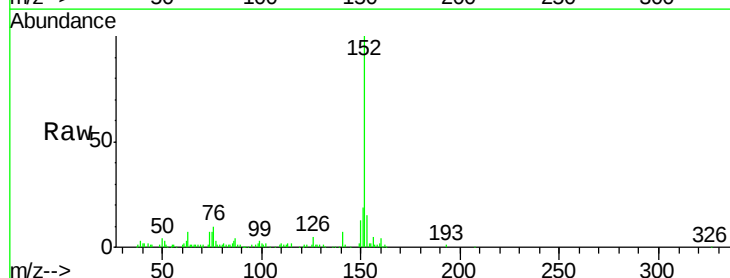



#49

Acenaphthene

Concen: 4.826 ng/ul

RT: 14.24 min Scan# 1914

Delta R.T. 0.01 min

Lab File: BM014388.D

Acq: 27 Feb 2018 18:26

Instrument :

BNA\_M





ClientSampleId :

BE5Z1

|           |       |       |       |
|-----------|-------|-------|-------|
| Tot Ion:  | 153   | Resp: | 83515 |
| Ion Ratio | Lower | Upper |       |
| 153       | 100   |       |       |
| 152       | 45.1  | 37.6  | 56.4  |
| 154       | 83.9  | 70.4  | 105.6 |

Manual Integrations  
APPROVED

Sohil  
2/28/2018 1:59:19 PM

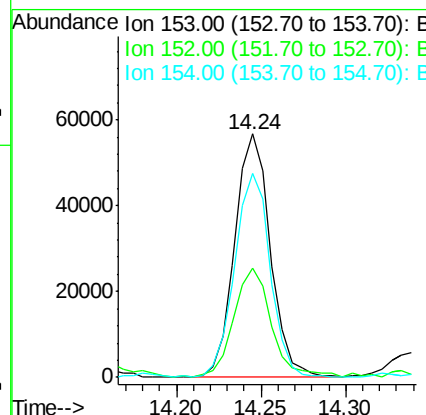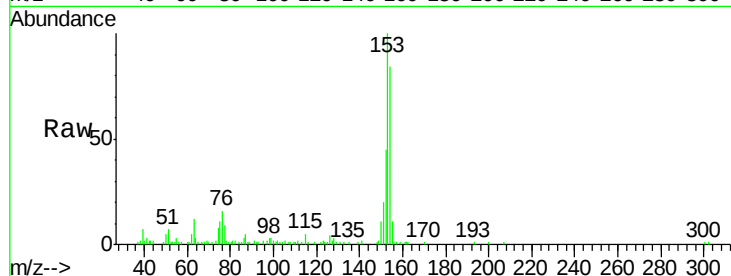

#53

Dibenzofuran

Concen: 3.548 ng/ul




RT: 14.59 min Scan# 1972


Delta R.T. 0.01 min

Lab File: BM014388.D

Acq: 27 Feb 2018 18:26

|           |       |       |       |
|-----------|-------|-------|-------|
| Tgt Ion:  | 168   | Resp: | 92064 |
| Ion Ratio | Lower | Upper |       |
| 168       | 100   |       |       |
| 139       | 44.3  | 30.8  | 46.2  |

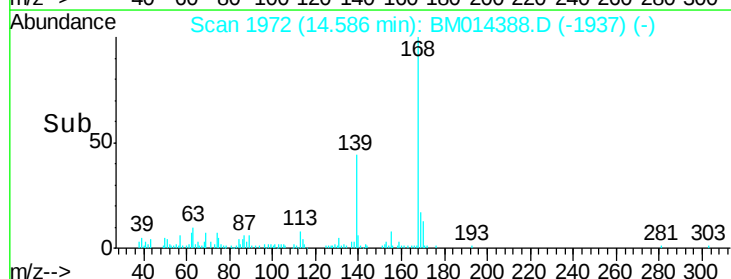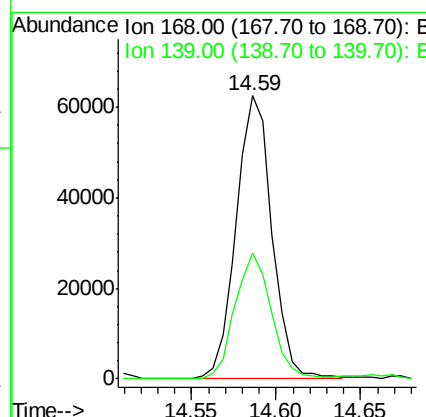




#56  
Diethylphthalate  
Concen: 1.635 ng/ul  
RT: 15.02 min Scan# 2046  
Delta R.T. -0.00 min  
Lab File: BM014388.D  
Acq: 27 Feb 2018 18:26

Instrument :  
BNA\_M  
ClientSampleId :  
BE5Z1




| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 149     | 100   |       |       |
| 177     | 15.0  | 20.5  | 30.7# |
| 150     | 11.1  | 10.6  | 15.8  |

Manual Integrations  
APPROVED

Sohil  
2/28/2018 1:59:19 PM

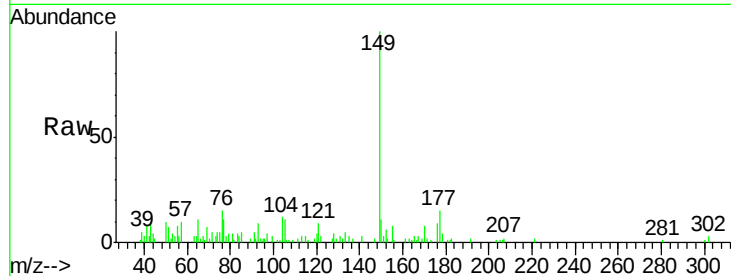


Abundance Ion 149.00 (148.70 to 149.70): E  
Ion 177.00 (176.70 to 177.70): E  
Ion 150.00 (149.70 to 150.70): E

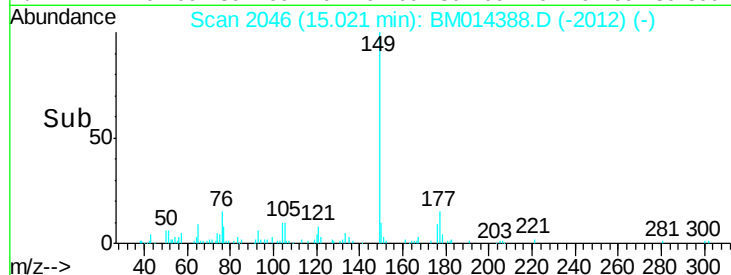
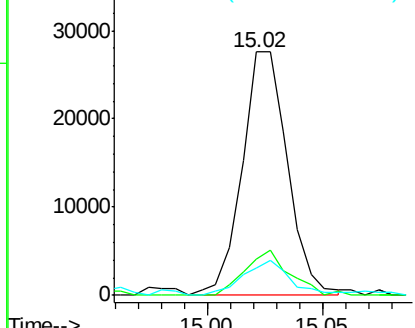



#58  
Fluorene  
Concen: 5.346 ng/ul  
RT: 15.24 min Scan# 2083  
Delta R.T. 0.01 min  
Lab File: BM014388.D  
Acq: 27 Feb 2018 18:26

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 166     | 100   |       |       |
| 165     | 100.2 | 77.9  | 116.9 |
| 167     | 16.4  | 10.6  | 16.0# |



Abundance Ion 166.00 (165.70 to 166.70): E  
Ion 165.00 (164.70 to 165.70): E  
Ion 167.00 (166.70 to 167.70): E

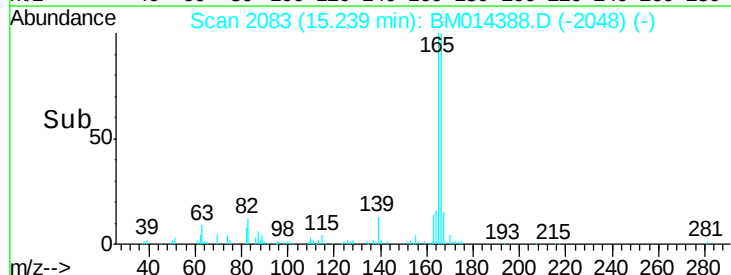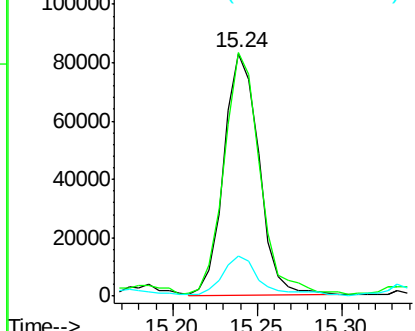

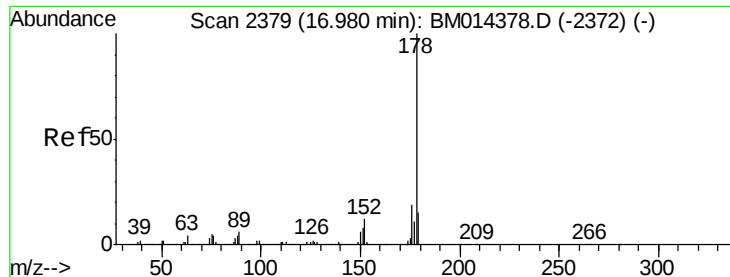

#69

Phenanthrene

Concen: 84.576 ng/ul

RT: 16.99 min Scan# 2380

Delta R.T. 0.01 min

Lab File: BM014388.D

Acq: 27 Feb 2018 18:26

Instrument :

BNA\_M

ClientSampled :

BE5Z1

Tot Ion:178 Resp: 2531911

Ion Ratio Lower Upper

178 100


179 15.4 12.6 19.0

176 18.5 14.9 22.3


Manual Integrations  
APPROVED

Sohil



2/28/2018 1:59:19 PM

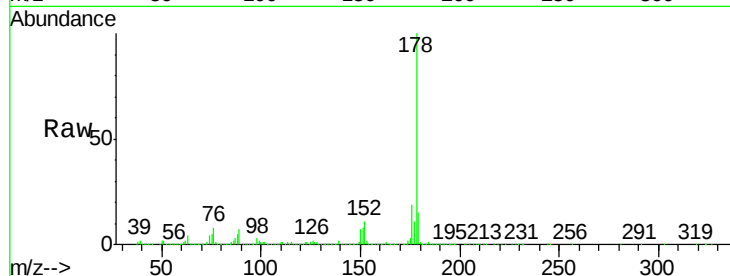

Abundance Ion 178.00 (177.70 to 178.70): E  
Ion 179.00 (178.70 to 179.70): E  
Ion 176.00 (175.70 to 176.70): E

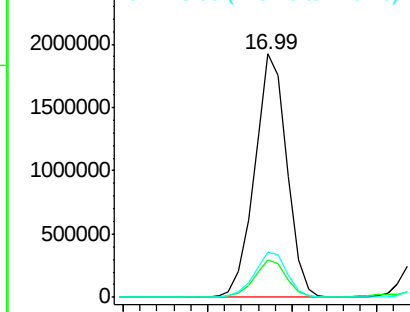

Time--> 16.90 16.95 17.00 17.05

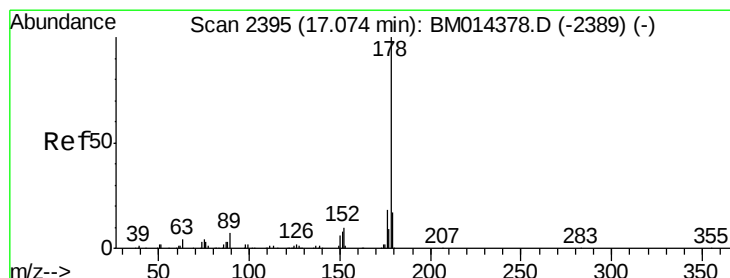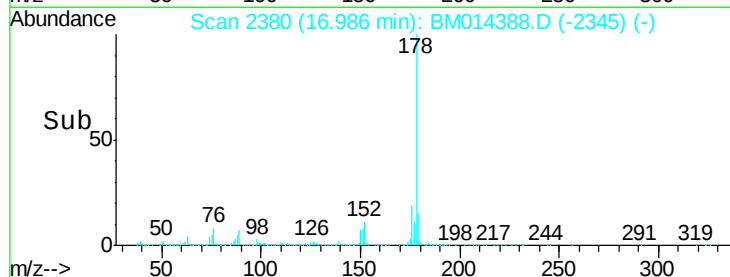

#71

Anthracene

Concen: 17.366 ng/ul

RT: 17.07 min Scan# 2395

Delta R.T. -0.00 min

Lab File: BM014388.D

Acq: 27 Feb 2018 18:26


Tgt Ion:178 Resp: 522847

Ion Ratio Lower Upper


178 100

179 14.9 11.7 17.5


176 16.6 14.6 21.8

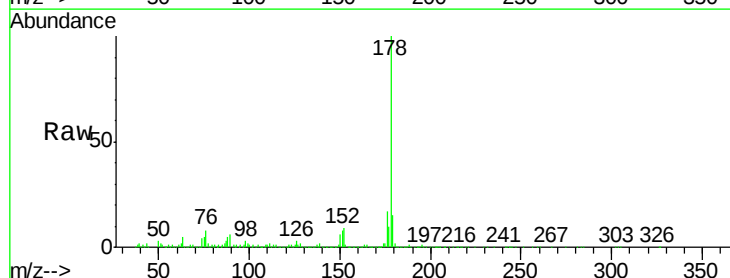


Abundance Ion 178.00 (177.70 to 178.70): E  
Ion 179.00 (178.70 to 179.70): E  
Ion 176.00 (175.70 to 176.70): E

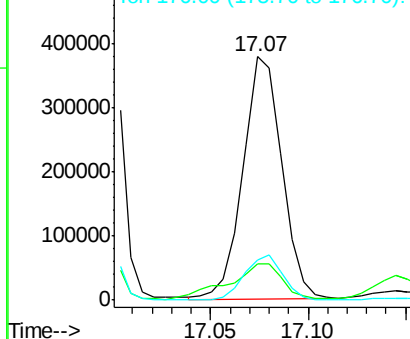

Time--> 17.05 17.10

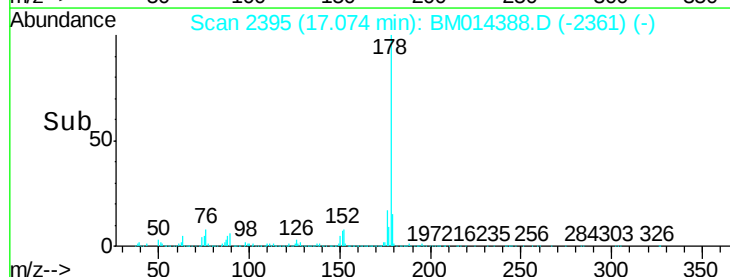

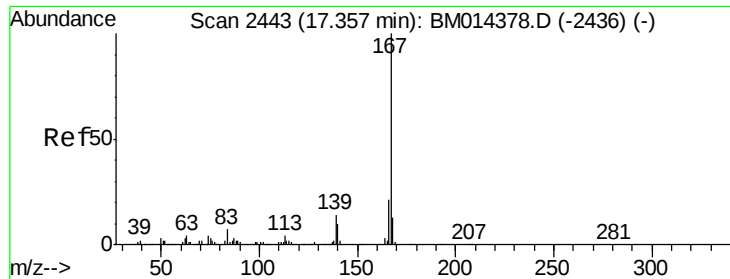





#72  
 Carbazole  
 Concen: 8.850 ng/ul  
 RT: 17.36 min Scan# 2444  
 Delta R.T. 0.01 min  
 Lab File: BM014388.D  
 Acq: 27 Feb 2018 18:26

Instrument :  
 BNA\_M  
 ClientSampleId :  
 BE5Z1

| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 167     | 100   |       |       |
| 166     | 19.8  | 17.1  | 25.7  |
| 139     | 12.4  | 10.0  | 15.0  |




Manual Integrations  
 APPROVED


Sohil  
 2/28/2018 1:59:19 PM

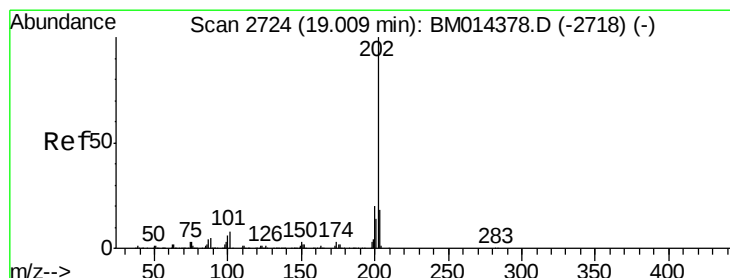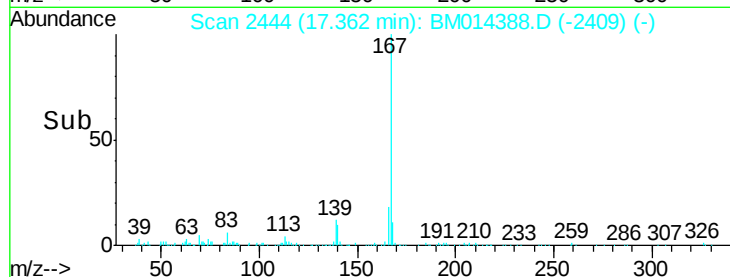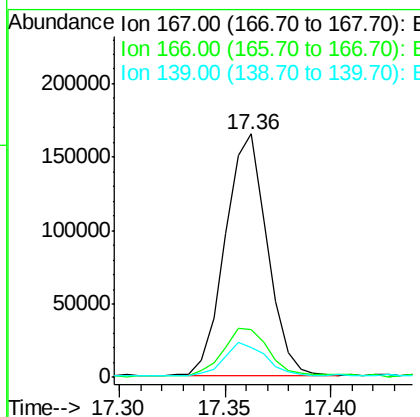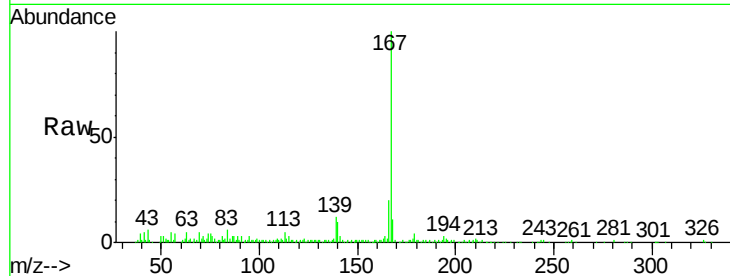

#74  
 Fluoranthene  
 Concen: 115.863 ng/ul  
 RT: 19.02 min Scan# 2726  
 Delta R.T. 0.01 min  
 Lab File: BM014388.D  
 Acq: 27 Feb 2018 18:26

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 202     | 100   |       |       |
| 101     | 8.3   | 4.6   | 7.0#  |
| 100     | 6.6   | 3.4   | 5.2#  |

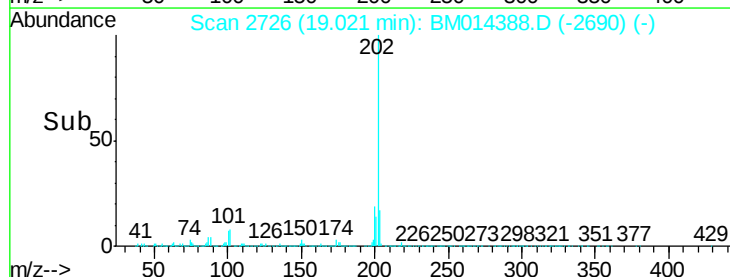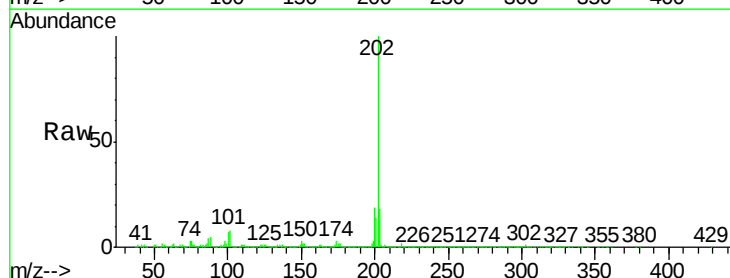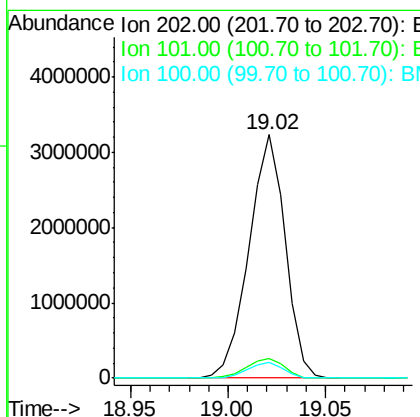

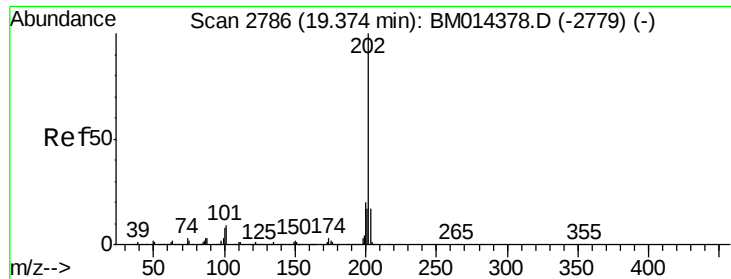

#77

Pvrene

Concen: 107.463 ng/ul

RT: 19.39 min Scan# 2788

Delta R.T. 0.01 min

Lab File: BM014388.D

Acq: 27 Feb 2018 18:26

Instrument :

BNA\_M


ClientSampleId :

BE5Z1




|           |       |       |         |
|-----------|-------|-------|---------|
| Tot Ion:  | 202   | Resp: | 3652275 |
| Ion Ratio | Lower | Upper |         |
| 202       | 100   |       |         |
| 101       | 10.3  | 5.1   | 7.7#    |
| 100       | 8.4   | 4.9   | 7.3#    |

Manual Integrations  
APPROVED

Sohil  
2/28/2018 1:59:19 PM

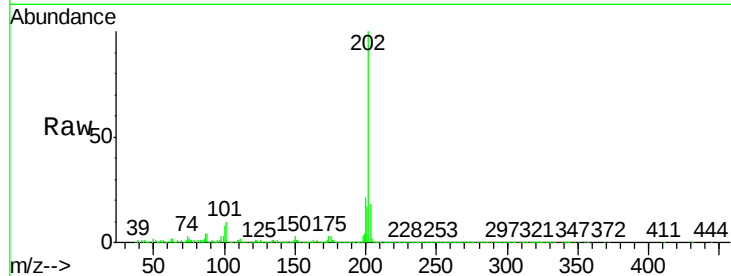

Abundance Ion 202.00 (201.70 to 202.70): E  
Ion 101.00 (100.70 to 101.70): E  
Ion 100.00 (99.70 to 100.70): B

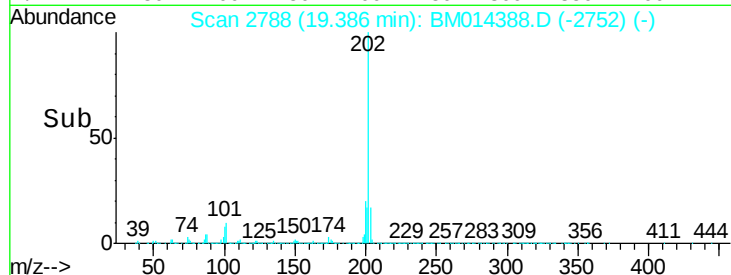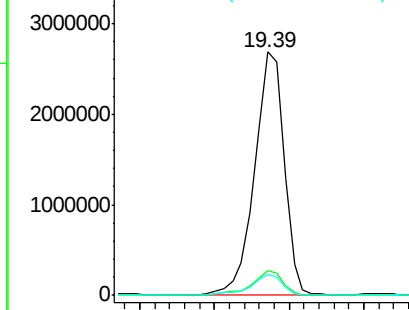

#80

Benzo(a)anthracene

Concen: 63.792 ng/ul

RT: 21.14 min Scan# 3087




Delta R.T. 0.01 min


Lab File: BM014388.D

Acq: 27 Feb 2018 18:26

|           |       |       |         |
|-----------|-------|-------|---------|
| Tgt Ion:  | 228   | Resp: | 2036044 |
| Ion Ratio | Lower | Upper |         |
| 228       | 100   |       |         |
| 229       | 20.6  | 15.4  | 23.0    |
| 226       | 26.7  | 21.4  | 32.0    |

Abundance Ion 228.00 (227.70 to 228.70): E  
Ion 229.00 (228.70 to 229.70): E  
Ion 226.00 (225.70 to 226.70): E

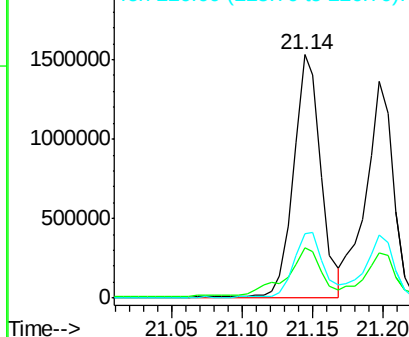

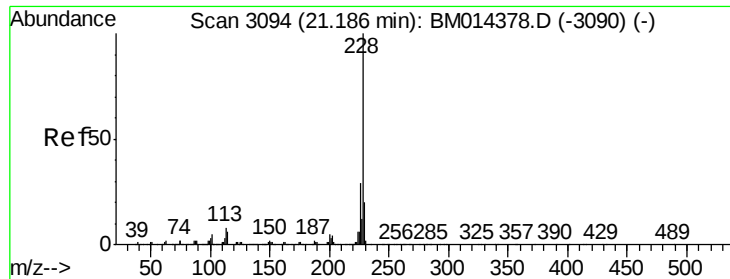

#82

Chrysene

Concen: 61.745 ng/ul

RT: 21.20 min Scan# 3096

Delta R.T. 0.01 min

Lab File: BM014388.D

Acq: 27 Feb 2018 18:26

Instrument :

BNA\_M

ClientSampled :

BE5Z1

Tot Ion:228 Resp: 1838395

Ion Ratio Lower Upper

228 100


226 29.2 23.4 35.2

229 21.2 15.5 23.3




Manual Integrations  
APPROVED

Sohil

2/28/2018 1:59:19 PM

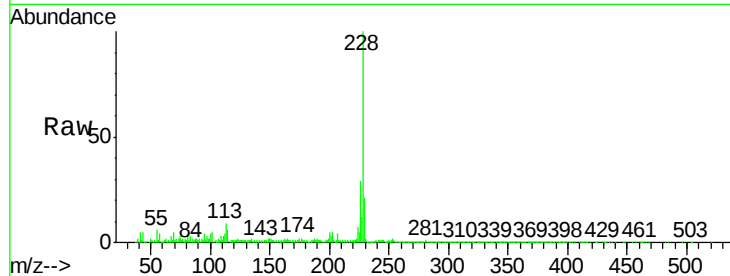

Abundance Ion 228.00 (227.70 to 228.70): E  
Ion 226.00 (225.70 to 226.70): E  
Ion 229.00 (228.70 to 229.70): E

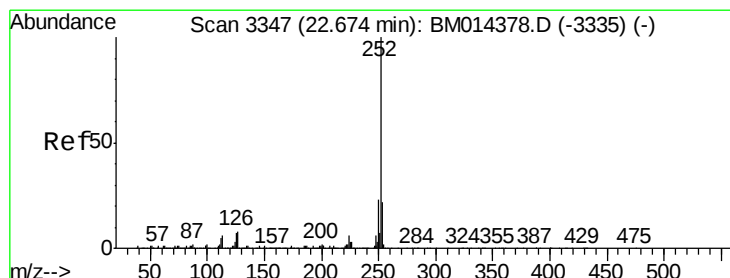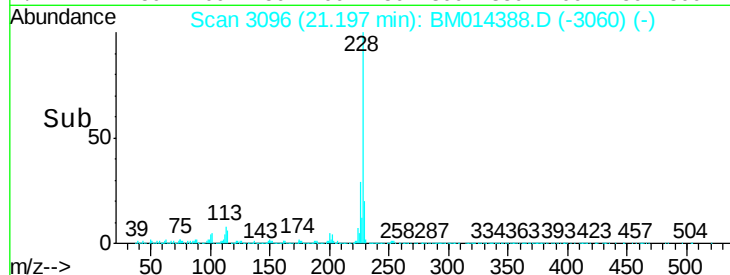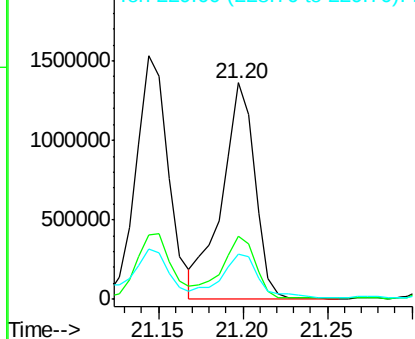

#85

Benzo(b)fluoranthene

Concen: 75.207 ng/ul

RT: 22.70 min Scan# 3352

Delta R.T. 0.03 min

Lab File: BM014388.D

Acq: 27 Feb 2018 18:26

Tgt Ion:252 Resp: 2458811




Ion Ratio Lower Upper


252 100

253 22.7 17.9 26.9

125 8.5 3.6 5.4#

Abundance Ion 252.00 (251.70 to 252.70): E  
Ion 253.00 (252.70 to 253.70): E  
Ion 125.00 (124.70 to 125.70): E

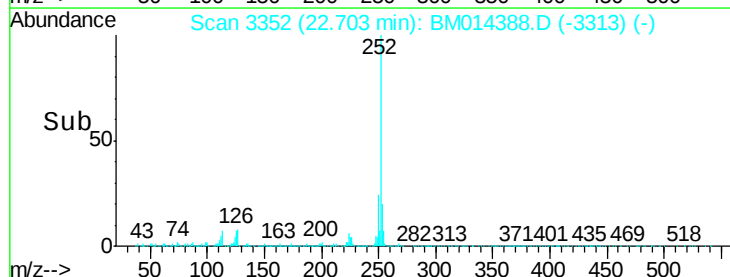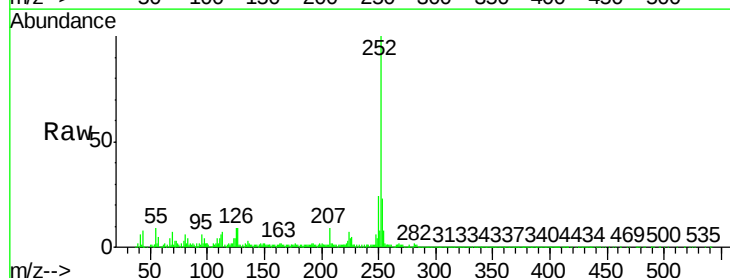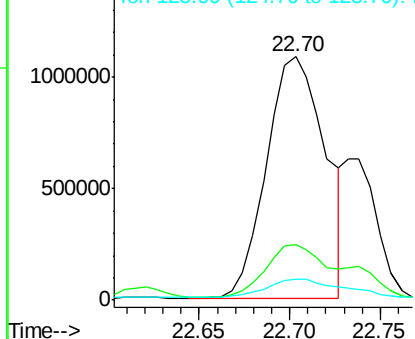

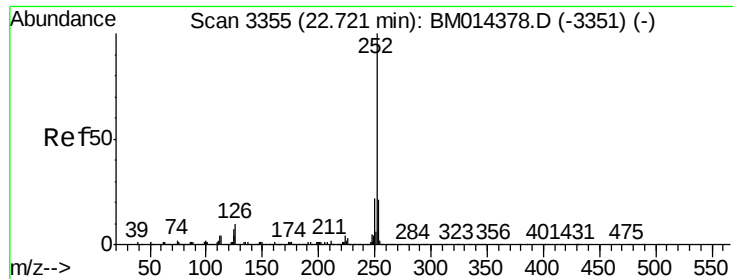





#86  
Benzo(k)fluoranthene  
Concen: 24.878 ng/ul m  
RT: 22.74 min Scan# 3358  
Delta R.T. 0.02 min  
Lab File: BM014388.D  
Acq: 27 Feb 2018 18:26

Instrument :  
BNA\_M  
ClientSampled :  
BE5Z1

| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 252     | 100   |       |       |
| 253     | 23.7  | 17.1  | 25.7  |
| 125     | 7.2   | 3.4   | 5.2#  |




Manual Integrations  
APPROVED


Sohil  
2/28/2018 1:59:19 PM

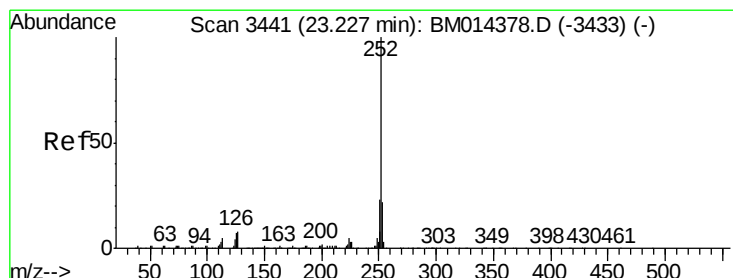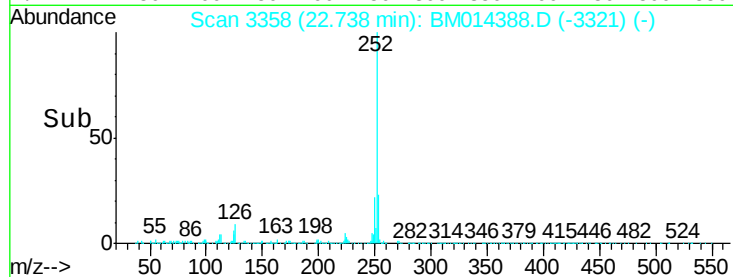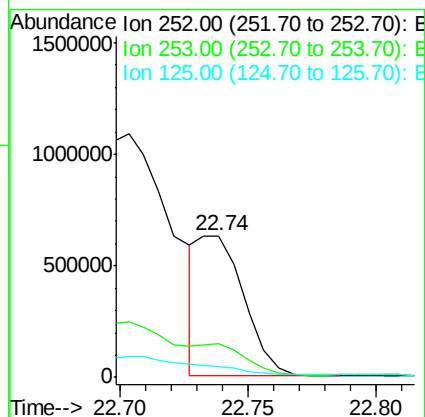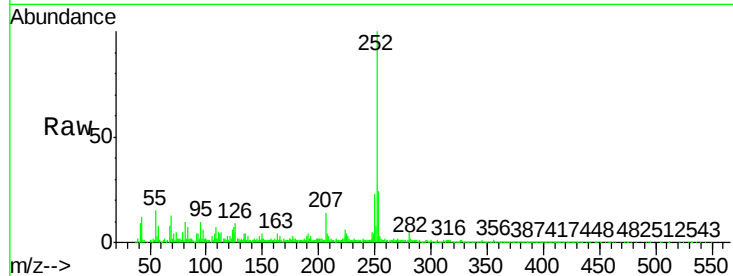

#88  
Benzo(a)pyrene  
Concen: 60.108 ng/ul  
RT: 23.26 min Scan# 3446  
Delta R.T. 0.03 min  
Lab File: BM014388.D  
Acq: 27 Feb 2018 18:26

| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 252     | 100   |       |       |
| 253     | 23.3  | 18.2  | 27.2  |
| 125     | 7.5   | 4.0   | 6.0#  |

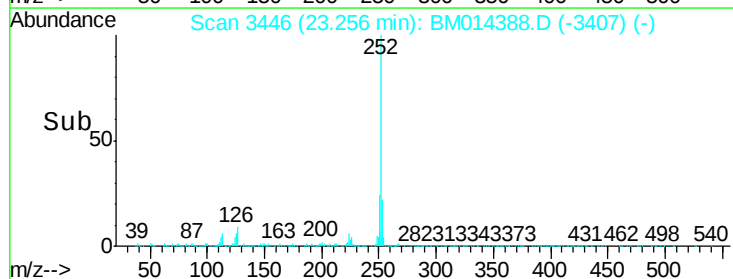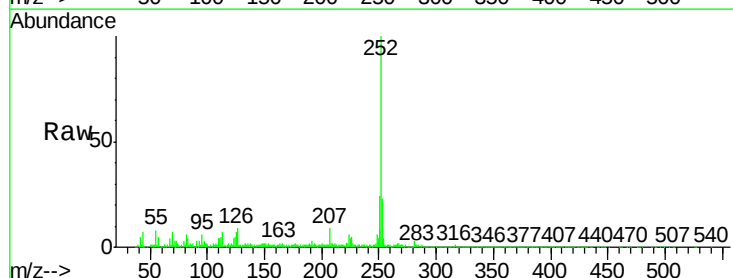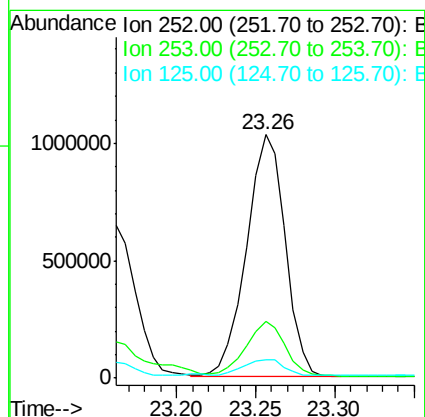

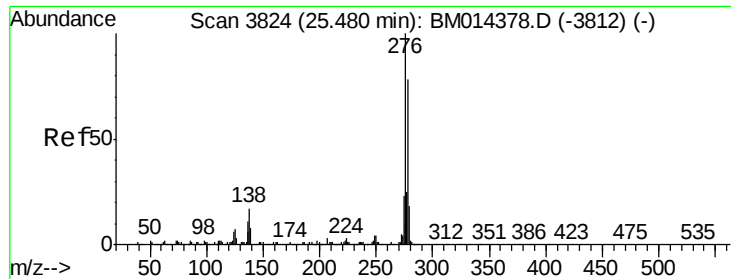

#89

Indeno(1,2,3-cd)pyrene

Concen: 40.434 ng/ul

RT: 25.53 min Scan# 3832

Delta R.T. 0.05 min

Lab File: BM014388.D

Acq: 27 Feb 2018 18:26

Instrument :

BNA\_M


ClientSampleID :

BE5Z1

| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 276     | 100   |       |       |
| 138     | 14.2  | 9.3   | 13.9# |
| 277     | 24.8  | 19.9  | 29.9  |

Manual Integrations  
APPROVED

Sohil  
2/28/2018 1:59:19 PM



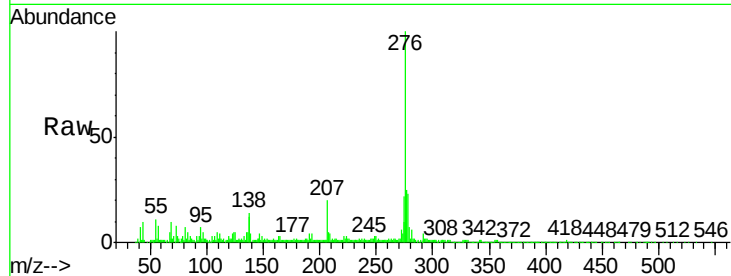


Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

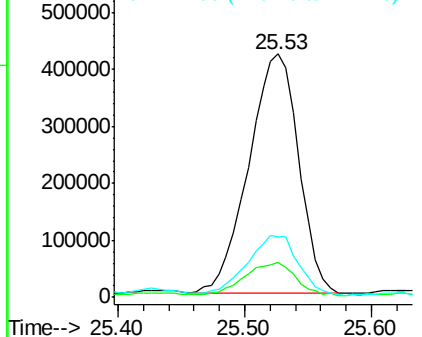

#90

Dibenzo(a,h)anthracene

Concen: 14.387 ng/ul

RT: 25.52 min Scan# 3831

Delta R.T. 0.04 min

Lab File: BM014388.D

Acq: 27 Feb 2018 18:26




| Tgt Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 278     | 100   |       |       |
| 139     | 15.2  | 5.8   | 8.8#  |
| 279     | 30.4  | 18.6  | 27.8# |


Abundance

Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

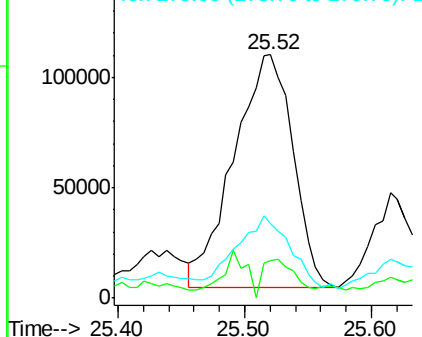

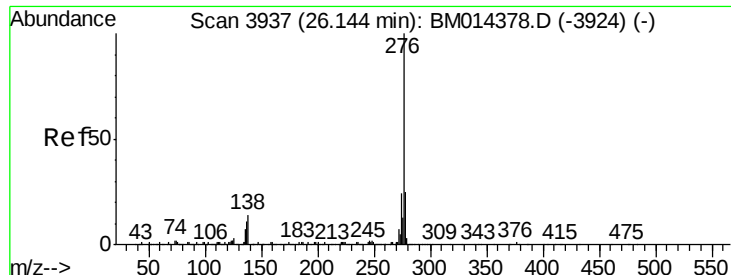


#91  
 Benzo(a,h,i)perylene  
 Concen: 37.825 ng/ul  
 RT: 26.20 min Scan# 3946  
 Delta R.T. 0.05 min  
 Lab File: BM014388.D  
 Acq: 27 Feb 2018 18:26

Instrument :  
 BNA\_M  
 ClientSampleId :  
 BE5Z1

| Tot Ion | Ratio | Lower | Upper |
|---------|-------|-------|-------|
| 276     | 100   |       |       |
| 138     | 15.2  | 8.5   | 12.7# |
| 277     | 25.7  | 18.6  | 28.0  |

Manual Integrations  
 APPROVED

Sohil  
 2/28/2018 1:59:19 PM



Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

