


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022721\
Data File : BM028933.D
Acq On : 26 Feb 2021 23:38
Operator : CG/JU
Sample : M1482-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBGM6

Manual Integrations
APPROVED

mohammad
3/1/2021 12:38:31 PM

Quant Time: Feb 27 00:36:00 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 26 15:22:35 2021
Response via : Initial Calibration

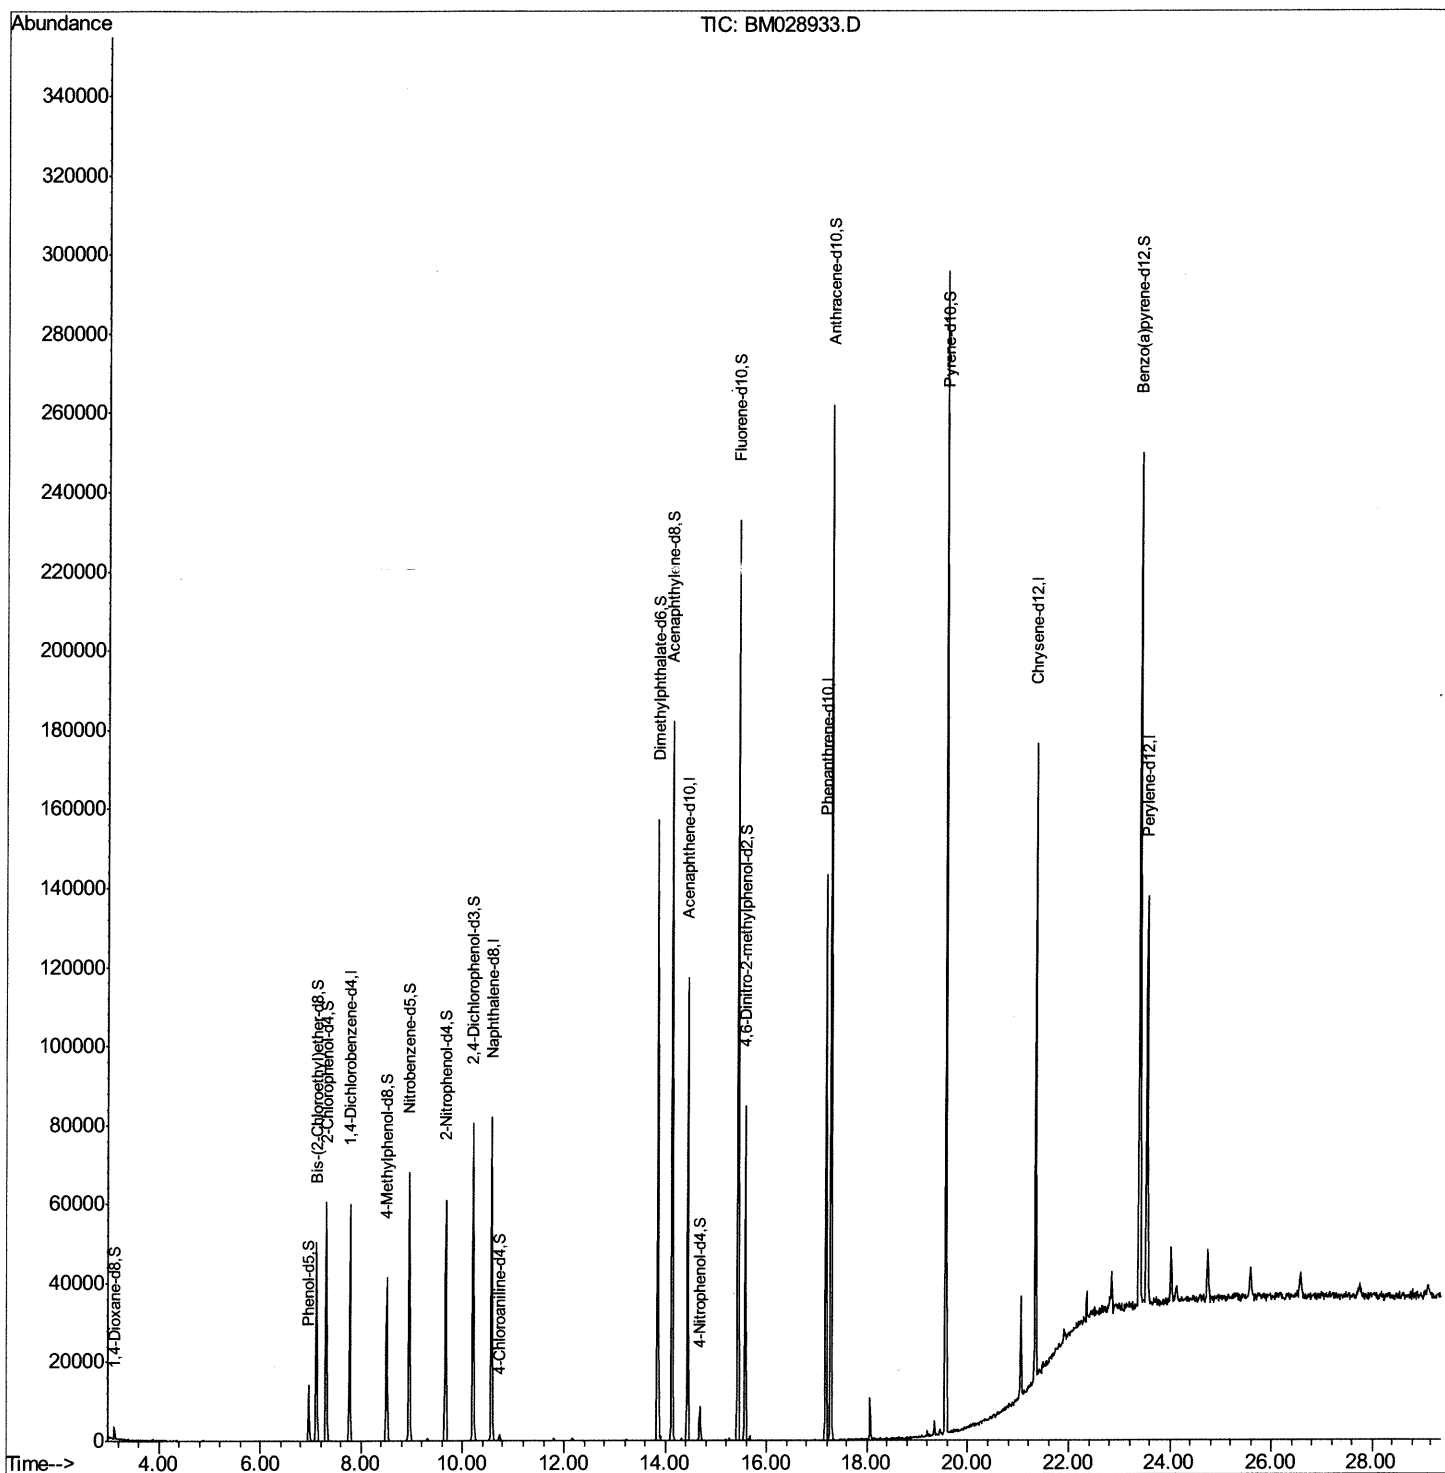

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022721\
 Data File : BM028933.D
 Acq On : 26 Feb 2021 23:38
 Operator : CG/JU
 Sample : M1482-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBGM6

Manual Integrations
 APPROVED

mohammad
 3/1/2021 12:38:31 PM

Quant Time: Feb 27 00:34:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 26 15:22:35 2021
 Response via : Initial Calibration

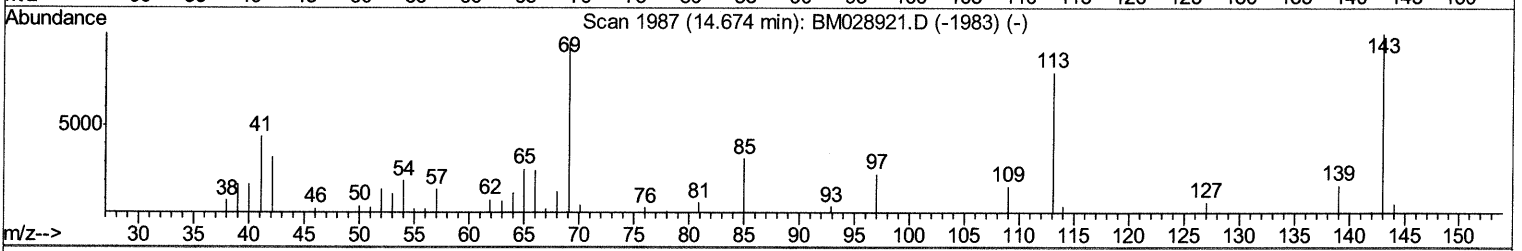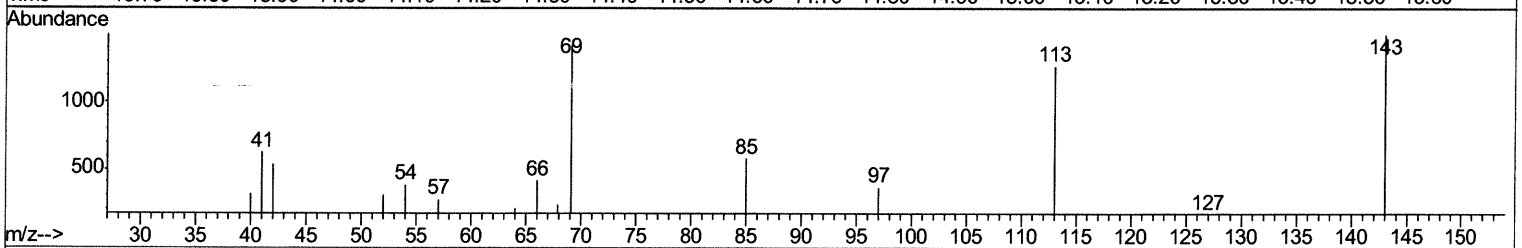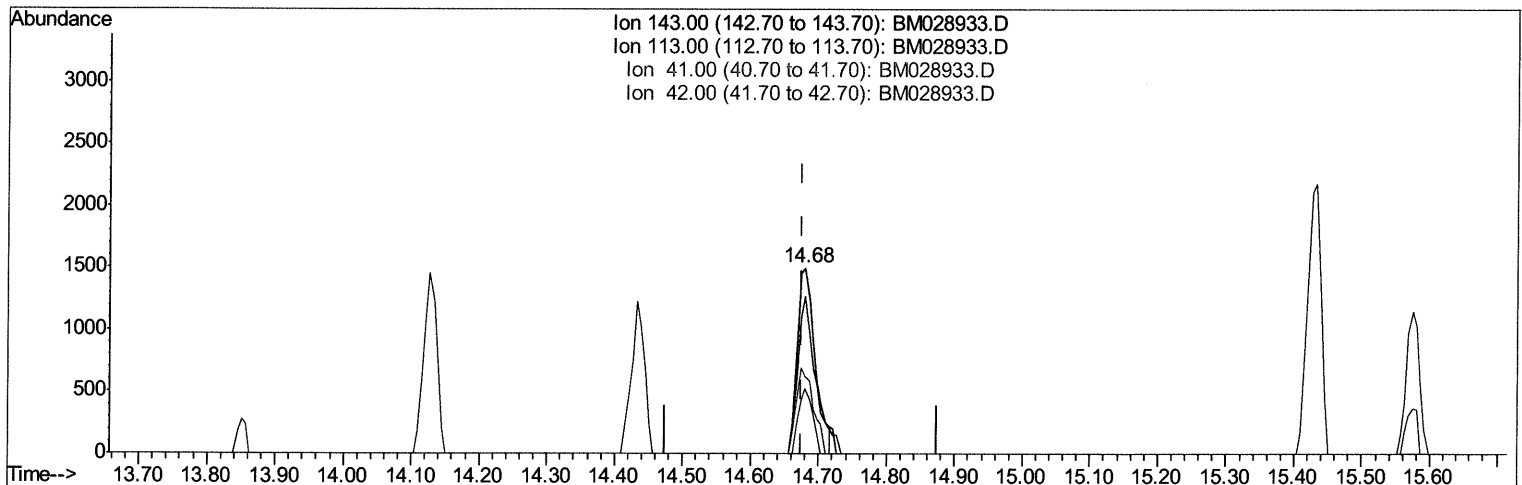

TIC: BM028933.D

(52) 4-Nitrophenol-d4 (S)

14.680min (+0.006) 5.61ng/ul

response 2701

Ion	Exp%	Act%
143.00	100	100
113.00	77.90	84.25
41.00	41.50	41.46
42.00	30.40	35.31

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022721\
Data File : BM028933.D
Acq On : 26 Feb 2021 23:38
Operator : CG/JU
Sample : M1482-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBGM6

Manual Integrations
APPROVED

mohammad
3/1/2021 12:38:31 PM

Quant Time: Feb 27 00:34:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 26 15:22:35 2021
Response via : Initial Calibration

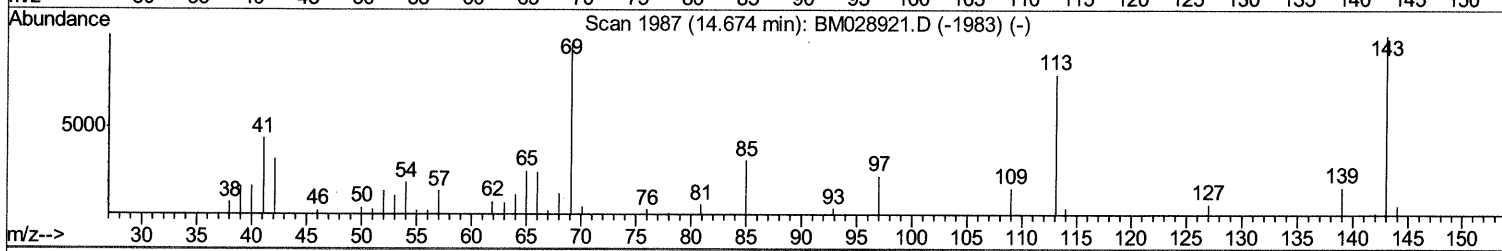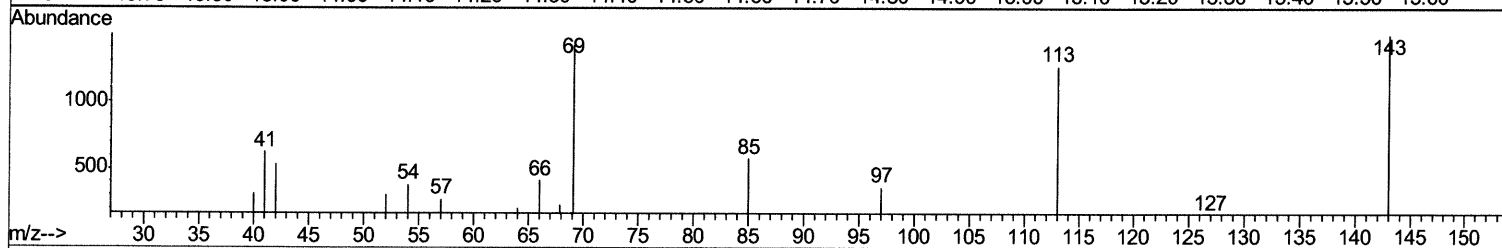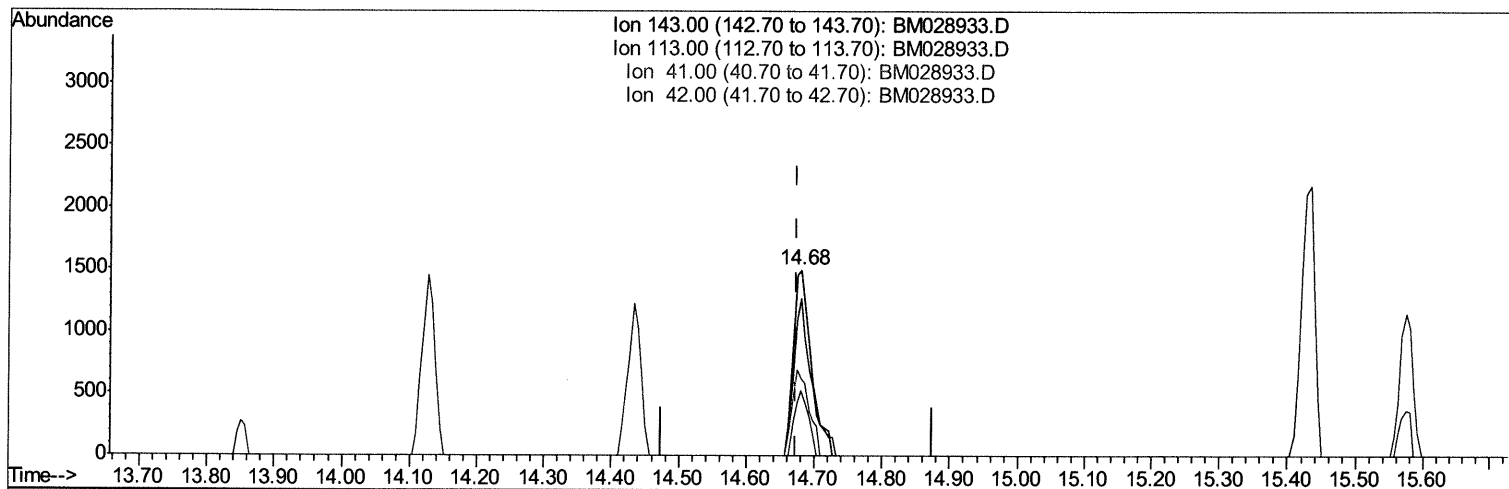

TIC: BM028933.D

(52) 4-Nitrophenol-d4 (S)

14.680min (+0.006) 5.75ng/ul m 03/01/21 Ju

response 2772

Ion	Exp%	Act%
143.00	100	100
113.00	77.90	84.25
41.00	41.50	41.46
42.00	30.40	35.31

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022721\
 Data File : BM028933.D
 Acq On : 26 Feb 2021 23:38
 Operator : CG/JU
 Sample : M1482-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBG6

Manual Integrations
 APPROVED

mohammad
 3/1/2021 12:38:31 PM

Quant Time: Feb 27 00:36:00 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 26 15:22:35 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	16182	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	65274	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.43	164	40289	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.18	188	79458	20.00	ng/ul	0.00
78) Chrysene-d12	21.34	240	69087	20.00	ng/ul	0.00
86) Perylene-d12	23.54	264	66016	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	1559	4.34	ng/uL	0.00
5) Phenol-d5	6.96	99	7569	6.47	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.11	67	21452	32.25	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	26348	25.21	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	15066	16.01	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	15266	32.52	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	17714	33.71	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	28441	29.20	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	1980	1.79	ng/ul	0.00
44) Dimethylphthalate-d6	13.85	166	98290	35.49	ng/ul	0.00
47) Acenaphthylene-d8	14.13	160	121248	32.63	ng/ul	0.00
52) 4-Nitrophenol-d4	14.68	143	2772m	5.75	ng/ul	0.00
58) Fluorene-d10	15.43	176	85437	35.36	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.57	200	15677	33.09	ng/ul	0.00
71) Anthracene-d10	17.28	188	139241	38.55	ng/ul	0.00
79) Pyrene-d10	19.56	212	141487	41.67	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.40	264	131716	39.28	ng/ul	0.00

03/01/2021

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed