

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022721\
 Data File : BM028953.D
 Acq On : 27 Feb 2021 12:18
 Operator : CG/JU
 Sample : M1498-11
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB8G0

Quant Time: Mar 01 00:39:26 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 26 15:22:35 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	16669	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	68672	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.43	164	41544	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.17	188	80649	20.00	ng/ul	-0.01
78) Chrysene-d12	21.34	240	66511	20.00	ng/ul	0.00
86) Perylene-d12	23.54	264	62676	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	1856	5.01	ng/uL	0.00
5) Phenol-d5	6.96	99	9259	7.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.11	67	24557	35.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.30	132	31085	28.87	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	18233	18.81	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	18196	36.84	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	21088	38.14	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	33782	32.97	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	2547	2.19	ng/ul	0.00
44) Dimethylphthalate-d6	13.85	166	111709	39.12	ng/ul	0.00
47) Acenaphthylene-d8	14.13	160	141644	36.97	ng/ul	0.00
52) 4-Nitrophenol-d4	14.69	143	3093	6.22	ng/ul	0.01
58) Fluorene-d10	15.43	176	95709	38.41	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.57	200	16828	34.99	ng/ul	0.00
71) Anthracene-d10	17.27	188	150641	41.09	ng/ul	0.00
79) Pyrene-d10	19.56	212	149054	45.60	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.40	264	131799	41.40	ng/ul	0.00


Target Compounds				Ovalue
45) Dimethylphthalate	13.90	163	4154	1.394 ng/ul# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022721\
Data File : BM028953.D
Acq On : 27 Feb 2021 12:18
Operator : CG/JU
Sample : M1498-11
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB8G0

Quant Time: Mar 01 00:39:26 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 26 15:22:35 2021
Response via : Initial Calibration

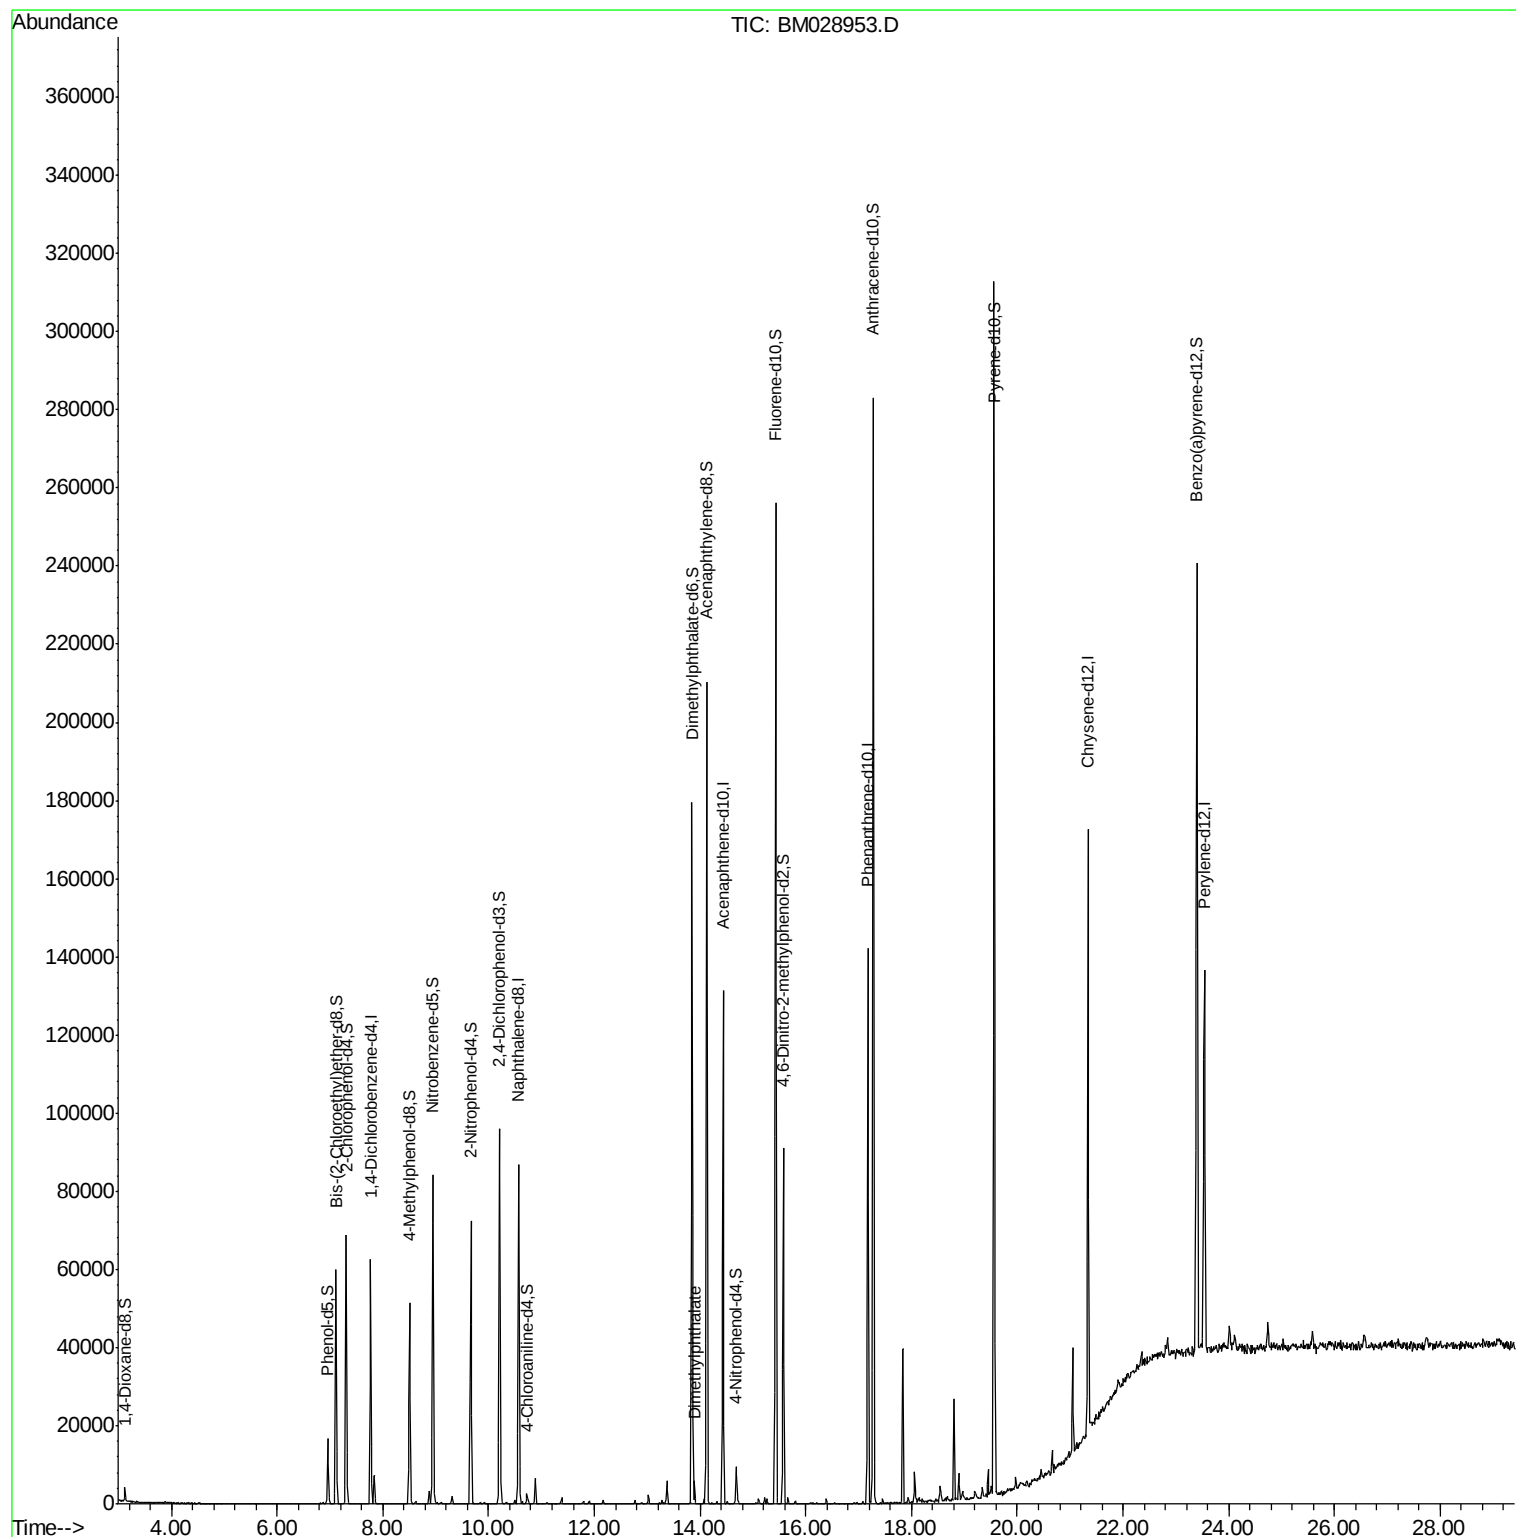

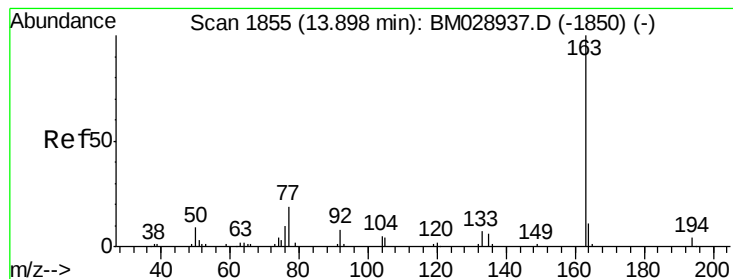

#45

Dimethylphthalate

Concen: 1.394 ng/ul

RT: 13.90 min Scan# 1855

Delta R.T. -0.01 min

Lab File: BM028953.D

Acq: 27 Feb 2021 12:18

Instrument :

BNA_M

ClientSampleId :

CB8G0


Tot Ion:163 Resp: 4154

Ion Ratio Lower Upper

163 100

194 0.0 3.3 4.9#

164 9.0 8.2 12.2

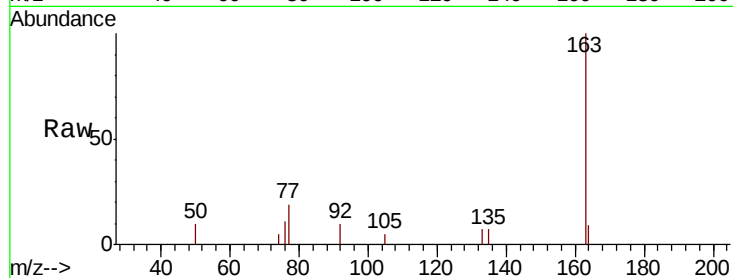

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

