

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022721\
 Data File : BM028922.D
 Acq On : 26 Feb 2021 16:56
 Operator : CG/JU
 Sample : PB134805BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK05

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	20	23	29	rBV	4558	5215	1.66%	0.144%
2	3.458	77	80	82	rBV	199	328	0.10%	0.009%
3	3.881	150	152	155	rBB	595	449	0.14%	0.012%
4	6.957	670	675	685	rBB	76392	115893	36.95%	3.208%
5	7.116	696	702	710	rBB	57077	83959	26.77%	2.324%
6	7.304	729	734	743	rBB	80056	124426	39.67%	3.444%
7	7.775	809	814	822	rBB	60110	87864	28.01%	2.432%
8	8.504	933	938	948	rBB	90532	137925	43.97%	3.818%
9	8.951	1008	1014	1023	rBB	71218	111049	35.40%	3.074%
10	9.669	1131	1136	1144	rBB	61876	95446	30.43%	2.642%
11	10.210	1222	1228	1239	rBB	89646	140040	44.64%	3.877%
12	10.575	1284	1290	1298	rBB	76003	120733	38.49%	3.342%
13	10.728	1310	1316	1328	rBB	90403	141212	45.02%	3.909%
14	12.175	1559	1562	1565	rBB	798	864	0.28%	0.024%
15	13.857	1842	1848	1855	rBB	152336	197158	62.85%	5.458%
16	14.133	1889	1895	1902	rBV	174361	240636	76.71%	6.661%
17	14.439	1941	1947	1953	rBB	107117	148859	47.46%	4.121%
18	14.674	1982	1987	1999	rBB	60046	86912	27.71%	2.406%
19	15.433	2110	2116	2122	rBB	210792	282888	90.18%	7.831%
20	15.580	2136	2141	2148	rBB	63556	81784	26.07%	2.264%
21	15.668	2154	2156	2160	rBB	878	1025	0.33%	0.028%
22	17.180	2408	2413	2420	rBB	117454	159025	50.70%	4.402%
23	17.280	2424	2430	2436	rBV	224273	293337	93.51%	8.120%
24	18.833	2691	2694	2695	rBV	376	443	0.14%	0.012%
25	18.927	2707	2710	2711	rBV	470	331	0.11%	0.009%
26	18.945	2711	2713	2715	rVV	473	498	0.16%	0.014%
27	18.968	2715	2717	2721	rVB2	519	554	0.18%	0.015%
28	19.092	2734	2738	2740	rBV	340	515	0.16%	0.014%
29	19.121	2740	2743	2745	rVB2	366	441	0.14%	0.012%
30	19.151	2745	2748	2749	rBV3	419	376	0.12%	0.010%
31	19.174	2749	2752	2754	rBV2	280	345	0.11%	0.010%
32	19.204	2754	2757	2762	rVV2	1633	2036	0.65%	0.056%
33	19.309	2774	2775	2778	rBV3	312	319	0.10%	0.009%
34	19.404	2788	2791	2792	rVB2	423	407	0.13%	0.011%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022721\
 Data File : BM028922.D
 Acq On : 26 Feb 2021 16:56
 Operator : CG/JU
 Sample : PB134805BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK05

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
 Title : SVOA CALIBRATION

35	19.427	2792	2795	2797	rBV2	357	487	0.16%	0.013%
36	19.451	2797	2799	2803	rBV2	1158	1518	0.48%	0.042%
37	19.521	2810	2811	2813	rBV2	525	396	0.13%	0.011%
38	19.568	2813	2819	2827	rVV	245338	313684	100.00%	8.683%
39	19.645	2830	2832	2834	rVV3	573	611	0.19%	0.017%
40	19.674	2835	2837	2840	rVB	668	503	0.16%	0.014%
41	19.703	2840	2842	2846	rBV2	634	814	0.26%	0.023%
42	19.892	2873	2874	2879	rBV3	672	1121	0.36%	0.031%
43	20.056	2900	2902	2903	rBV	602	407	0.13%	0.011%
44	20.074	2903	2905	2908	rVB4	927	840	0.27%	0.023%
45	20.098	2908	2909	2910	rBV	970	468	0.15%	0.013%
46	20.115	2910	2912	2913	rBV	734	470	0.15%	0.013%
47	20.509	2977	2979	2980	rBV2	946	543	0.17%	0.015%
48	21.345	3116	3121	3126	rBV	138911	161107	51.36%	4.460%
49	23.403	3465	3471	3479	rVB	175333	304775	97.16%	8.437%
50	23.544	3489	3495	3503	rVB2	87886	161416	51.46%	4.468%


Sum of corrected areas: 3612452

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022721\
Data File : BM028922.D
Acq On : 26 Feb 2021 16:56
Operator : CG/JU
Sample : PB134805BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK05

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

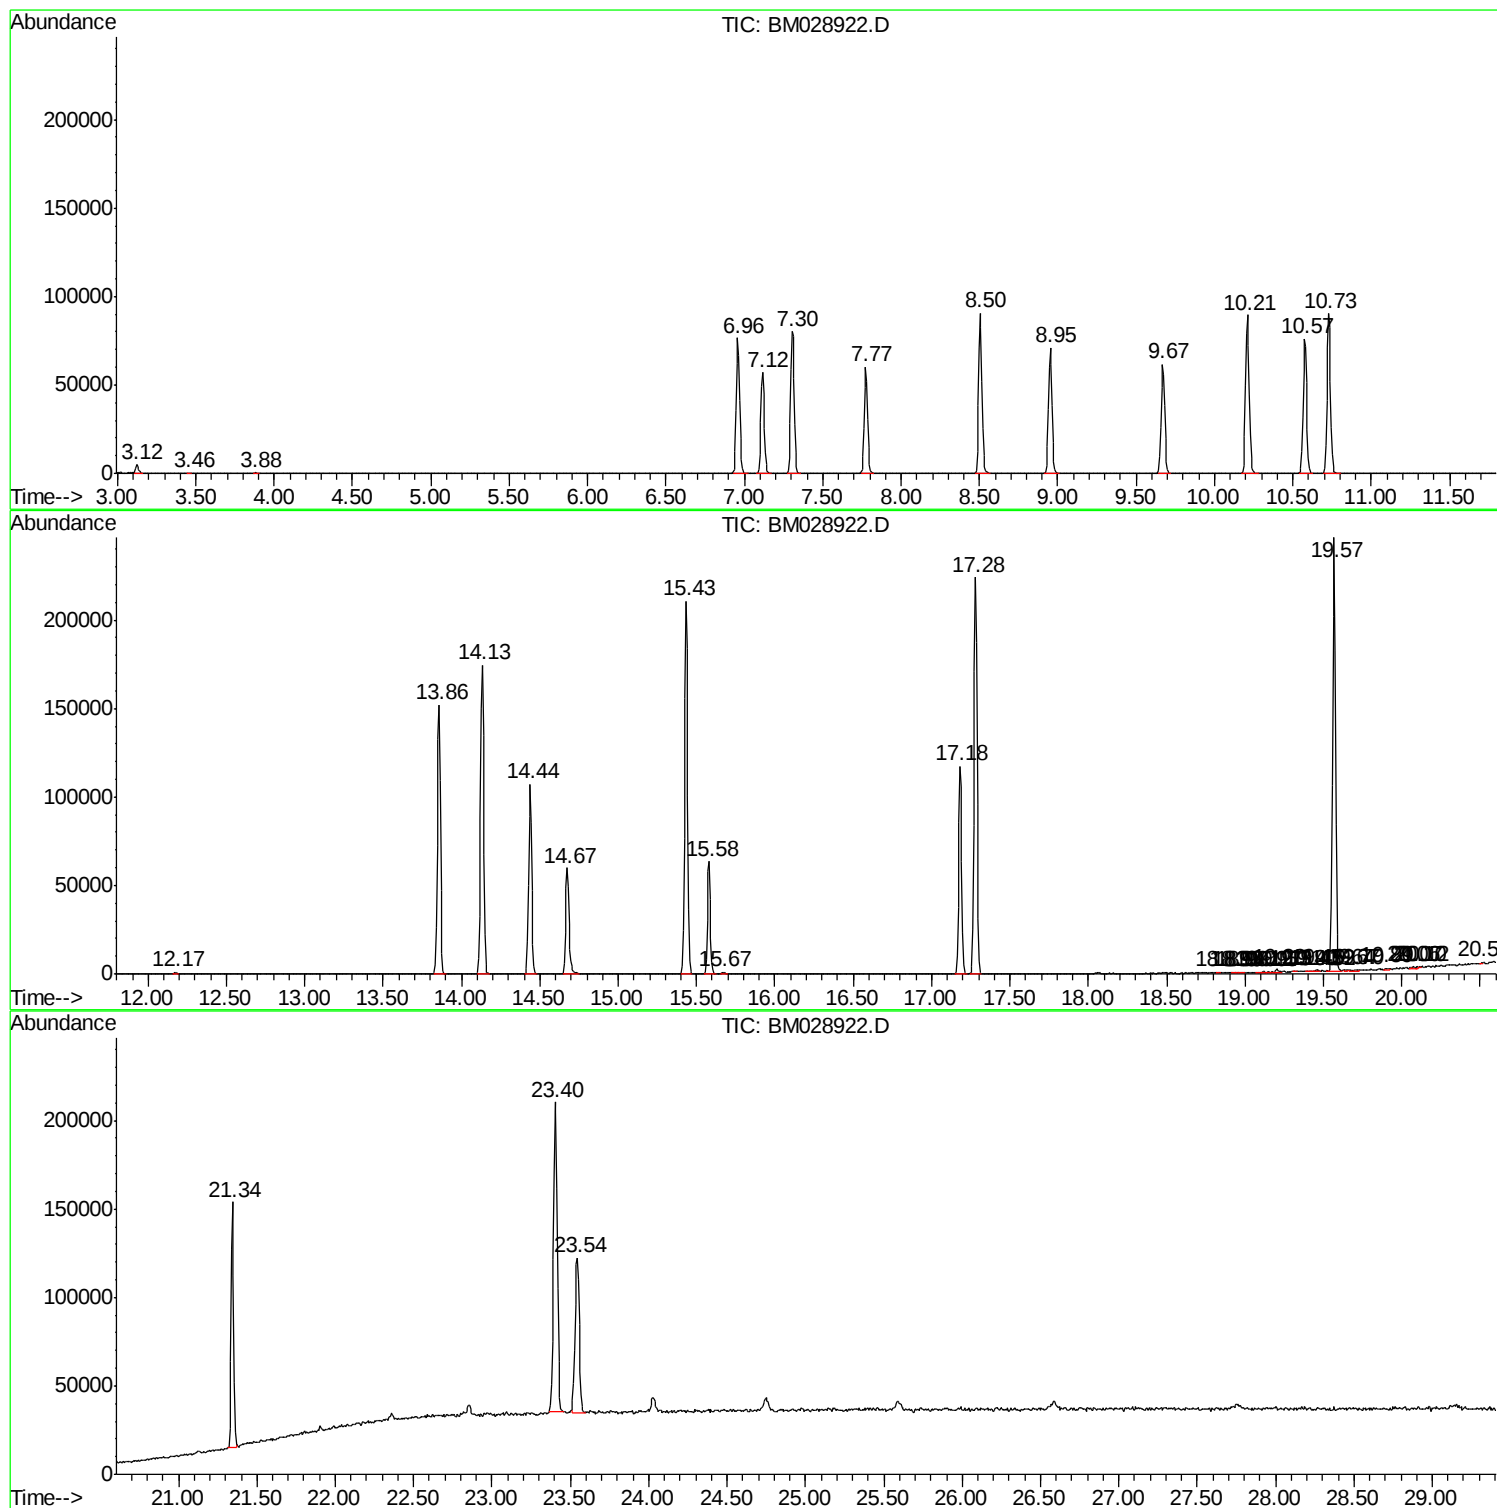

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022721\
Data File : BM028922.D
Acq On : 26 Feb 2021 16:56
Operator : CG/JU
Sample : PB134805BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK05

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022721\
Data File : BM028922.D
Acq On : 26 Feb 2021 16:56
Operator : CG/JU
Sample : PB134805BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK05

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc