

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022721\
 Data File : BM028935.D
 Acq On : 27 Feb 2021 00:50
 Operator : CG/JU
 Sample : M1482-10DL2 50X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBGN1DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.016	3	5	7	rVV	330	255	0.12%	0.020%
2	3.281	49	50	55	rVB	260	231	0.11%	0.018%
3	3.340	57	60	61	rBV	206	228	0.10%	0.017%
4	3.887	149	153	156	rVB	333	383	0.18%	0.029%
5	7.128	701	704	705	rBB	389	395	0.18%	0.030%
6	7.769	808	813	821	rBB	61216	96073	43.97%	7.367%
7	8.134	874	875	879	rBB	410	402	0.18%	0.031%
8	8.310	901	905	910	rBB	3209	4793	2.19%	0.368%
9	8.957	1013	1015	1018	rBB	393	377	0.17%	0.029%
10	10.575	1283	1290	1294	rBV	86426	141446	64.74%	10.847%
11	10.622	1294	1298	1306	rVB	82896	130334	59.65%	9.994%
12	10.745	1314	1319	1325	rBB	2785	4024	1.84%	0.309%
13	12.463	1607	1611	1616	rBB	4991	7177	3.28%	0.550%
14	13.269	1744	1748	1752	rBB	1371	1958	0.90%	0.150%
15	13.851	1843	1847	1851	rBB	1787	2245	1.03%	0.172%
16	14.133	1891	1895	1898	rBB	1779	2047	0.94%	0.157%
17	14.433	1941	1946	1952	rBB	131655	186845	85.52%	14.328%
18	14.498	1953	1957	1962	rBB	11771	15299	7.00%	1.173%
19	14.586	1968	1972	1977	rBB	2381	3301	1.51%	0.253%
20	14.839	2011	2015	2019	rBV	4162	5654	2.59%	0.434%
21	14.880	2019	2022	2026	rVB	803	974	0.45%	0.075%
22	15.433	2112	2116	2119	rBB	3061	3593	1.64%	0.276%
23	15.486	2120	2125	2129	rBB	4359	5577	2.55%	0.428%
24	16.968	2375	2377	2379	rBB	285	246	0.11%	0.019%
25	17.180	2407	2413	2418	rBV	152358	215780	98.76%	16.547%
26	17.221	2418	2420	2425	rVB	2662	2860	1.31%	0.219%
27	17.280	2426	2430	2435	rBB2	3534	4494	2.06%	0.345%
28	17.515	2468	2470	2474	rBB	208	316	0.14%	0.024%
29	17.592	2478	2483	2489	rVB	11435	15232	6.97%	1.168%
30	18.104	2568	2570	2572	rBV	402	273	0.12%	0.021%
31	18.457	2626	2630	2633	rBV	168	255	0.12%	0.020%
32	18.868	2698	2700	2703	rBV	256	279	0.13%	0.021%
33	18.933	2708	2711	2714	rVB	337	496	0.23%	0.038%
34	18.968	2714	2717	2719	rBV	320	395	0.18%	0.030%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022721\
 Data File : BM028935.D
 Acq On : 27 Feb 2021 00:50
 Operator : CG/JU
 Sample : M1482-10DL2 50X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBGN1DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
 Title : SVOA CALIBRATION

35	18.998	2719	2722	2723	rVB	419	323	0.15%	0.025%
36	19.015	2723	2725	2726	rBV	431	259	0.12%	0.020%
37	19.039	2727	2729	2730	rVB	413	225	0.10%	0.017%
38	19.051	2730	2731	2734	rBV	238	256	0.12%	0.020%
39	19.104	2737	2740	2741	rBV	358	252	0.12%	0.019%
40	19.127	2741	2744	2745	rBV	254	286	0.13%	0.022%
41	19.157	2748	2749	2752	rBV	436	453	0.21%	0.035%
42	19.180	2752	2753	2755	rBV	413	283	0.13%	0.022%
43	19.327	2776	2778	2780	rBV	528	414	0.19%	0.032%
44	19.345	2780	2781	2783	rVV	334	256	0.12%	0.020%
45	19.362	2783	2784	2787	rBV2	327	377	0.17%	0.029%
46	19.433	2794	2796	2799	rBV2	355	237	0.11%	0.018%
47	19.504	2806	2808	2812	rVB2	375	247	0.11%	0.019%
48	19.562	2814	2818	2825	rBV2	4878	6248	2.86%	0.479%
49	19.792	2855	2857	2860	rBV2	480	501	0.23%	0.038%
50	19.833	2862	2864	2865	rBV2	398	381	0.17%	0.029%
51	19.892	2870	2874	2875	rBV	493	504	0.23%	0.039%
52	19.909	2875	2877	2878	rBV	431	301	0.14%	0.023%
53	19.945	2882	2883	2884	rBV	669	300	0.14%	0.023%
54	19.974	2887	2888	2889	rBV	449	284	0.13%	0.022%
55	20.027	2894	2897	2899	rVB3	747	842	0.39%	0.065%
56	20.051	2899	2901	2902	rBV2	439	447	0.20%	0.034%
57	20.080	2905	2906	2908	rBV2	797	614	0.28%	0.047%
58	20.662	3003	3005	3006	rBV2	1227	831	0.38%	0.064%
59	21.339	3115	3120	3128	rBV	187577	218493	100.00%	16.755%
60	22.845	3373	3376	3382	rVB2	8380	11916	5.45%	0.914%
61	23.533	3488	3493	3503	rVB2	114270	204299	93.50%	15.666%


Sum of corrected areas: 1304066

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022721\
Data File : BM028935.D
Acq On : 27 Feb 2021 00:50
Operator : CG/JU
Sample : M1482-10DL2 50X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBGN1DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

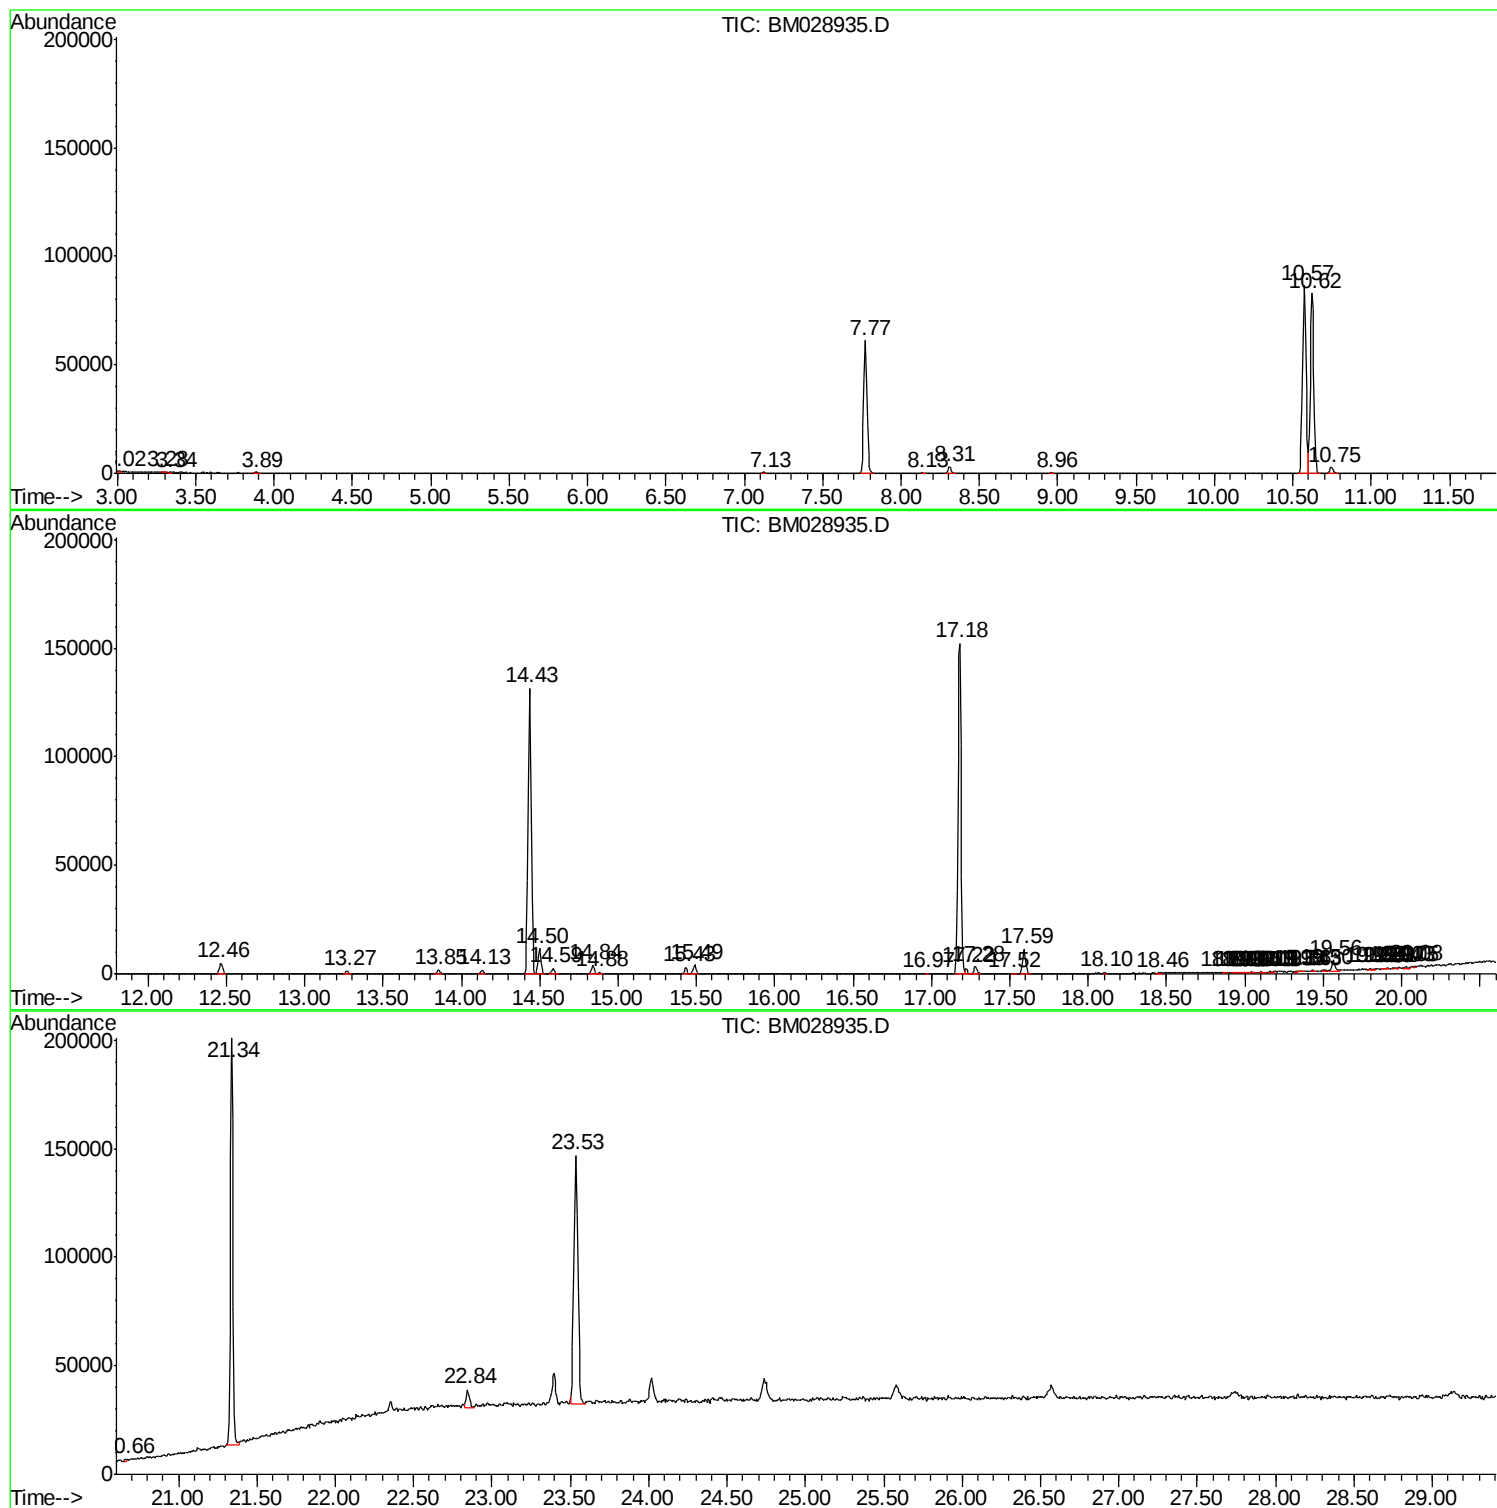

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022721\
Data File : BM028935.D
Acq On : 27 Feb 2021 00:50
Operator : CG/JU
Sample : M1482-10DL2 50X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBGN1DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022721\
Data File : BM028935.D
Acq On : 27 Feb 2021 00:50
Operator : CG/JU
Sample : M1482-10DL2 50X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBGN1DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc